

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113021\
 Data File : PP041469.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2021 6:32
 Operator : AJ\MA
 Sample : M4068-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 07:45:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.746	3.750	408773	617794	18.128	20.338
2)	SA Decachlor...	10.640	9.007	430746	312013	20.004	20.188
Target Compounds							
26)	L6 AR-1254-1	6.967	5.866	23738	32473	27.969	23.328
27)	L6 AR-1254-2	7.196	6.026	36085	29993	27.392	25.115
28)	L6 AR-1254-3	7.578	6.444	36189	44855	25.407	25.338
29)	L6 AR-1254-4	7.874	6.684	24550	20877	23.662	20.255
30)	L6 AR-1254-5	8.300	7.112	21373	30690	19.043	21.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113021\
Data File : PP041469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2021 6:32
Operator : AJ\MA
Sample : M4068-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 07:45:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

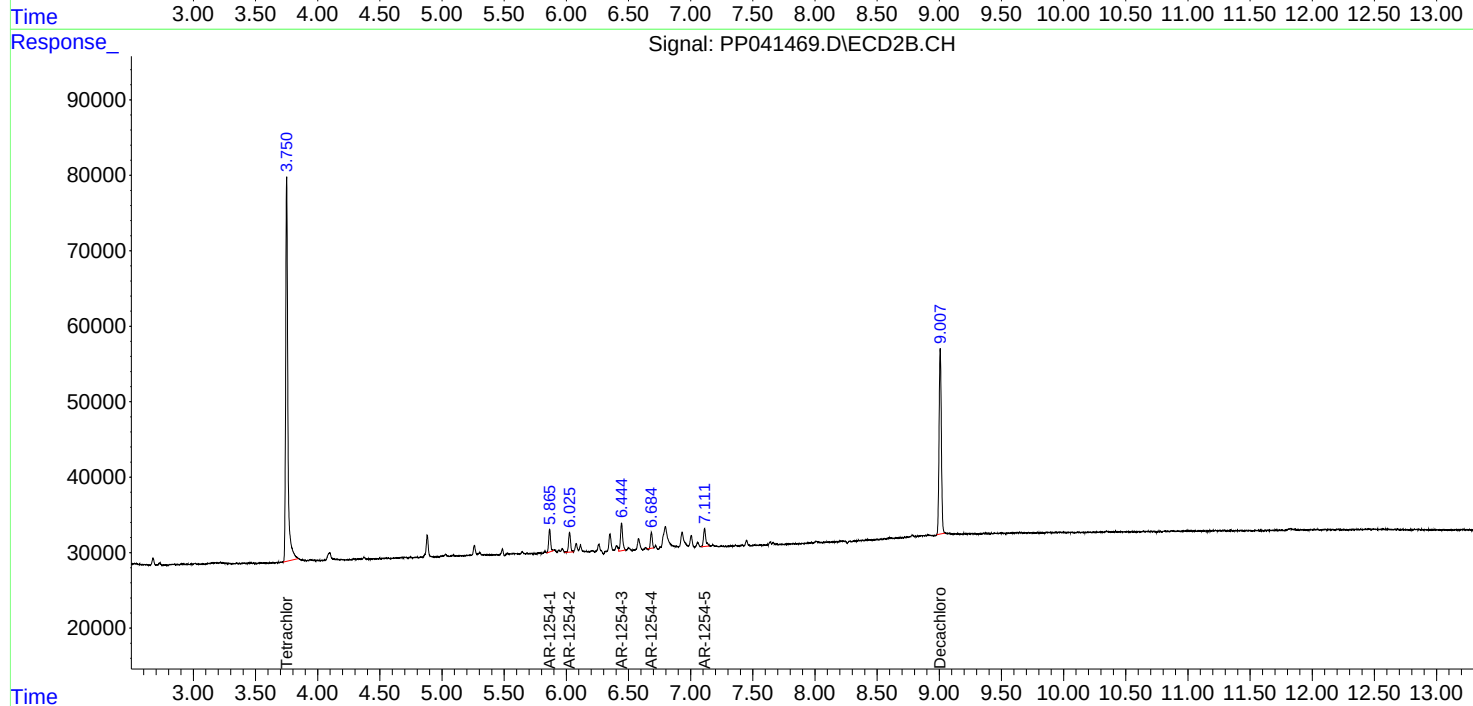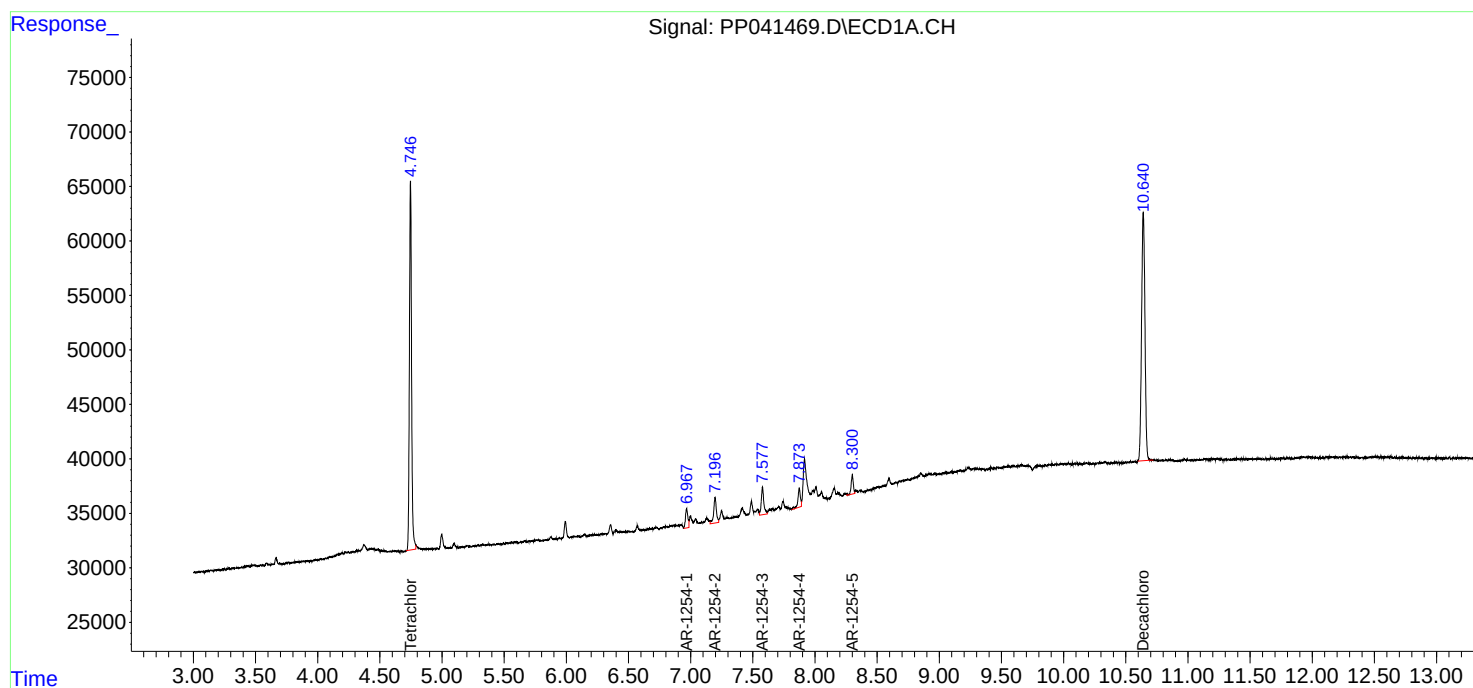


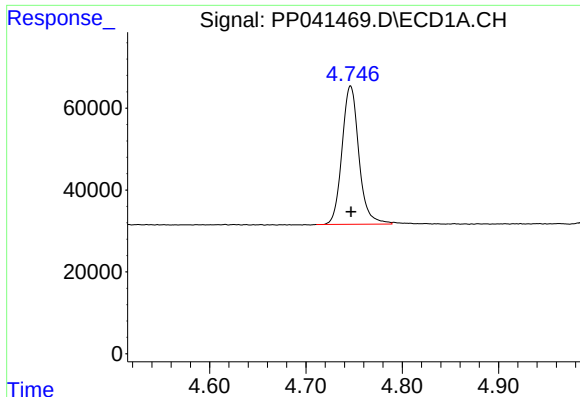

#1 Tetrachloro-m-xylene


R.T.: 4.746 min
Delta R.T.: 0.000 min
Response: 408773
Conc: 18.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2021

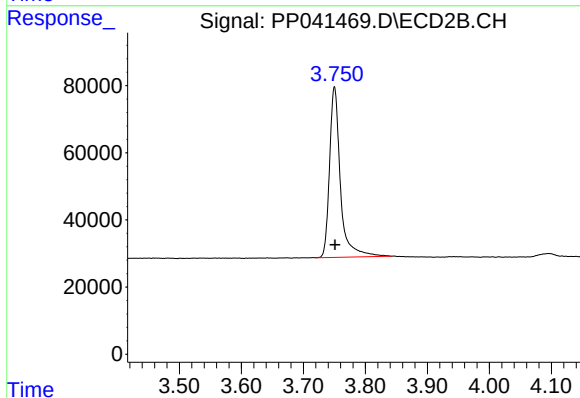


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.001 min
Response: 617794
Conc: 20.34 ng/ml

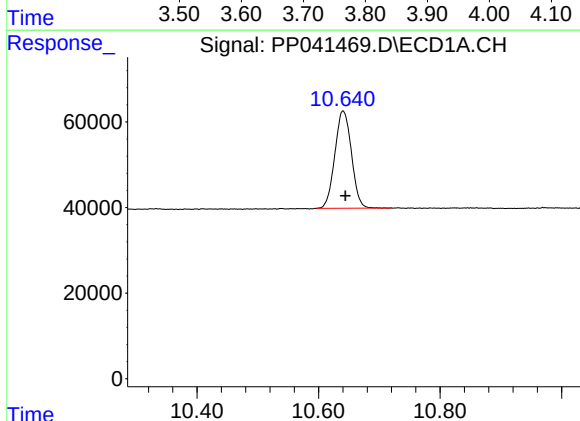


#2 Decachlorobiphenyl

R.T.: 10.640 min
Delta R.T.: -0.004 min
Response: 430746
Conc: 20.00 ng/ml

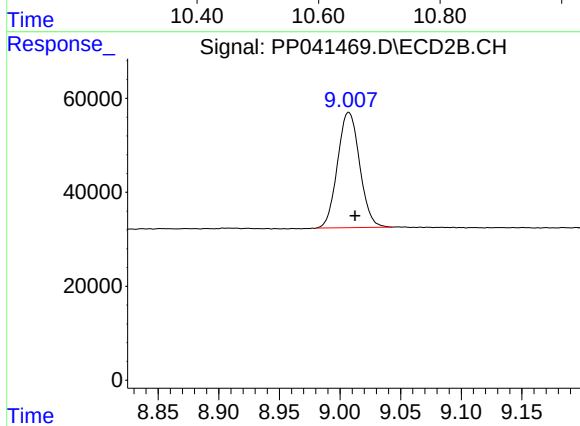

#2 Decachlorobiphenyl


R.T.: 9.007 min
Delta R.T.: -0.005 min
Response: 312013
Conc: 20.19 ng/ml

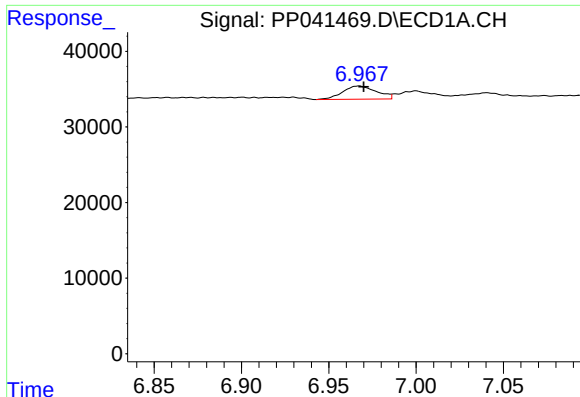

#26 AR-1254-1


R.T.: 6.967 min
Delta R.T.: -0.003 min
Response: 23738
Conc: 27.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2021

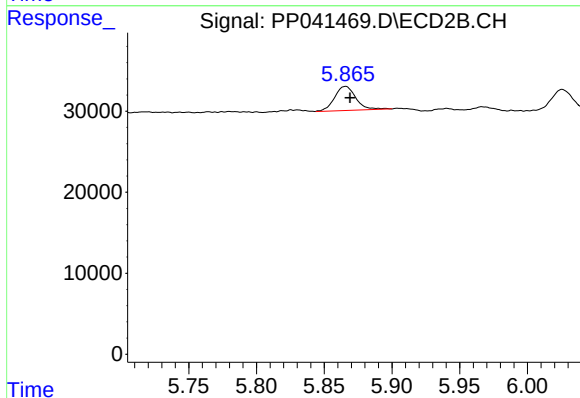


#26 AR-1254-1

R.T.: 5.866 min
Delta R.T.: -0.003 min
Response: 32473
Conc: 23.33 ng/ml

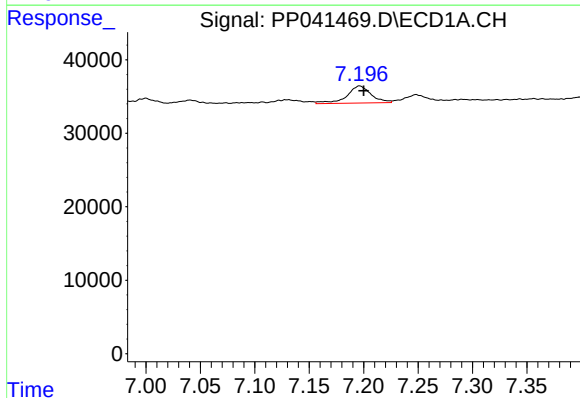


#27 AR-1254-2

R.T.: 7.196 min
Delta R.T.: -0.004 min
Response: 36085
Conc: 27.39 ng/ml

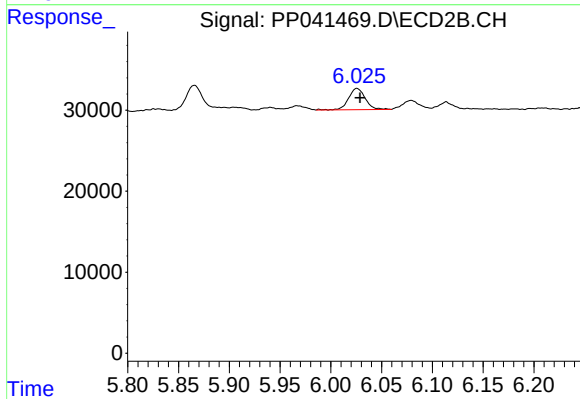

#27 AR-1254-2


R.T.: 6.026 min
Delta R.T.: -0.003 min
Response: 29993
Conc: 25.11 ng/ml

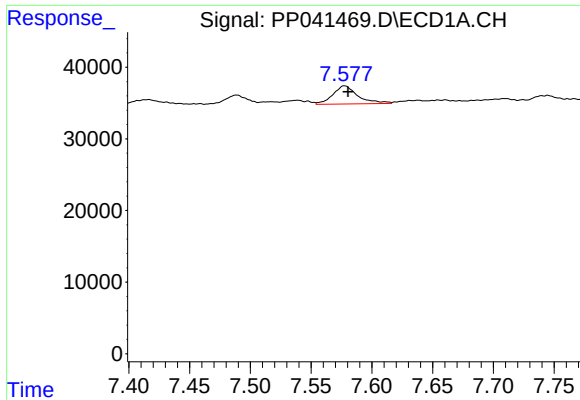

#28 AR-1254-3


R.T.: 7.578 min
Delta R.T.: -0.003 min
Response: 36189
Conc: 25.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2021

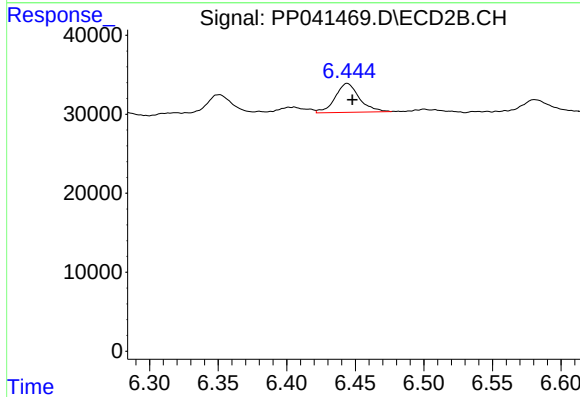


#28 AR-1254-3

R.T.: 6.444 min
Delta R.T.: -0.004 min
Response: 44855
Conc: 25.34 ng/ml

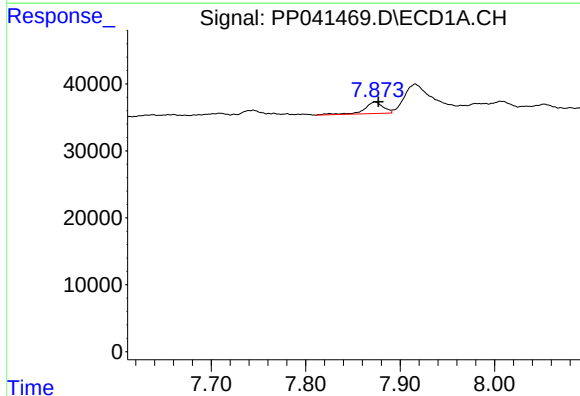


#29 AR-1254-4

R.T.: 7.874 min
Delta R.T.: -0.004 min
Response: 24550
Conc: 23.66 ng/ml

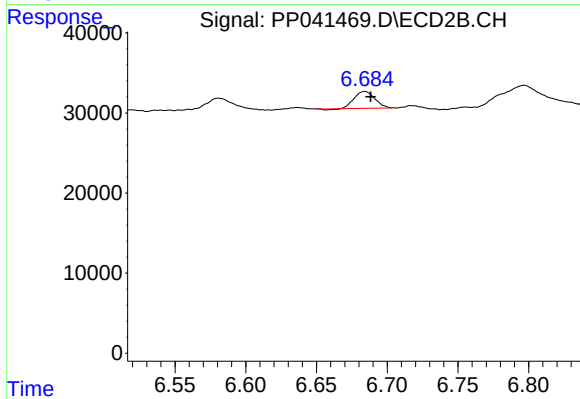

#29 AR-1254-4


R.T.: 6.684 min
Delta R.T.: -0.004 min
Response: 20877
Conc: 20.26 ng/ml

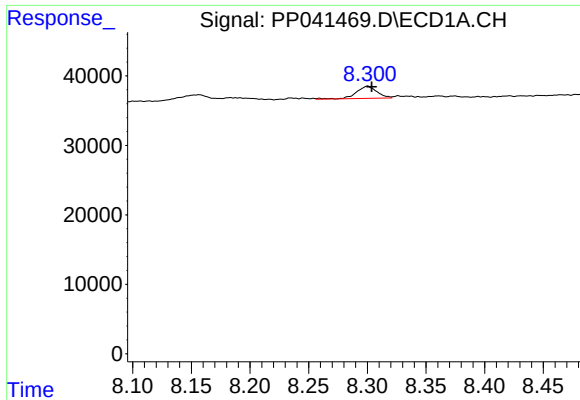

#30 AR-1254-5

R.T.: 8.300 min
Delta R.T.: -0.004 min
Response: 21373
Conc: 19.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2021

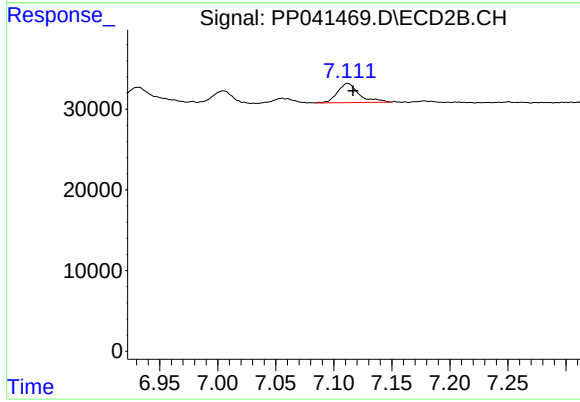

#30 AR-1254-5

R.T.: 7.112 min
Delta R.T.: -0.005 min
Response: 30690
Conc: 21.05 ng/ml