

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113022\
 Data File : PP053573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2022 16:54
 Operator : YP\AJ
 Sample : N5809-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HOWE-DRUM-B-1129

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2022
 Supervised By :Ankita Jodhani 12/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 20:30:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 09 05:50:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.646	32619613	29577208	16.969	19.662
2) SA Decachlor...	10.211	8.728	24044170	25708278	17.732	13.716m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP113022\
Data File : PP053573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2022 16:54
Operator : YP\AJ
Sample : N5809-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HOWE-DRUM-B-1129


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2022
Supervised By :Ankita Jodhani 12/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 20:30:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 09 05:50:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

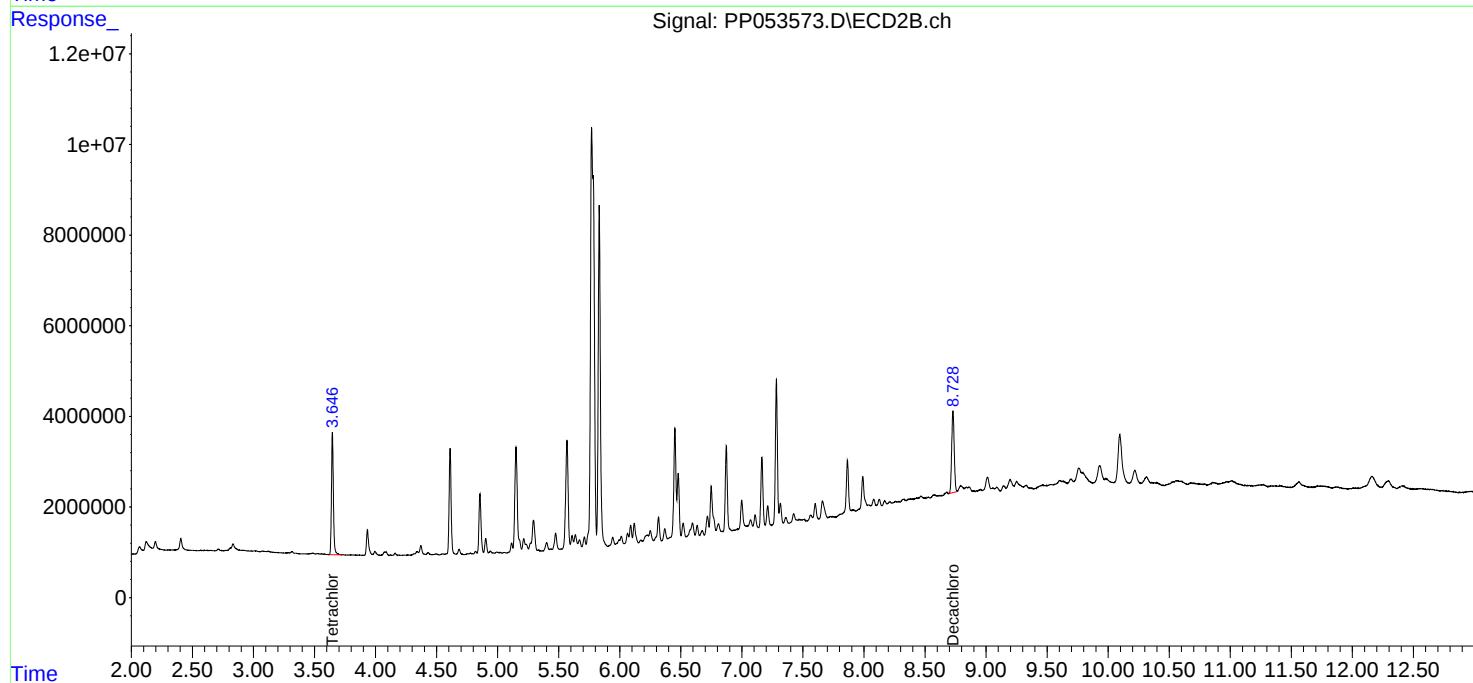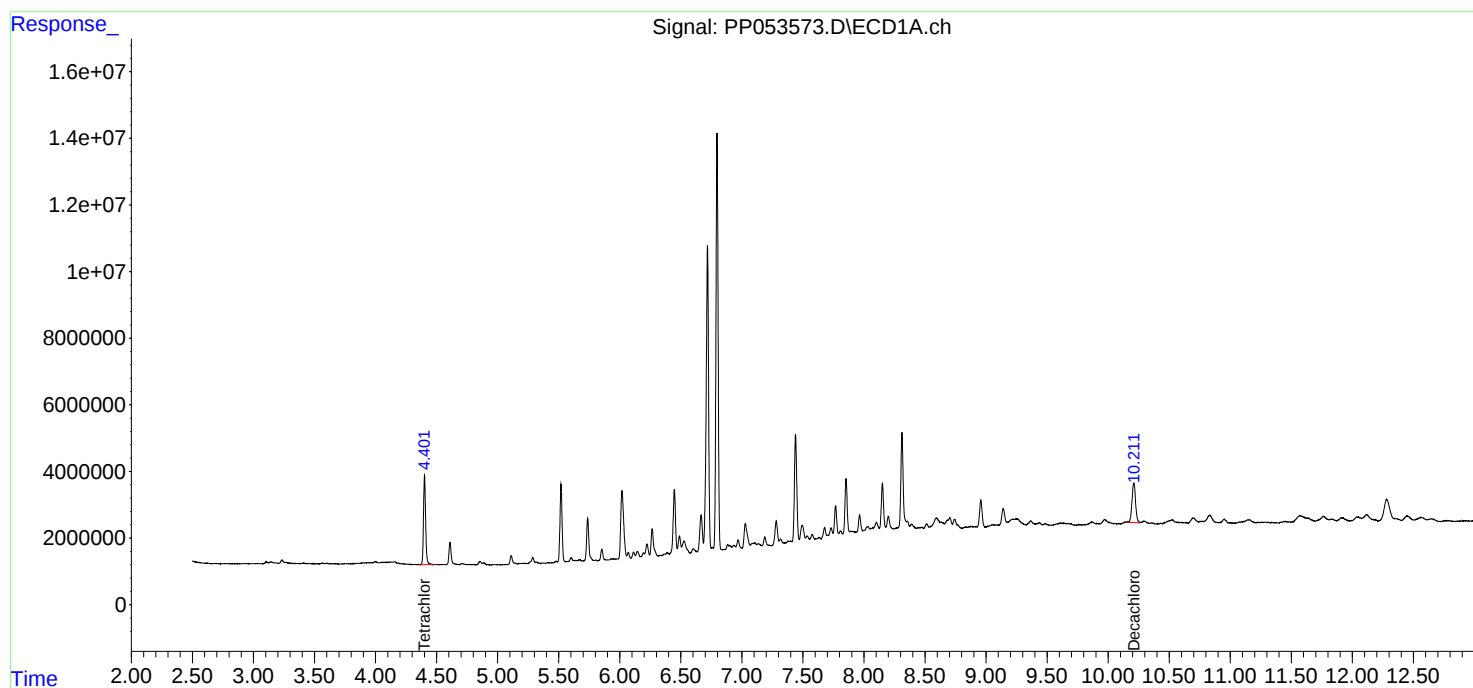

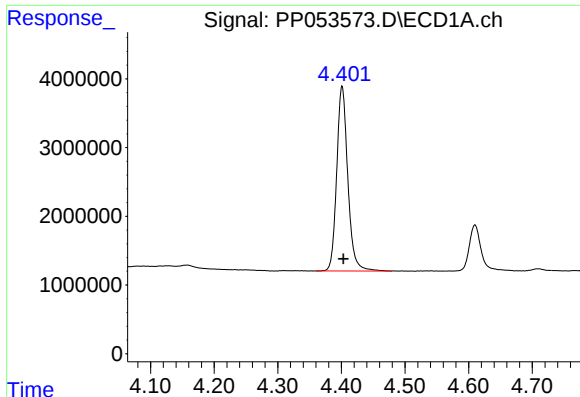


#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.002 min
Response: 32619613
Conc: 16.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOWE-DRUM-B-1129


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2022
Supervised By :Ankita Jodhani 12/01/2022

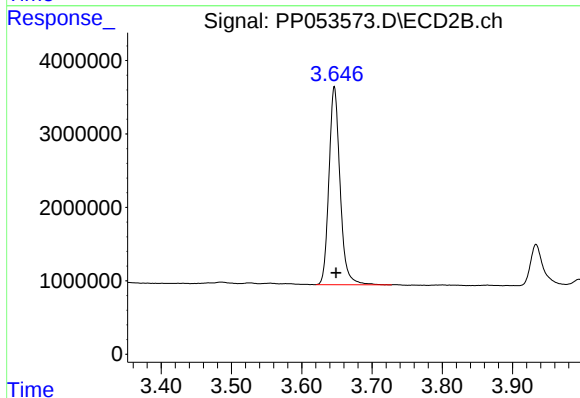


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.002 min
Response: 29577208
Conc: 19.66 ng/ml

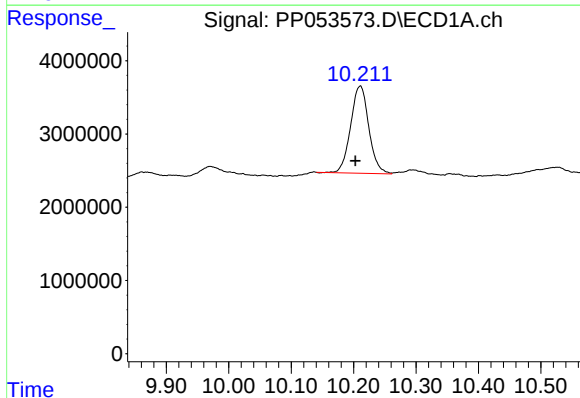

#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: 0.008 min
Response: 24044170
Conc: 17.73 ng/ml

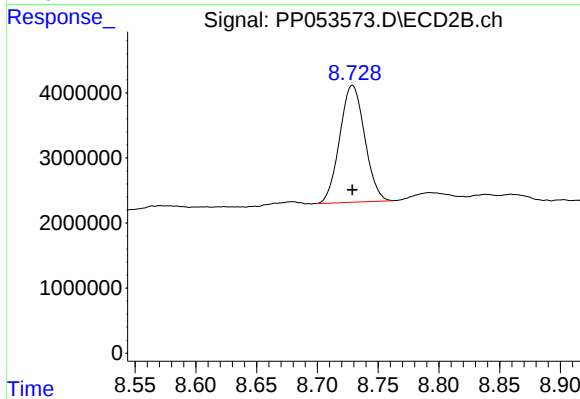

#2 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 25708278
Conc: 13.72 ng/ml m