

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
 Data File : PP041556.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 8:54
 Operator : AJ\MA
 Sample : PB141048BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 17:22:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.746	3.750	513186	732314	22.758	24.108
2)	SA Decachlor...	10.641	9.007	518117	355646	24.062	23.011
Target Compounds							
8)	L2 AR-1221-1	4.996	0.000	21670	0	82.445	N.D. #
9)	L2 AR-1221-2	5.098	4.098	8114	9971	43.296	36.220
24)	L5 AR-1248-4	6.977f	0.000	3647	0	4.354	N.D. #
26)	L6 AR-1254-1	6.977	0.000	3647	0	4.297	N.D. #
28)	L6 AR-1254-3	7.596f	0.000	3229	0	2.267	N.D. #
32)	L7 AR-1260-2	8.019	0.000	1327	0	1.056	N.D. #
33)	L7 AR-1260-3	0.000	6.949	0	15928	N.D.	11.908 #
45)	L9 AR-1268-5	10.355f	0.000	42122	0	5.827	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
Data File : PP041556.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 8:54
Operator : AJ\MA
Sample : PB141048BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 17:22:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

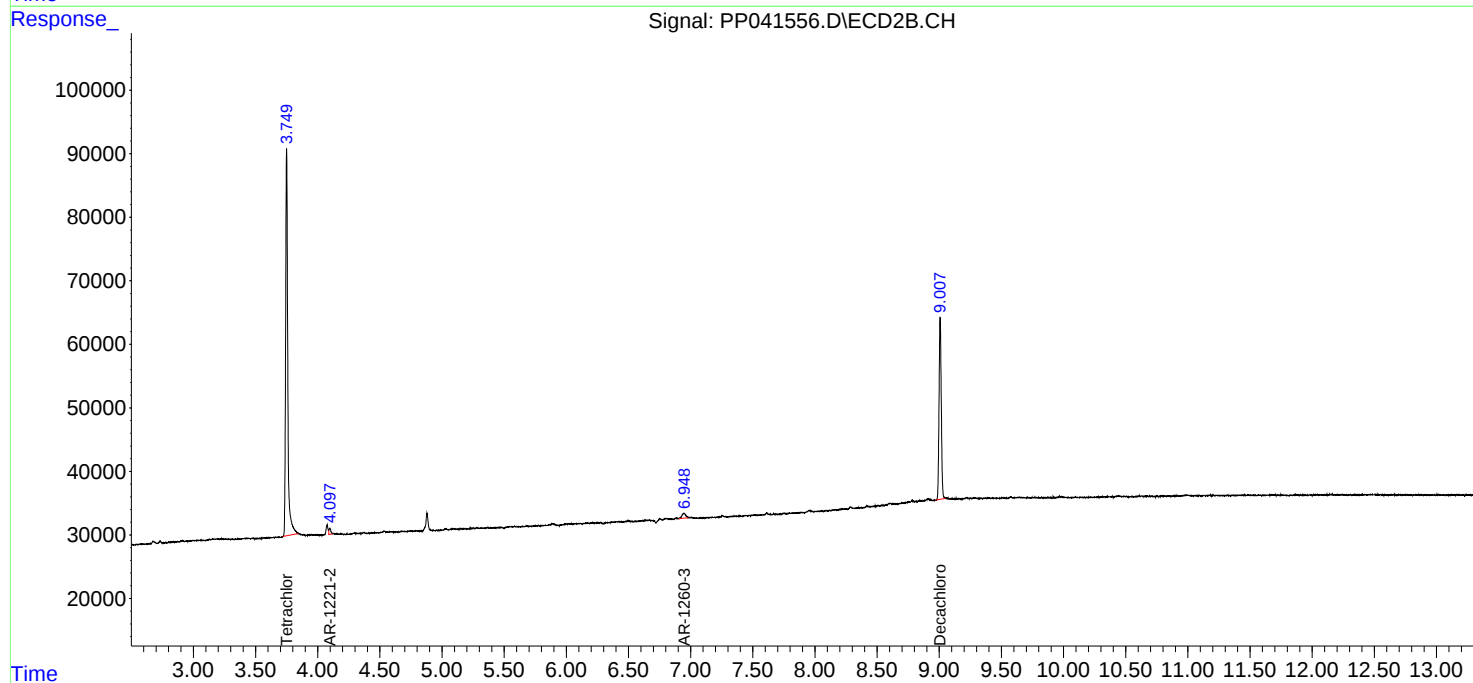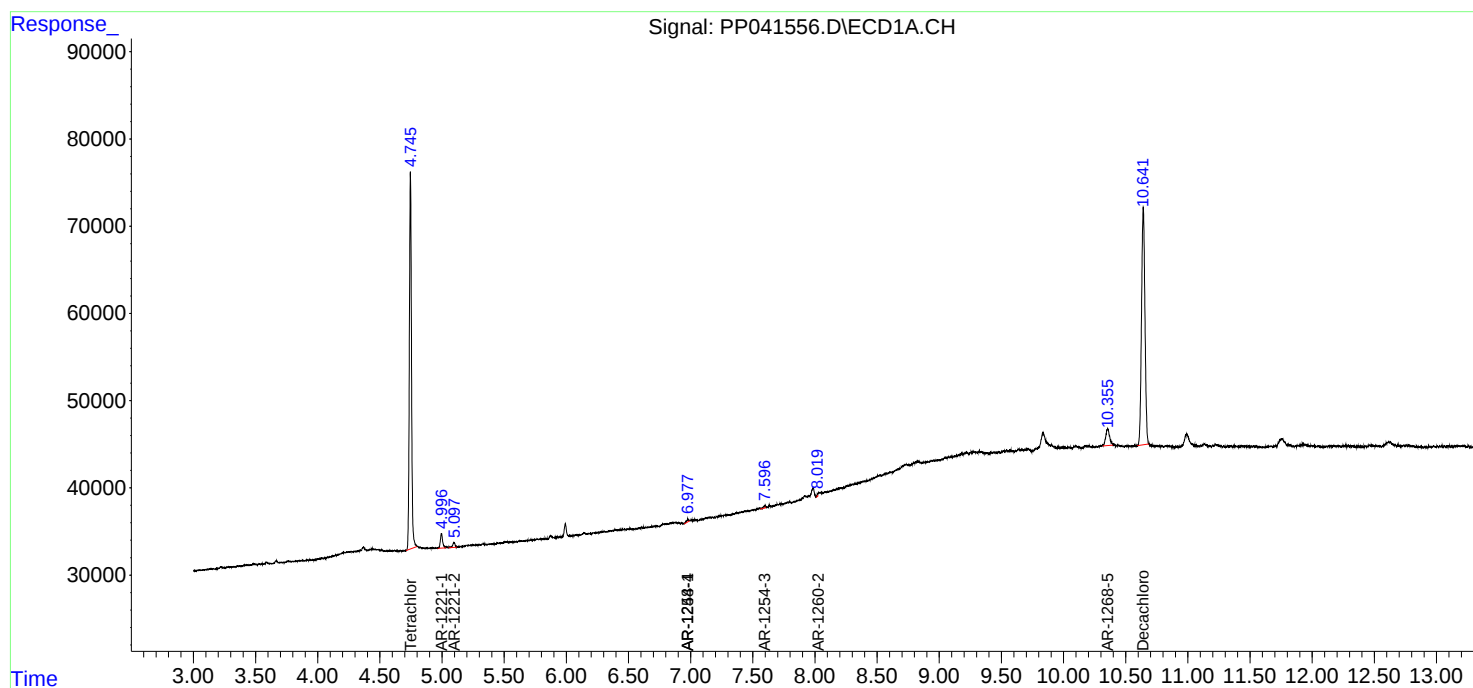


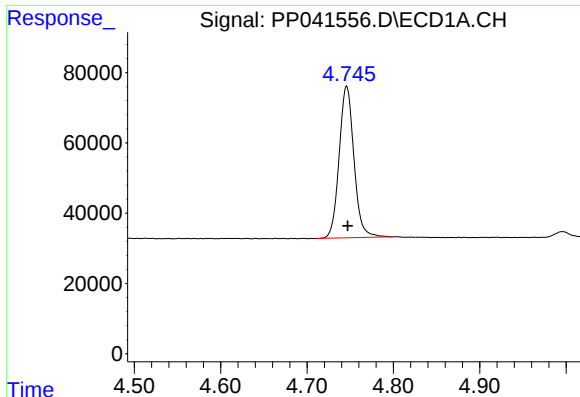

#1 Tetrachloro-m-xylene


R.T.: 4.746 min
Delta R.T.: -0.001 min
Response: 513186
Conc: 22.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

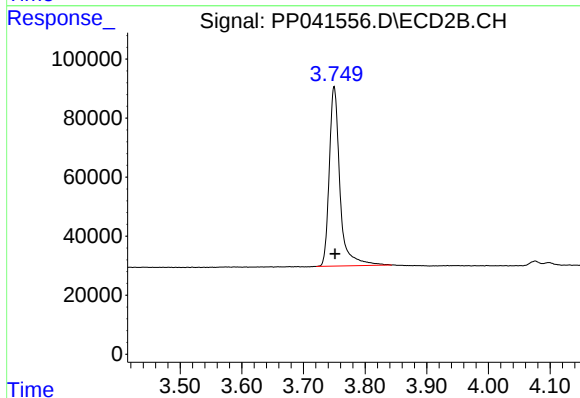


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.001 min
Response: 732314
Conc: 24.11 ng/ml

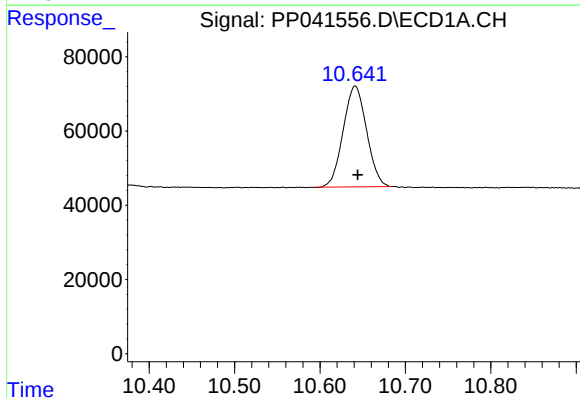


#2 Decachlorobiphenyl

R.T.: 10.641 min
Delta R.T.: -0.003 min
Response: 518117
Conc: 24.06 ng/ml

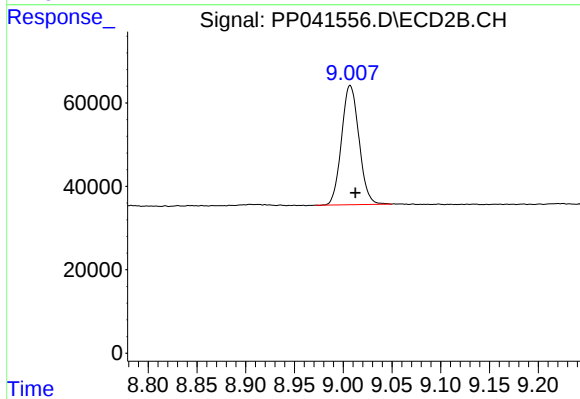

#2 Decachlorobiphenyl


R.T.: 9.007 min
Delta R.T.: -0.005 min
Response: 355646
Conc: 23.01 ng/ml

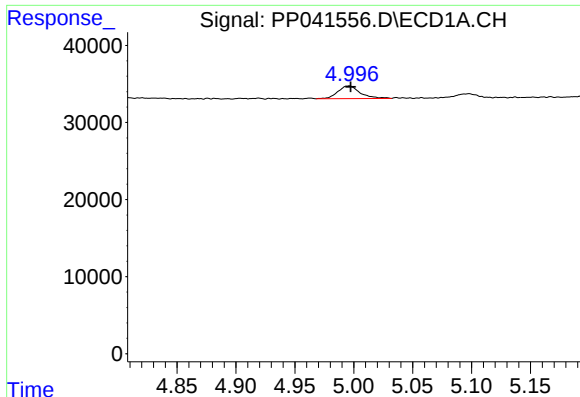

#8 AR-1221-1


R.T.: 4.996 min
Delta R.T.: -0.001 min
Response: 21670
Conc: 82.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

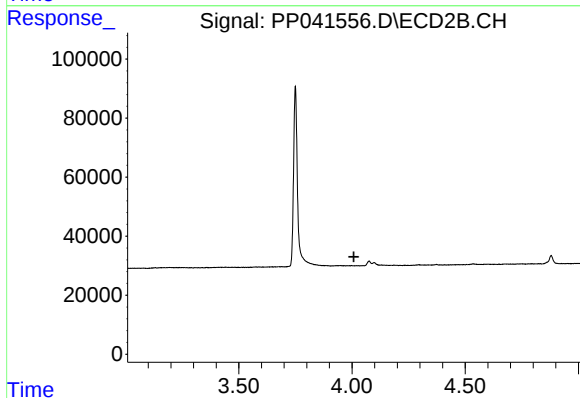


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.008 min
Response: 0
Conc: N.D.

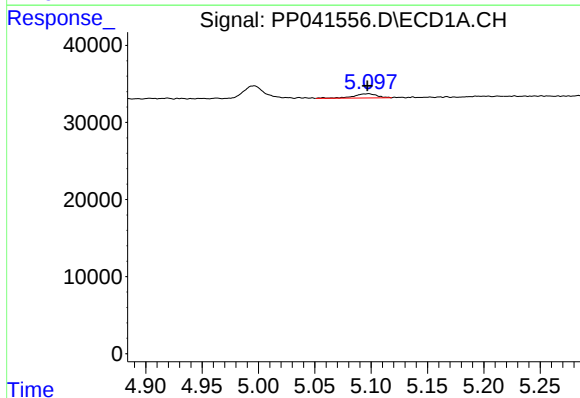


#9 AR-1221-2

R.T.: 5.098 min
Delta R.T.: 0.001 min
Response: 8114
Conc: 43.30 ng/ml

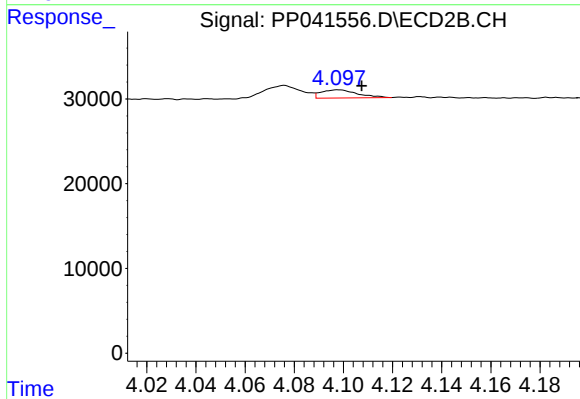

#9 AR-1221-2


R.T.: 4.098 min
Delta R.T.: -0.010 min
Response: 9971
Conc: 36.22 ng/ml

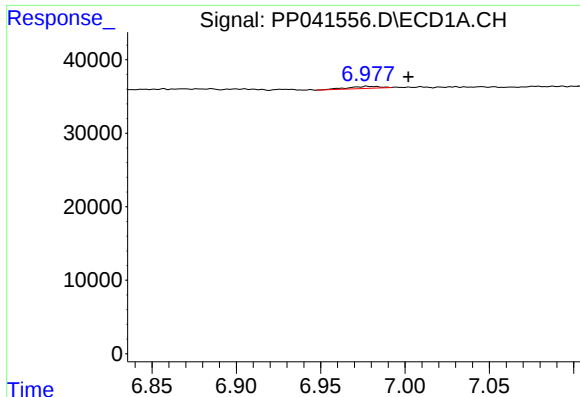

#24 AR-1248-4


R.T.: 6.977 min
Delta R.T.: -0.025 min
Response: 3647
Conc: 4.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

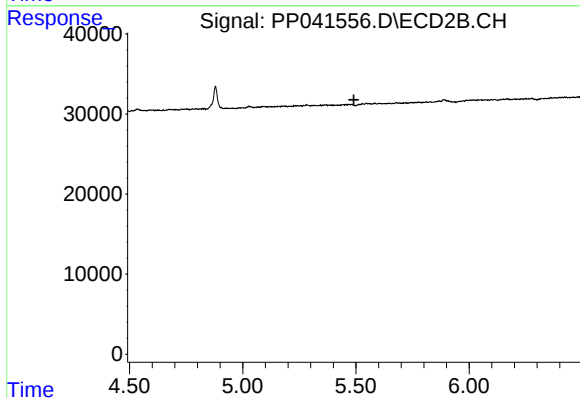


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

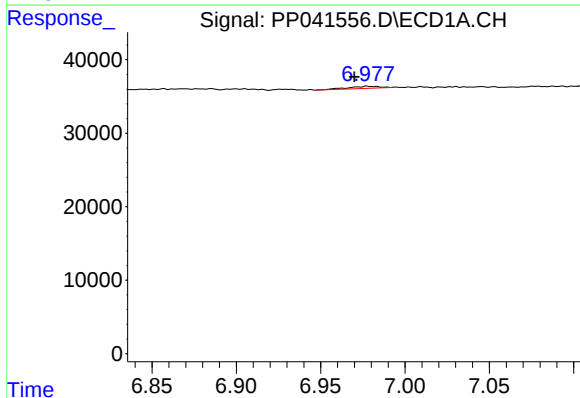


#26 AR-1254-1

R.T.: 6.977 min
Delta R.T.: 0.007 min
Response: 3647
Conc: 4.30 ng/ml

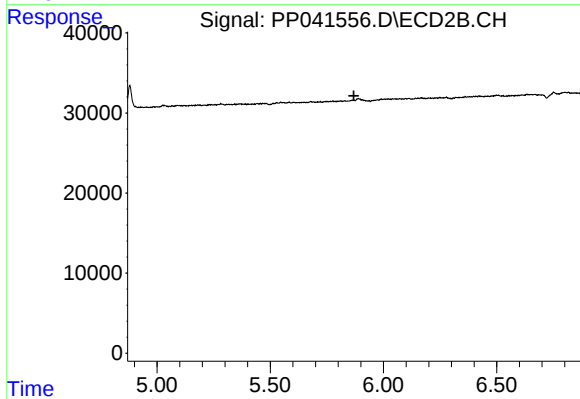

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.869 min
Response: 0
Conc: N.D.

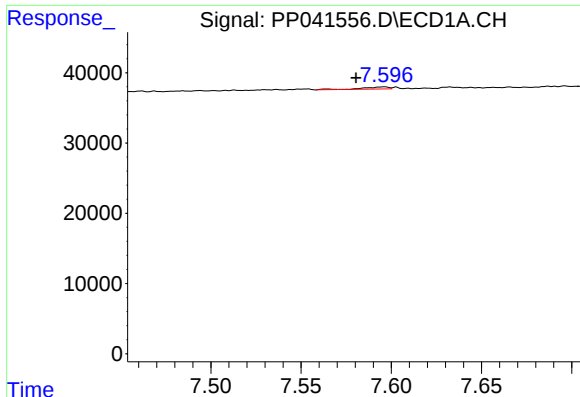

#28 AR-1254-3


R.T.: 7.596 min
Delta R.T.: 0.016 min
Response: 3229
Conc: 2.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

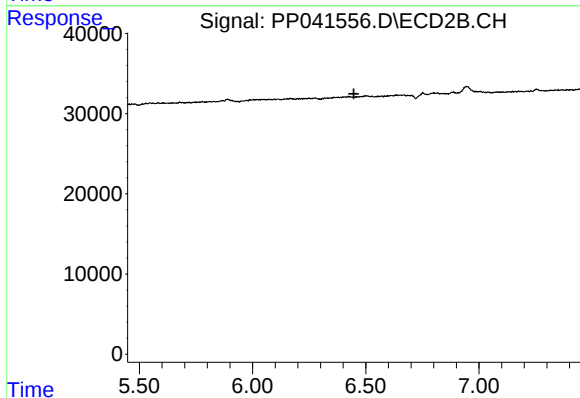


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.448 min
Response: 0
Conc: N.D.

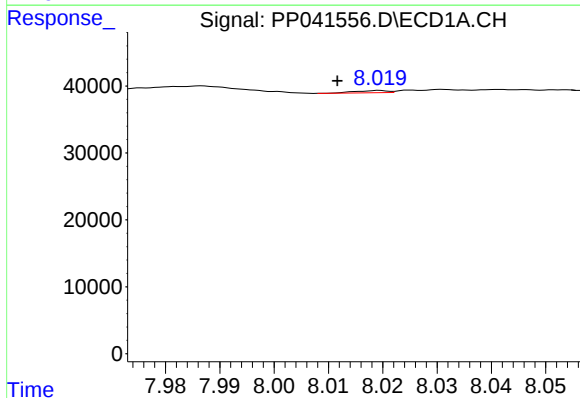


#32 AR-1260-2

R.T.: 8.019 min
Delta R.T.: 0.008 min
Response: 1327
Conc: 1.06 ng/ml

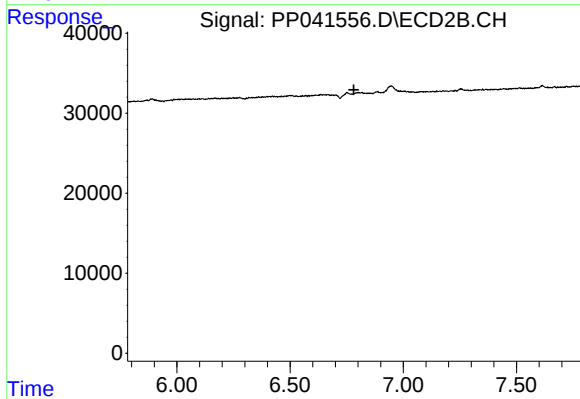

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

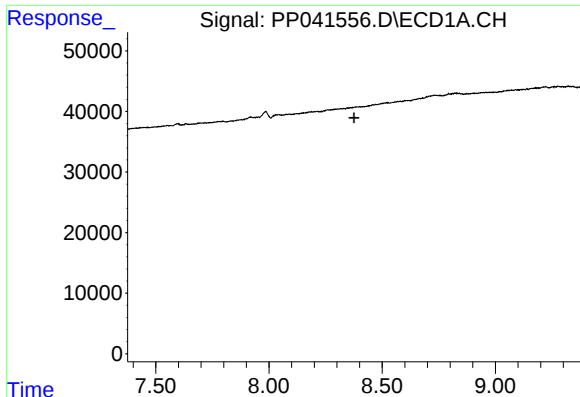

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

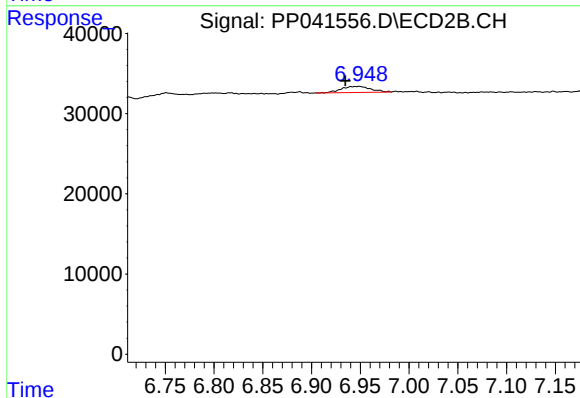


#33 AR-1260-3

R.T.: 6.949 min
Delta R.T.: 0.014 min
Response: 15928
Conc: 11.91 ng/ml

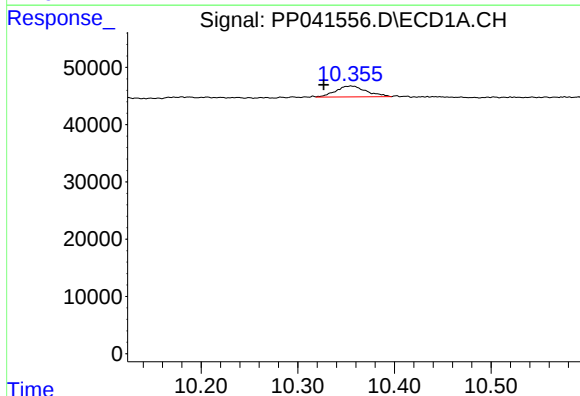

#45 AR-1268-5

R.T.: 10.355 min
Delta R.T.: 0.028 min
Response: 42122
Conc: 5.83 ng/ml

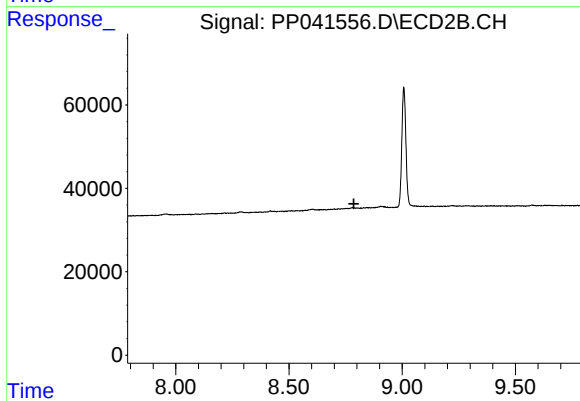

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 8.786 min
Response: 0
Conc: N.D.