

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
Data File : PP041536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 2:40
Operator : AJ\MA
Sample : M4866-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
30938

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 02:53:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.746	3.751	424704	484176	18.834	15.939
2) SA Decachlor...	10.642	9.008	291766	203566	13.550	13.171

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
Data File : PP041536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 2:40
Operator : AJ\MA
Sample : M4866-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
30938

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 02:53:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

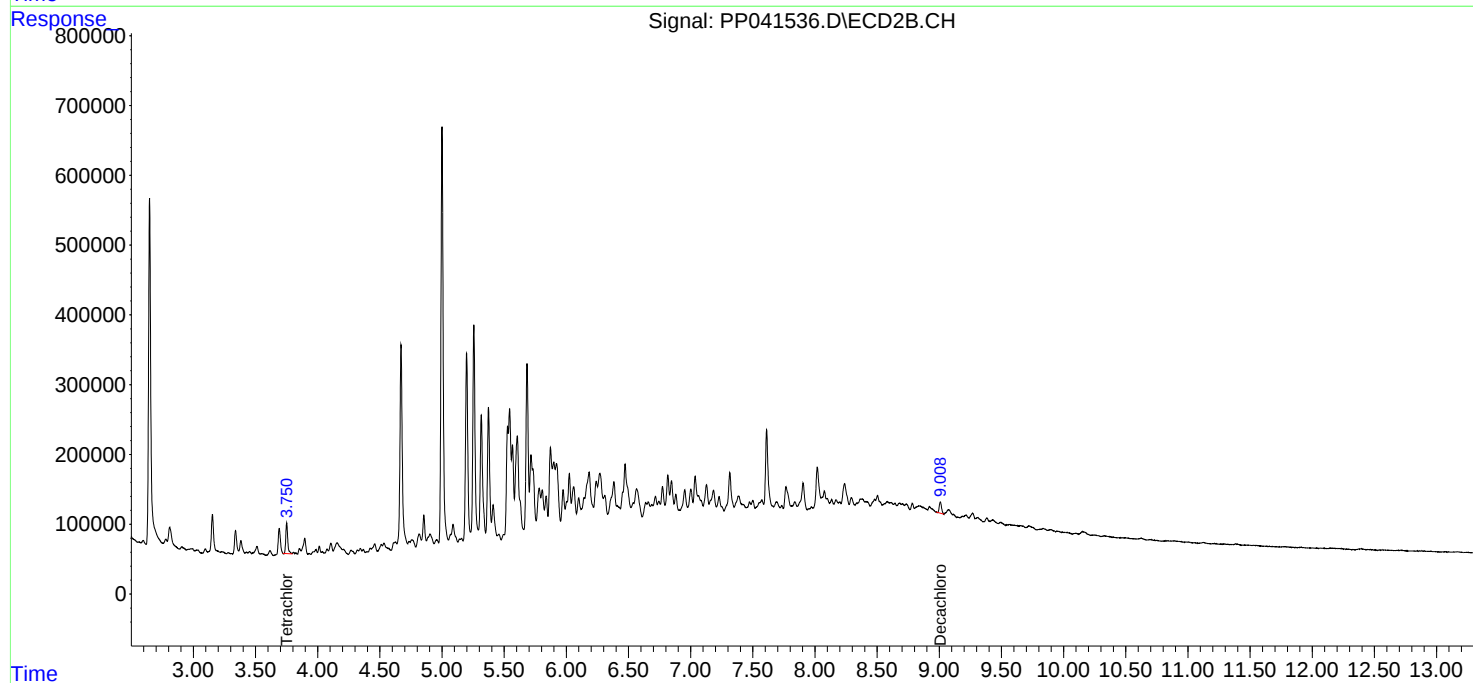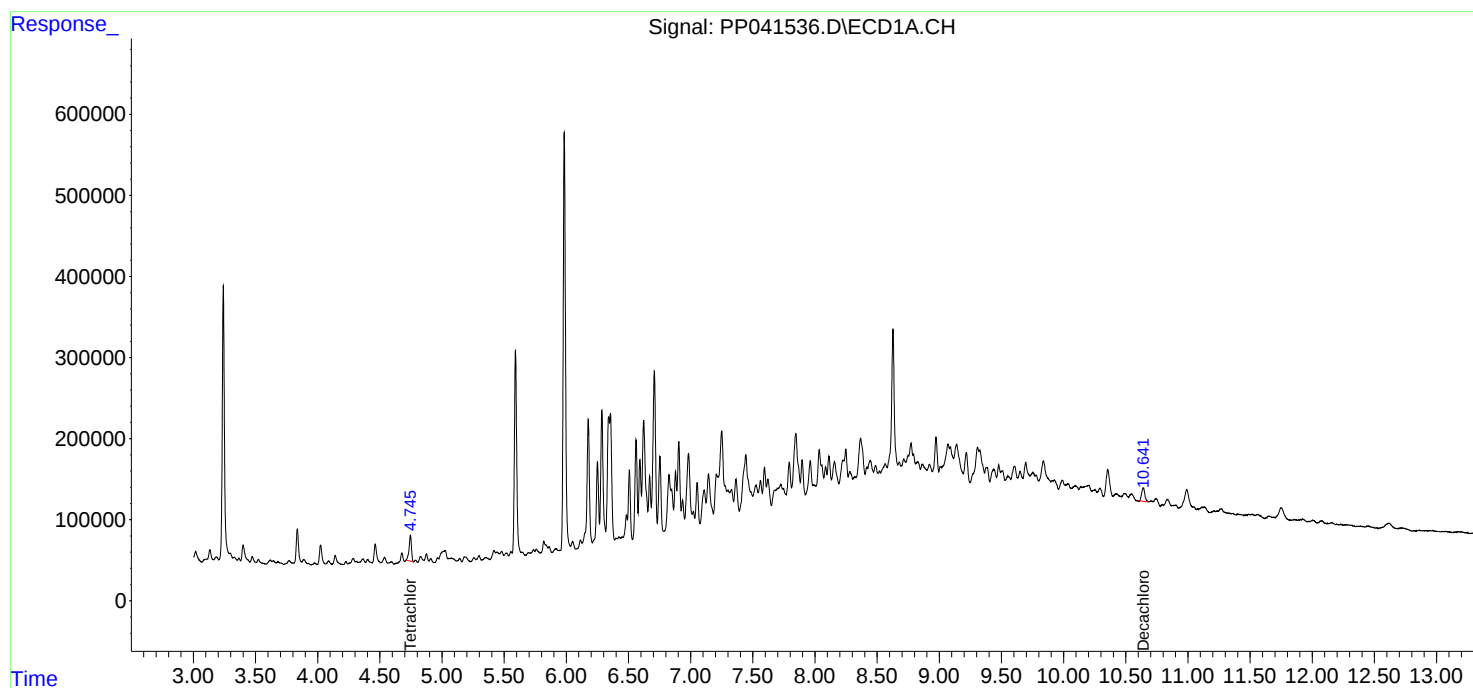


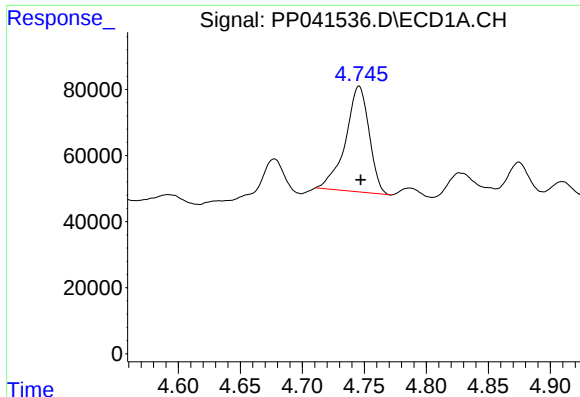

#1 Tetrachloro-m-xylene


R.T.: 4.746 min
Delta R.T.: -0.001 min
Response: 424704
Conc: 18.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
30938

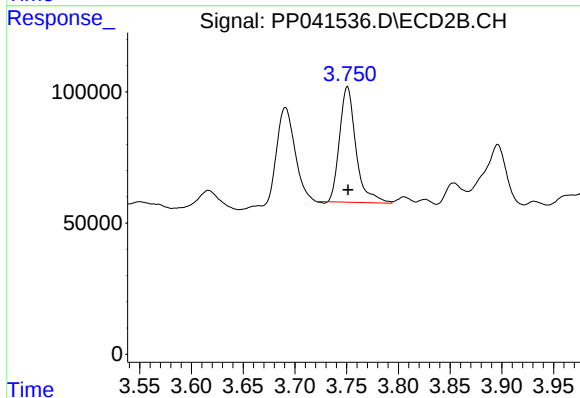


#1 Tetrachloro-m-xylene

R.T.: 3.751 min
Delta R.T.: 0.000 min
Response: 484176
Conc: 15.94 ng/ml

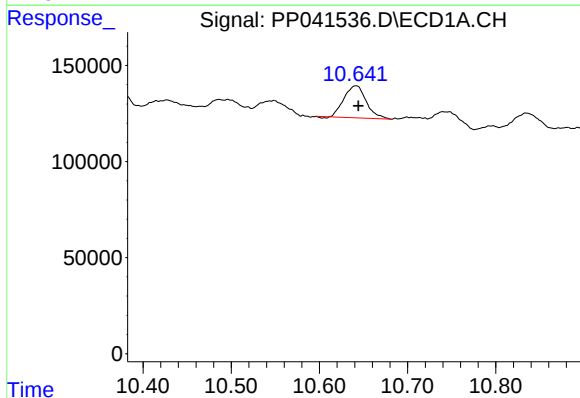

#2 Decachlorobiphenyl

R.T.: 10.642 min
Delta R.T.: -0.003 min
Response: 291766
Conc: 13.55 ng/ml

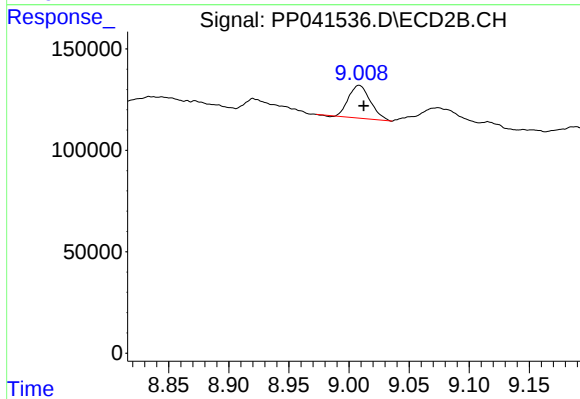

#2 Decachlorobiphenyl

R.T.: 9.008 min
Delta R.T.: -0.004 min
Response: 203566
Conc: 13.17 ng/ml