

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
 Data File : PP041538.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 3:13
 Operator : AJ\MA
 Sample : M4866-06 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 16941

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/02/2021
 Supervised By :mohammad ahmed 12/02/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 04:28:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.743	3.748	56890	77760	2.523m	2.560m
2) SA Decachlor...	10.637	9.006	112063	56094	5.204m	3.629m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
Data File : PP041538.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 3:13
Operator : AJ\MA
Sample : M4866-06 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
16941


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/02/2021
Supervised By :mohammad ahmed 12/02/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 04:28:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

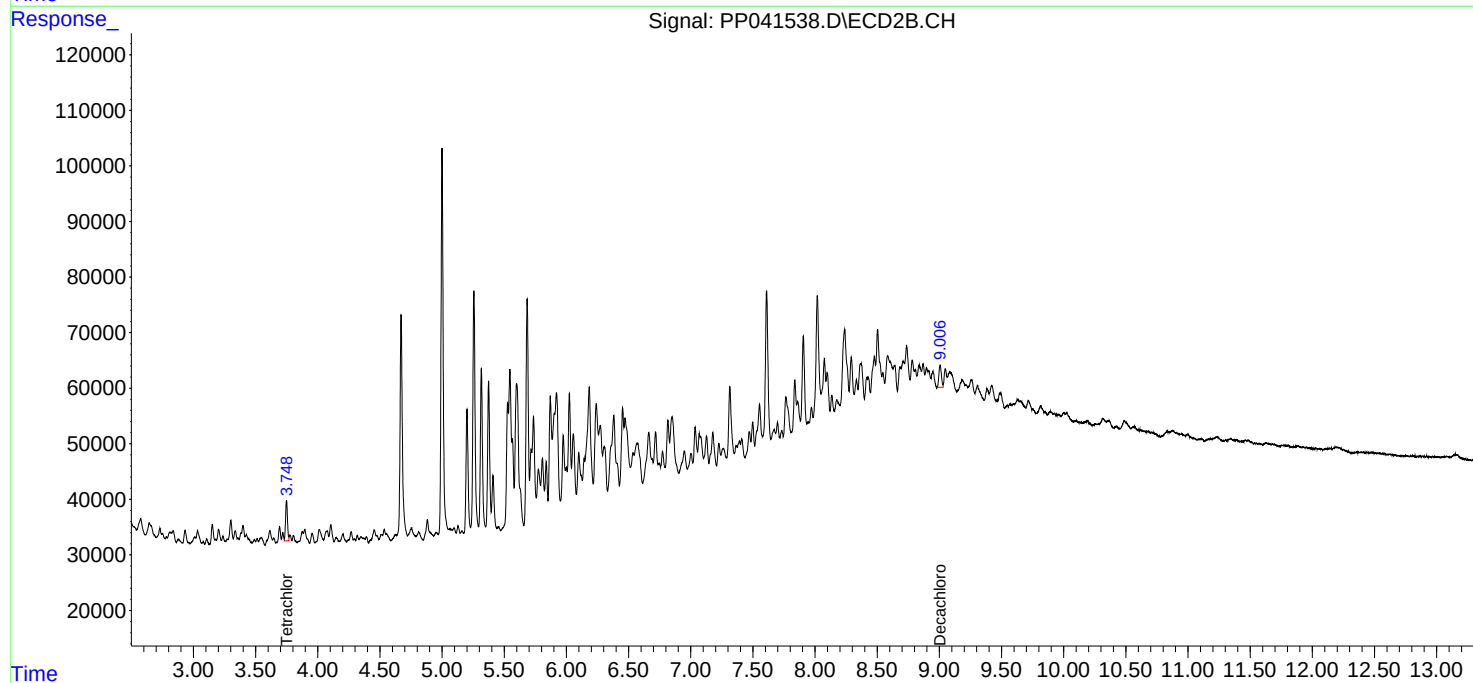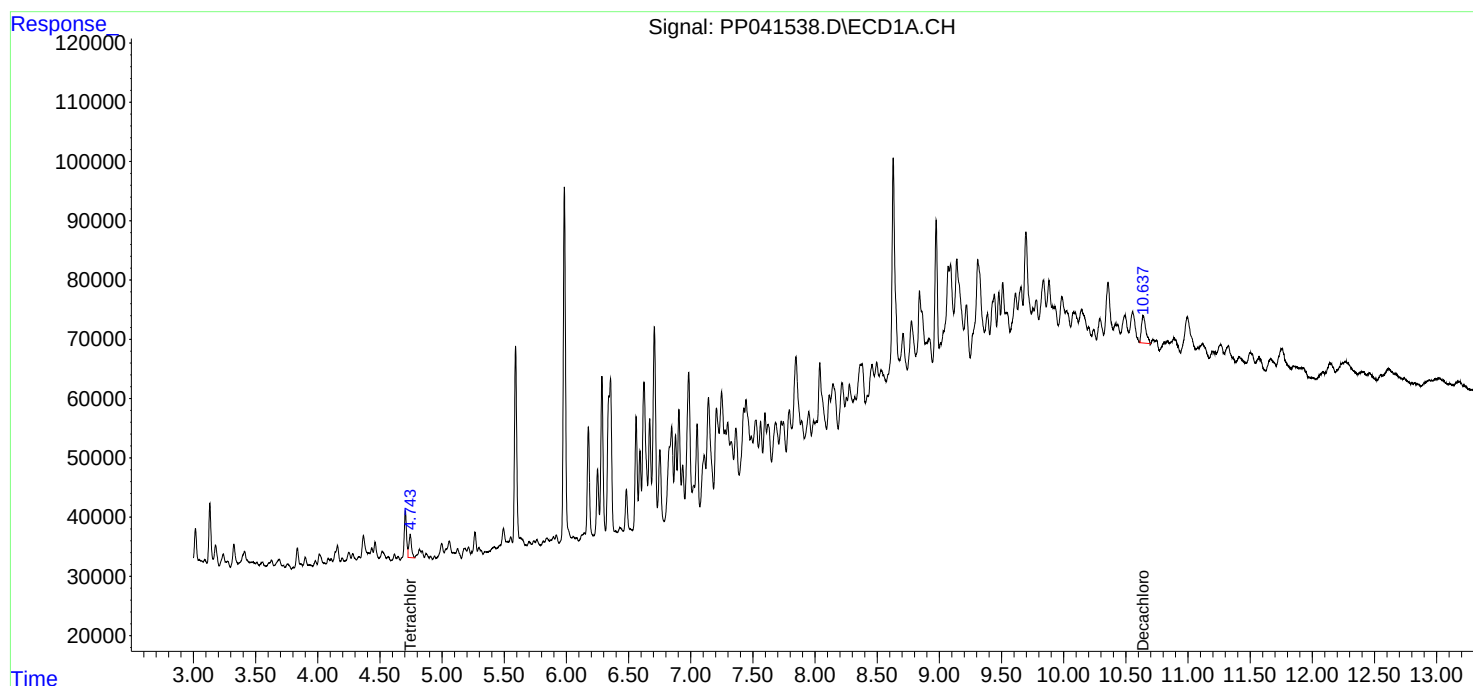

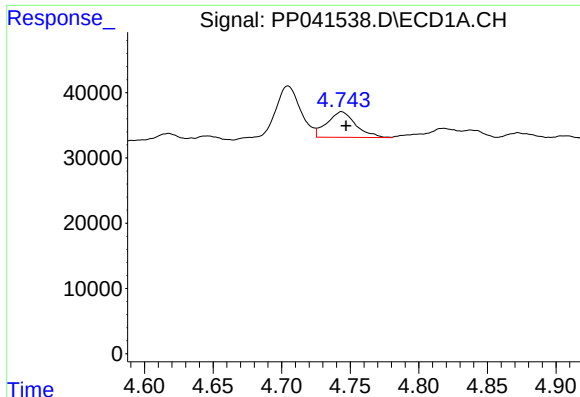


#1 Tetrachloro-m-xylene

R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 56890
Conc: 2.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
16941


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/02/2021
Supervised By :mohammad ahmed 12/02/2021

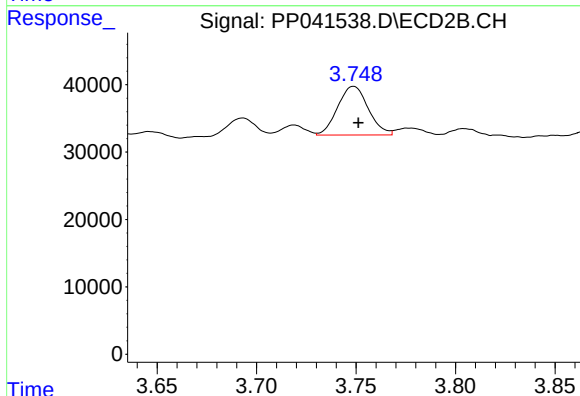


#1 Tetrachloro-m-xylene

R.T.: 3.748 min
Delta R.T.: -0.003 min
Response: 77760
Conc: 2.56 ng/ml m

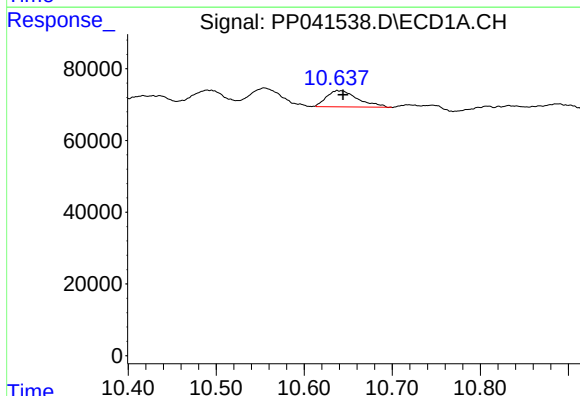

#2 Decachlorobiphenyl

R.T.: 10.637 min
Delta R.T.: -0.007 min
Response: 112063
Conc: 5.20 ng/ml m

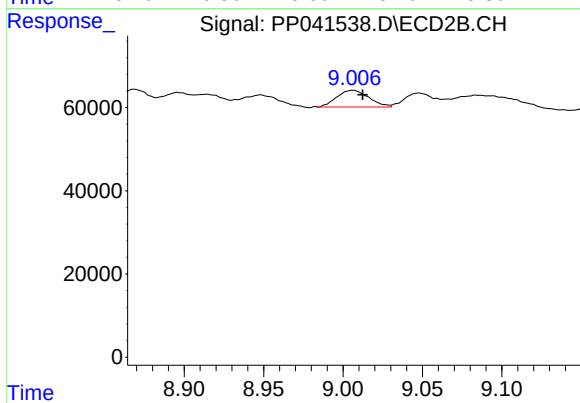

#2 Decachlorobiphenyl

R.T.: 9.006 min
Delta R.T.: -0.007 min
Response: 56094
Conc: 3.63 ng/ml m