

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
 Data File : PP041561.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 10:18
 Operator : AJ\MA
 Sample : M4068-07
 Misc : AR1248 LOD 25 PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 17:23:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.748	3.751	506223	720390	22.449	23.716
2) SA Decachlor...	10.645	9.009	522169	362908	24.250	23.481
Target Compounds						
21) L5 AR-1248-1	6.063	4.998	11663	14016	26.642	25.647
22) L5 AR-1248-2	6.356	5.260	15084	19954	24.323	24.509
23) L5 AR-1248-3	6.571	5.304	18618	20460	24.920	24.160
24) L5 AR-1248-4	7.001	5.488	22689	23008	27.086	23.592
25) L5 AR-1248-5	7.039	5.909	19357	24167	23.261	26.991



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
Data File : PP041561.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 10:18
Operator : AJ\MA
Sample : M4068-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 17:23:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

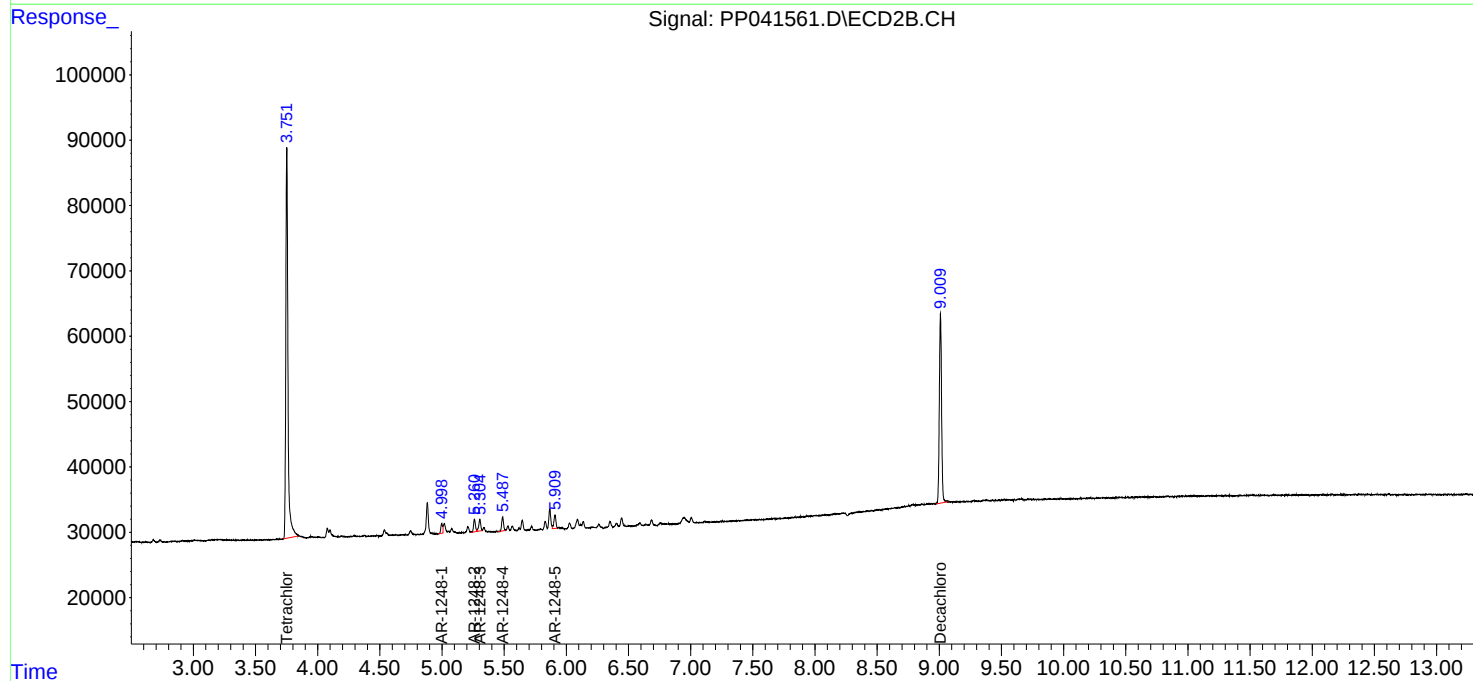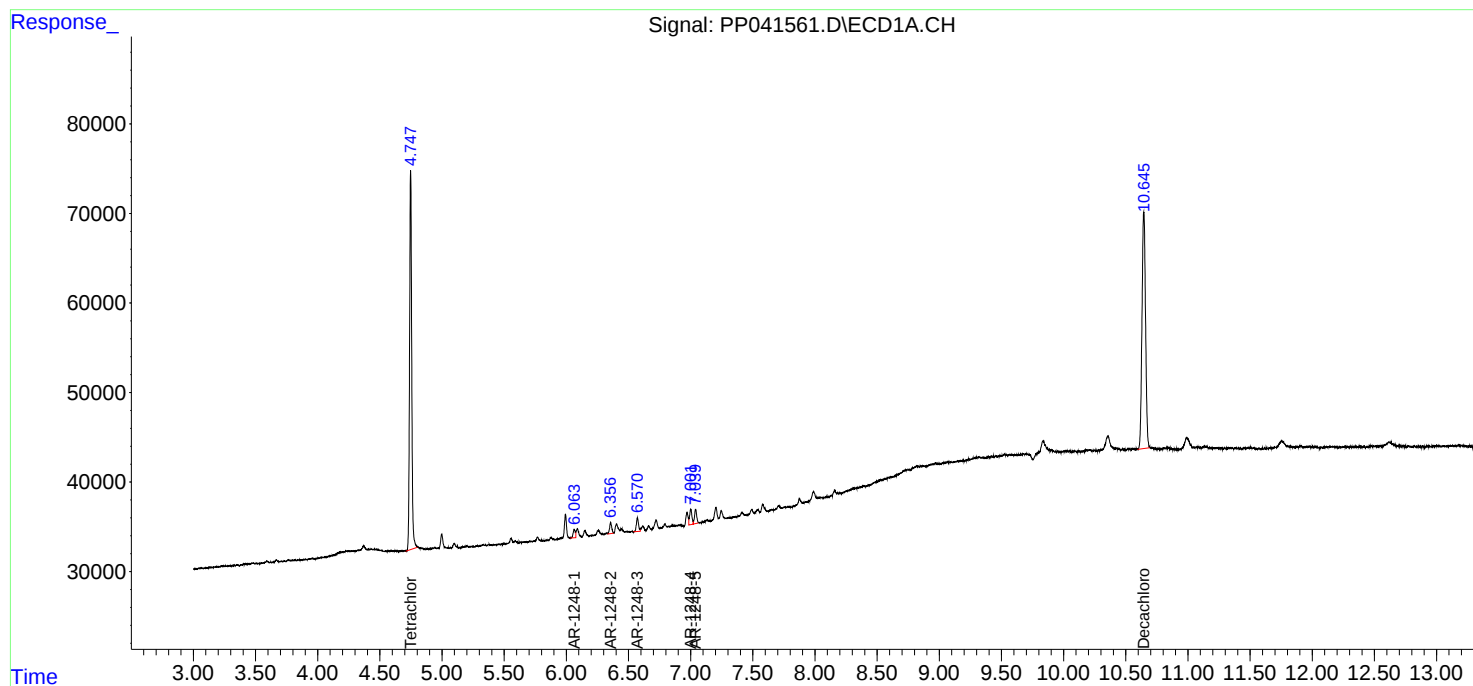


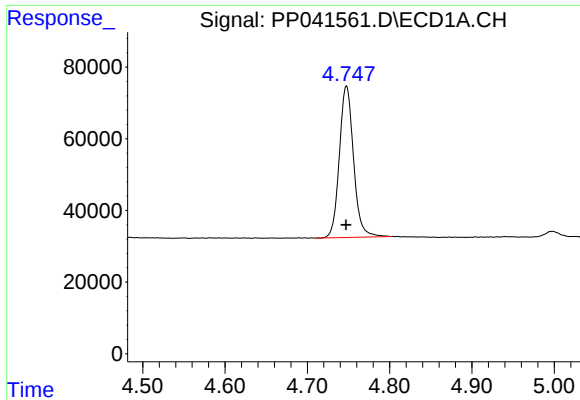

#1 Tetrachloro-m-xylene


R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 506223
Conc: 22.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

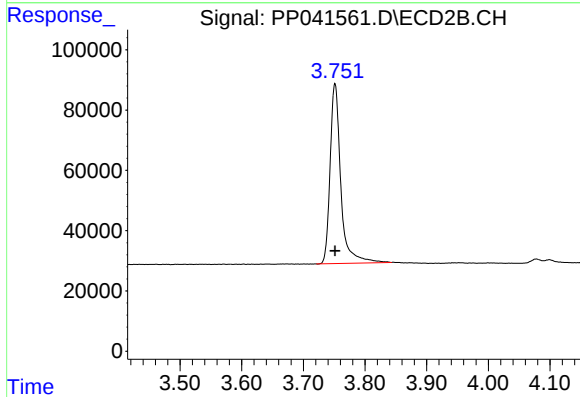


#1 Tetrachloro-m-xylene

R.T.: 3.751 min
Delta R.T.: 0.000 min
Response: 720390
Conc: 23.72 ng/ml

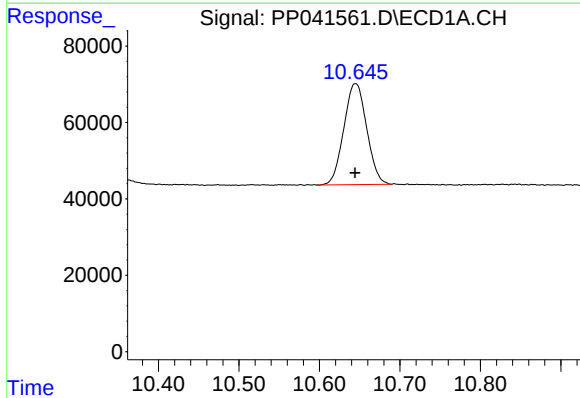


#2 Decachlorobiphenyl

R.T.: 10.645 min
Delta R.T.: 0.000 min
Response: 522169
Conc: 24.25 ng/ml

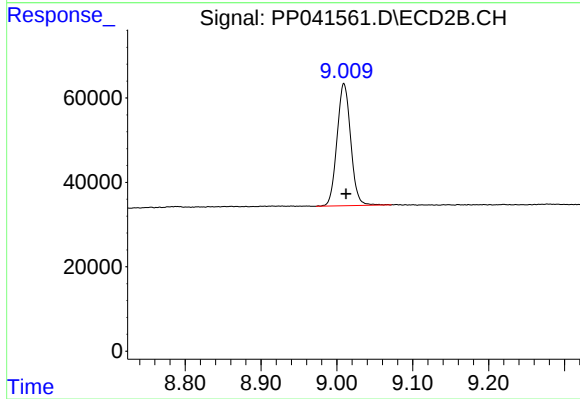

#2 Decachlorobiphenyl


R.T.: 9.009 min
Delta R.T.: -0.003 min
Response: 362908
Conc: 23.48 ng/ml

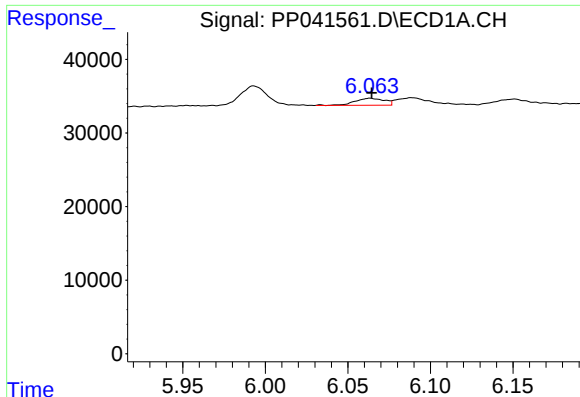

#21 AR-1248-1


R.T.: 6.063 min
Delta R.T.: -0.001 min
Response: 11663
Conc: 26.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

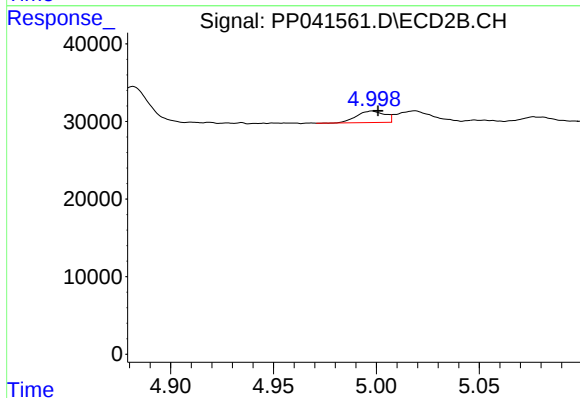


#21 AR-1248-1

R.T.: 4.998 min
Delta R.T.: -0.003 min
Response: 14016
Conc: 25.65 ng/ml

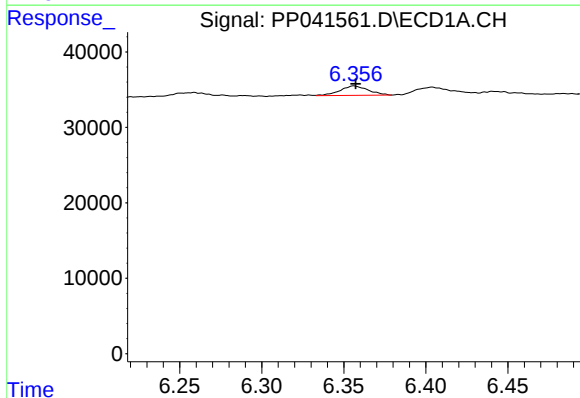


#22 AR-1248-2

R.T.: 6.356 min
Delta R.T.: -0.001 min
Response: 15084
Conc: 24.32 ng/ml

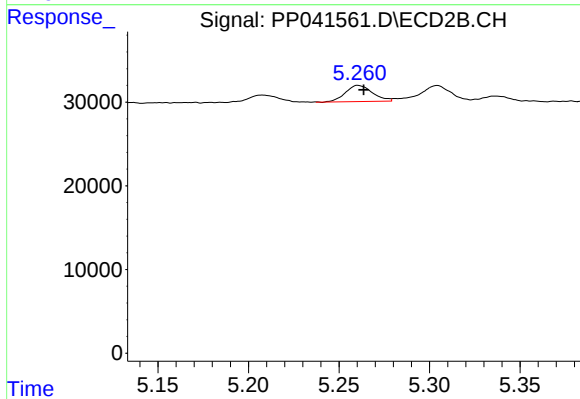

#22 AR-1248-2


R.T.: 5.260 min
Delta R.T.: -0.003 min
Response: 19954
Conc: 24.51 ng/ml

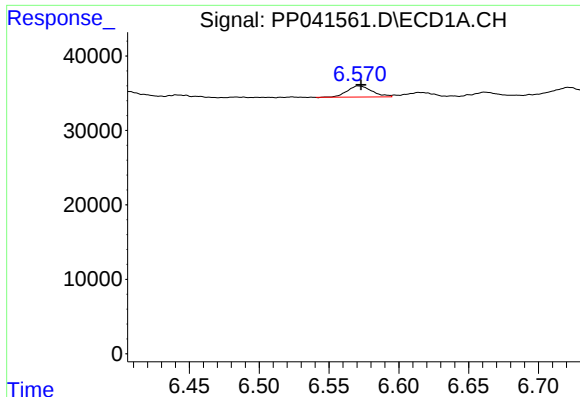

#23 AR-1248-3


R.T.: 6.571 min
Delta R.T.: -0.002 min
Response: 18618
Conc: 24.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

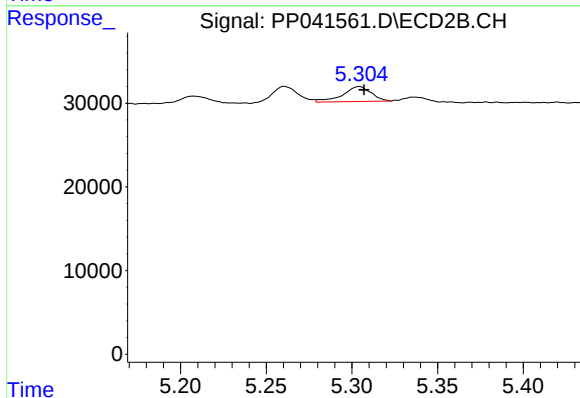


#23 AR-1248-3

R.T.: 5.304 min
Delta R.T.: -0.003 min
Response: 20460
Conc: 24.16 ng/ml

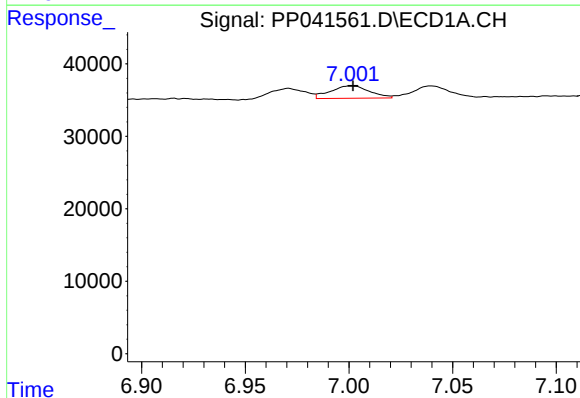


#24 AR-1248-4

R.T.: 7.001 min
Delta R.T.: 0.000 min
Response: 22689
Conc: 27.09 ng/ml

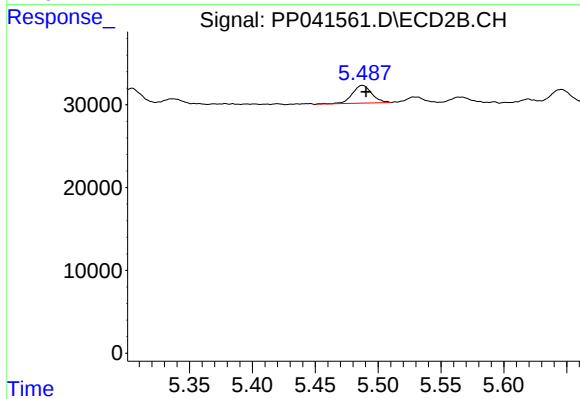

#24 AR-1248-4


R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 23008
Conc: 23.59 ng/ml

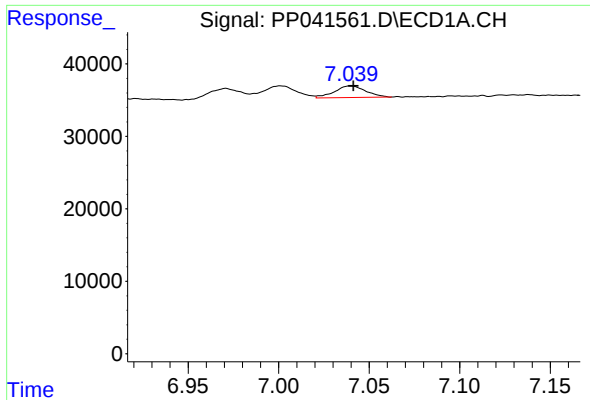

#25 AR-1248-5

R.T.: 7.039 min
Delta R.T.: -0.002 min
Response: 19357
Conc: 23.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

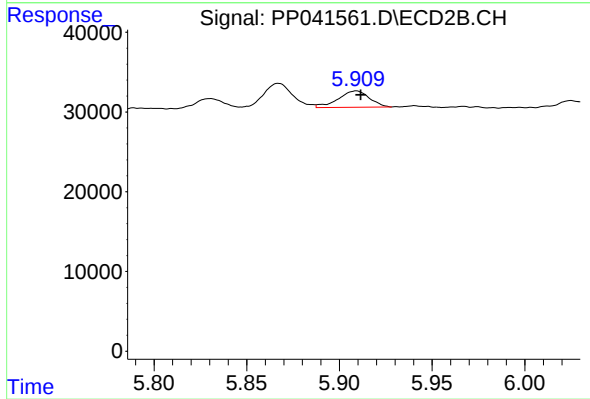

#25 AR-1248-5

R.T.: 5.909 min
Delta R.T.: -0.002 min
Response: 24167
Conc: 26.99 ng/ml