

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
 Data File : PP041562.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 10:35
 Operator : AJ\MA
 Sample : M4068-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 17:23:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.746	3.750	513180	740746	22.758	24.386
2)	SA Decachlor...	10.642	9.008	516466	358287	23.985	23.182
Target Compounds							
26)	L6 AR-1254-1	6.968	5.865	23217	36979	27.356	26.565
27)	L6 AR-1254-2	7.197	6.025	37577	34131	28.524	28.580
28)	L6 AR-1254-3	7.578	6.444	36063	48834	25.318	27.586
29)	L6 AR-1254-4	7.874	6.685	30150	26003	29.060	25.228
30)	L6 AR-1254-5	8.301	7.112	30460	37385	27.140	25.640



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
Data File : PP041562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 10:35
Operator : AJ\MA
Sample : M4068-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 17:23:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

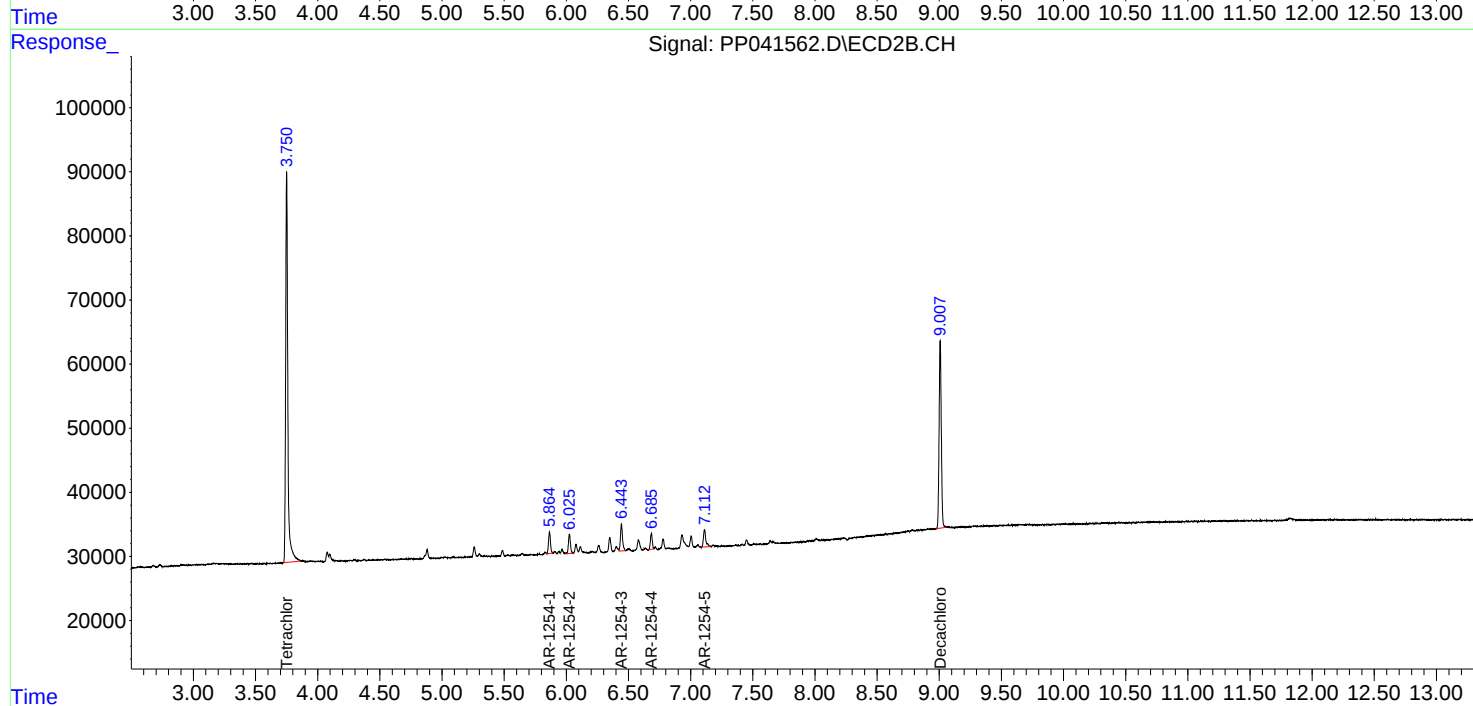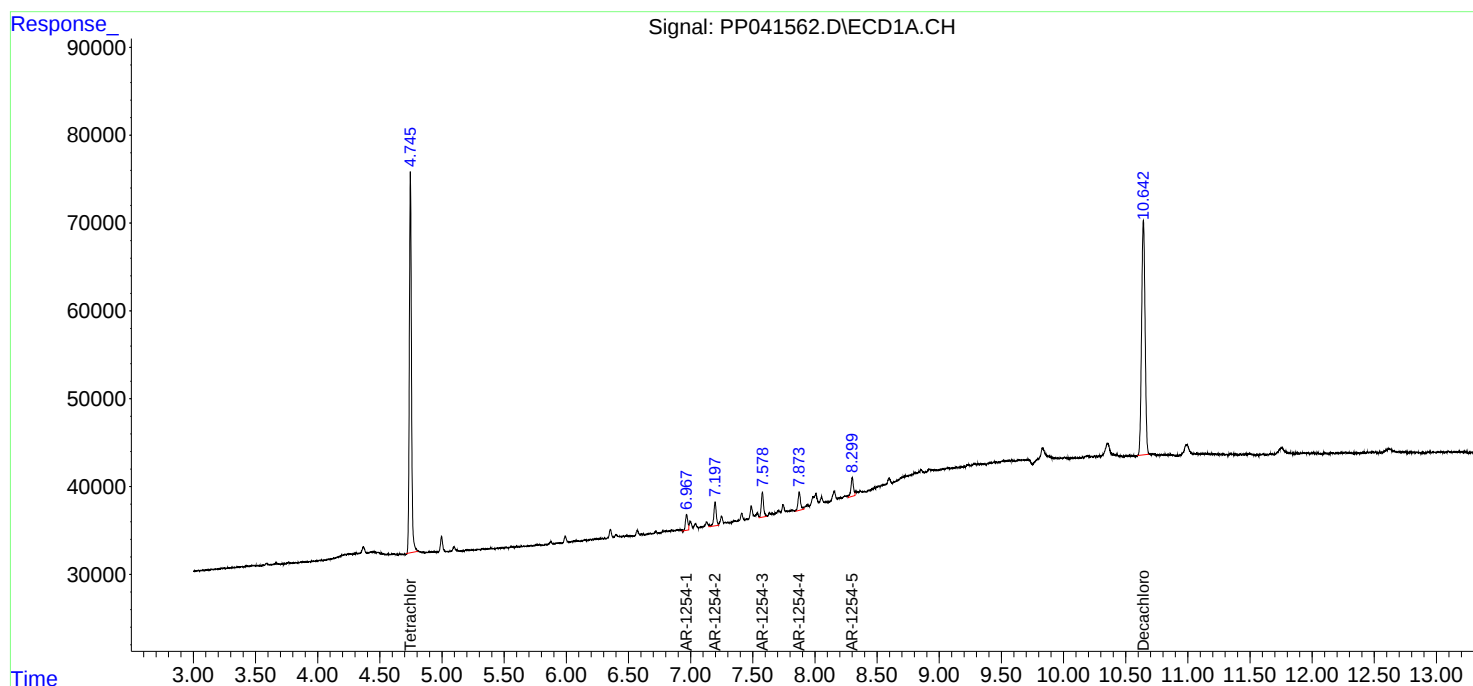


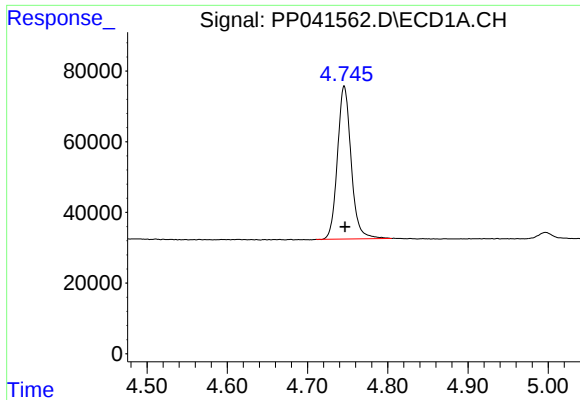

#1 Tetrachloro-m-xylene


R.T.: 4.746 min
Delta R.T.: -0.001 min
Response: 513180
Conc: 22.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

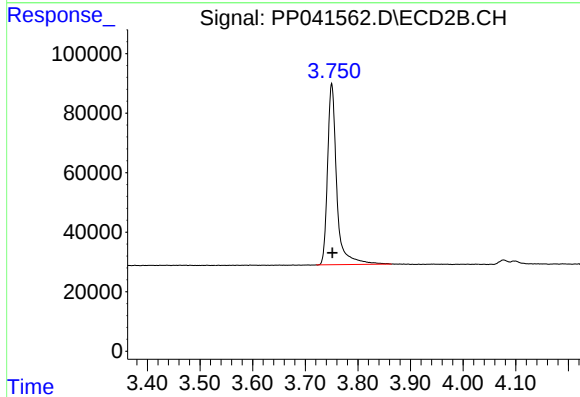


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: 0.000 min
Response: 740746
Conc: 24.39 ng/ml

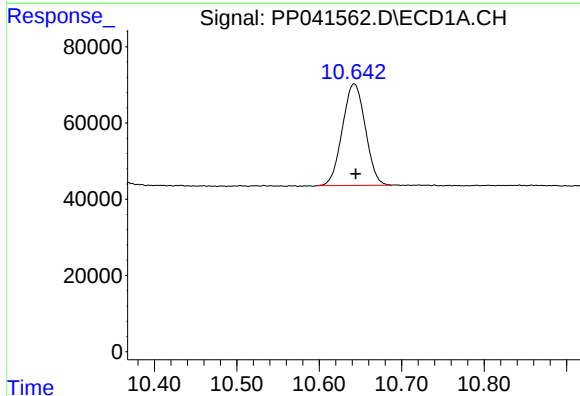


#2 Decachlorobiphenyl

R.T.: 10.642 min
Delta R.T.: -0.002 min
Response: 516466
Conc: 23.99 ng/ml

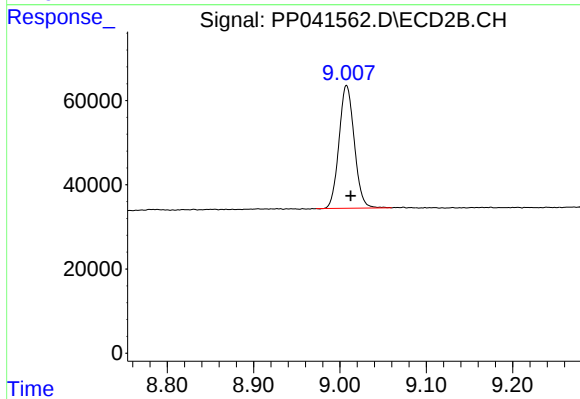

#2 Decachlorobiphenyl


R.T.: 9.008 min
Delta R.T.: -0.005 min
Response: 358287
Conc: 23.18 ng/ml

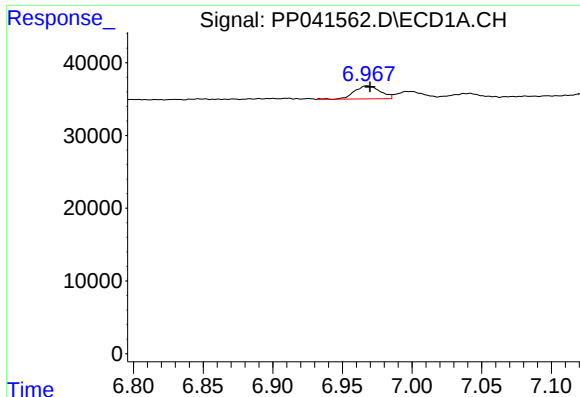

#26 AR-1254-1


R.T.: 6.968 min
Delta R.T.: -0.002 min
Response: 23217
Conc: 27.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

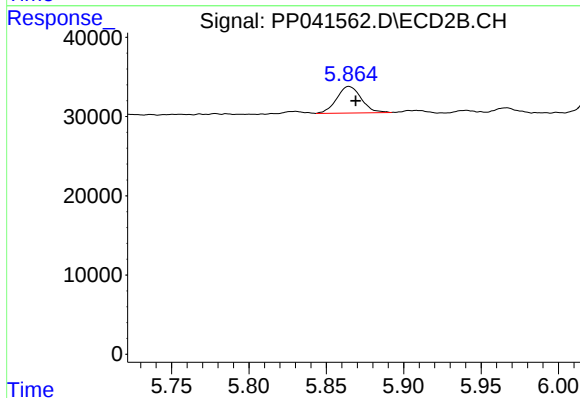


#26 AR-1254-1

R.T.: 5.865 min
Delta R.T.: -0.004 min
Response: 36979
Conc: 26.56 ng/ml

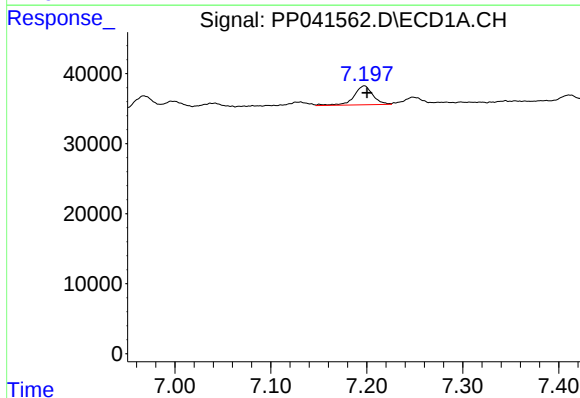


#27 AR-1254-2

R.T.: 7.197 min
Delta R.T.: -0.003 min
Response: 37577
Conc: 28.52 ng/ml

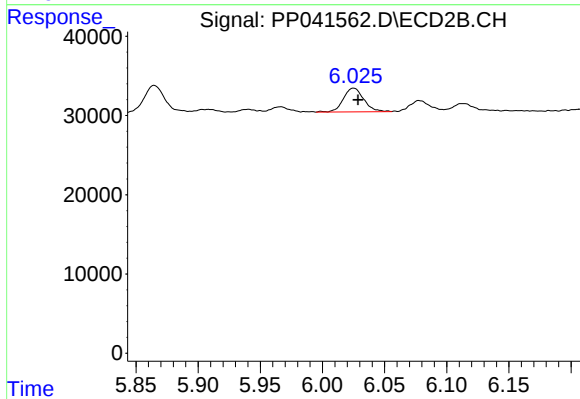

#27 AR-1254-2


R.T.: 6.025 min
Delta R.T.: -0.004 min
Response: 34131
Conc: 28.58 ng/ml

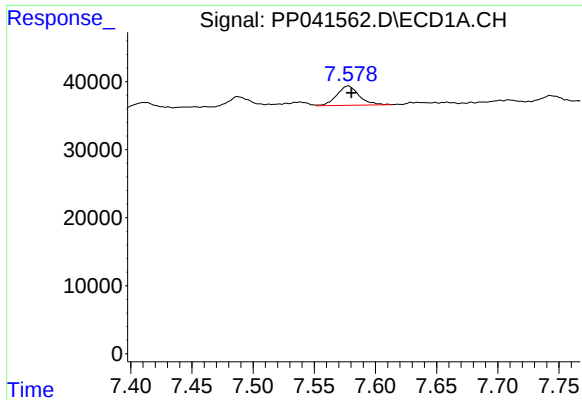

#28 AR-1254-3


R.T.: 7.578 min
Delta R.T.: -0.003 min
Response: 36063
Conc: 25.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

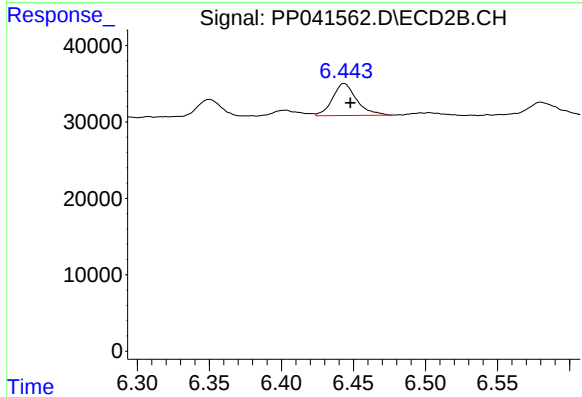


#28 AR-1254-3

R.T.: 6.444 min
Delta R.T.: -0.004 min
Response: 48834
Conc: 27.59 ng/ml

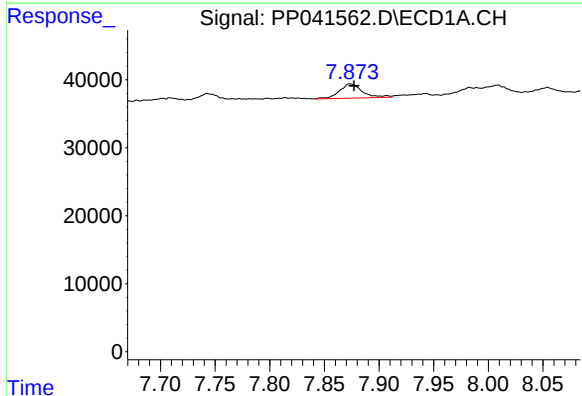


#29 AR-1254-4

R.T.: 7.874 min
Delta R.T.: -0.004 min
Response: 30150
Conc: 29.06 ng/ml

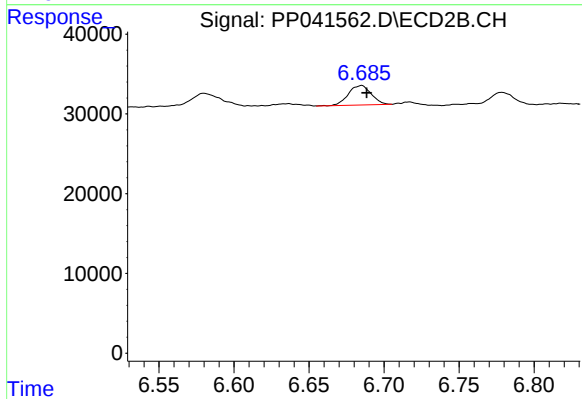

#29 AR-1254-4


R.T.: 6.685 min
Delta R.T.: -0.003 min
Response: 26003
Conc: 25.23 ng/ml

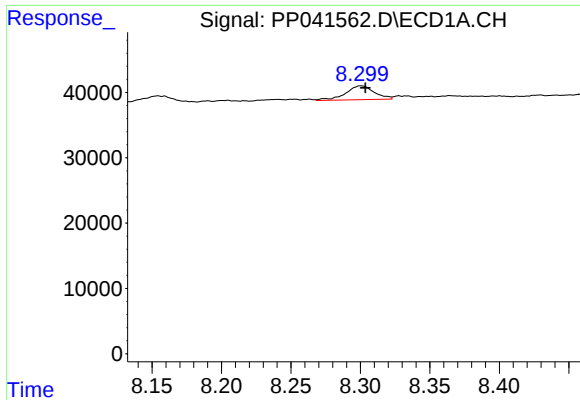

#30 AR-1254-5

R.T.: 8.301 min
Delta R.T.: -0.003 min
Response: 30460
Conc: 27.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

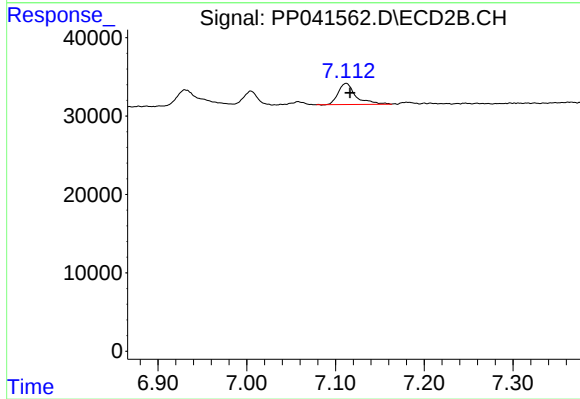

#30 AR-1254-5

R.T.: 7.112 min
Delta R.T.: -0.004 min
Response: 37385
Conc: 25.64 ng/ml