

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
 Data File : PP041563.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 10:51
 Operator : AJ\MA
 Sample : M4068-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 17:24:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.746	3.750	521860	756978	23.143	24.920
2)	SA Decachlor...	10.642	9.008	519199	360284	24.112	23.311
Target Compounds							
36)	L8 AR-1262-1	8.374	7.112	35006	21618	27.567	28.924
37)	L8 AR-1262-2	8.919	7.665	56338	65148	24.936	30.878
38)	L8 AR-1262-3	9.214	7.949	24116	28082	22.219	31.512 #
39)	L8 AR-1262-4	9.298	8.013	16372	48480	23.920	30.187 #
40)	L8 AR-1262-5	9.937	8.513	20825	19056	23.276	26.249



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120121\
Data File : PP041563.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 10:51
Operator : AJ\MA
Sample : M4068-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 17:24:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

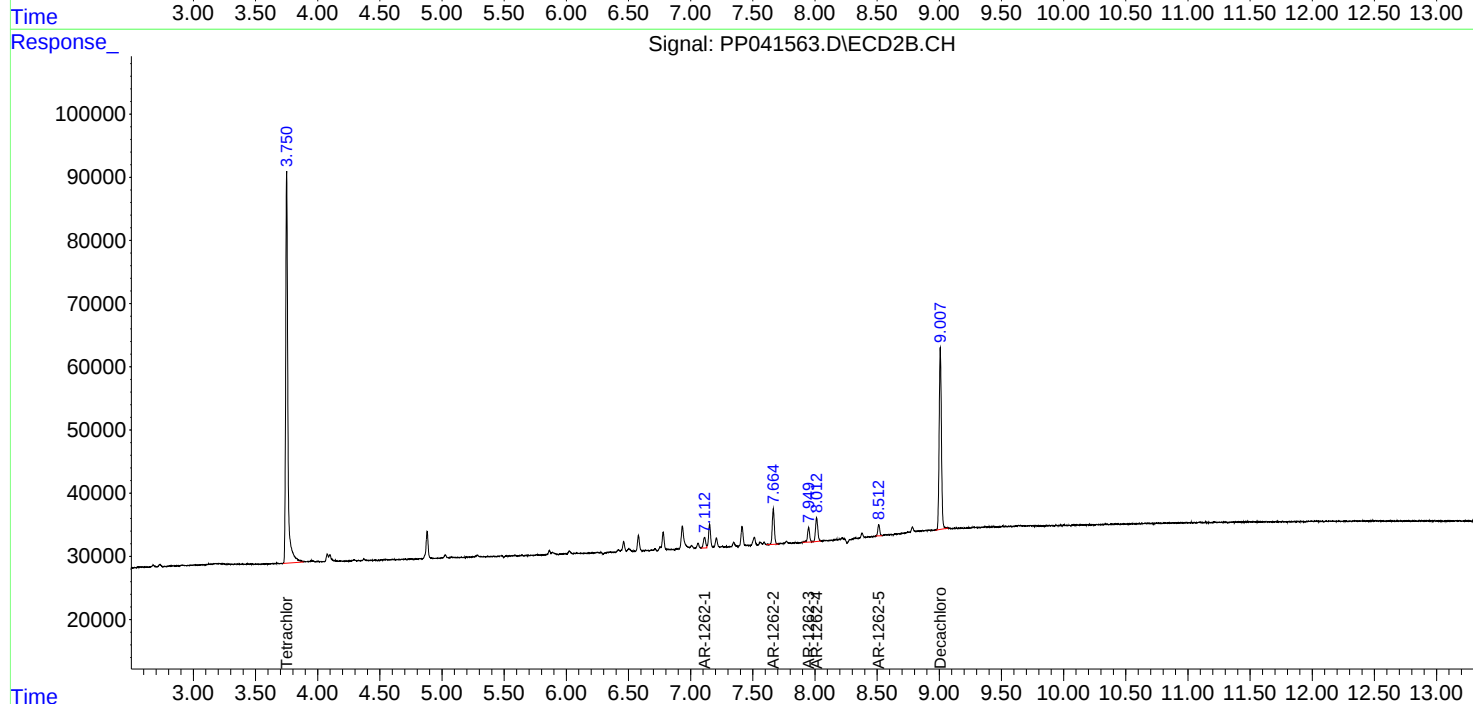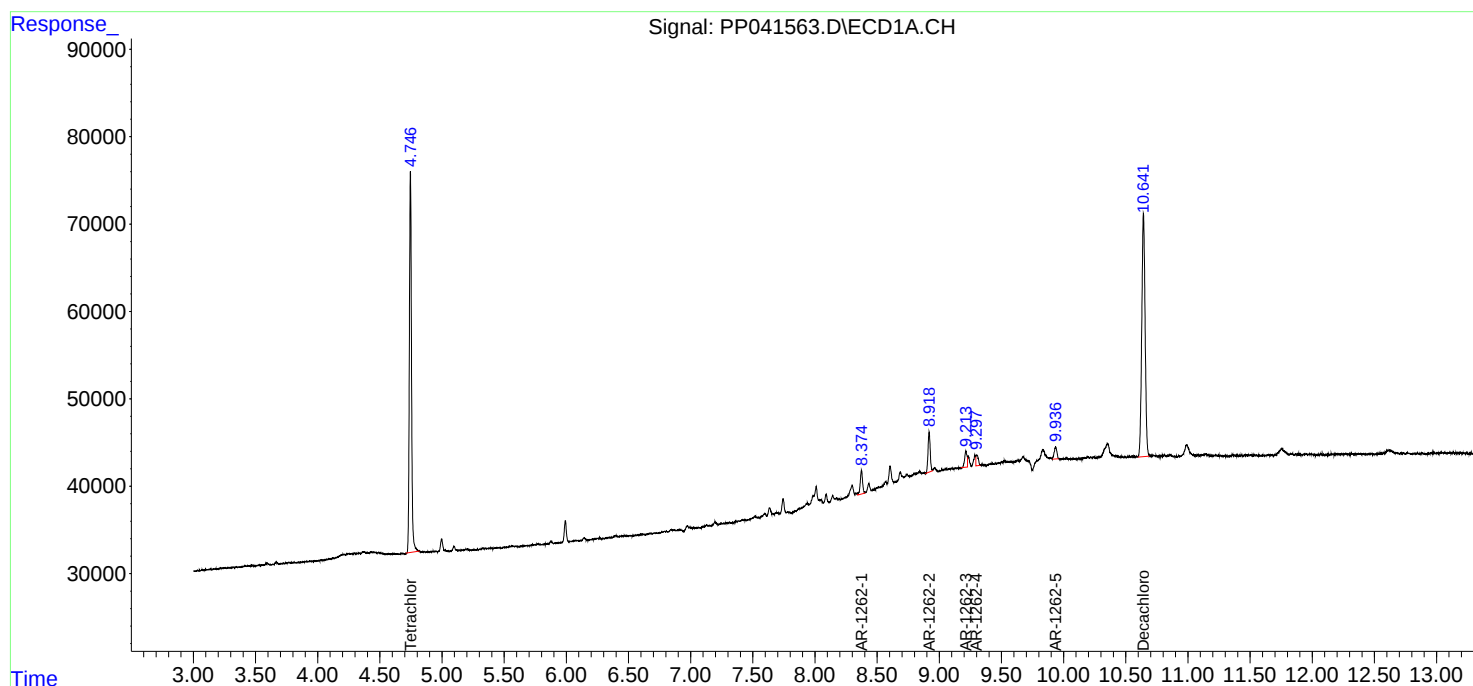


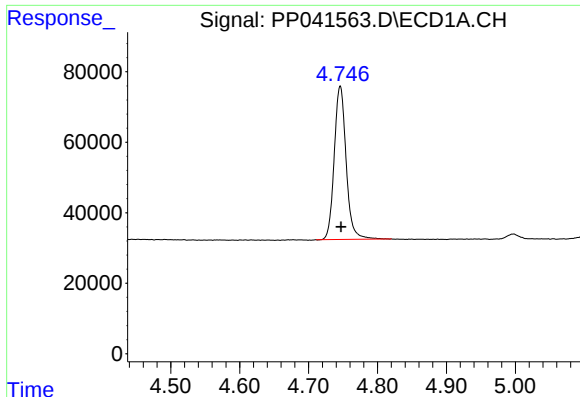

#1 Tetrachloro-m-xylene


R.T.: 4.746 min
Delta R.T.: -0.001 min
Response: 521860
Conc: 23.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

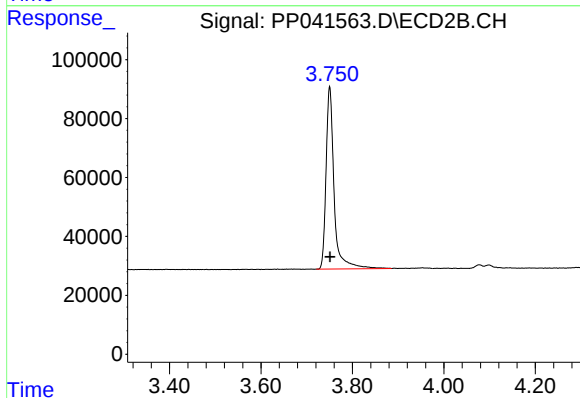


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.001 min
Response: 756978
Conc: 24.92 ng/ml

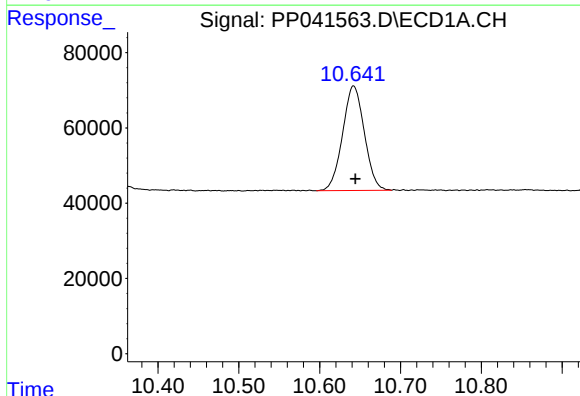


#2 Decachlorobiphenyl

R.T.: 10.642 min
Delta R.T.: -0.002 min
Response: 519199
Conc: 24.11 ng/ml

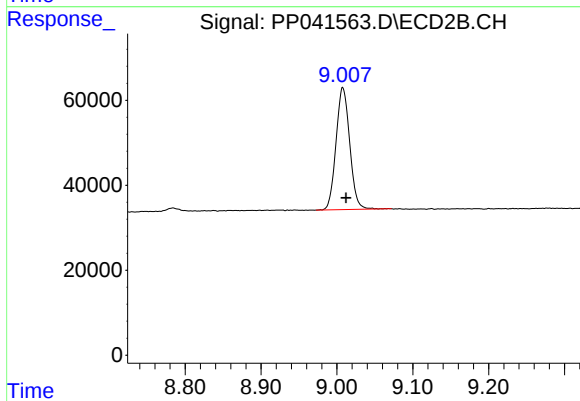

#2 Decachlorobiphenyl


R.T.: 9.008 min
Delta R.T.: -0.005 min
Response: 360284
Conc: 23.31 ng/ml

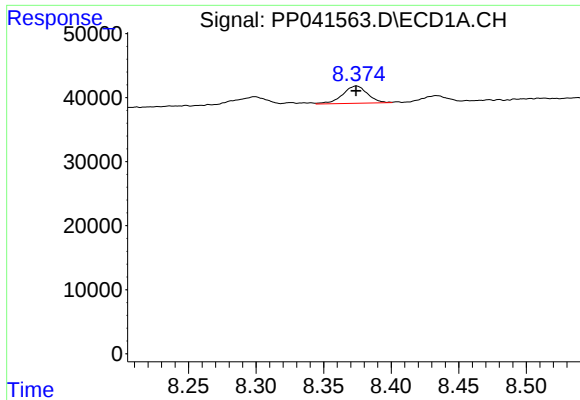

#36 AR-1262-1


R.T.: 8.374 min
Delta R.T.: 0.000 min
Response: 35006
Conc: 27.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

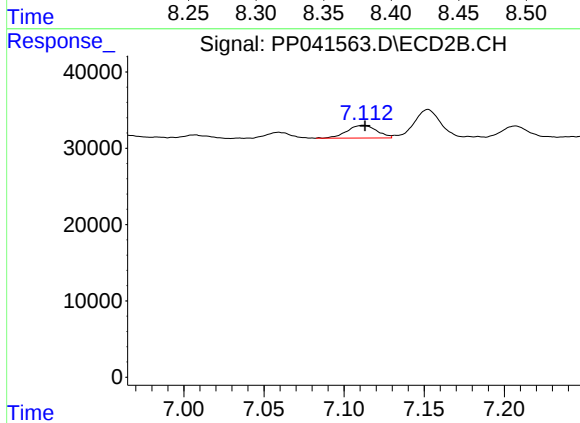


#36 AR-1262-1

R.T.: 7.112 min
Delta R.T.: 0.000 min
Response: 21618
Conc: 28.92 ng/ml

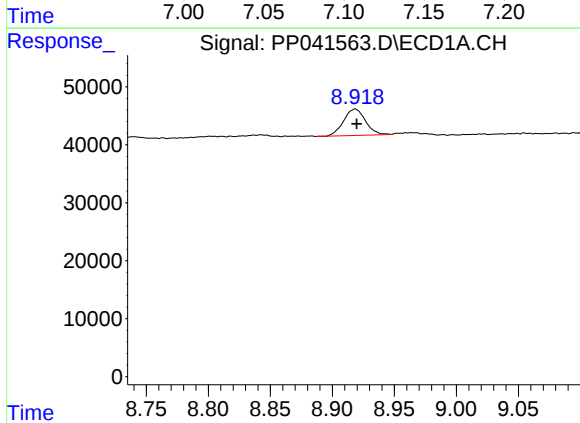


#37 AR-1262-2

R.T.: 8.919 min
Delta R.T.: -0.001 min
Response: 56338
Conc: 24.94 ng/ml

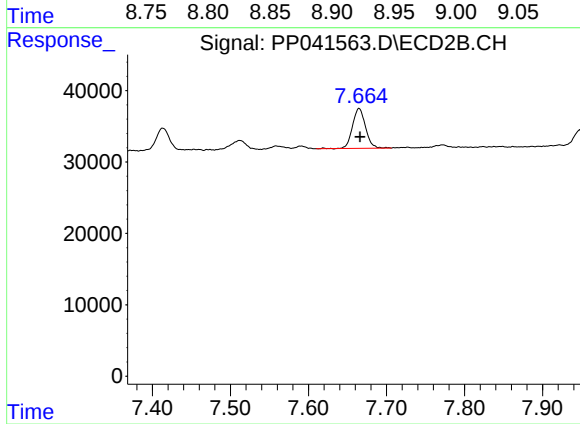

#37 AR-1262-2


R.T.: 7.665 min
Delta R.T.: -0.001 min
Response: 65148
Conc: 30.88 ng/ml

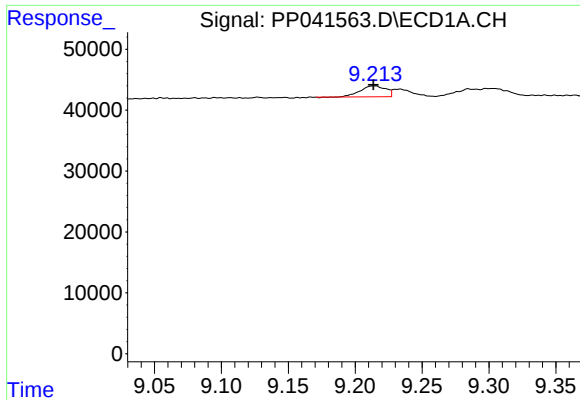

#38 AR-1262-3


R.T.: 9.214 min
Delta R.T.: 0.000 min
Response: 24116
Conc: 22.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

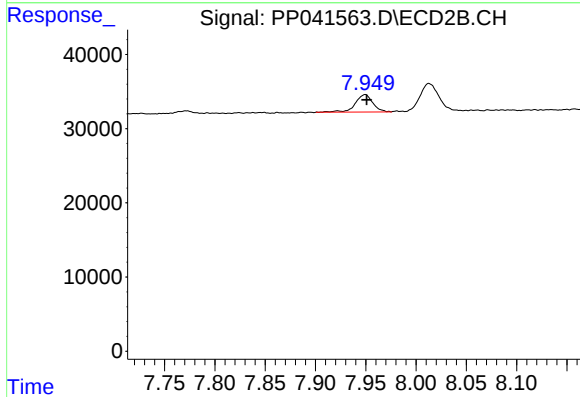


#38 AR-1262-3

R.T.: 7.949 min
Delta R.T.: -0.001 min
Response: 28082
Conc: 31.51 ng/ml

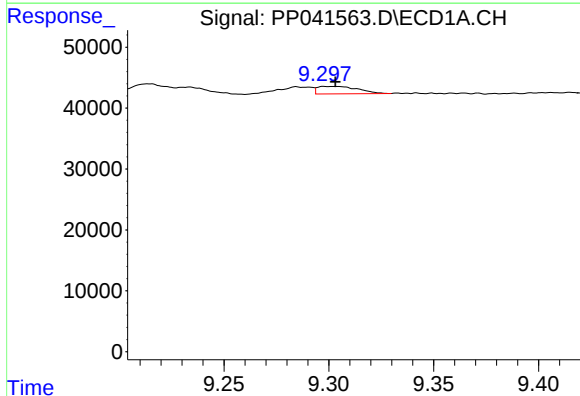


#39 AR-1262-4

R.T.: 9.298 min
Delta R.T.: -0.005 min
Response: 16372
Conc: 23.92 ng/ml

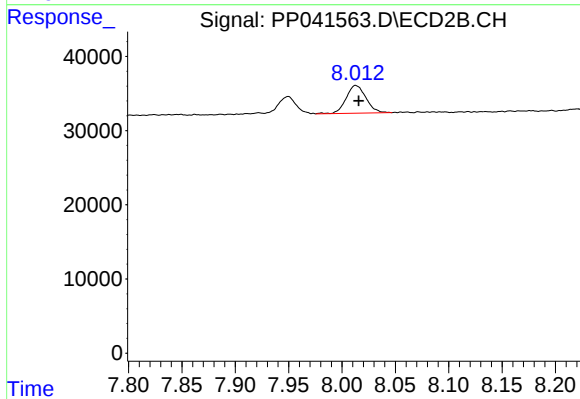

#39 AR-1262-4


R.T.: 8.013 min
Delta R.T.: -0.003 min
Response: 48480
Conc: 30.19 ng/ml

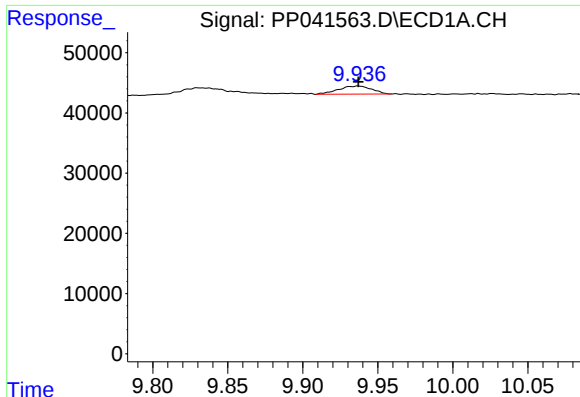

#40 AR-1262-5

R.T.: 9.937 min
Delta R.T.: 0.000 min
Response: 20825
Conc: 23.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

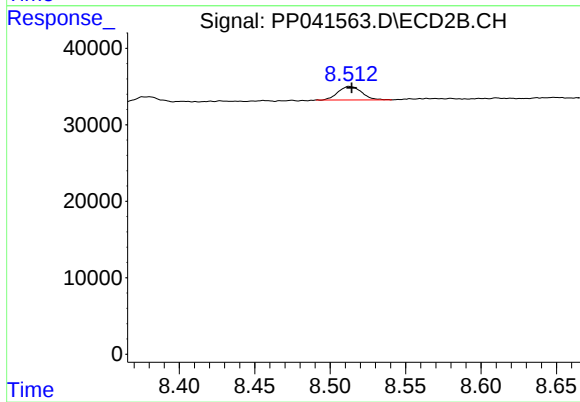

#40 AR-1262-5

R.T.: 8.513 min
Delta R.T.: -0.001 min
Response: 19056
Conc: 26.25 ng/ml