

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120123\
 Data File : PP062081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2023 17:29
 Operator : YP\AJ
 Sample : 05590-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 22:15:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.453	3.724	34456383	43582319	26.174	24.221
2) SA Decachlor...	10.242	8.846	24037562	42271240	23.292	20.481

Target Compounds

7) L1 AR-1016-5	0.000	5.288	0	353116	N.D.	6.108 #
9) L2 AR-1221-2	4.760	4.032	495637	806868	37.164	42.419
15) L3 AR-1232-5	0.000	5.288	0	353116	N.D.	13.876 #
24) L5 AR-1248-4	0.000	5.288	0	353116	N.D.	4.587 #
34) L7 AR-1260-4	8.064f	7.150f	395090	232128	6.474	2.354 #
35) L7 AR-1260-5	0.000	7.384f	0	517801	N.D.	2.418 #
37) L8 AR-1262-2	0.000	7.150f	0	232128	N.D.	1.718 #
43) L9 AR-1268-3	0.000	7.980	0	69747	N.D.	0.287 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120123\
Data File : PP062081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2023 17:29
Operator : YP\AJ
Sample : 05590-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 22:15:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

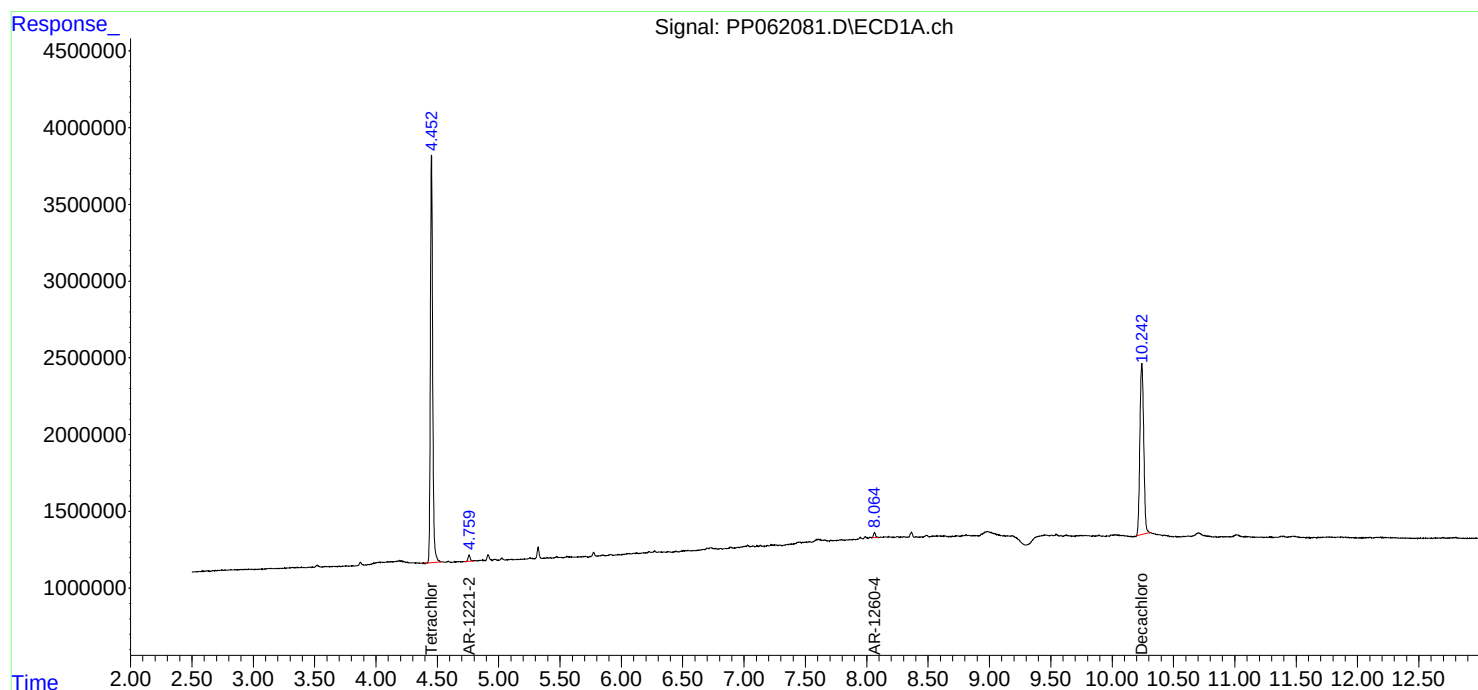


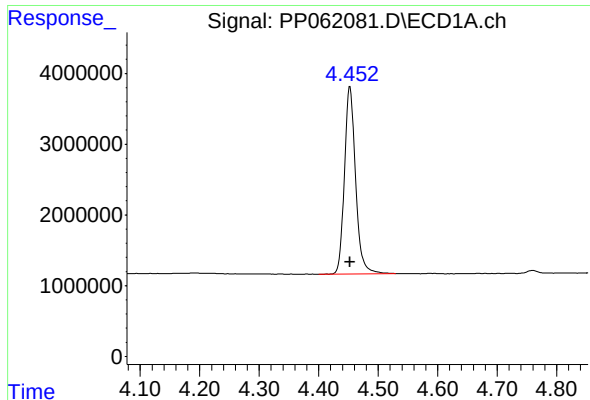

#1 Tetrachloro-m-xylene


R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 34456383
Conc: 26.17 ng/ml

Instrument :
ECD_P
ClientSampleId :

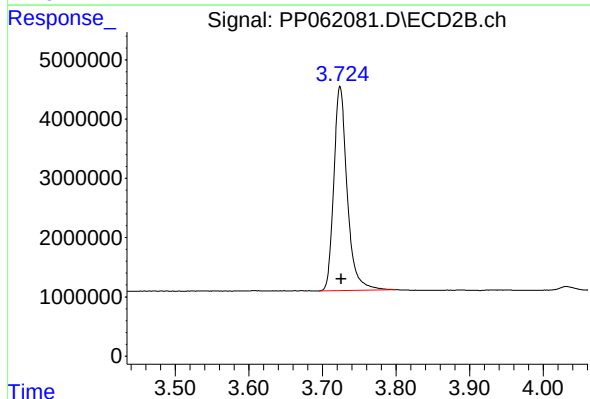


#1 Tetrachloro-m-xylene

R.T.: 3.724 min
Delta R.T.: -0.002 min
Response: 43582319
Conc: 24.22 ng/ml

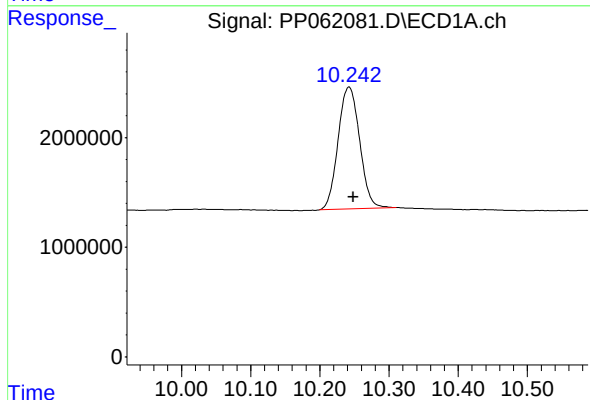


#2 Decachlorobiphenyl

R.T.: 10.242 min
Delta R.T.: -0.006 min
Response: 24037562
Conc: 23.29 ng/ml

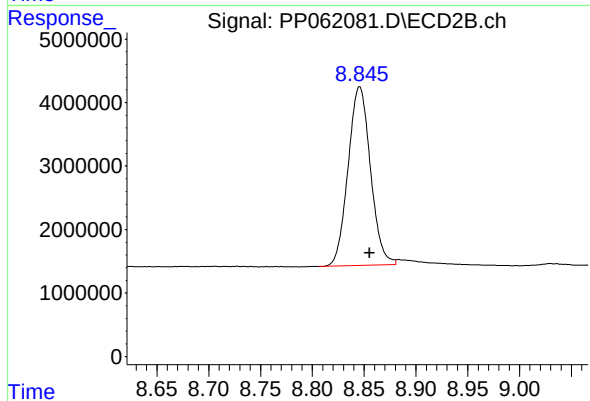

#2 Decachlorobiphenyl


R.T.: 8.846 min
Delta R.T.: -0.010 min
Response: 42271240
Conc: 20.48 ng/ml

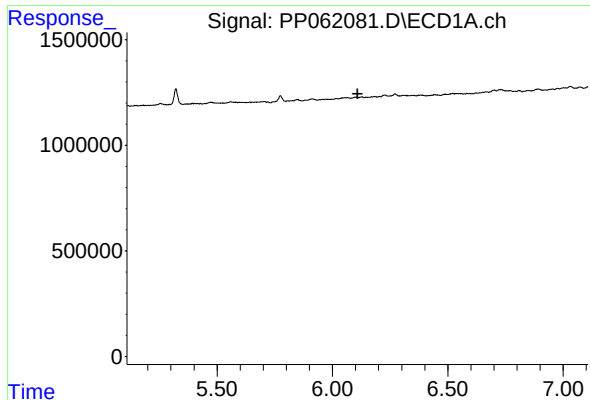

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

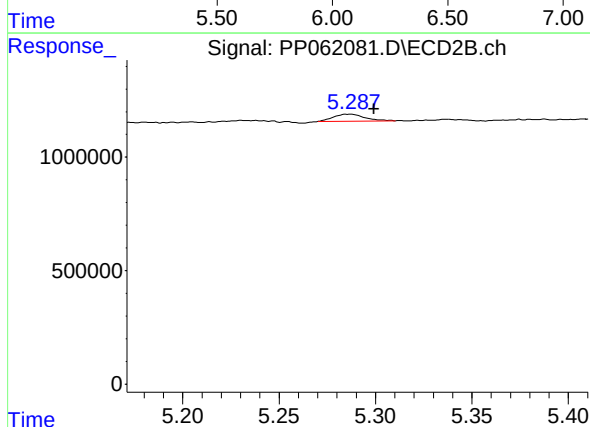


#7 AR-1016-5

R.T.: 5.288 min
Delta R.T.: -0.012 min
Response: 353116
Conc: 6.11 ng/ml

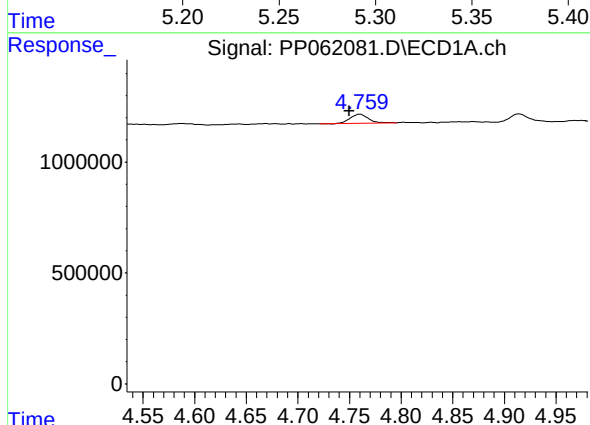


#9 AR-1221-2

R.T.: 4.760 min
Delta R.T.: 0.010 min
Response: 495637
Conc: 37.16 ng/ml

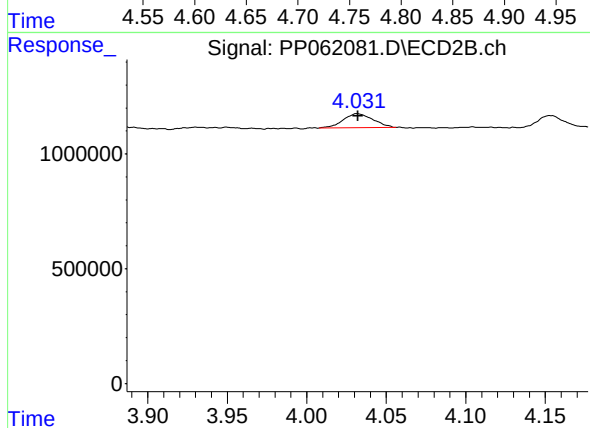

#9 AR-1221-2


R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 806868
Conc: 42.42 ng/ml

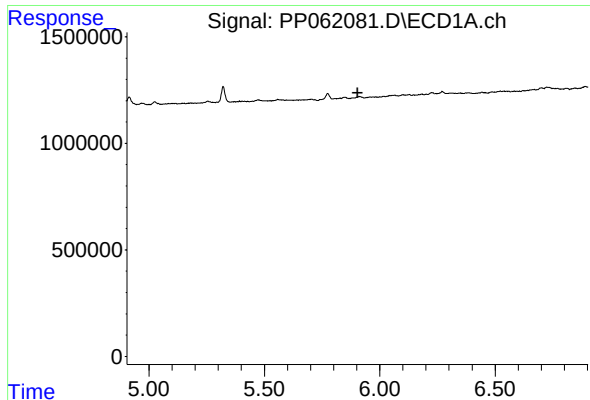

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

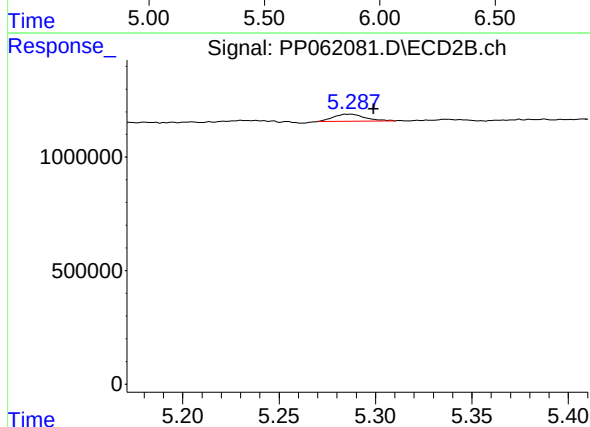


#15 AR-1232-5

R.T.: 5.288 min
Delta R.T.: -0.012 min
Response: 353116
Conc: 13.88 ng/ml

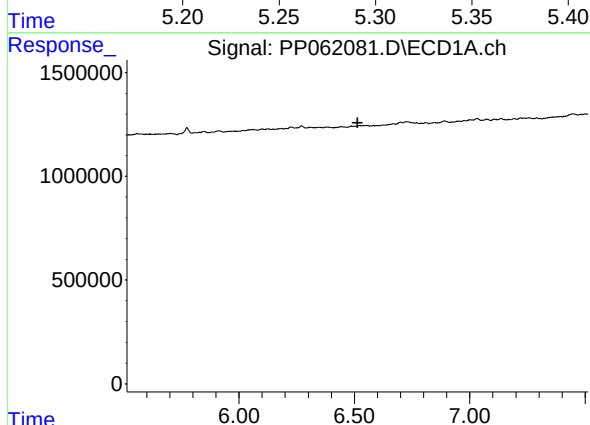


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.514 min
Response: 0
Conc: N.D.

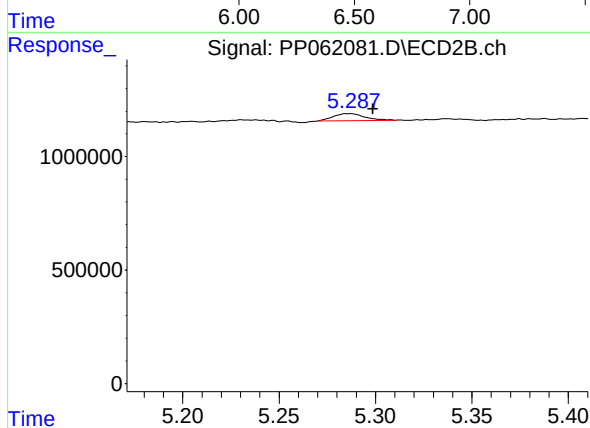

#24 AR-1248-4


R.T.: 5.288 min
Delta R.T.: -0.011 min
Response: 353116
Conc: 4.59 ng/ml

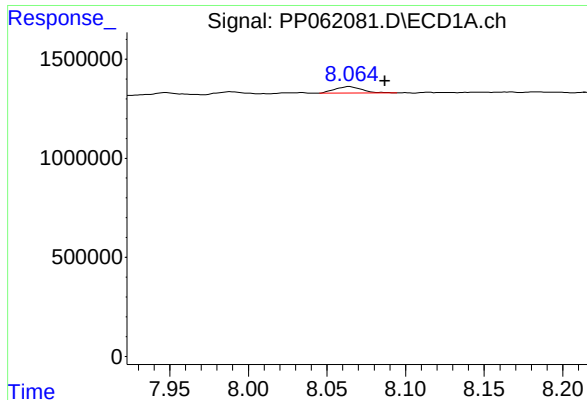

#34 AR-1260-4


R.T.: 8.064 min
Delta R.T.: -0.022 min
Response: 395090
Conc: 6.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

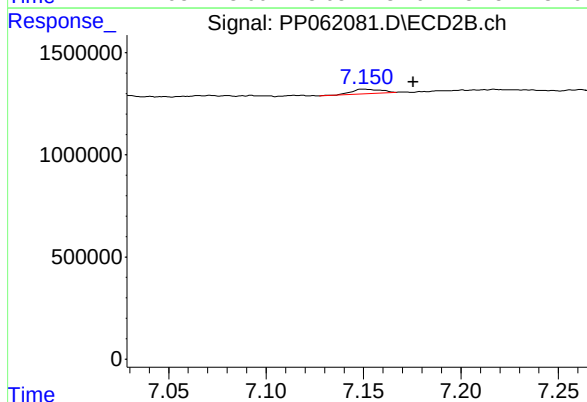


#34 AR-1260-4

R.T.: 7.150 min
Delta R.T.: -0.026 min
Response: 232128
Conc: 2.35 ng/ml

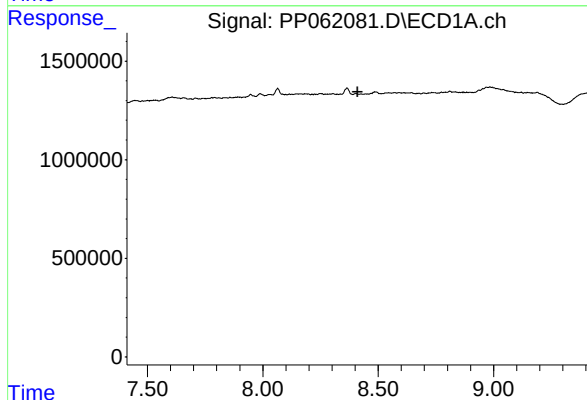


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.410 min
Response: 0
Conc: N.D.

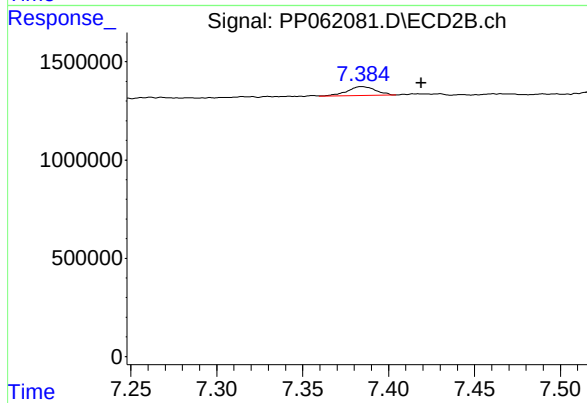

#35 AR-1260-5


R.T.: 7.384 min
Delta R.T.: -0.035 min
Response: 517801
Conc: 2.42 ng/ml

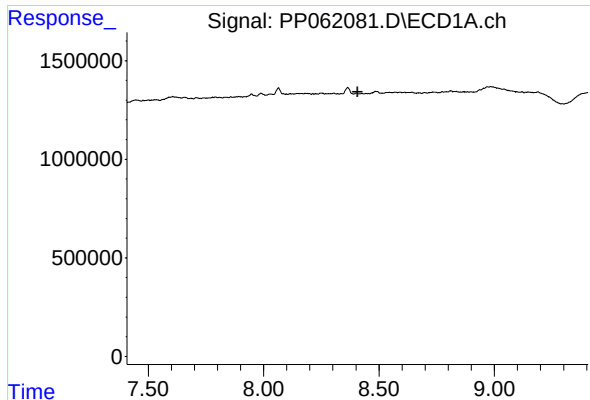

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

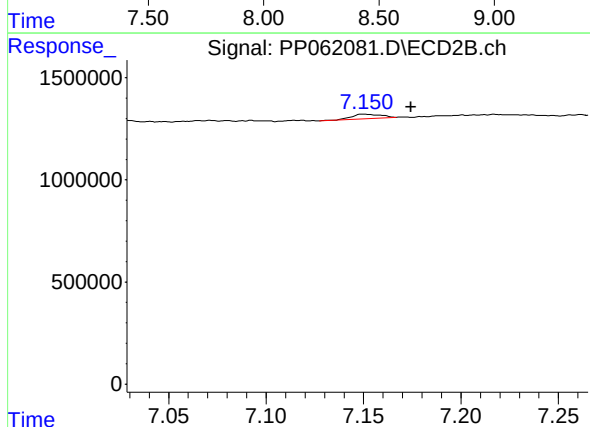


#37 AR-1262-2

R.T.: 7.150 min
Delta R.T.: -0.024 min
Response: 232128
Conc: 1.72 ng/ml

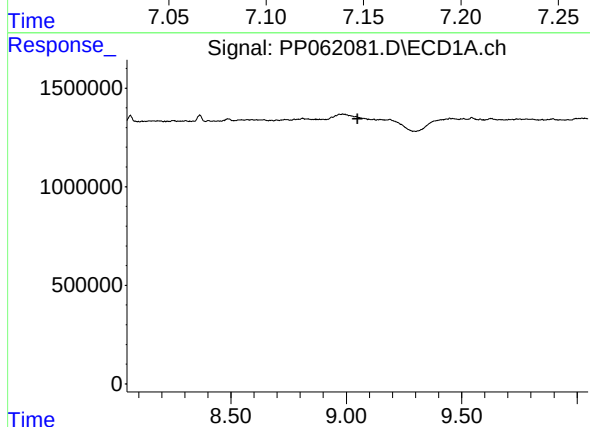

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.049 min
Response: 0
Conc: N.D.

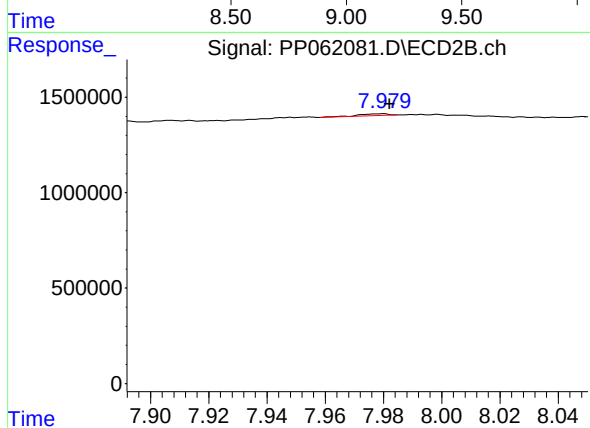

#43 AR-1268-3

R.T.: 7.980 min
Delta R.T.: -0.002 min
Response: 69747
Conc: 0.29 ng/ml