

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120123\
 Data File : PP062088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2023 19:23
 Operator : YP\AJ
 Sample : PB157523BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 22:17:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.454	3.724	27429940	34357535	20.836	19.094
2) SA Decachlor...	10.243	8.845	21910348	35537922	21.231	17.218
Target Compounds						
9) L2 AR-1221-2	4.762	4.032	499435	473104	37.449	24.872 #
20) L4 AR-1242-5	0.000	5.673f	0	92000	N.D.	1.758 #
25) L5 AR-1248-5	0.000	5.673f	0	92000	N.D.	0.921 #
26) L6 AR-1254-1	0.000	5.673f	0	92000	N.D.	0.845 #
28) L6 AR-1254-3	7.072	0.000	877531	0	10.607	N.D. #
29) L6 AR-1254-4	0.000	6.449	0	401845	N.D.	5.056 #
32) L7 AR-1260-2	7.523f	6.523	1074110	600556	14.260	4.408 #
33) L7 AR-1260-3	0.000	6.694	0	55866	N.D.	0.427 #
35) L7 AR-1260-5	0.000	7.420	0	19119	N.D.	0.089 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120123\
Data File : PP062088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2023 19:23
Operator : YP\AJ
Sample : PB157523BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 22:17:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

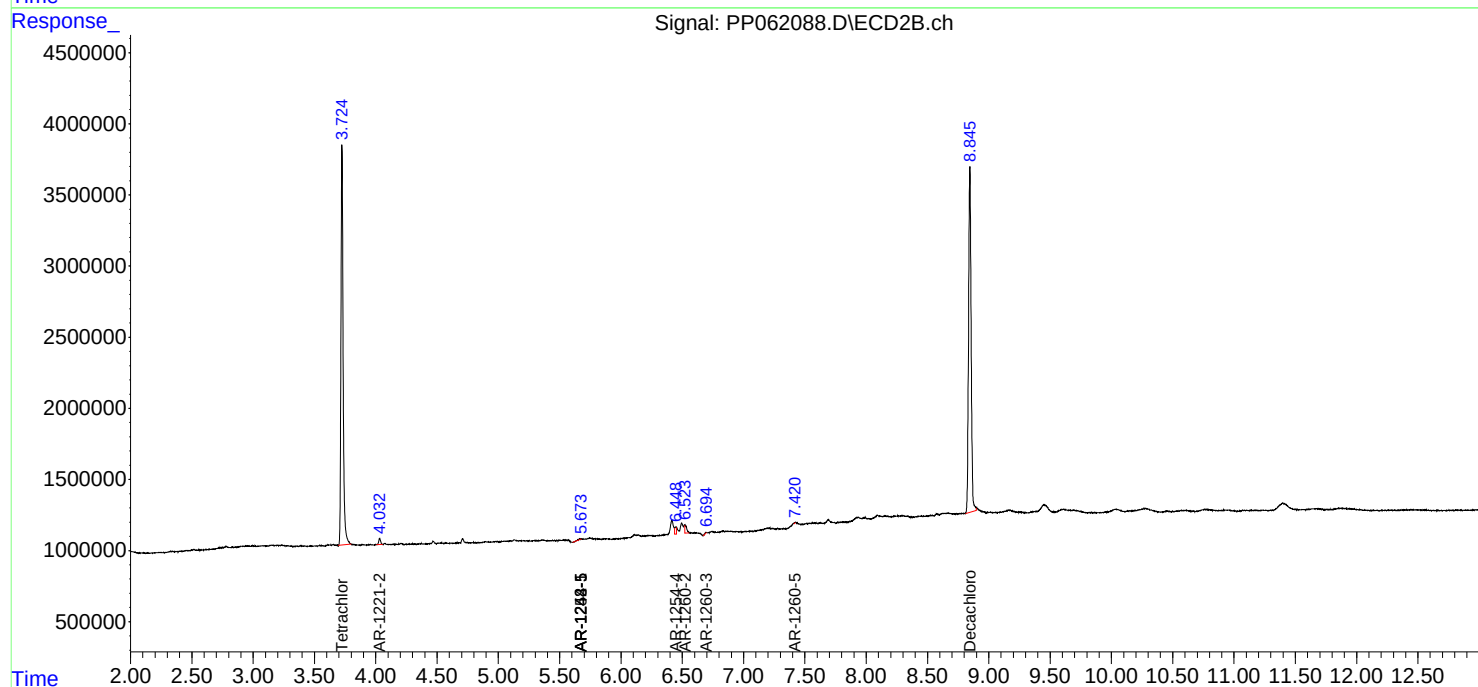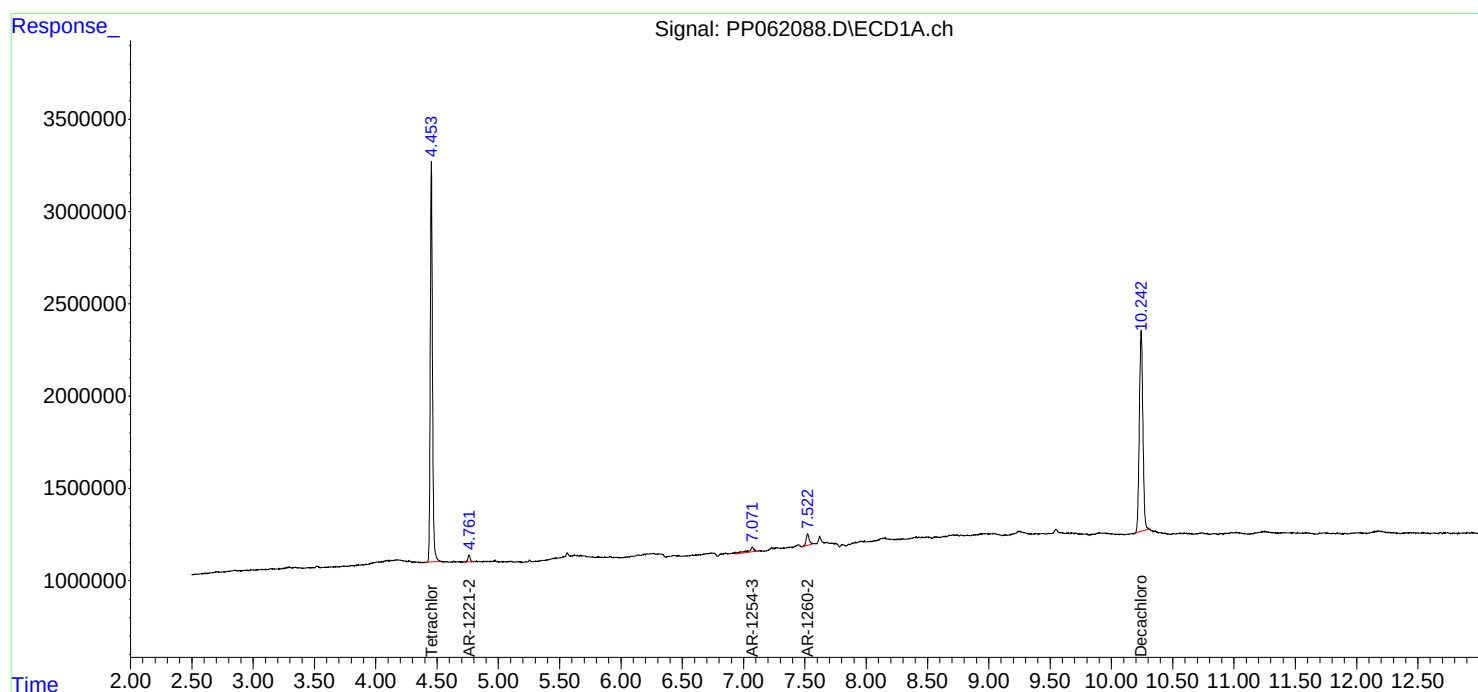


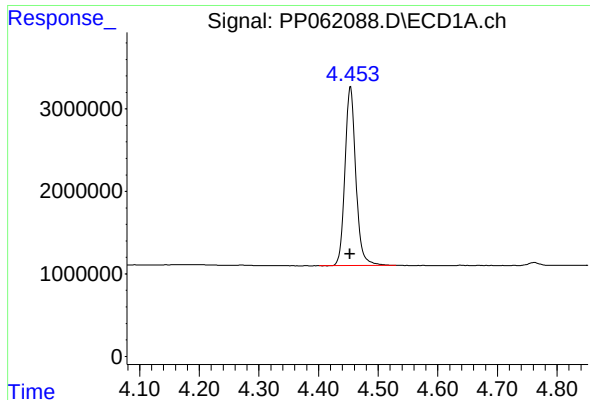

#1 Tetrachloro-m-xylene


R.T.: 4.454 min
Delta R.T.: 0.000 min
Response: 27429940
Conc: 20.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

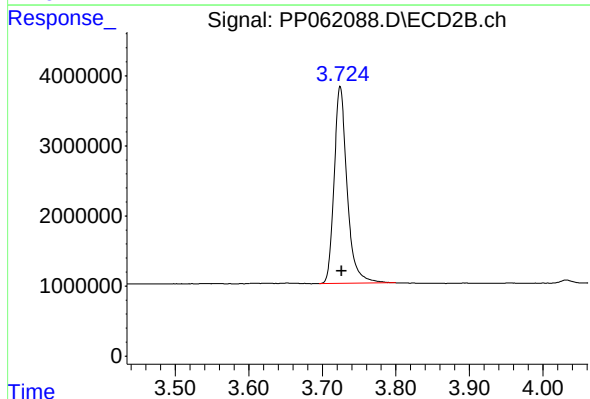


#1 Tetrachloro-m-xylene

R.T.: 3.724 min
Delta R.T.: -0.002 min
Response: 34357535
Conc: 19.09 ng/ml

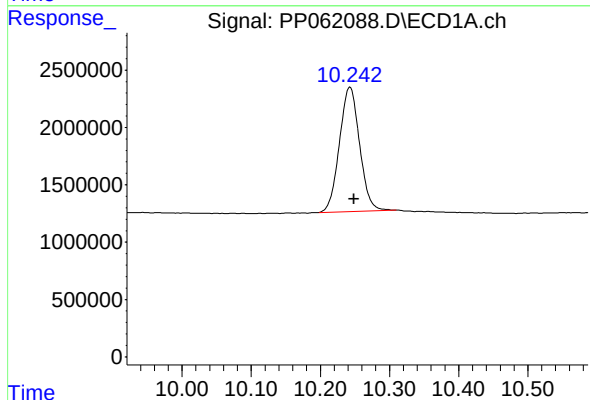


#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: -0.006 min
Response: 21910348
Conc: 21.23 ng/ml

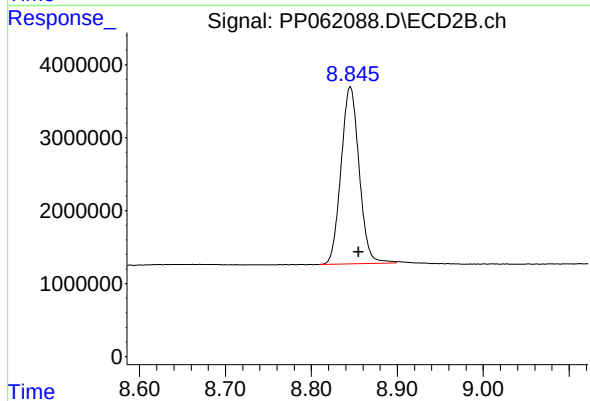

#2 Decachlorobiphenyl


R.T.: 8.845 min
Delta R.T.: -0.010 min
Response: 35537922
Conc: 17.22 ng/ml

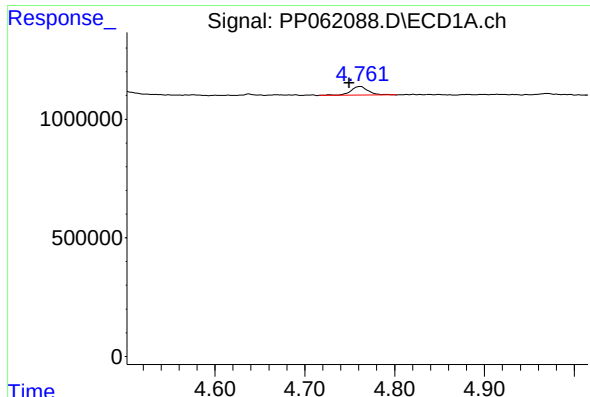

#9 AR-1221-2


R.T.: 4.762 min
Delta R.T.: 0.012 min
Response: 499435
Conc: 37.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

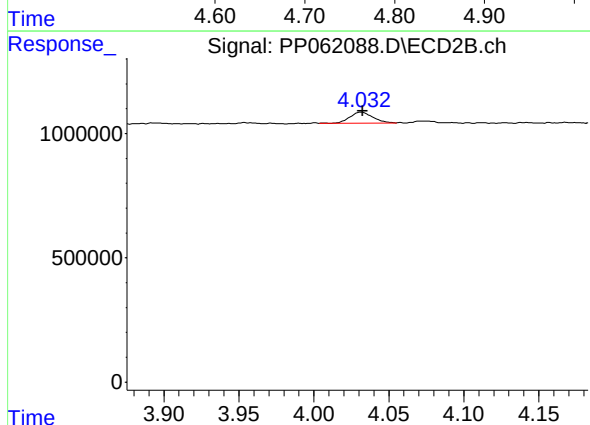


#9 AR-1221-2

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 473104
Conc: 24.87 ng/ml

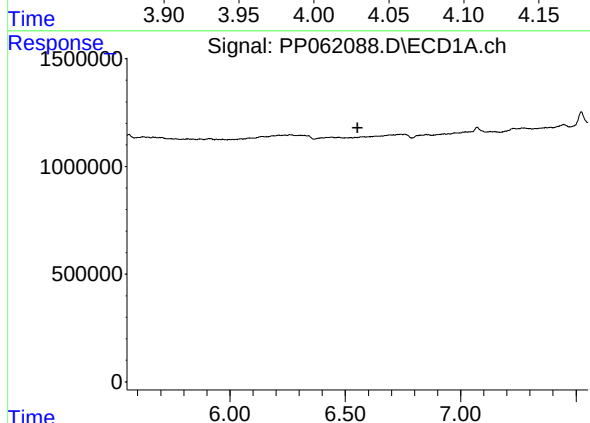


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.553 min
Response: 0
Conc: N.D.

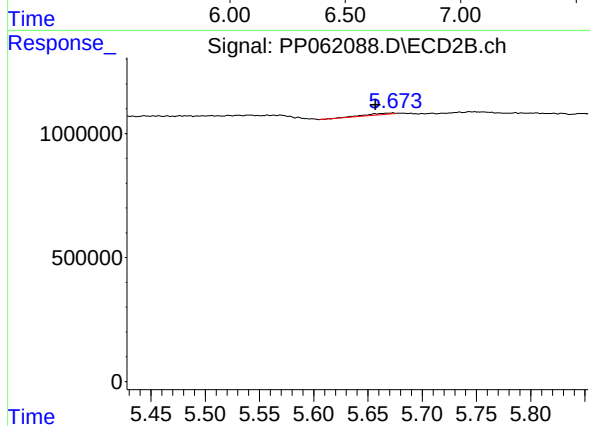

#20 AR-1242-5


R.T.: 5.673 min
Delta R.T.: 0.016 min
Response: 92000
Conc: 1.76 ng/ml

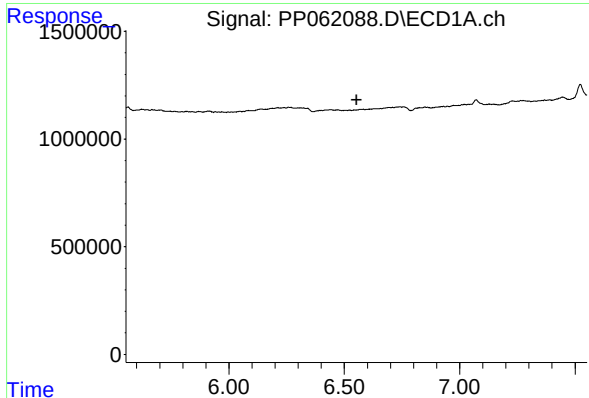

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.553 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

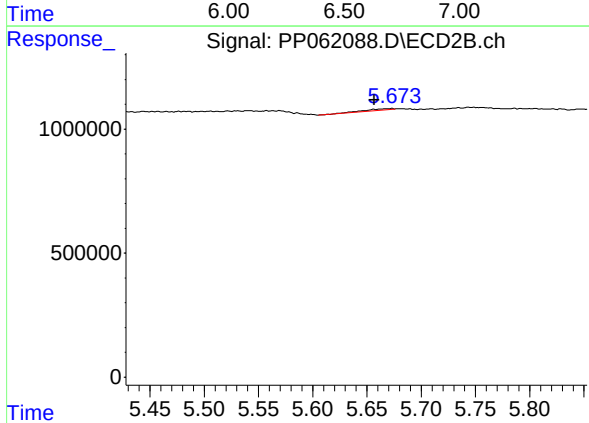


#25 AR-1248-5

R.T.: 5.673 min
Delta R.T.: 0.016 min
Response: 92000
Conc: 0.92 ng/ml

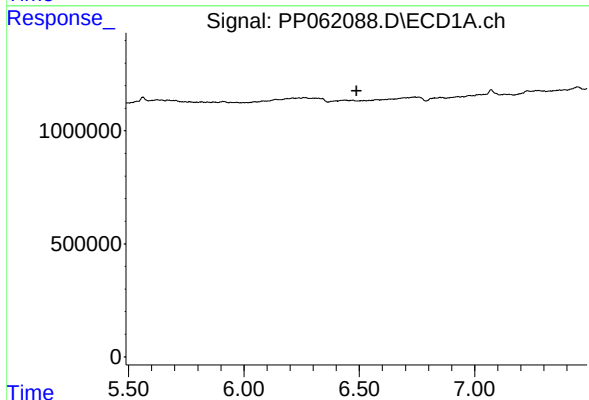


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.488 min
Response: 0
Conc: N.D.

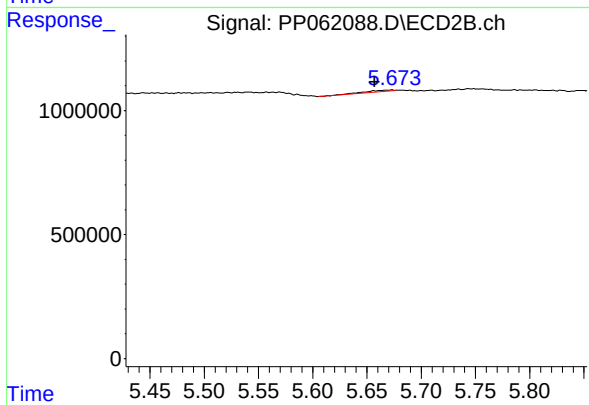

#26 AR-1254-1


R.T.: 5.673 min
Delta R.T.: 0.016 min
Response: 92000
Conc: 0.84 ng/ml

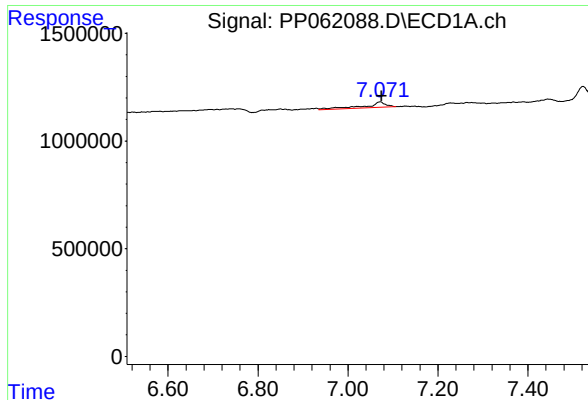

#28 AR-1254-3


R.T.: 7.072 min
Delta R.T.: -0.003 min
Response: 877531
Conc: 10.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

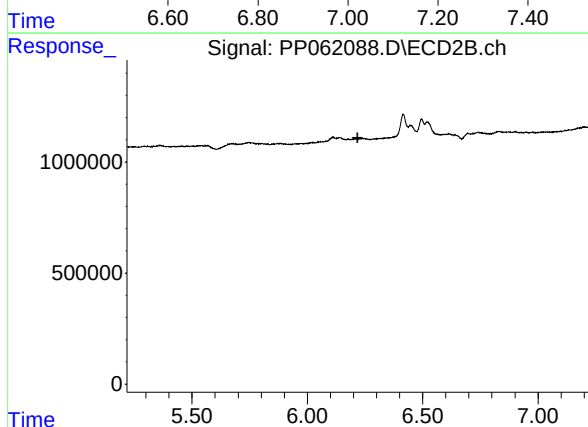


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.217 min
Response: 0
Conc: N.D.

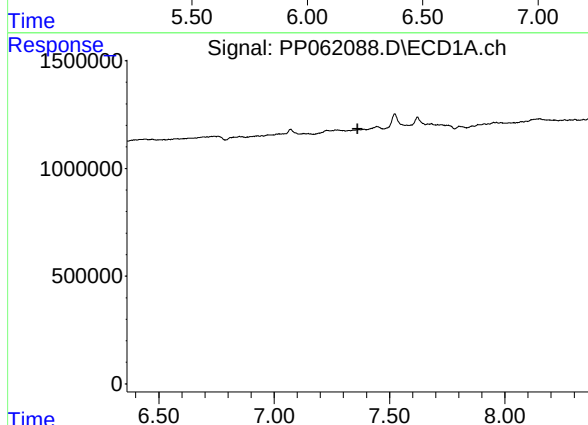


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

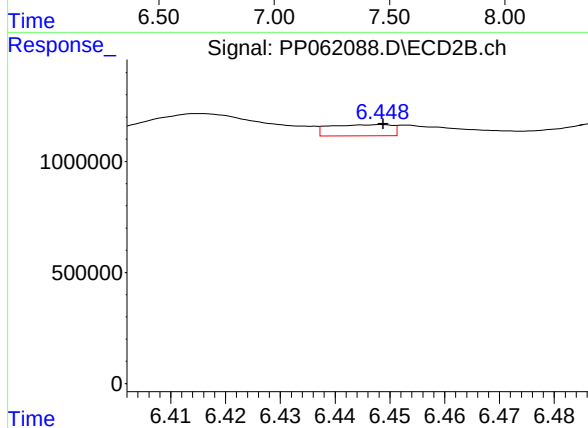

#29 AR-1254-4


R.T.: 6.449 min
Delta R.T.: 0.000 min
Response: 401845
Conc: 5.06 ng/ml

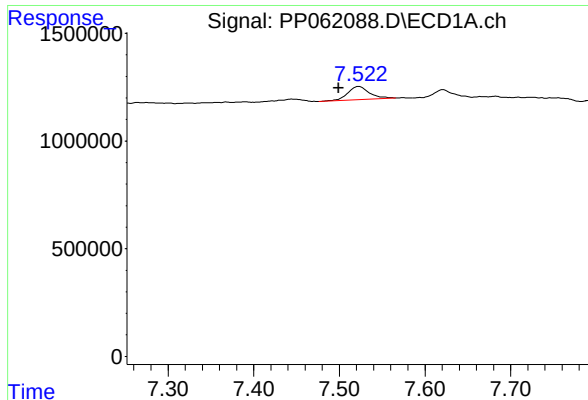

#32 AR-1260-2


R.T.: 7.523 min
Delta R.T.: 0.024 min
Response: 1074110
Conc: 14.26 ng/ml

Instrument :
ECD_P
ClientSampleId :

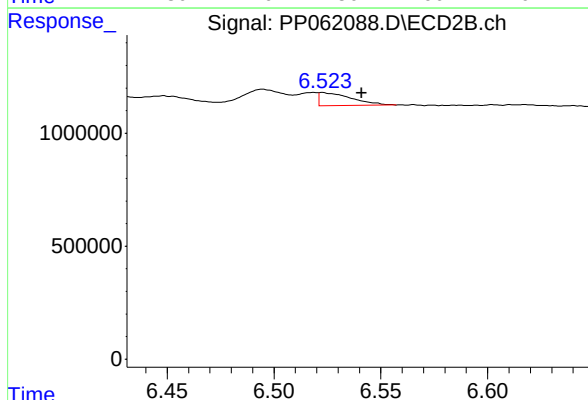


#32 AR-1260-2

R.T.: 6.523 min
Delta R.T.: -0.018 min
Response: 600556
Conc: 4.41 ng/ml

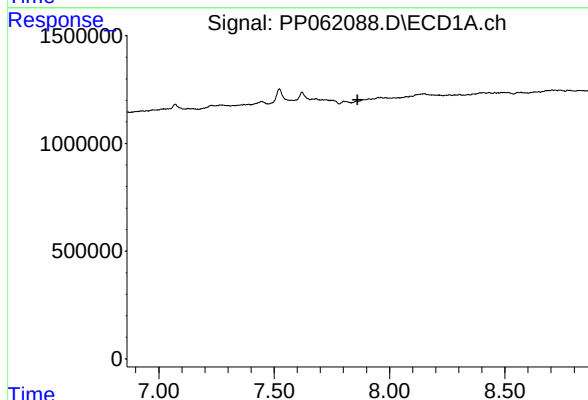


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.861 min
Response: 0
Conc: N.D.

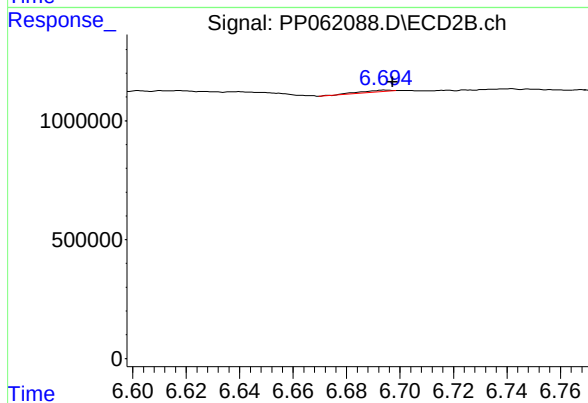

#33 AR-1260-3


R.T.: 6.694 min
Delta R.T.: -0.003 min
Response: 55866
Conc: 0.43 ng/ml

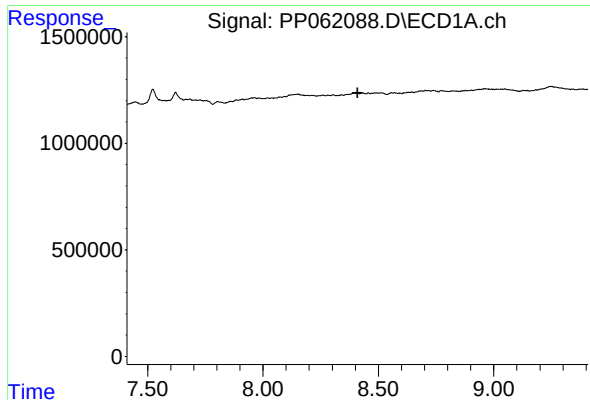

#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

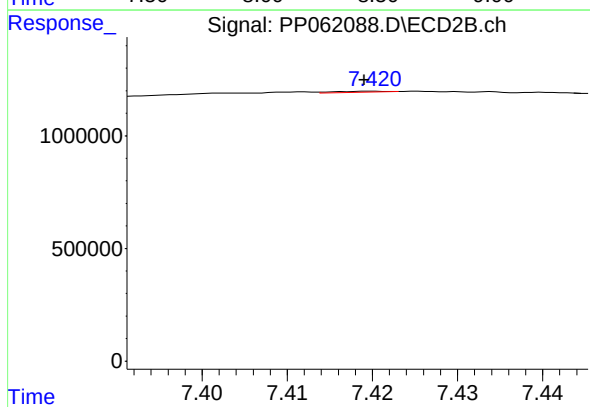

#35 AR-1260-5

R.T.: 7.420 min
Delta R.T.: 0.001 min
Response: 19119
Conc: 0.09 ng/ml