

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 12:37
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1221-WATER-01-QT4-2025
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/02/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:53:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.612	3.771	42227981	51953593	23.006	24.943
2) SA Decachlor...	10.360	8.763	32919754	41927447	21.966	23.761
Target Compounds						
8) L2 AR-1221-1	4.808	3.980	496787	671589	19.230m	25.136 #
9) L2 AR-1221-2	4.910	4.066	1096341	1188161	55.017m	59.433m
10) L2 AR-1221-3	4.972	4.141	1312173	1623243	23.533m	26.932

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 12:37
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1221-WATER-01-QT4-2025
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:53:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

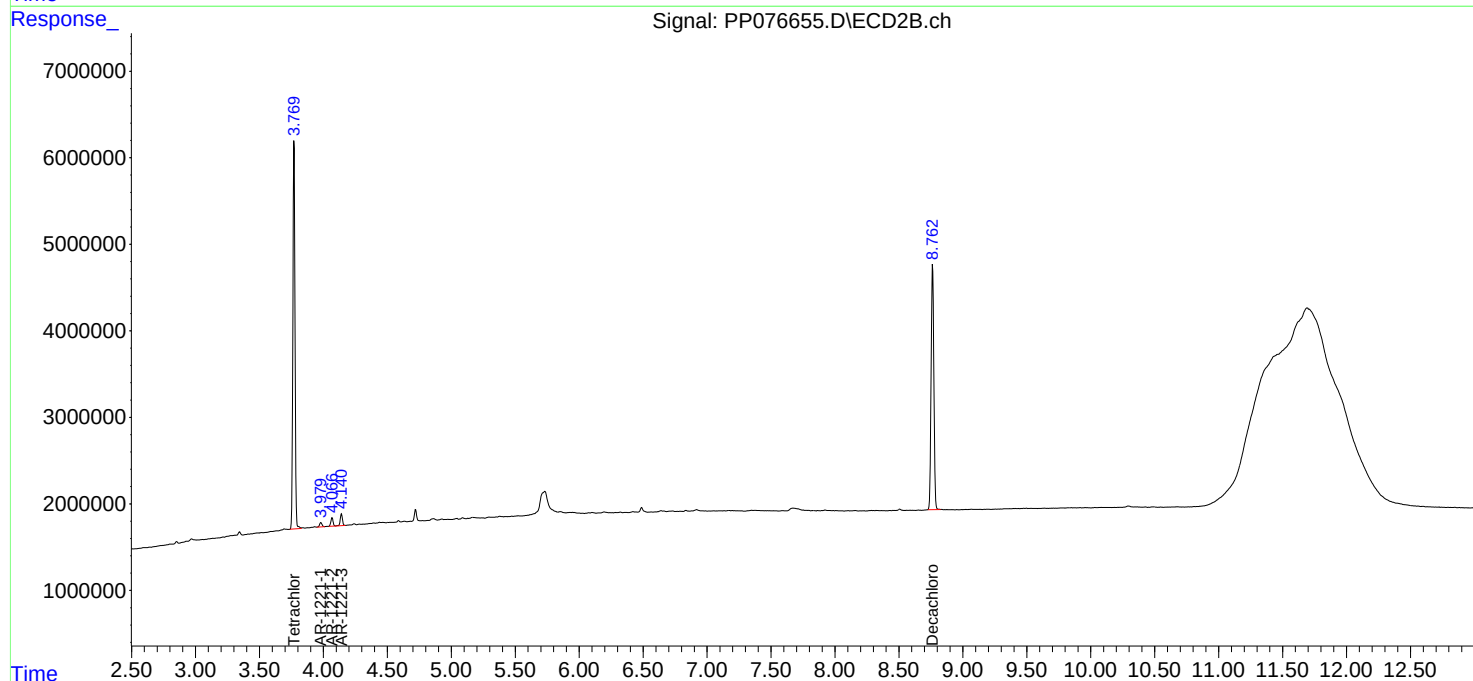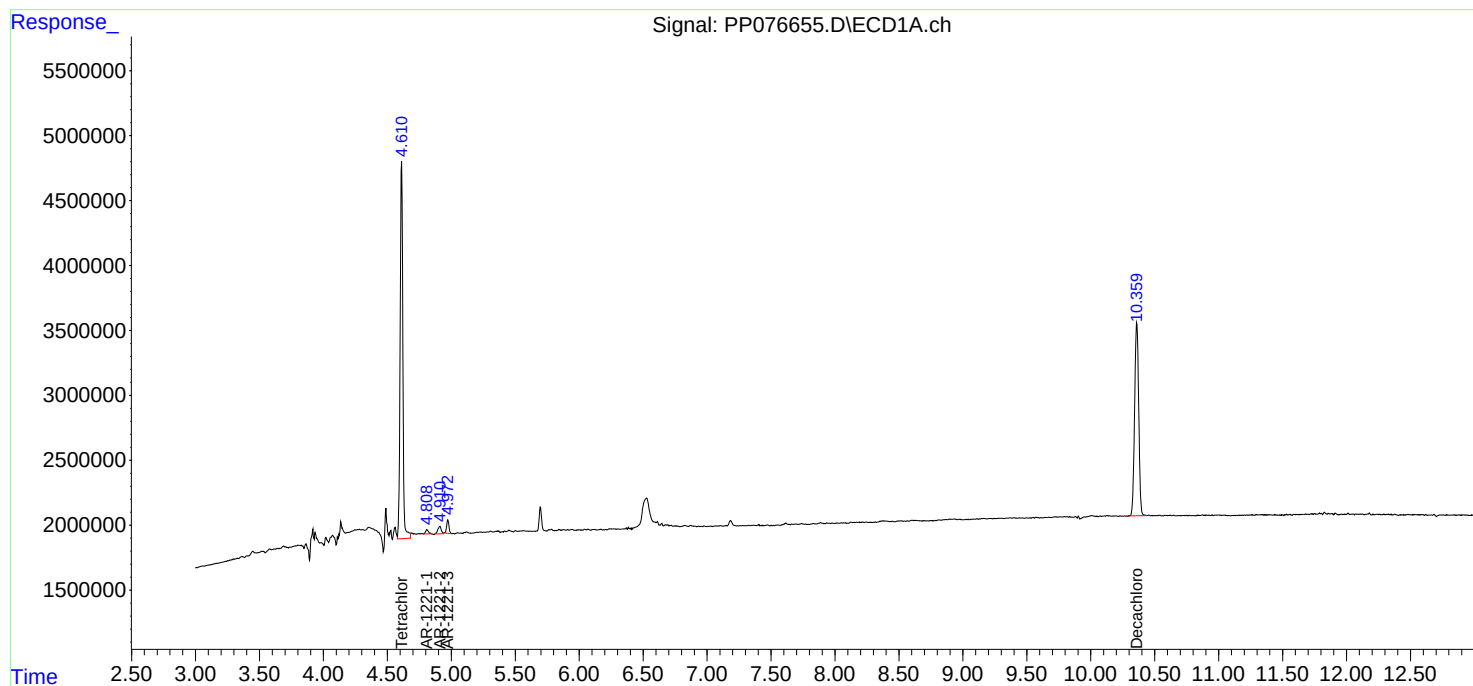

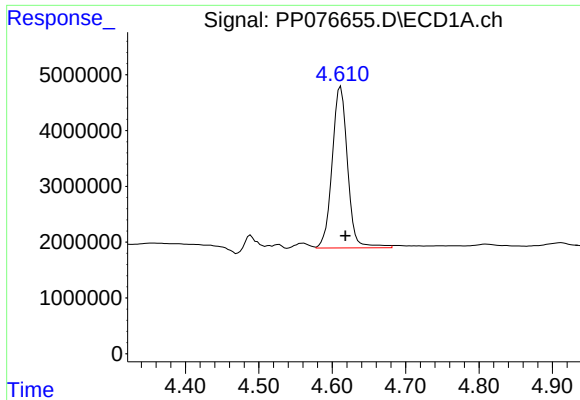


#1 Tetrachloro-m-xylene

R.T.: 4.612 min
Delta R.T.: -0.006 min
Response: 42227981
Conc: 23.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

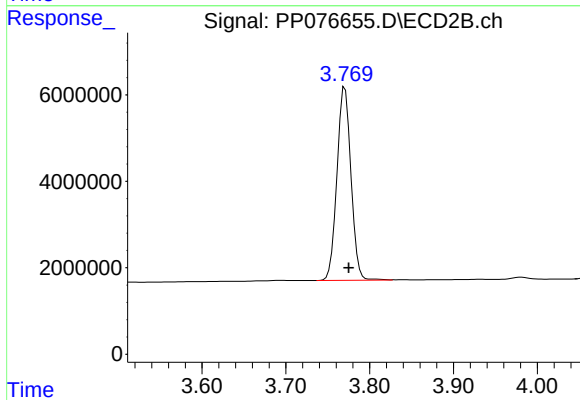


#1 Tetrachloro-m-xylene

R.T.: 3.771 min
Delta R.T.: -0.004 min
Response: 51953593
Conc: 24.94 ng/ml

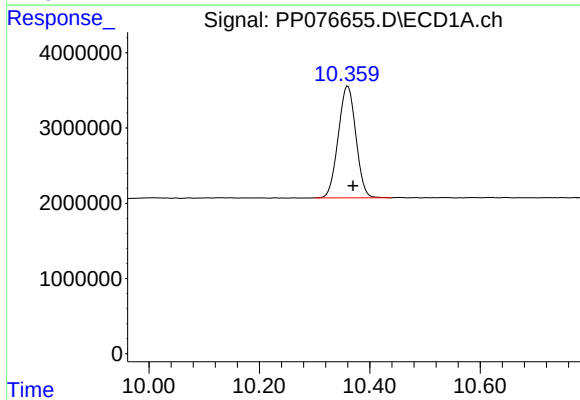


#2 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: -0.009 min
Response: 32919754
Conc: 21.97 ng/ml

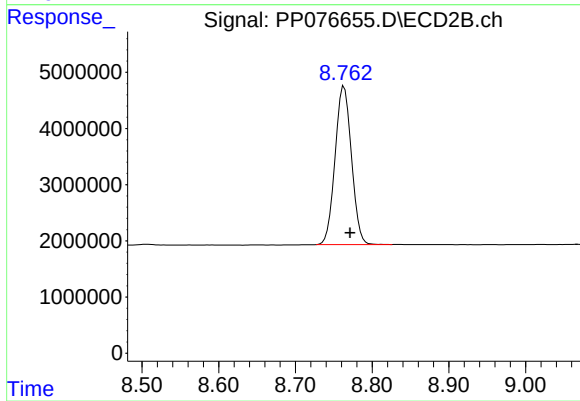

#2 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: -0.008 min
Response: 41927447
Conc: 23.76 ng/ml

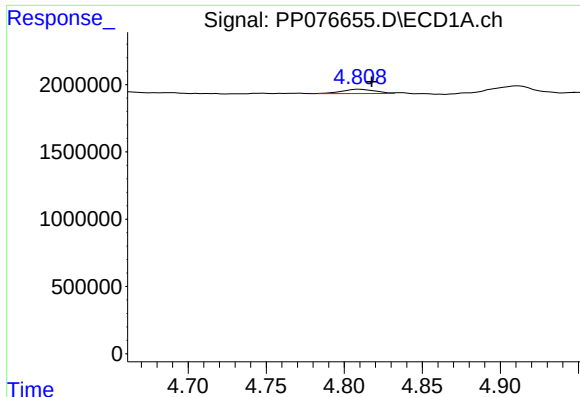


#8 AR-1221-1

R.T.: 4.808 min
Delta R.T.: -0.009 min
Response: 496787
Conc: 19.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

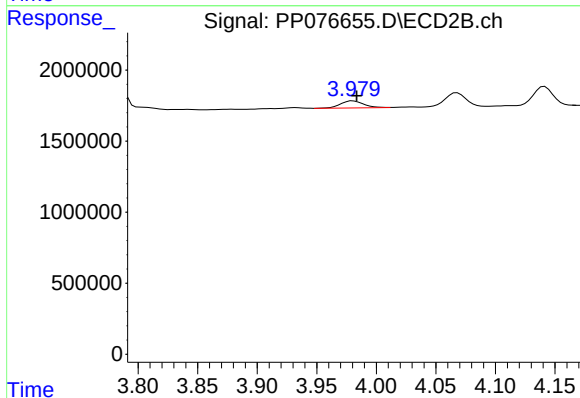


#8 AR-1221-1

R.T.: 3.980 min
Delta R.T.: -0.003 min
Response: 671589
Conc: 25.14 ng/ml

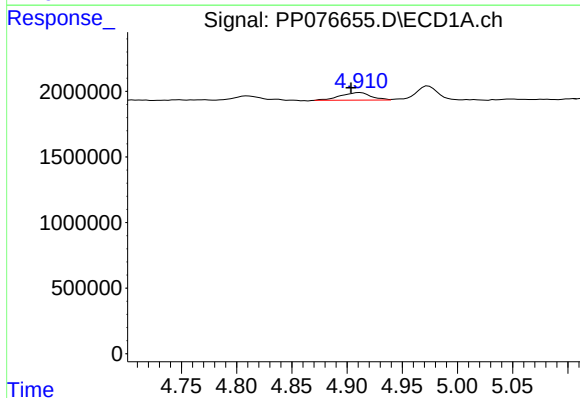


#9 AR-1221-2

R.T.: 4.910 min
Delta R.T.: 0.007 min
Response: 1096341
Conc: 55.02 ng/ml m

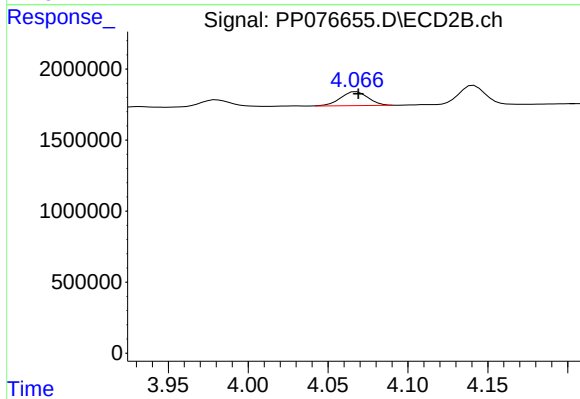

#9 AR-1221-2

R.T.: 4.066 min
Delta R.T.: -0.003 min
Response: 1188161
Conc: 59.43 ng/ml m

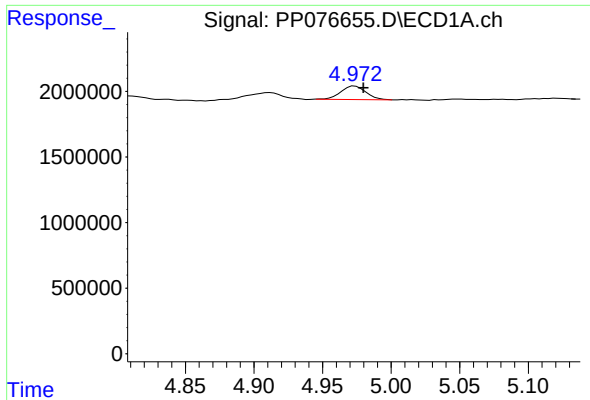


#10 AR-1221-3

R.T.: 4.972 min
Delta R.T.: -0.008 min
Response: 1312173
Conc: 23.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

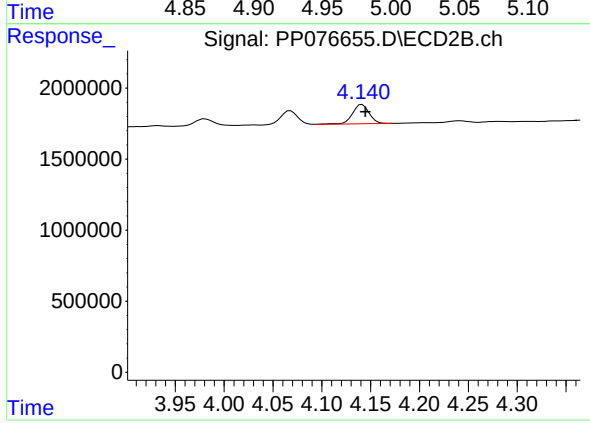

#10 AR-1221-3

R.T.: 4.141 min
Delta R.T.: -0.003 min
Response: 1623243
Conc: 26.93 ng/ml