

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 12:53
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1232-WATER-01-QT4-2025
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:54:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.615	3.774	39001022	50296853	21.248	24.147
2) SA Decachlor...	10.362	8.767	32477947	41110681	21.671	23.299
Target Compounds						
11) L3 AR-1232-1	4.977	4.145	1023472	1171205	23.543	24.876
12) L3 AR-1232-2	5.502	4.869	622712	1057238	27.844	22.926
13) L3 AR-1232-3	5.789	5.045	971141	560568	22.109	23.124
14) L3 AR-1232-4	5.949	5.129	598531	415932	26.357	19.316 #
15) L3 AR-1232-5	6.039	5.298	462154	714411	27.468	30.354m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 12:53
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1232-WATER-01-QT4-2025
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/03/2025
Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:54:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

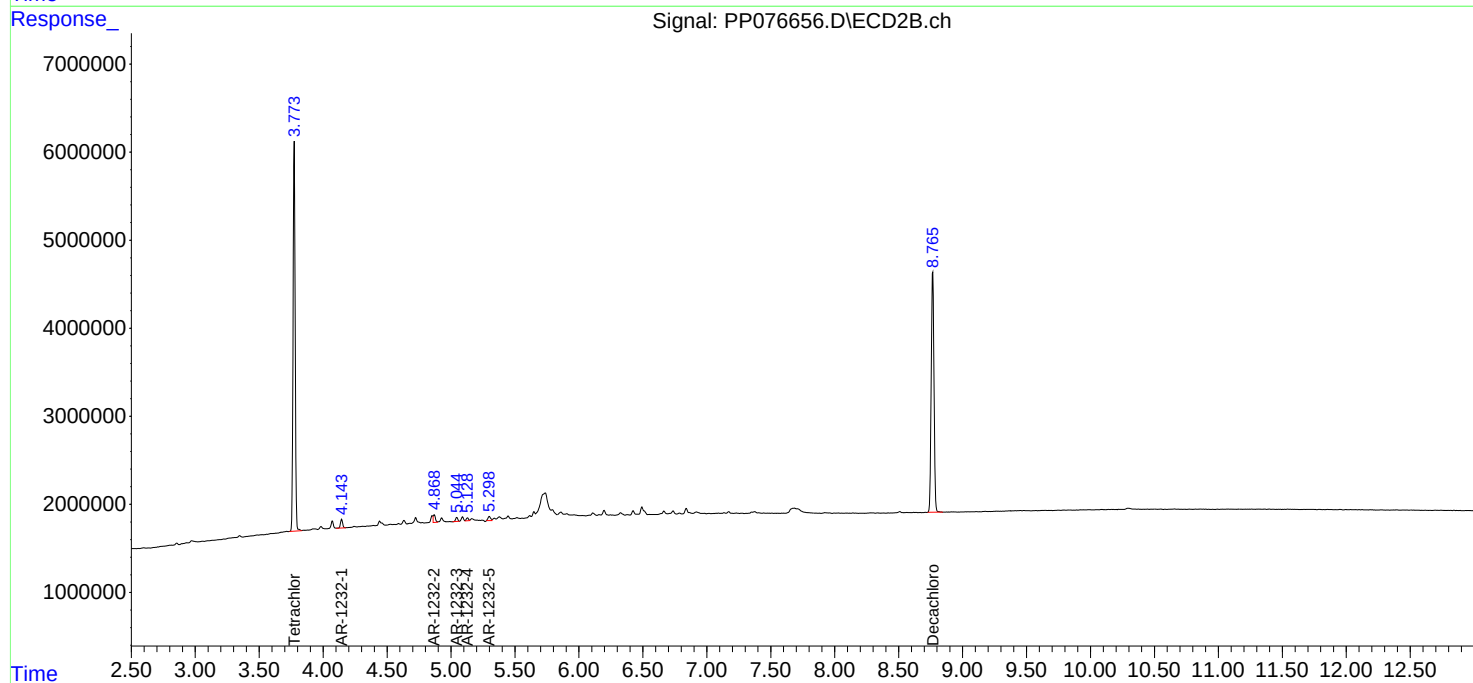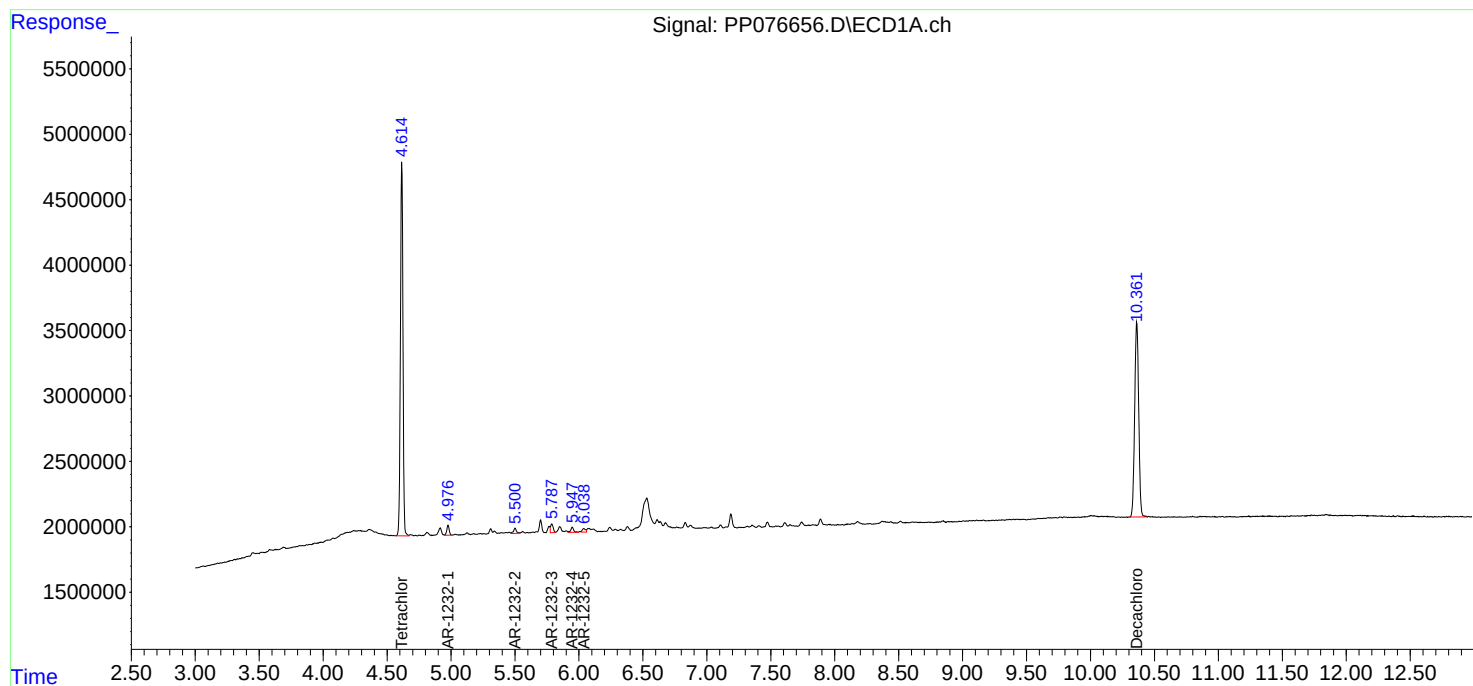

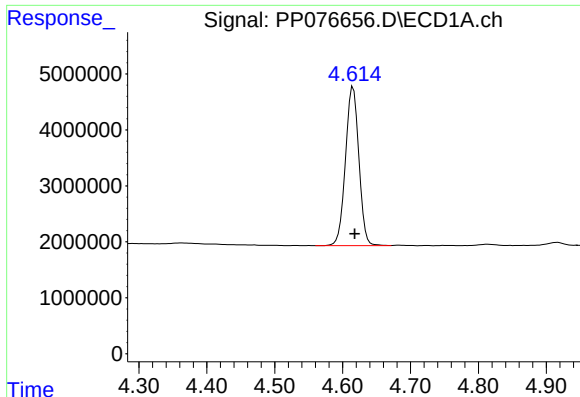


#1 Tetrachloro-m-xylene

R.T.: 4.615 min
Delta R.T.: -0.003 min
Response: 39001022
Conc: 21.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

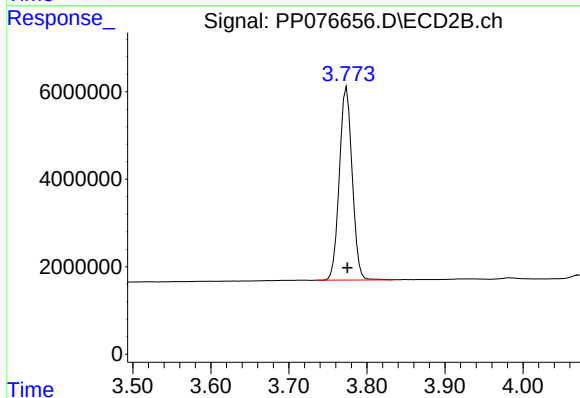


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 50296853
Conc: 24.15 ng/ml

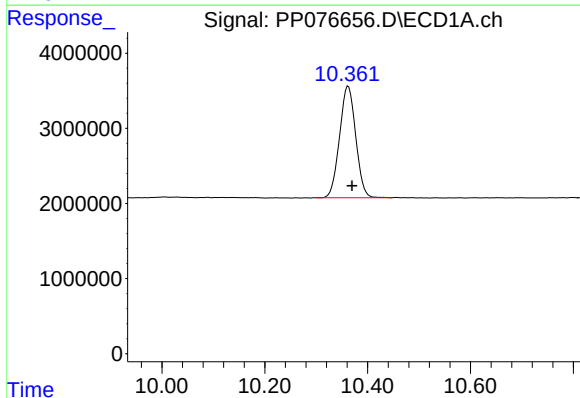


#2 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: -0.007 min
Response: 32477947
Conc: 21.67 ng/ml

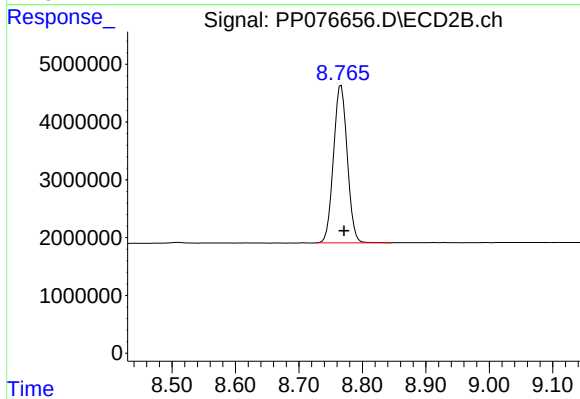

#2 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: -0.005 min
Response: 41110681
Conc: 23.30 ng/ml

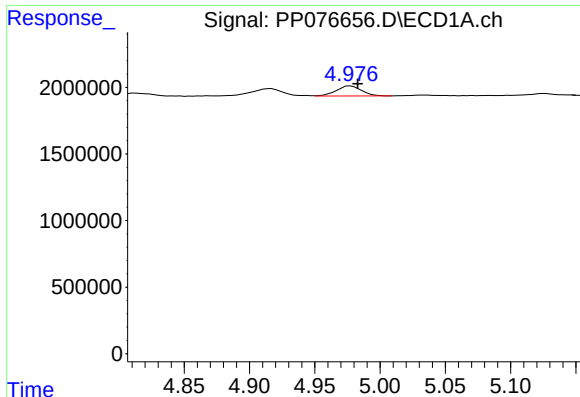


#11 AR-1232-1

R.T.: 4.977 min
Delta R.T.: -0.005 min
Response: 1023472
Conc: 23.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

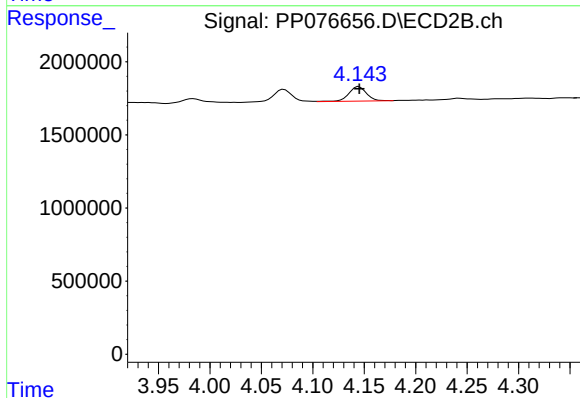


#11 AR-1232-1

R.T.: 4.145 min
Delta R.T.: 0.000 min
Response: 1171205
Conc: 24.88 ng/ml

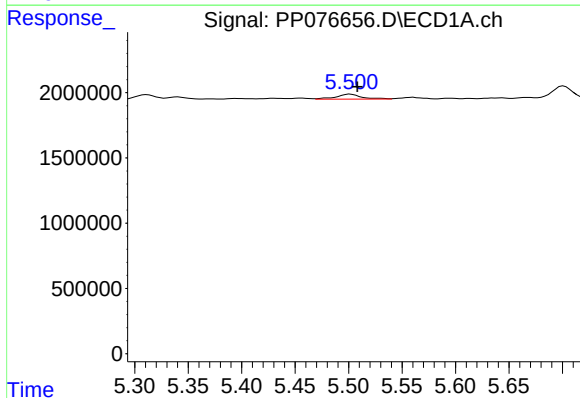


#12 AR-1232-2

R.T.: 5.502 min
Delta R.T.: -0.007 min
Response: 622712
Conc: 27.84 ng/ml

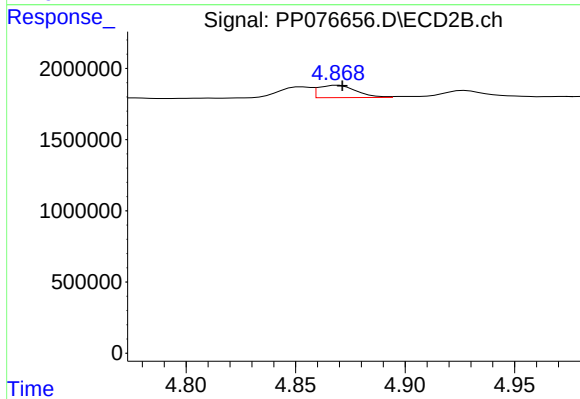

#12 AR-1232-2

R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 1057238
Conc: 22.93 ng/ml

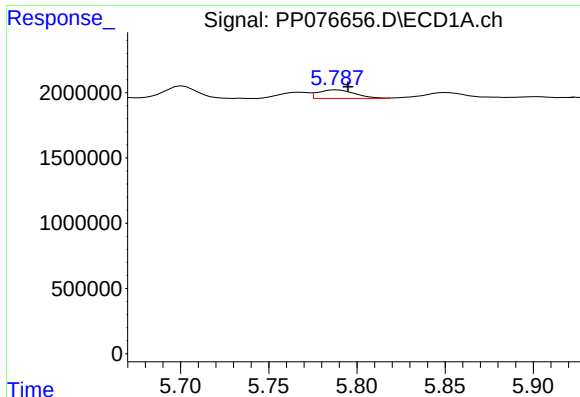


#13 AR-1232-3

R.T.: 5.789 min
Delta R.T.: -0.006 min
Response: 971141
Conc: 22.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

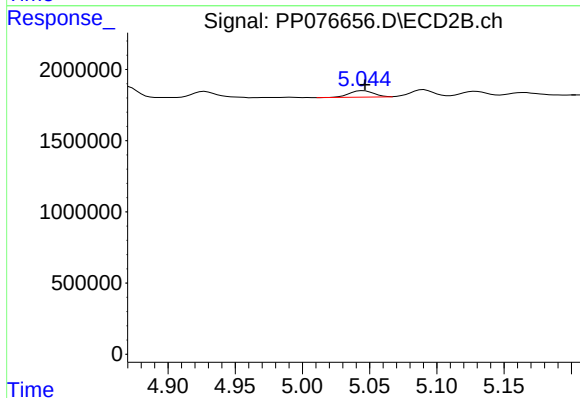


#13 AR-1232-3

R.T.: 5.045 min
Delta R.T.: -0.001 min
Response: 560568
Conc: 23.12 ng/ml

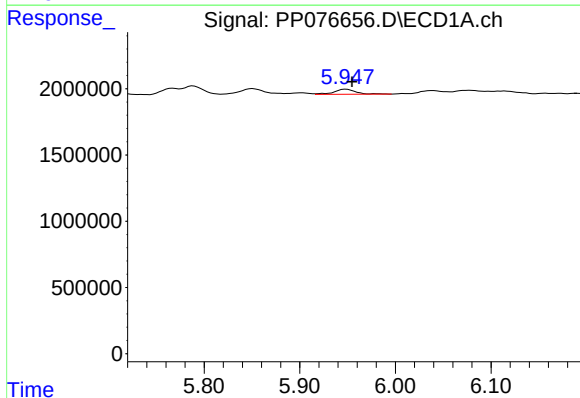


#14 AR-1232-4

R.T.: 5.949 min
Delta R.T.: -0.006 min
Response: 598531
Conc: 26.36 ng/ml

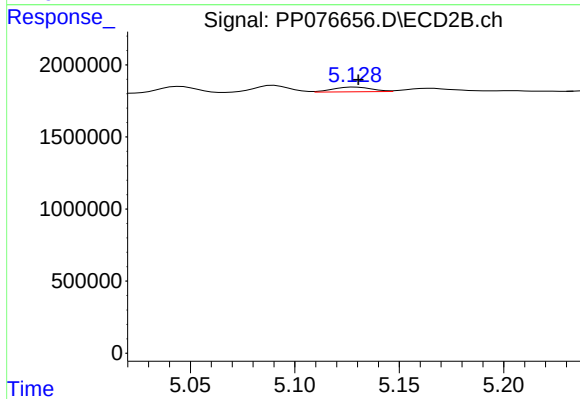

#14 AR-1232-4

R.T.: 5.129 min
Delta R.T.: -0.002 min
Response: 415932
Conc: 19.32 ng/ml

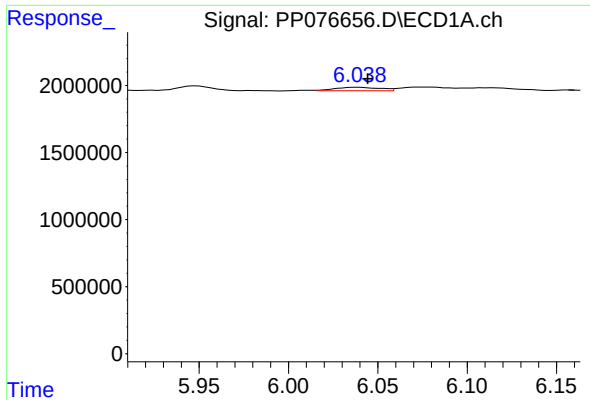


#15 AR-1232-5

R.T.: 6.039 min
Delta R.T.: -0.005 min
Response: 462154
Conc: 27.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

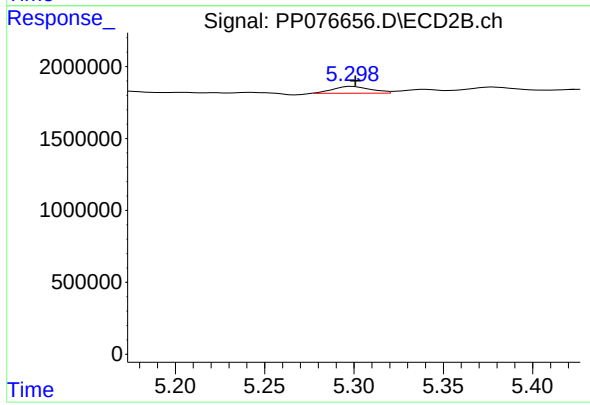

#15 AR-1232-5

R.T.: 5.298 min
Delta R.T.: -0.003 min
Response: 714411
Conc: 30.35 ng/ml m