

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 13:43
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1254-WATER-01-QT4-2025
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/02/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:55:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.615	3.774	39101751	48922711	21.303	23.488
2) SA Decachlor...	10.361	8.766	32264302	40601888	21.528	23.010
Target Compounds						
26) L6 AR-1254-1	6.613	5.648	2429765	3556423	30.289m	30.078m
27) L6 AR-1254-2	6.831	5.794	3362571	3935947	29.829	36.402m
28) L6 AR-1254-3	7.192	6.197	4339600	4973238	36.120	30.290
29) L6 AR-1254-4	7.475	6.424	2494889	3077052	27.685	29.646
30) L6 AR-1254-5	7.890	6.839	3220638	4190957	33.273	29.771

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 13:43
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1254-WATER-01-QT4-2025
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:55:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

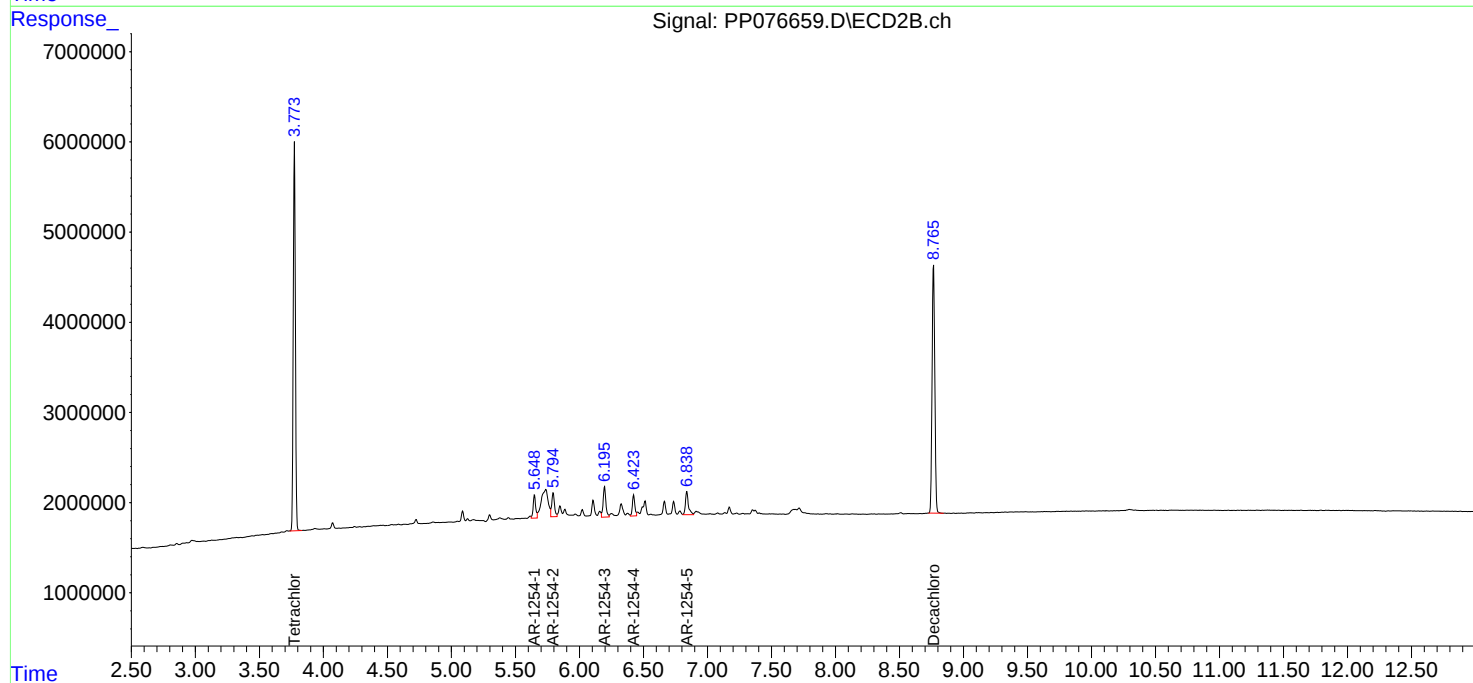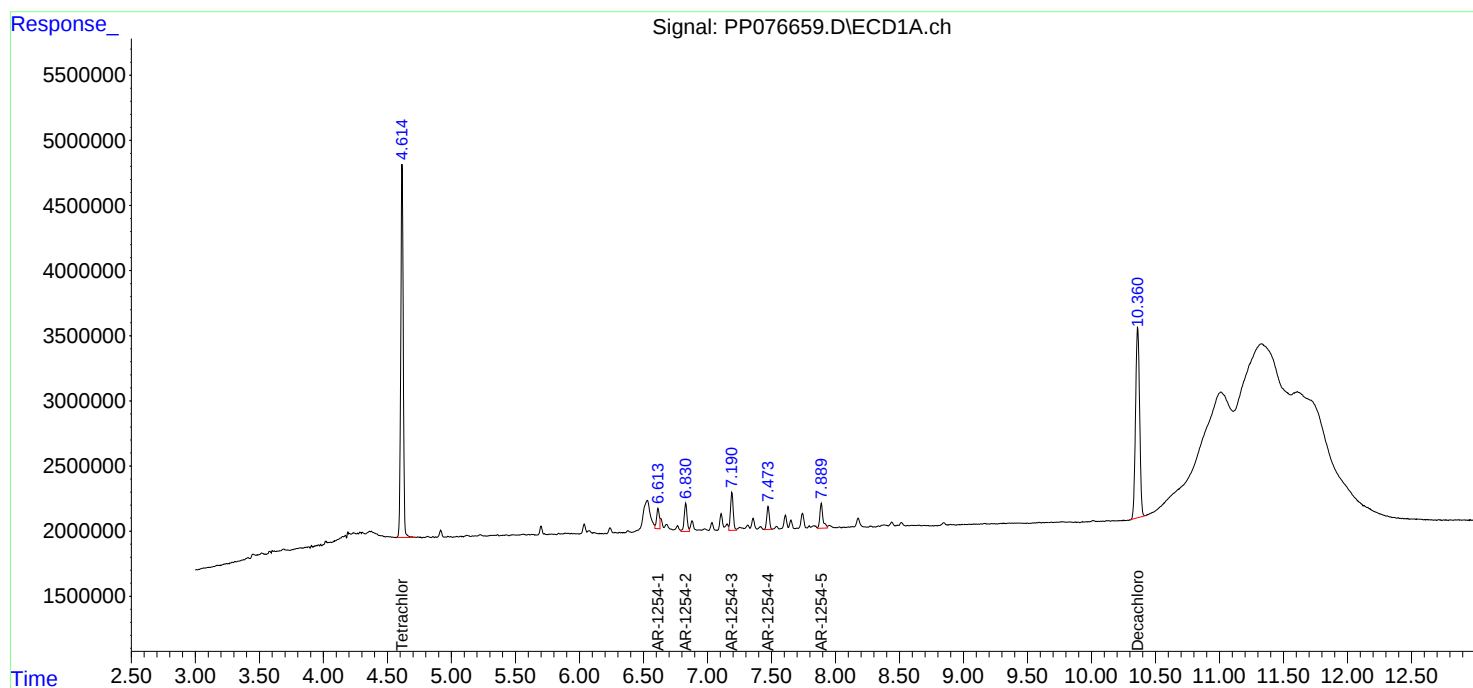

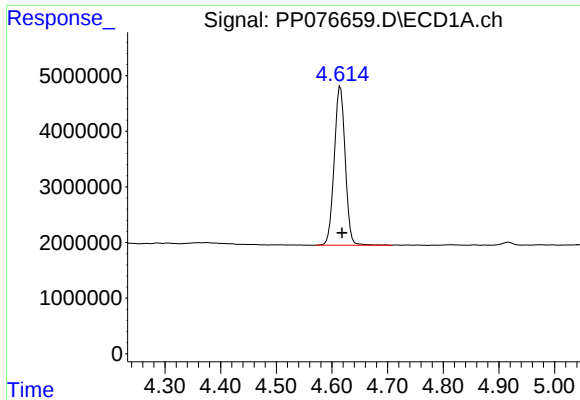


#1 Tetrachloro-m-xylene

R.T.: 4.615 min
Delta R.T.: -0.003 min
Response: 39101751
Conc: 21.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

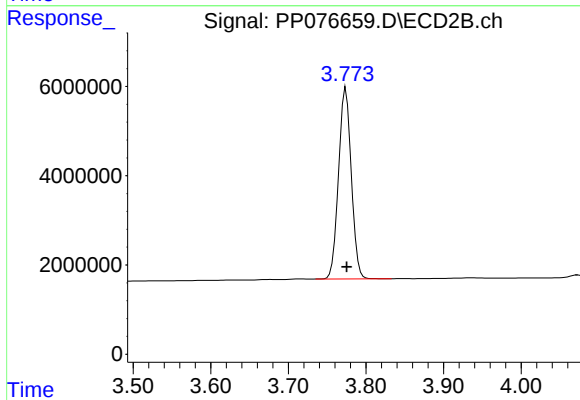


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 48922711
Conc: 23.49 ng/ml

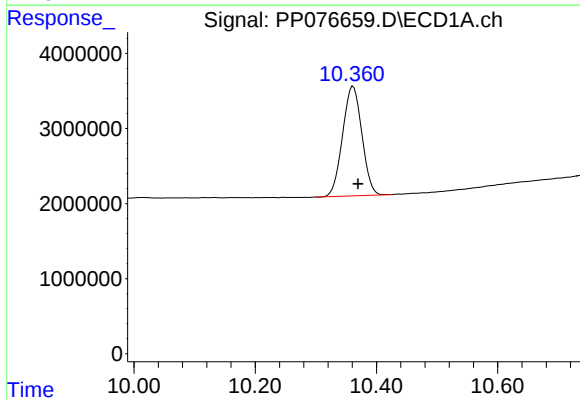


#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.008 min
Response: 32264302
Conc: 21.53 ng/ml

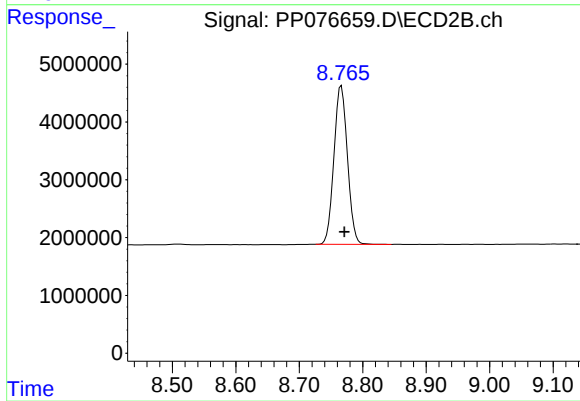

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.005 min
Response: 40601888
Conc: 23.01 ng/ml

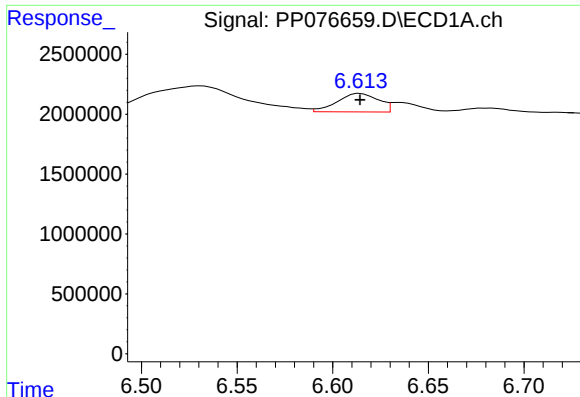


#26 AR-1254-1

R.T.: 6.613 min
Delta R.T.: -0.001 min
Response: 2429765
Conc: 30.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

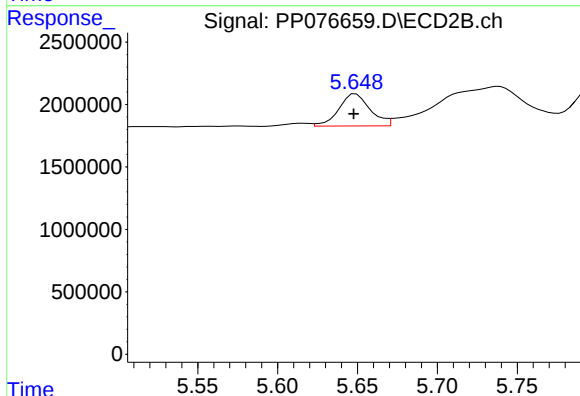


#26 AR-1254-1

R.T.: 5.648 min
Delta R.T.: 0.000 min
Response: 3556423
Conc: 30.08 ng/ml m

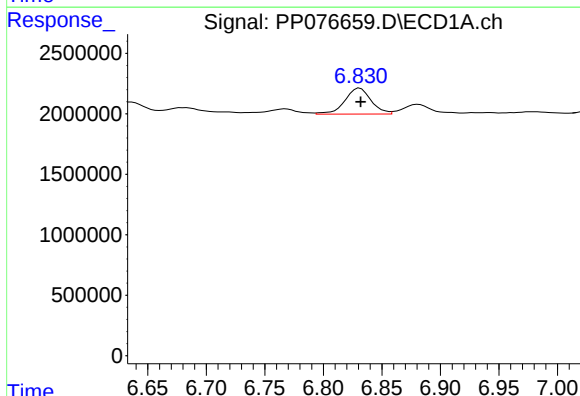


#27 AR-1254-2

R.T.: 6.831 min
Delta R.T.: 0.000 min
Response: 3362571
Conc: 29.83 ng/ml

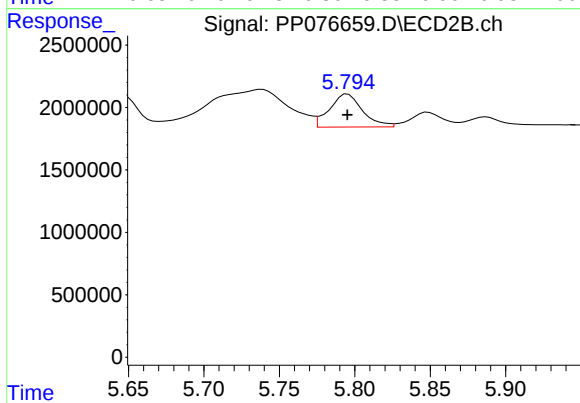

#27 AR-1254-2

R.T.: 5.794 min
Delta R.T.: -0.001 min
Response: 3935947
Conc: 36.40 ng/ml m

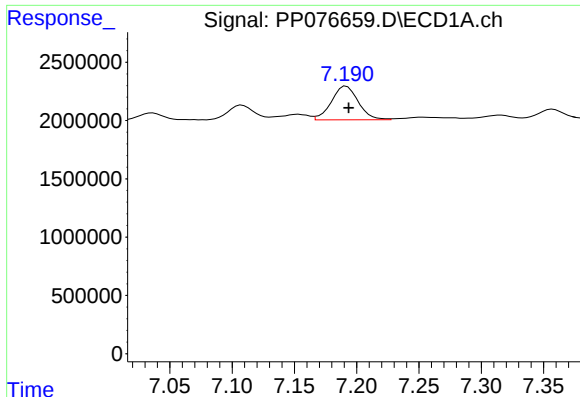


#28 AR-1254-3

R.T.: 7.192 min
Delta R.T.: -0.002 min
Response: 4339600
Conc: 36.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

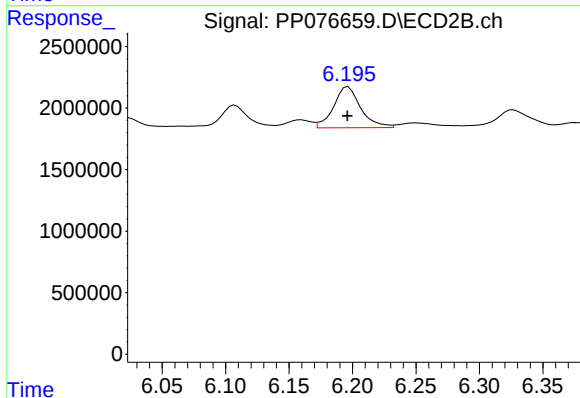


#28 AR-1254-3

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 4973238
Conc: 30.29 ng/ml

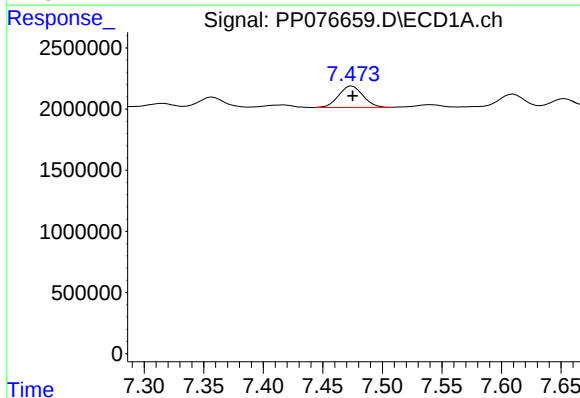


#29 AR-1254-4

R.T.: 7.475 min
Delta R.T.: 0.000 min
Response: 2494889
Conc: 27.68 ng/ml

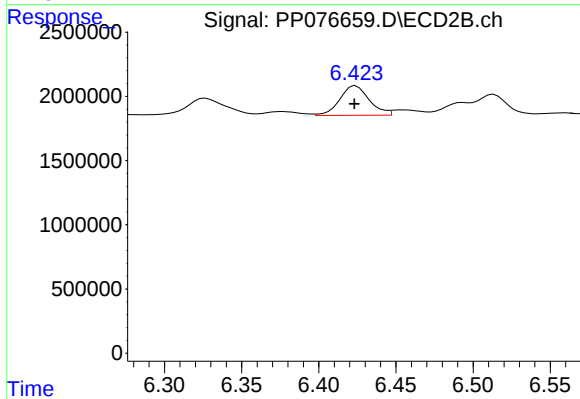

#29 AR-1254-4

R.T.: 6.424 min
Delta R.T.: 0.001 min
Response: 3077052
Conc: 29.65 ng/ml

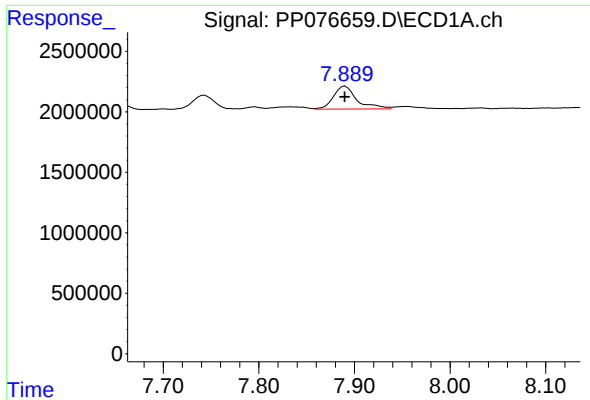


#30 AR-1254-5

R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 3220638
Conc: 33.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

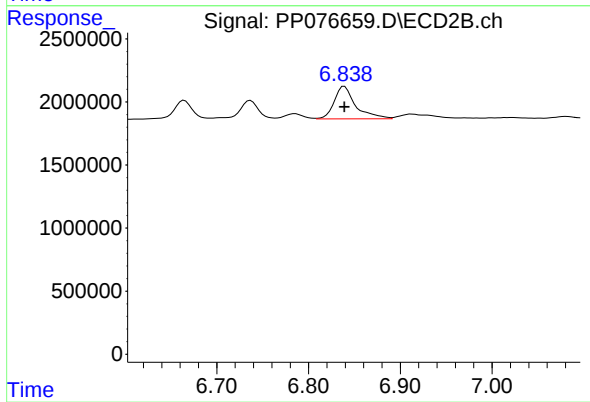

#30 AR-1254-5

R.T.: 6.839 min
Delta R.T.: 0.000 min
Response: 4190957
Conc: 29.77 ng/ml