

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 13:59
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1262-WATER-01-QT4-2025
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/02/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:55:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.615	3.773	47451562	59598517	25.852	28.613
2) SA Decachlor...	10.361	8.766	39584763	49604861	26.413	28.112
Target Compounds						
36) L8 AR-1262-1	8.192	6.877	2923262	4248942	29.541	31.871
37) L8 AR-1262-2	8.516	7.134	5349972	4004542	31.023	33.394
38) L8 AR-1262-3	8.838	7.656	3600480	4533821	28.638	46.022m#
39) L8 AR-1262-4	8.923	7.718	2668183	6113776	26.892	35.039m#
40) L8 AR-1262-5	9.588	8.214	2064474	2253221	29.060	28.040

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 13:59
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1262-WATER-01-QT4-2025
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:55:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

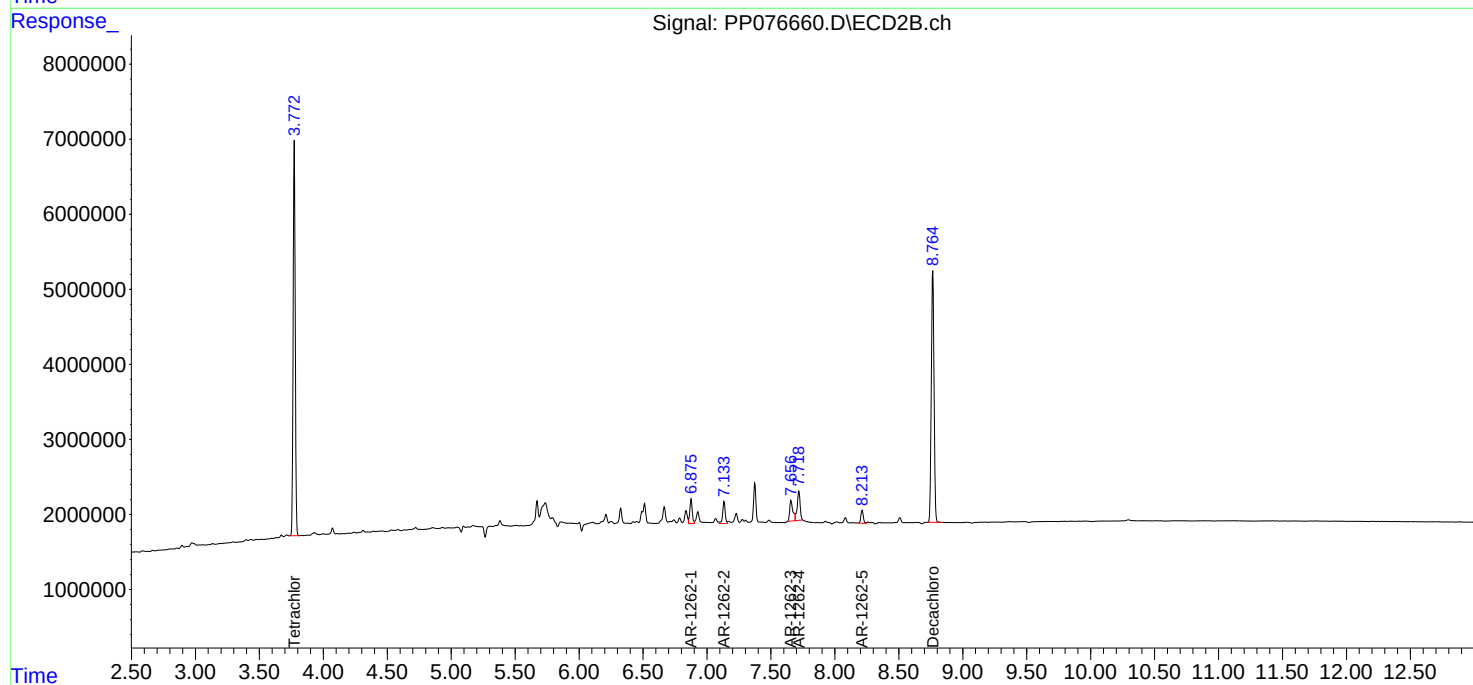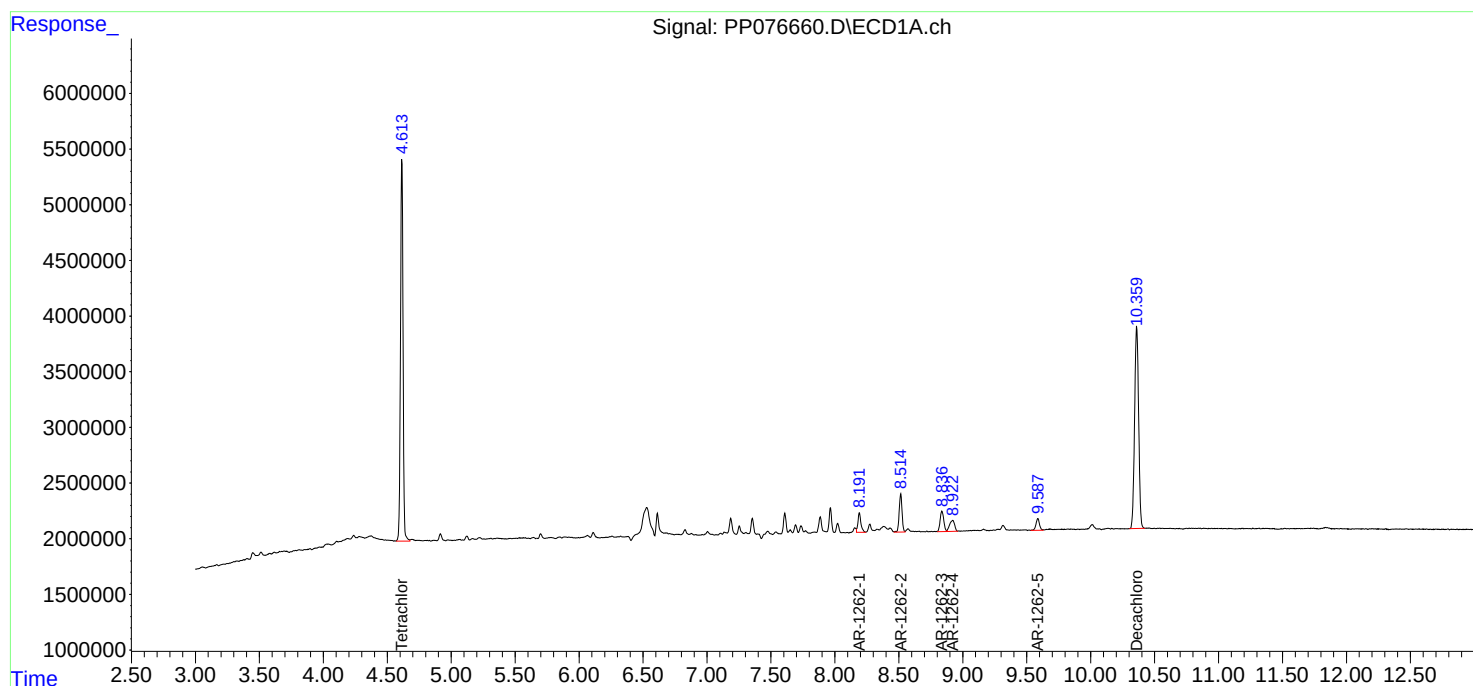

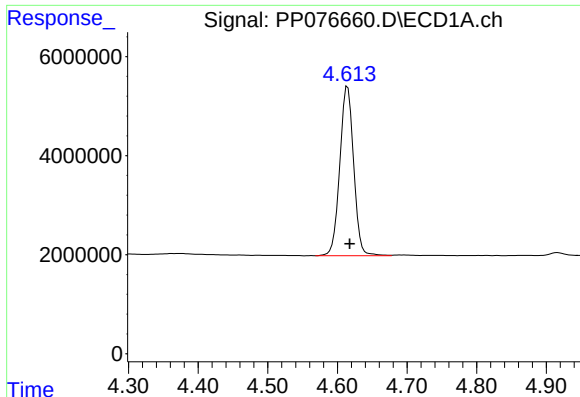


#1 Tetrachloro-m-xylene

R.T.: 4.615 min
Delta R.T.: -0.003 min
Response: 47451562
Conc: 25.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

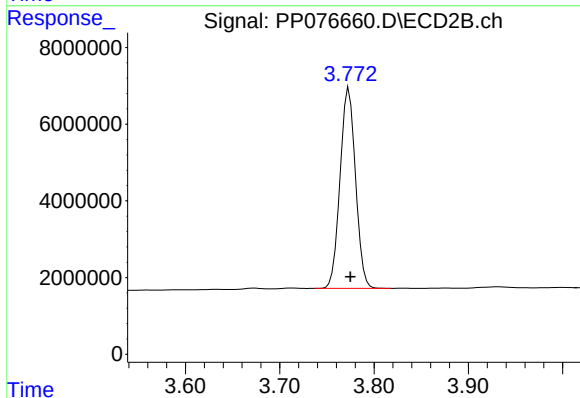


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: -0.002 min
Response: 59598517
Conc: 28.61 ng/ml

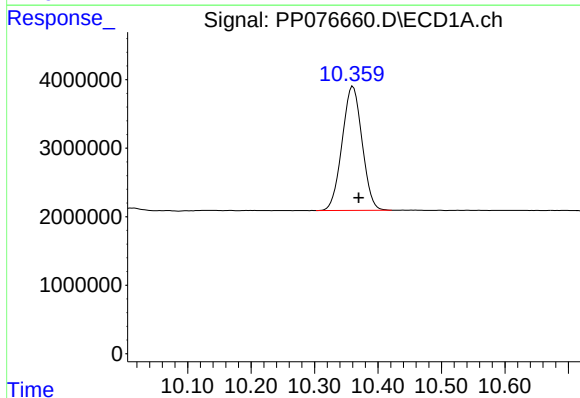


#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.009 min
Response: 39584763
Conc: 26.41 ng/ml

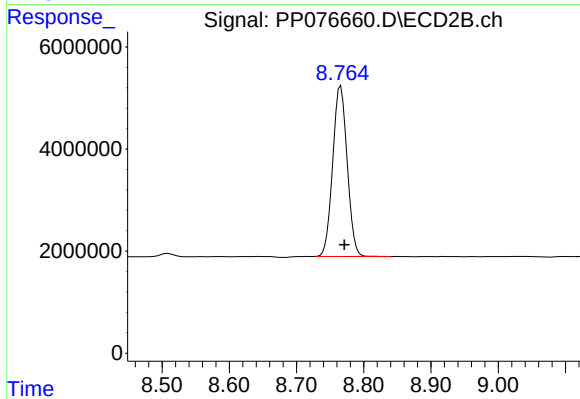

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.005 min
Response: 49604861
Conc: 28.11 ng/ml

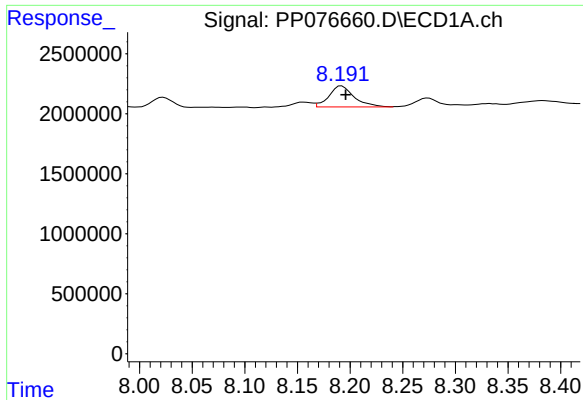


#36 AR-1262-1

R.T.: 8.192 min
Delta R.T.: -0.004 min
Response: 2923262
Conc: 29.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

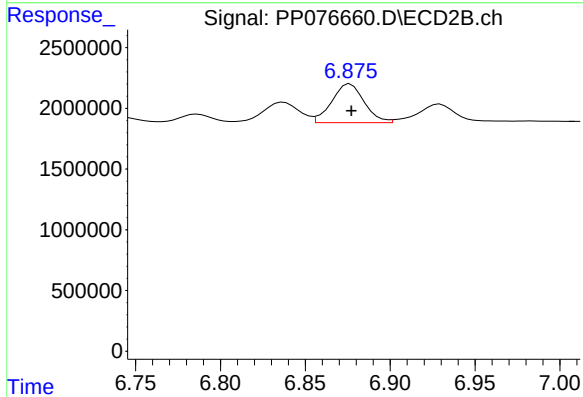


#36 AR-1262-1

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 4248942
Conc: 31.87 ng/ml

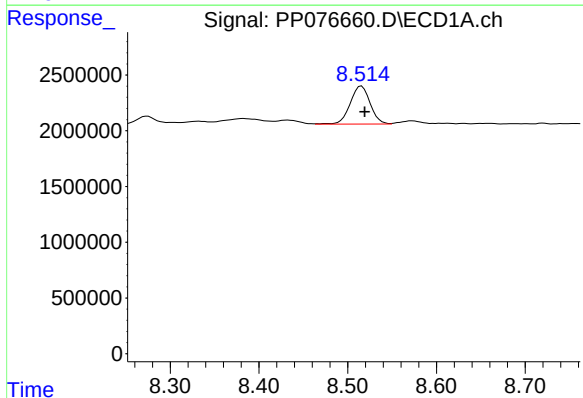


#37 AR-1262-2

R.T.: 8.516 min
Delta R.T.: -0.003 min
Response: 5349972
Conc: 31.02 ng/ml

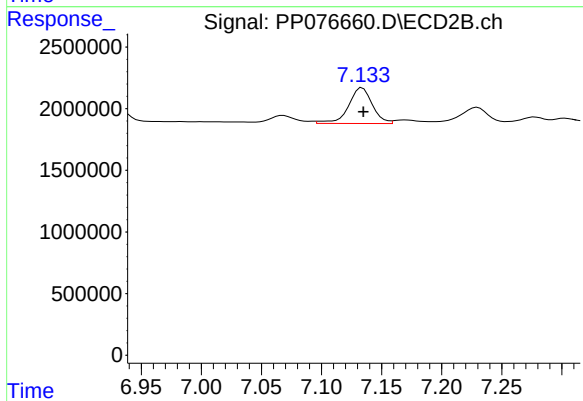

#37 AR-1262-2

R.T.: 7.134 min
Delta R.T.: 0.000 min
Response: 4004542
Conc: 33.39 ng/ml

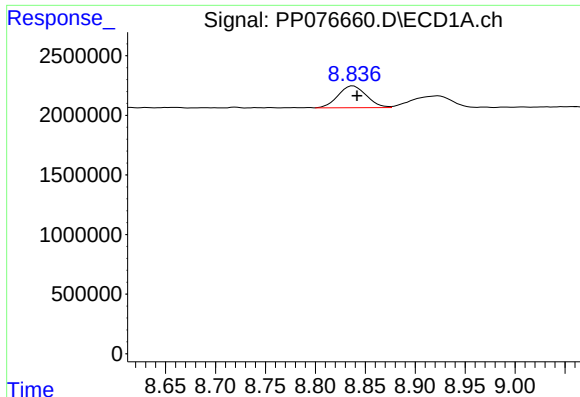


#38 AR-1262-3

R.T.: 8.838 min
Delta R.T.: -0.004 min
Response: 3600480
Conc: 28.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

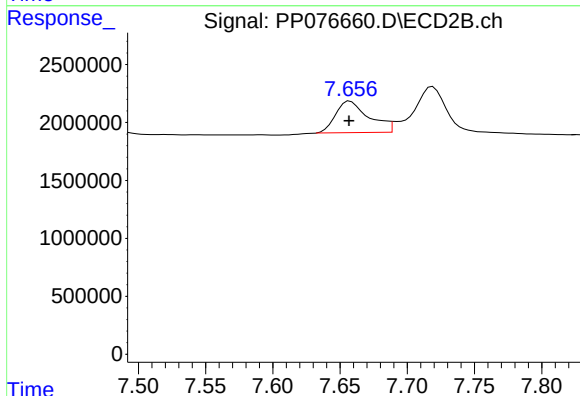


#38 AR-1262-3

R.T.: 7.656 min
Delta R.T.: 0.000 min
Response: 4533821
Conc: 46.02 ng/ml m

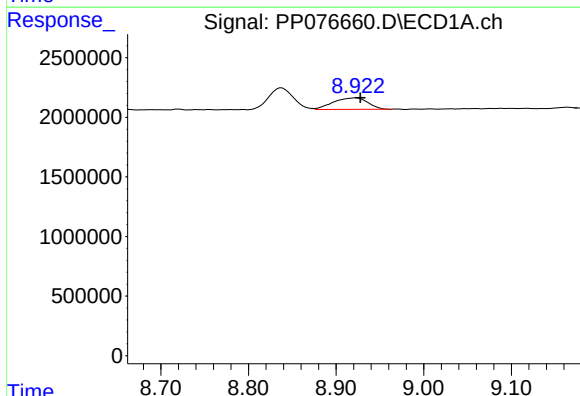


#39 AR-1262-4

R.T.: 8.923 min
Delta R.T.: -0.004 min
Response: 2668183
Conc: 26.89 ng/ml

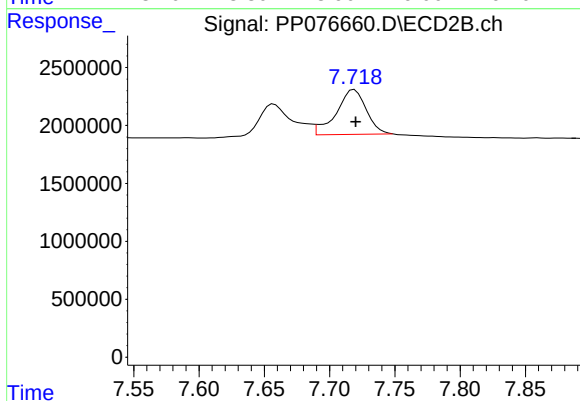

#39 AR-1262-4

R.T.: 7.718 min
Delta R.T.: -0.002 min
Response: 6113776
Conc: 35.04 ng/ml m

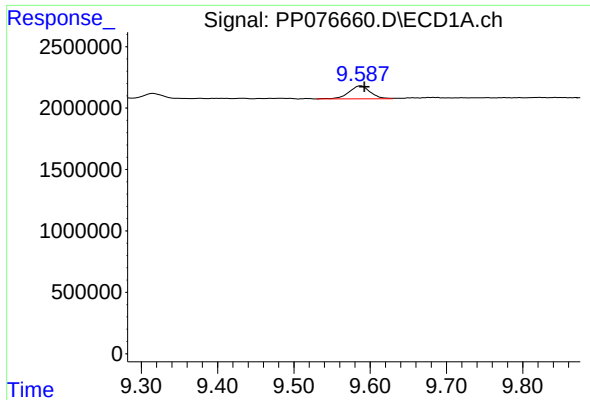


#40 AR-1262-5

R.T.: 9.588 min
Delta R.T.: -0.004 min
Response: 2064474
Conc: 29.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/02/2025
Supervised By :Sohil Jodhani 12/03/2025

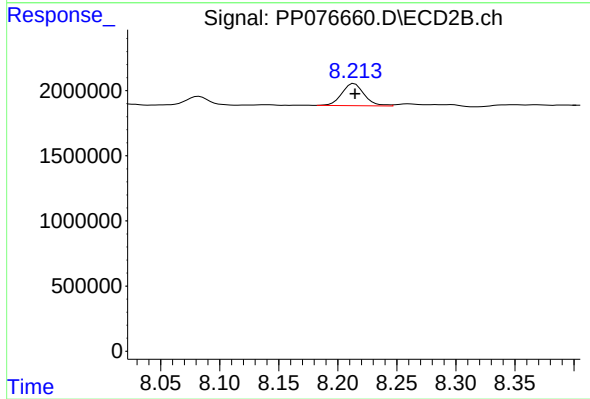

#40 AR-1262-5

R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 2253221
Conc: 28.04 ng/ml