

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076665.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 15:38
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1221-WATER-40 PPB-QT4-2025
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:02:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.617	3.776	44762639	53973387	24.387	25.912
2) SA Decachlor...	10.362	8.767	37654002	45456718	25.125	25.762
Target Compounds						
8) L2 AR-1221-1	4.816	3.985	1055511	1121979	40.858	41.994
9) L2 AR-1221-2	4.916	4.072	1561182	1541138	78.344	77.089
10) L2 AR-1221-3	4.978	4.146	2466582	2593220	44.237	43.025



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076665.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 15:38
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1221-WATER-40 PPB-QT4-2025
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:02:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

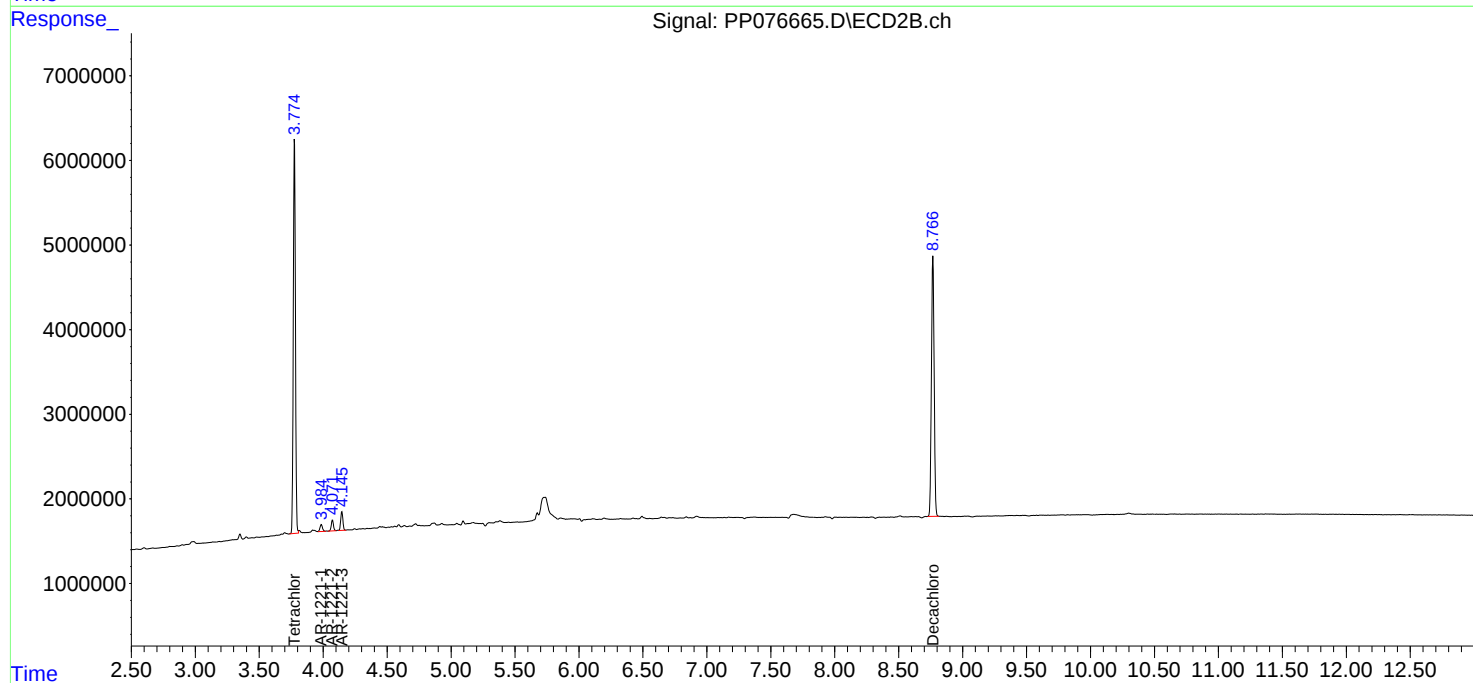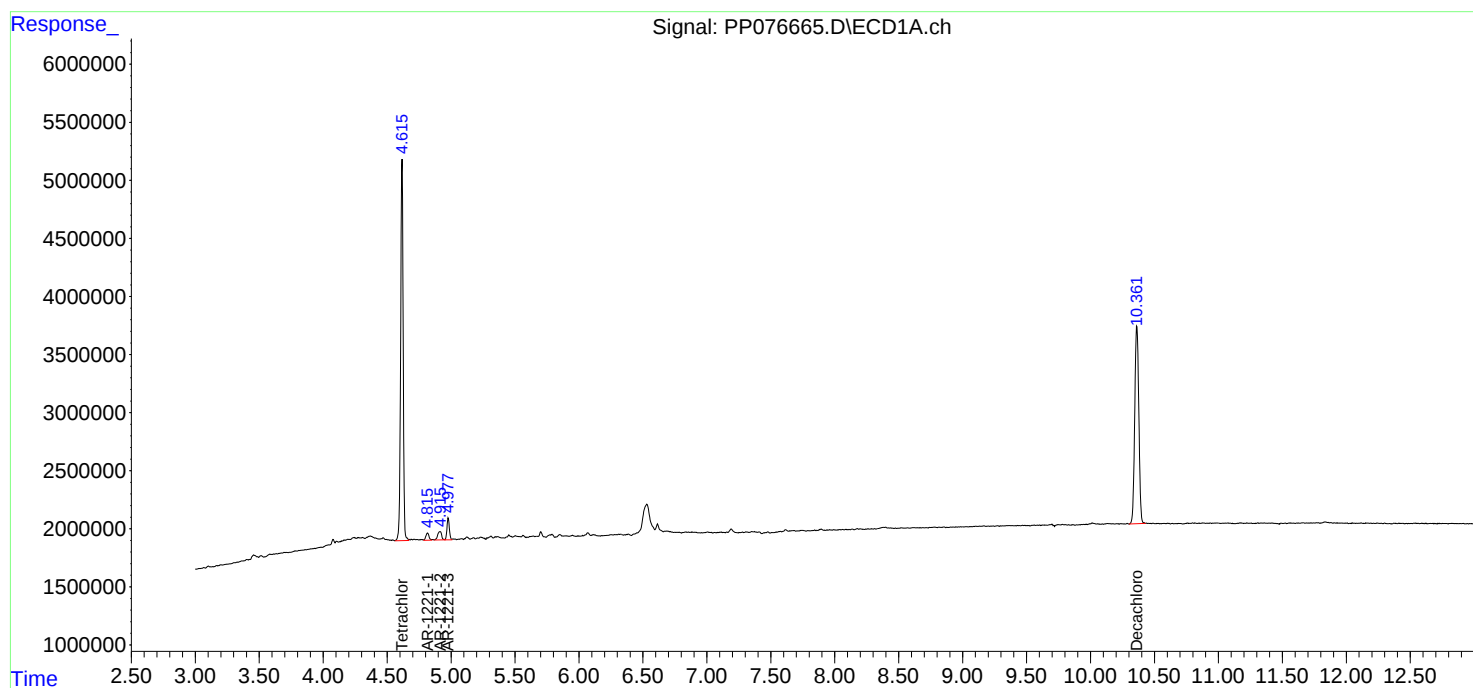


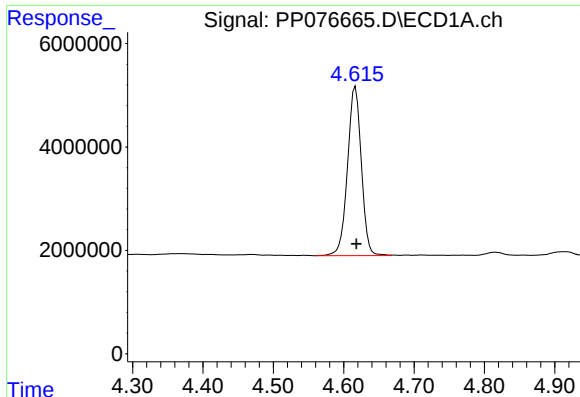

#1 Tetrachloro-m-xylene


R.T.: 4.617 min
Delta R.T.: -0.001 min
Response: 44762639
Conc: 24.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

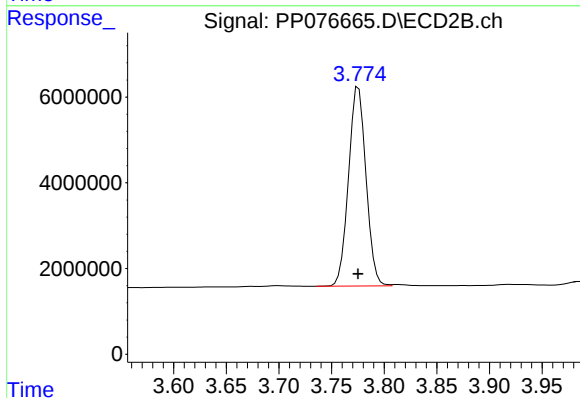


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 53973387
Conc: 25.91 ng/ml

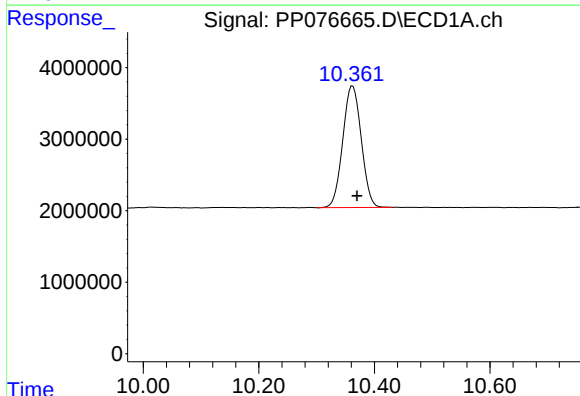


#2 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: -0.007 min
Response: 37654002
Conc: 25.12 ng/ml

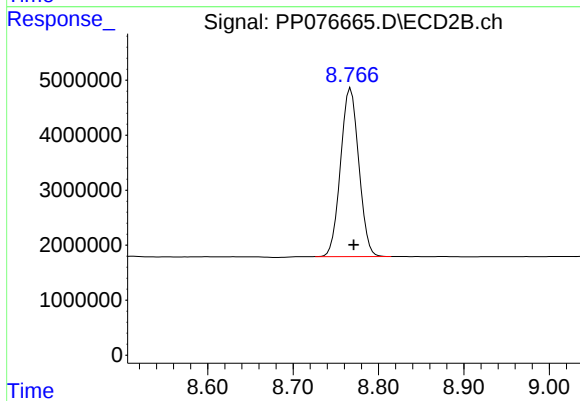

#2 Decachlorobiphenyl


R.T.: 8.767 min
Delta R.T.: -0.004 min
Response: 45456718
Conc: 25.76 ng/ml

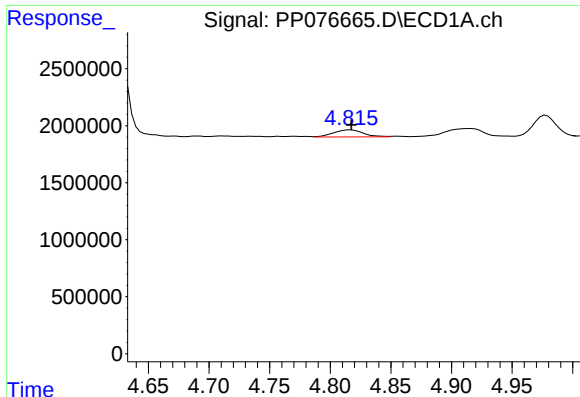

#8 AR-1221-1


R.T.: 4.816 min
Delta R.T.: -0.001 min
Response: 1055511
Conc: 40.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

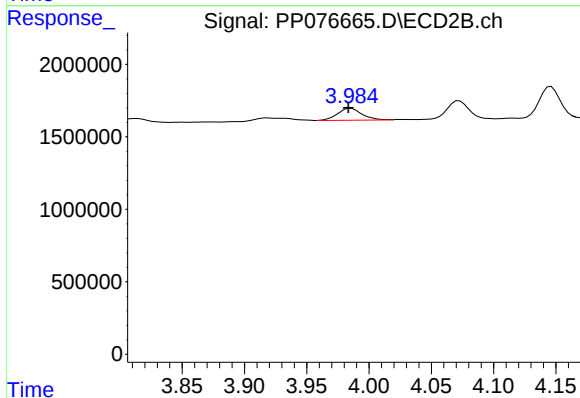


#8 AR-1221-1

R.T.: 3.985 min
Delta R.T.: 0.002 min
Response: 1121979
Conc: 41.99 ng/ml

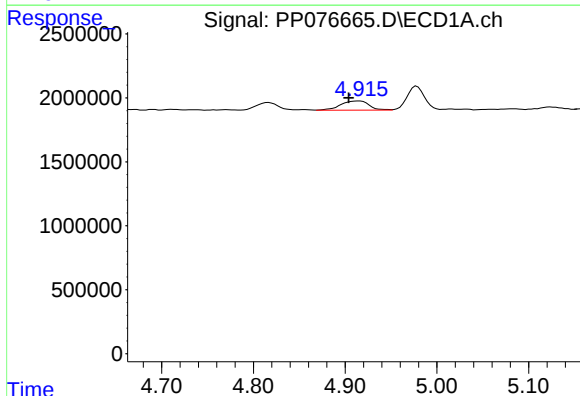


#9 AR-1221-2

R.T.: 4.916 min
Delta R.T.: 0.012 min
Response: 1561182
Conc: 78.34 ng/ml

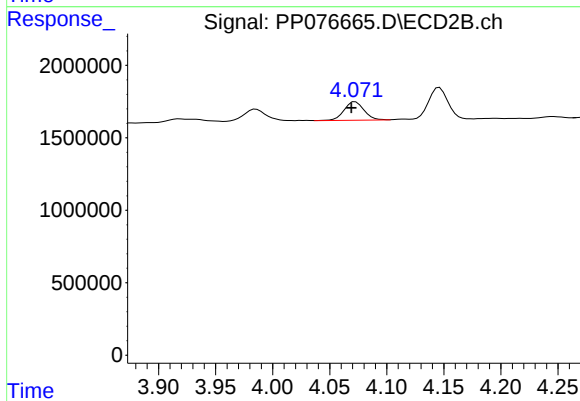

#9 AR-1221-2


R.T.: 4.072 min
Delta R.T.: 0.003 min
Response: 1541138
Conc: 77.09 ng/ml

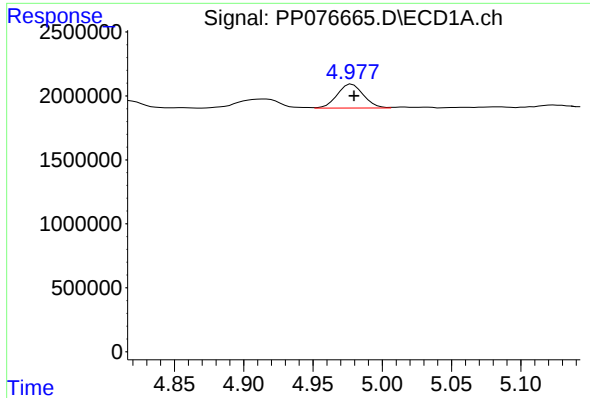

#10 AR-1221-3

R.T.: 4.978 min
Delta R.T.: -0.002 min
Response: 2466582
Conc: 44.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

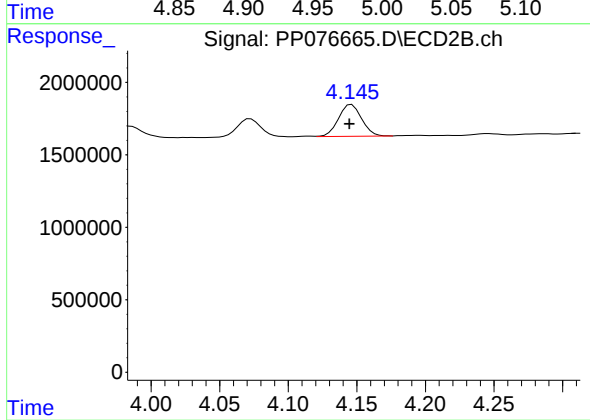

#10 AR-1221-3

R.T.: 4.146 min
Delta R.T.: 0.002 min
Response: 2593220
Conc: 43.03 ng/ml