

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 16:44
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1254-WATER-40 PPB-QT4-2025
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:04:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.614	3.773	40975890	48367833	22.324	23.221
2) SA Decachlor...	10.359	8.764	34893660	41639261	23.283	23.598
Target Compounds						
26) L6 AR-1254-1	6.611	5.645	4397691	4900239	54.821m	41.443m
27) L6 AR-1254-2	6.828	5.792	4518315	5107725	40.082m	47.239m
28) L6 AR-1254-3	7.189	6.193	5313427	6582021	44.225m	40.089m
29) L6 AR-1254-4	7.471	6.422	3695514	4420037	41.007m	42.585
30) L6 AR-1254-5	7.887	6.837	3681221	5766131	38.031m	40.960

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 16:44
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1254-WATER-40 PPB-QT4-2025
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/03/2025
Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:04:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

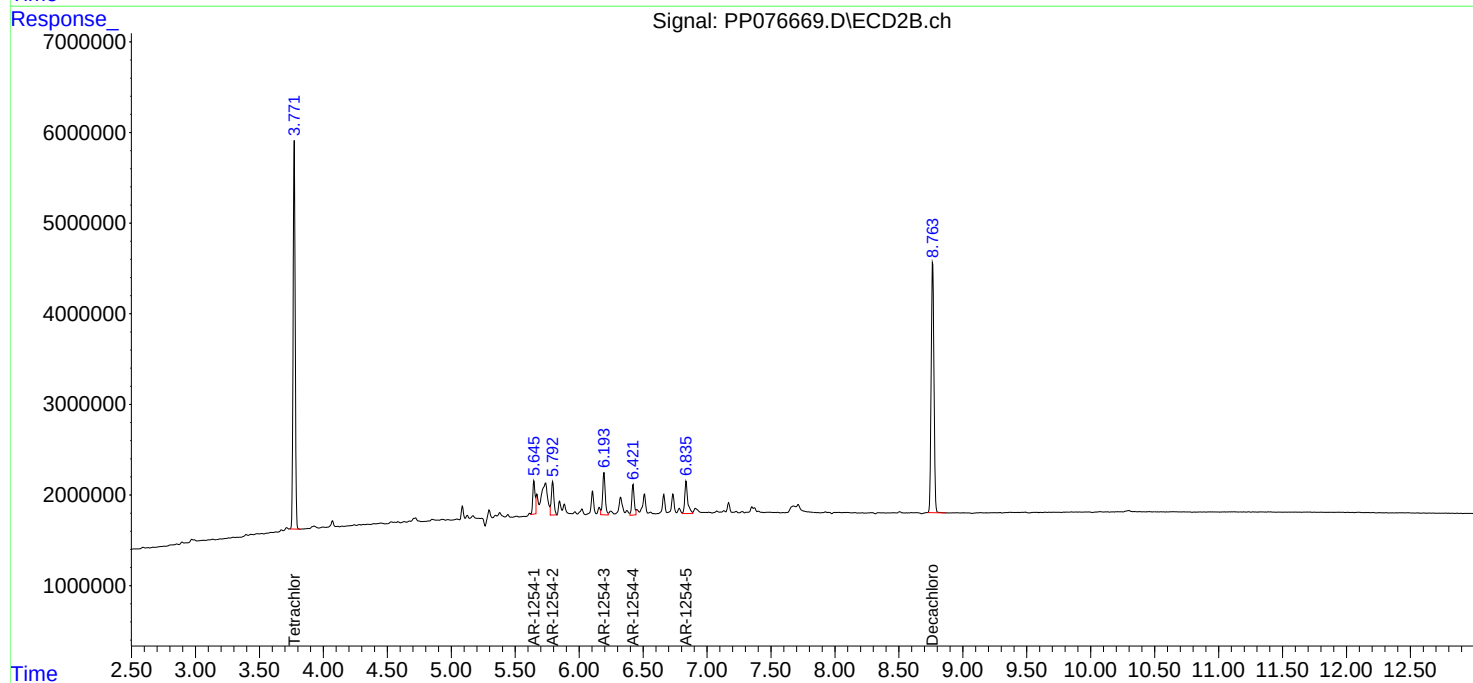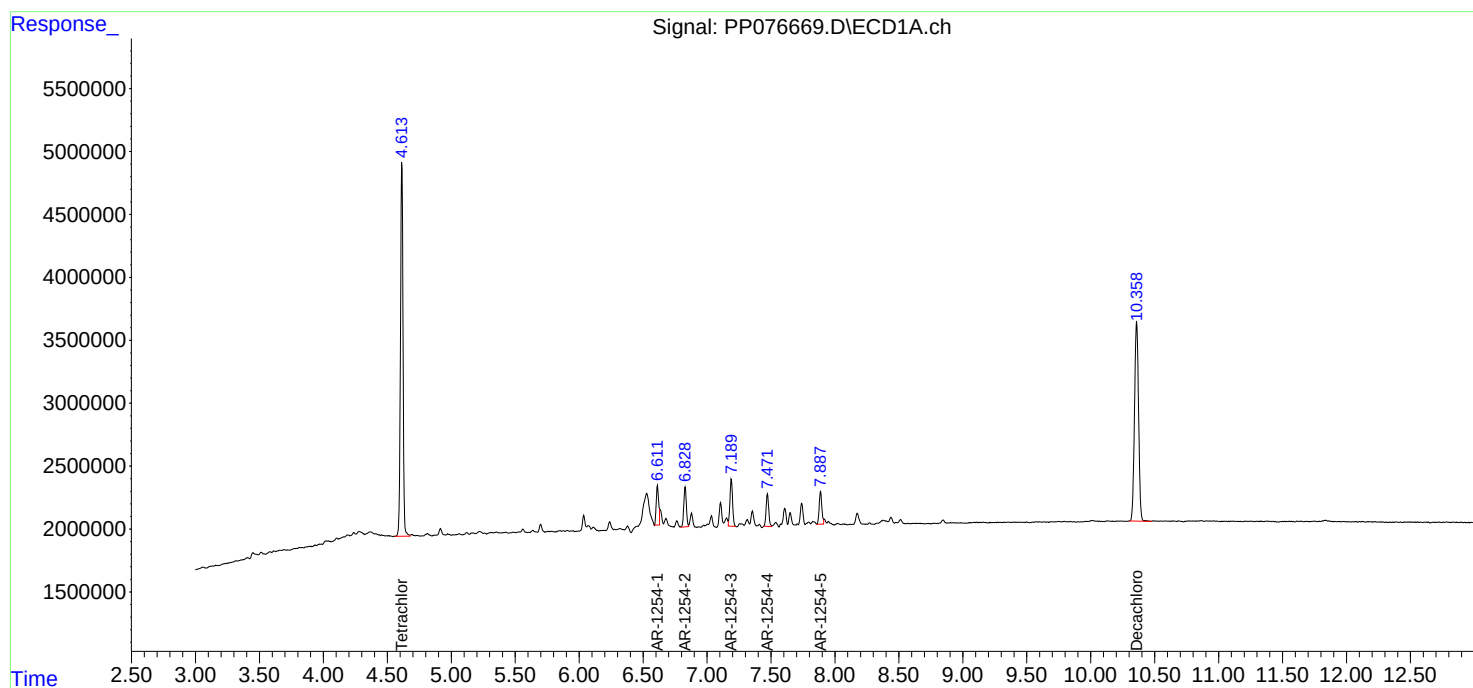

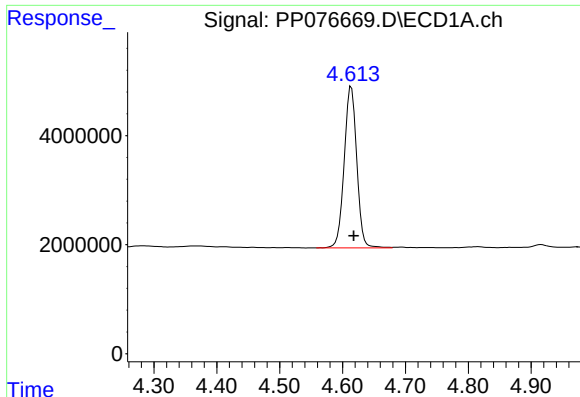


#1 Tetrachloro-m-xylene

R.T.: 4.614 min
Delta R.T.: -0.004 min
Response: 40975890
Conc: 22.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

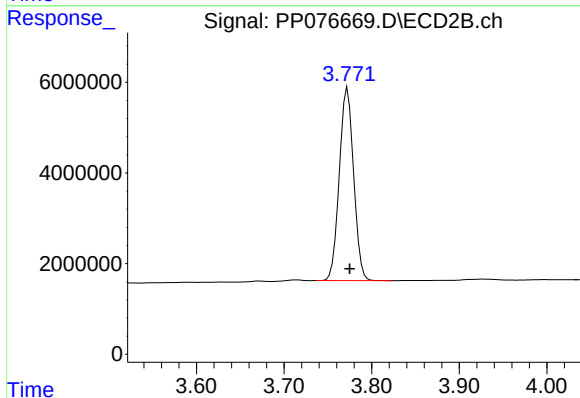


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: -0.002 min
Response: 48367833
Conc: 23.22 ng/ml

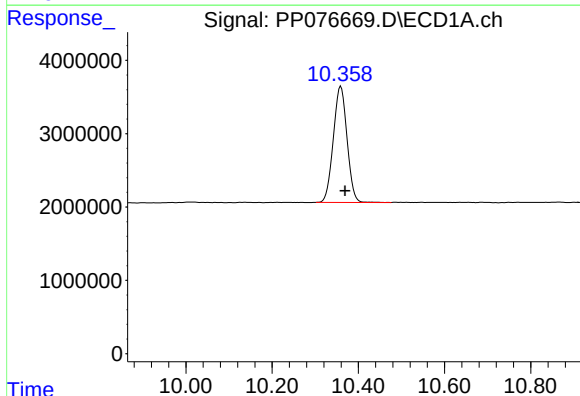


#2 Decachlorobiphenyl

R.T.: 10.359 min
Delta R.T.: -0.010 min
Response: 34893660
Conc: 23.28 ng/ml

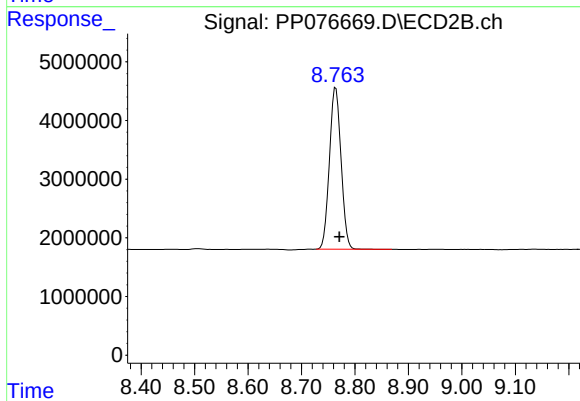

#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.007 min
Response: 41639261
Conc: 23.60 ng/ml

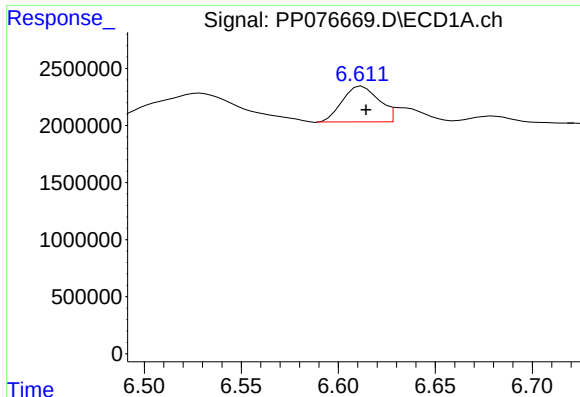


#26 AR-1254-1

R.T.: 6.611 min
Delta R.T.: -0.003 min
Response: 4397691
Conc: 54.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

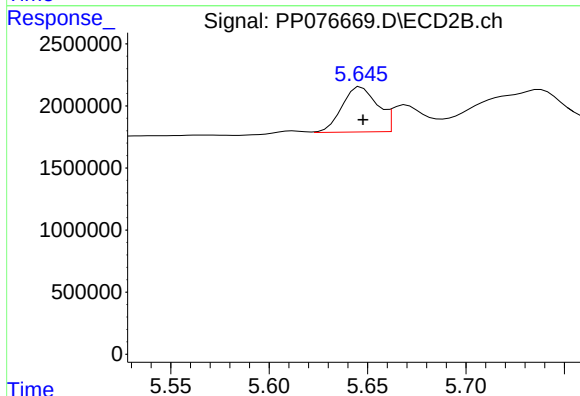


#26 AR-1254-1

R.T.: 5.645 min
Delta R.T.: -0.002 min
Response: 4900239
Conc: 41.44 ng/ml m

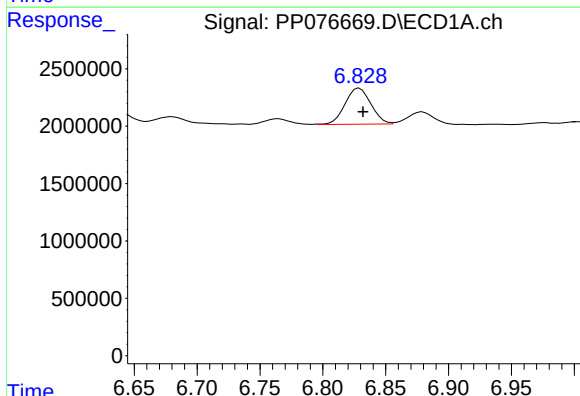


#27 AR-1254-2

R.T.: 6.828 min
Delta R.T.: -0.004 min
Response: 4518315
Conc: 40.08 ng/ml m

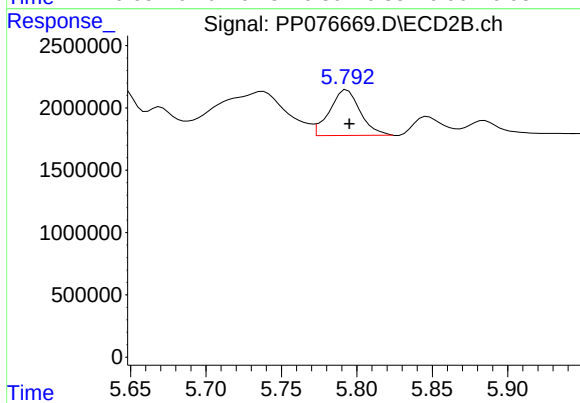

#27 AR-1254-2

R.T.: 5.792 min
Delta R.T.: -0.003 min
Response: 5107725
Conc: 47.24 ng/ml m

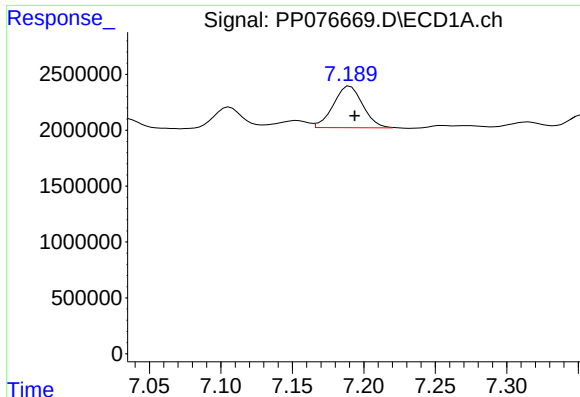


#28 AR-1254-3

R.T.: 7.189 min
Delta R.T.: -0.005 min
Response: 5313427
Conc: 44.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

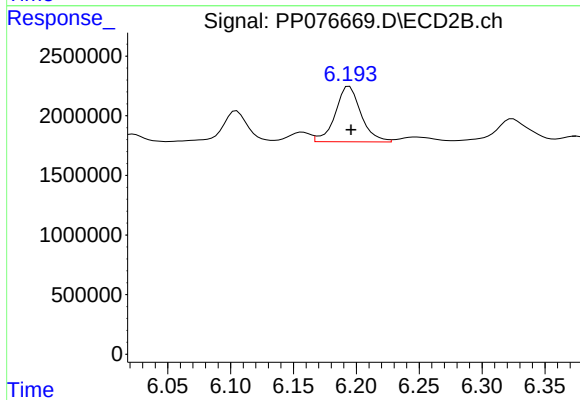


#28 AR-1254-3

R.T.: 6.193 min
Delta R.T.: -0.003 min
Response: 6582021
Conc: 40.09 ng/ml m

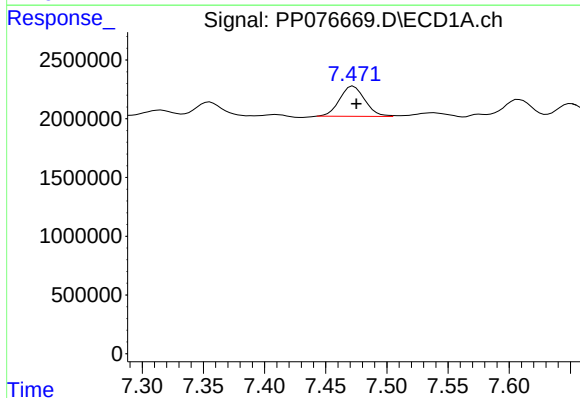


#29 AR-1254-4

R.T.: 7.471 min
Delta R.T.: -0.004 min
Response: 3695514
Conc: 41.01 ng/ml m

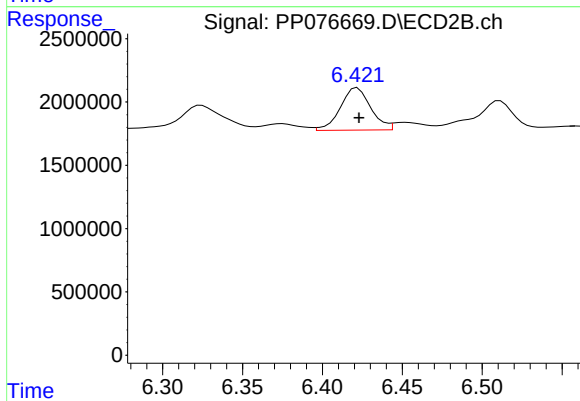

#29 AR-1254-4

R.T.: 6.422 min
Delta R.T.: -0.001 min
Response: 4420037
Conc: 42.59 ng/ml

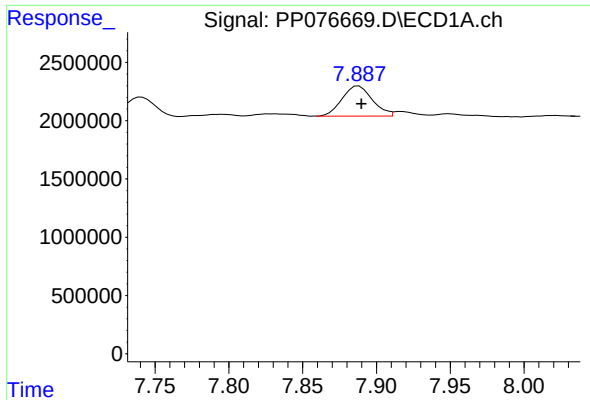


#30 AR-1254-5

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 3681221
Conc: 38.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

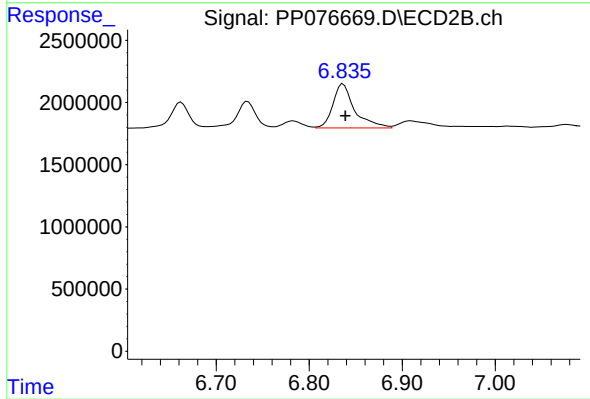

#30 AR-1254-5

R.T.: 6.837 min
Delta R.T.: -0.002 min
Response: 5766131
Conc: 40.96 ng/ml