

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 17:00
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1262-WATER-40 PPB-QT4-2025
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:04:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.615	3.774	41217627	48616761	22.456	23.341
2) SA Decachlor...	10.361	8.766	35159601	41506213	23.460	23.523
Target Compounds						
36) L8 AR-1262-1	8.193	6.877	4034466	5445291	40.770	40.845
37) L8 AR-1262-2	8.516	7.134	7364250	4888810	42.704	40.768
38) L8 AR-1262-3	8.838	7.656	5061242	5463984	40.257	55.463m#
39) L8 AR-1262-4	8.925	7.718	3747775	8319385	37.773	47.680m#
40) L8 AR-1262-5	9.588	8.214	2727276	2965524	38.390	36.904

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 17:00
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1262-WATER-40 PPB-QT4-2025
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/03/2025
Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:04:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

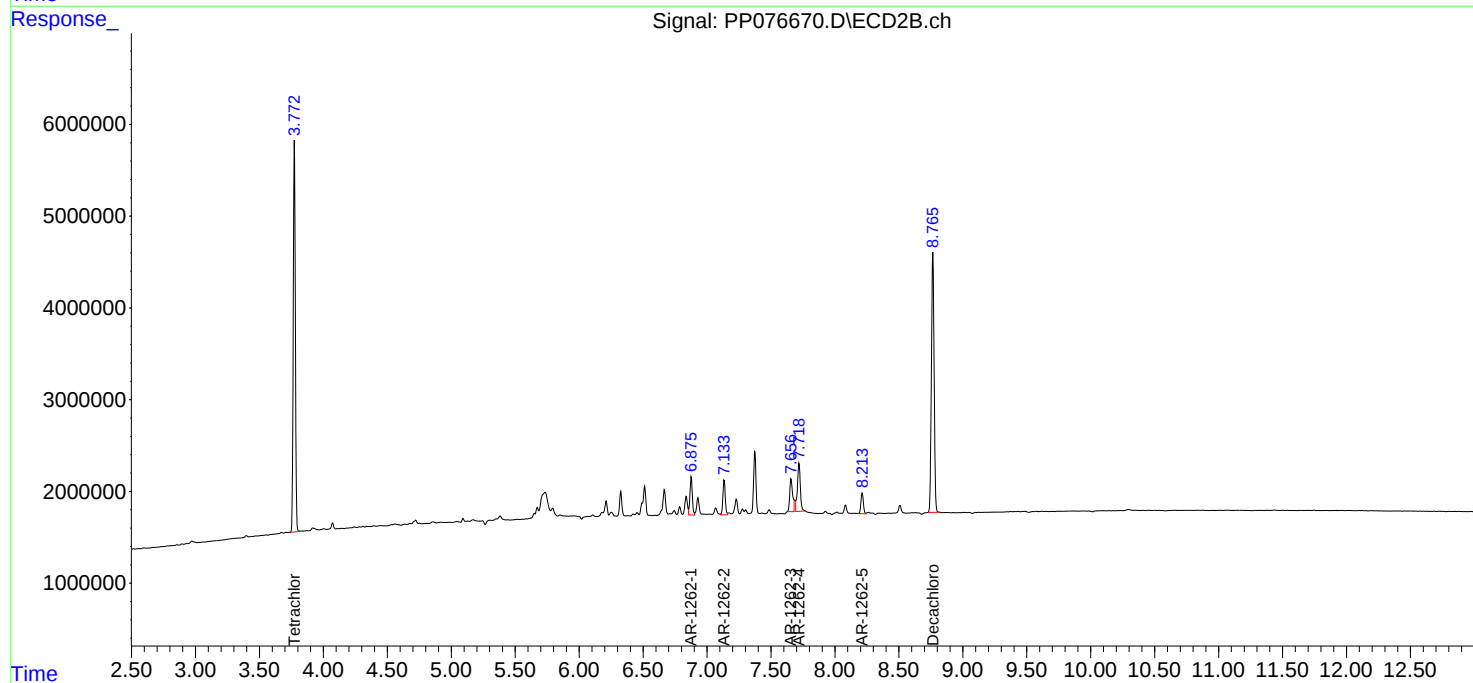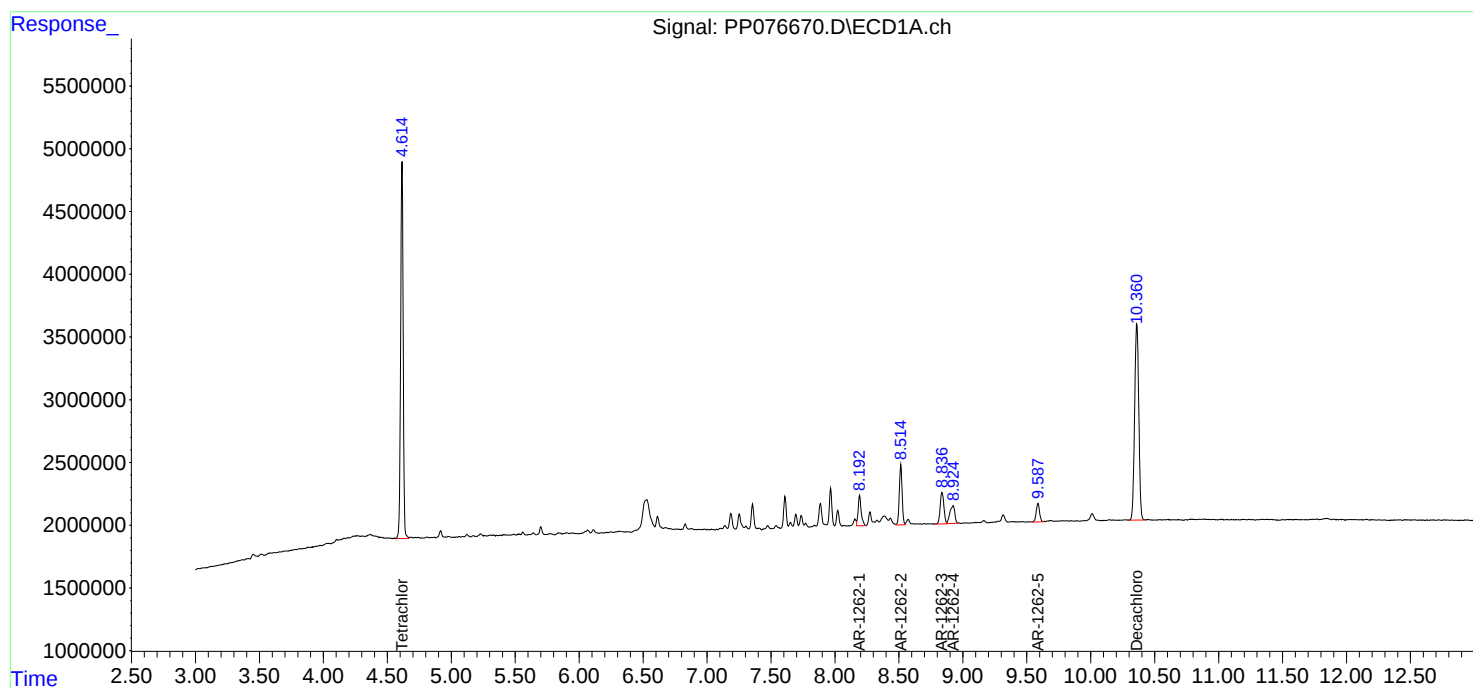

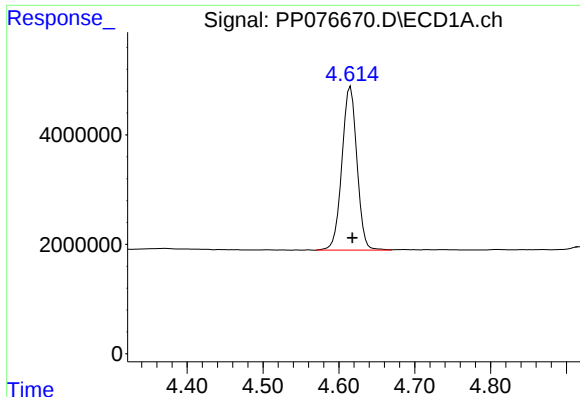


#1 Tetrachloro-m-xylene

R.T.: 4.615 min
Delta R.T.: -0.003 min
Response: 41217627
Conc: 22.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

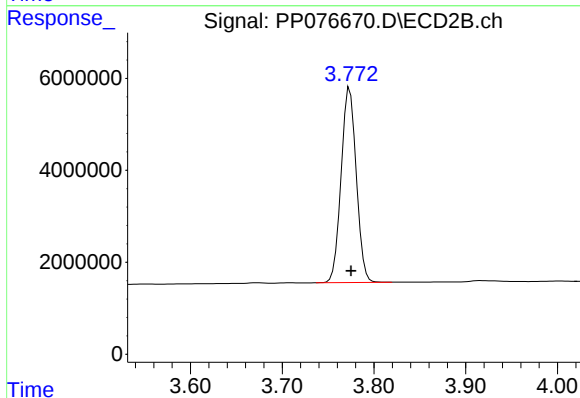


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: -0.001 min
Response: 48616761
Conc: 23.34 ng/ml

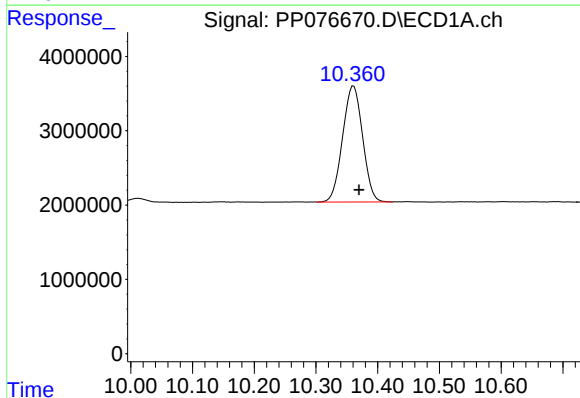


#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.009 min
Response: 35159601
Conc: 23.46 ng/ml

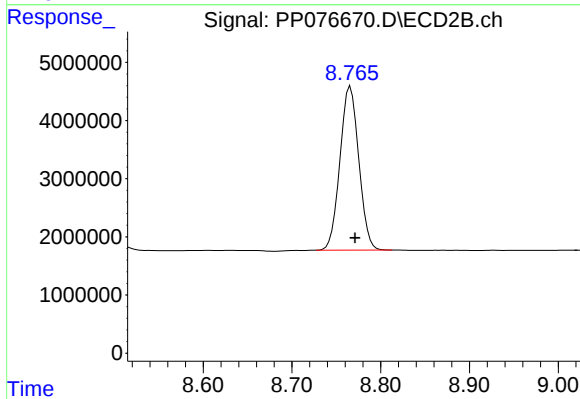

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.005 min
Response: 41506213
Conc: 23.52 ng/ml

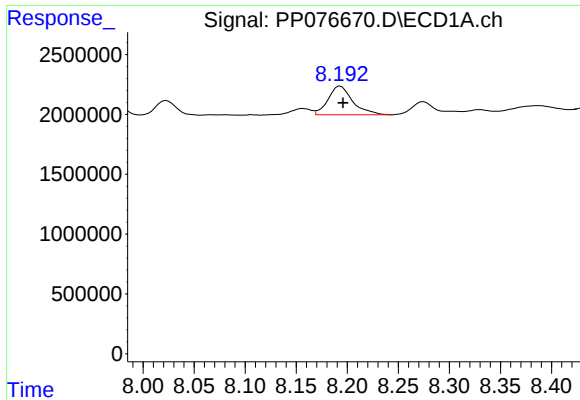


#36 AR-1262-1

R.T.: 8.193 min
Delta R.T.: -0.003 min
Response: 4034466
Conc: 40.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

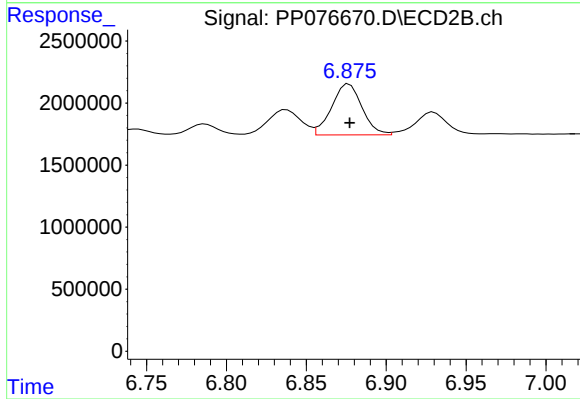


#36 AR-1262-1

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 5445291
Conc: 40.85 ng/ml

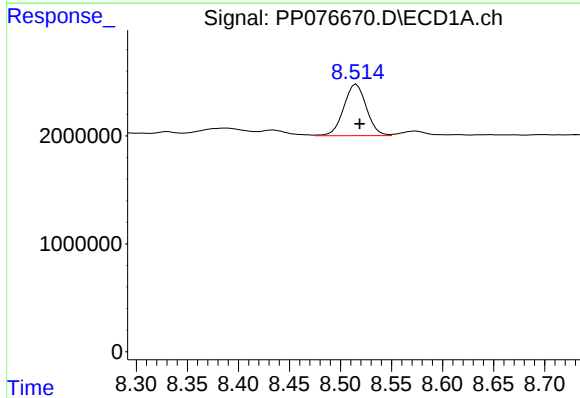


#37 AR-1262-2

R.T.: 8.516 min
Delta R.T.: -0.003 min
Response: 7364250
Conc: 42.70 ng/ml

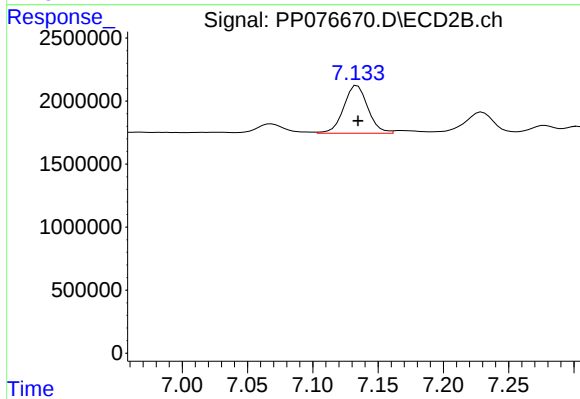

#37 AR-1262-2

R.T.: 7.134 min
Delta R.T.: 0.000 min
Response: 4888810
Conc: 40.77 ng/ml

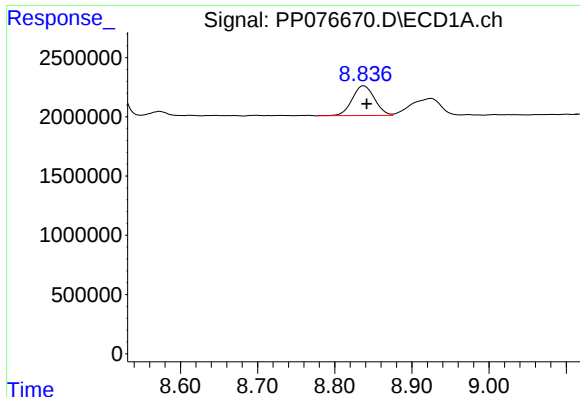


#38 AR-1262-3

R.T.: 8.838 min
Delta R.T.: -0.004 min
Response: 5061242
Conc: 40.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

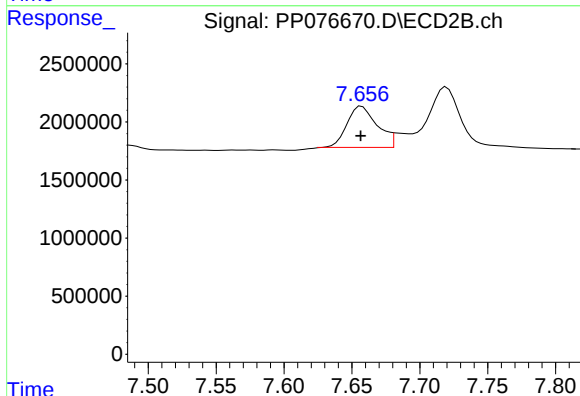


#38 AR-1262-3

R.T.: 7.656 min
Delta R.T.: 0.000 min
Response: 5463984
Conc: 55.46 ng/ml m

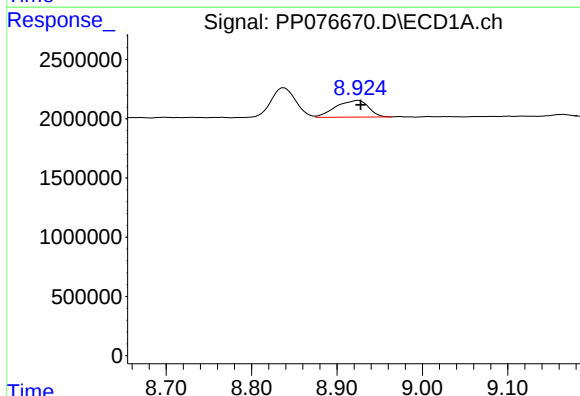


#39 AR-1262-4

R.T.: 8.925 min
Delta R.T.: -0.002 min
Response: 3747775
Conc: 37.77 ng/ml

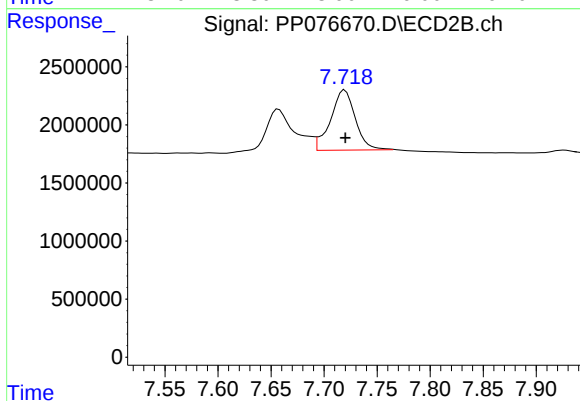

#39 AR-1262-4

R.T.: 7.718 min
Delta R.T.: -0.002 min
Response: 8319385
Conc: 47.68 ng/ml m

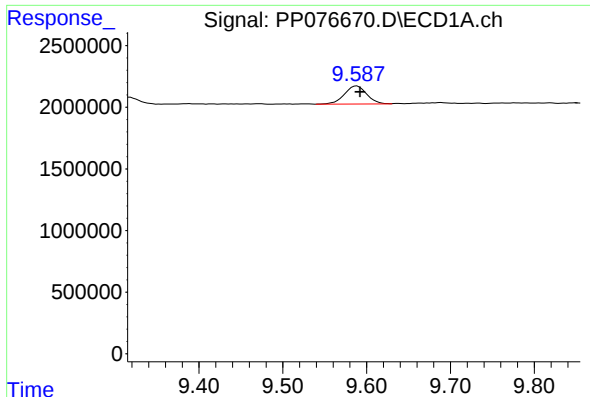


#40 AR-1262-5

R.T.: 9.588 min
Delta R.T.: -0.004 min
Response: 2727276
Conc: 38.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

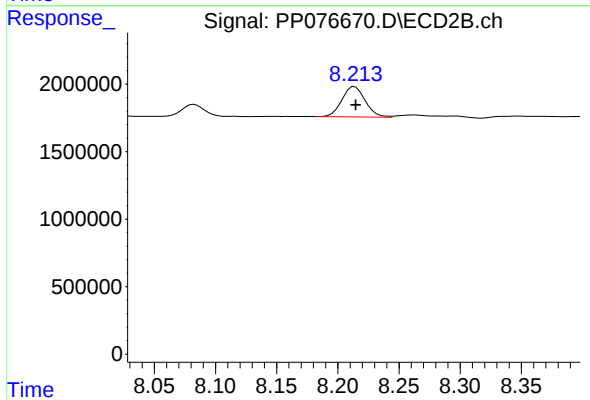

#40 AR-1262-5

R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 2965524
Conc: 36.90 ng/ml