

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
 Data File : PP076671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 17:17
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : LOD-MDL-1268-WATER-40 PPB-QT4-2025
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 01:05:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.613	3.772	42625089	50235019	23.222	24.118
2) SA Decachlor...	10.358	8.763	39202757	46304262	26.158	26.242
Target Compounds						
41) L9 AR-1268-1	8.832	7.653	7907121	12043936	36.792	42.809m
42) L9 AR-1268-2	8.925	7.717	7225891	10348071	35.908	40.656m
43) L9 AR-1268-3	9.162	7.923	6029736	7794765	36.290	37.761
44) L9 AR-1268-4	9.586	8.211	2769311	2982645	33.246	31.758
45) L9 AR-1268-5	10.010	8.506	18344318	20784678	36.374	32.653

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120125\
Data File : PP076671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 17:17
Operator : YP\AJ
Sample : Q3530-07
Misc : LOD-MDL-1268-WATER-40 PPB-QT4-2025
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/03/2025
Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 01:05:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

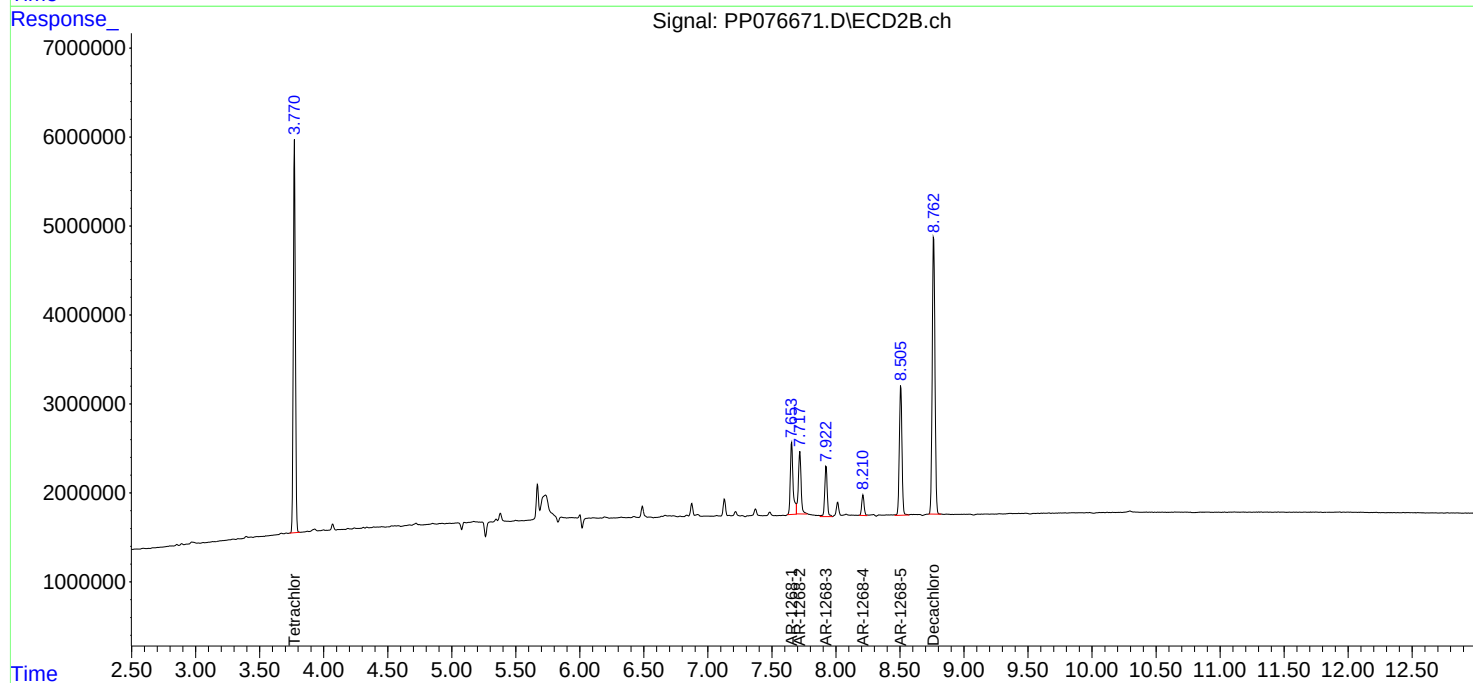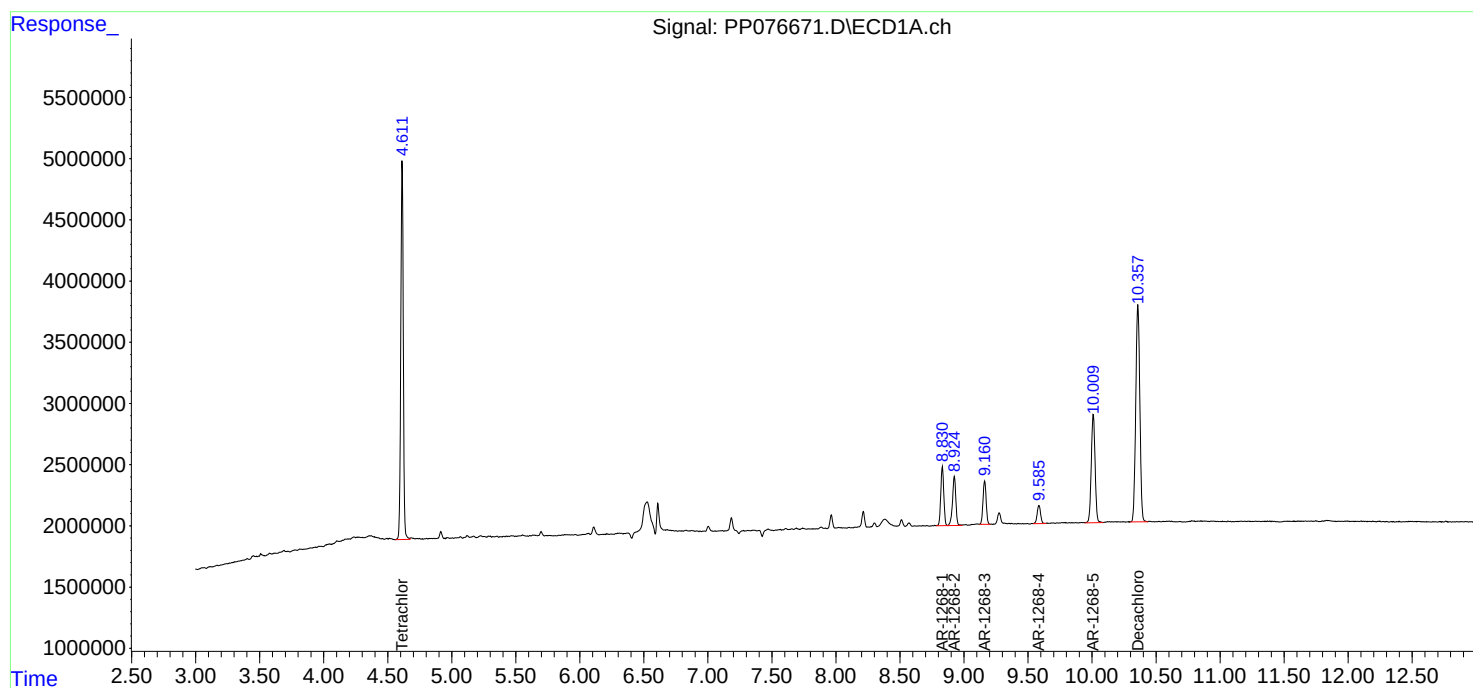

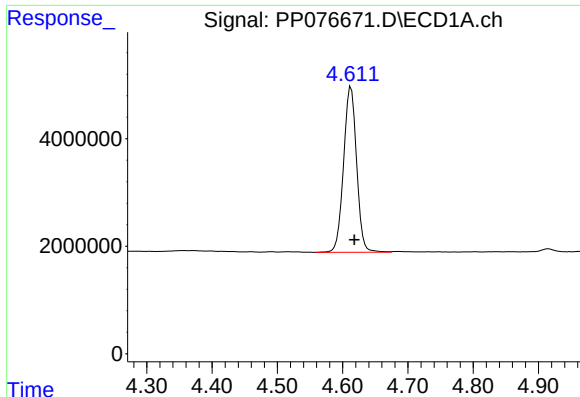


#1 Tetrachloro-m-xylene

R.T.: 4.613 min
Delta R.T.: -0.005 min
Response: 42625089
Conc: 23.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

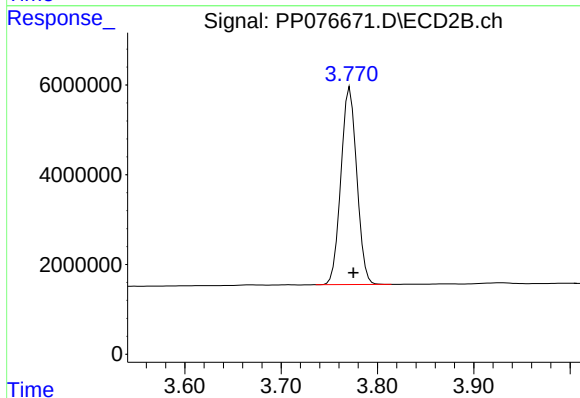


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: -0.003 min
Response: 50235019
Conc: 24.12 ng/ml

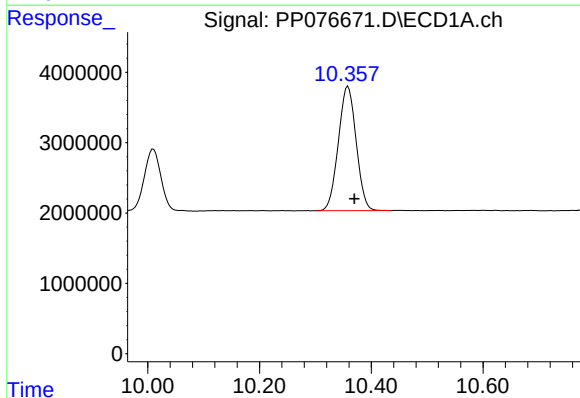


#2 Decachlorobiphenyl

R.T.: 10.358 min
Delta R.T.: -0.011 min
Response: 39202757
Conc: 26.16 ng/ml

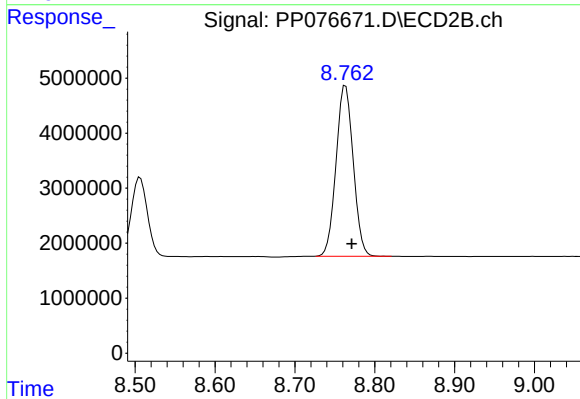

#2 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: -0.008 min
Response: 46304262
Conc: 26.24 ng/ml

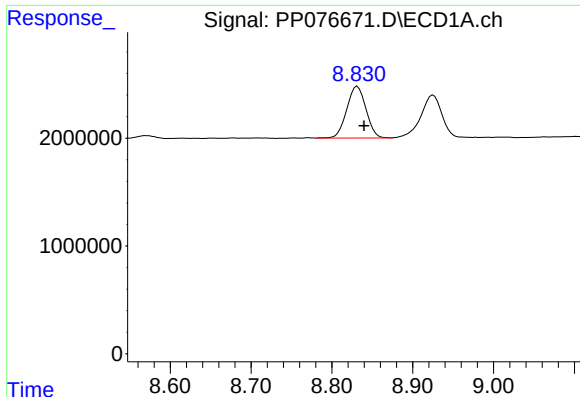


#41 AR-1268-1

R.T.: 8.832 min
Delta R.T.: -0.008 min
Response: 7907121
Conc: 36.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

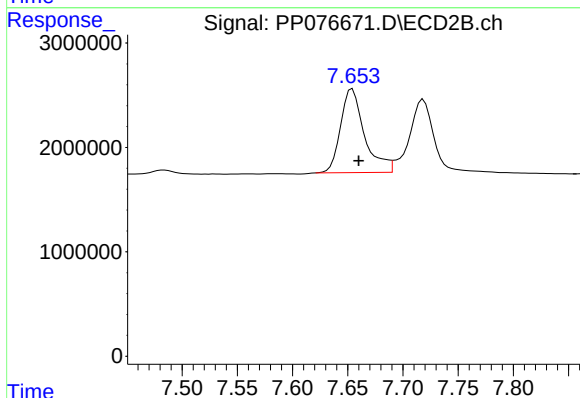


#41 AR-1268-1

R.T.: 7.653 min
Delta R.T.: -0.007 min
Response: 12043936
Conc: 42.81 ng/ml m

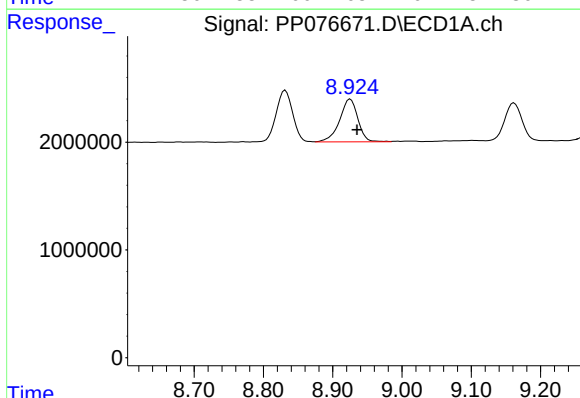


#42 AR-1268-2

R.T.: 8.925 min
Delta R.T.: -0.010 min
Response: 7225891
Conc: 35.91 ng/ml

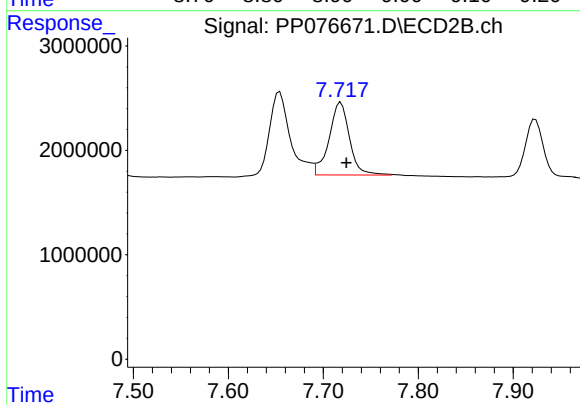

#42 AR-1268-2

R.T.: 7.717 min
Delta R.T.: -0.007 min
Response: 10348071
Conc: 40.66 ng/ml m

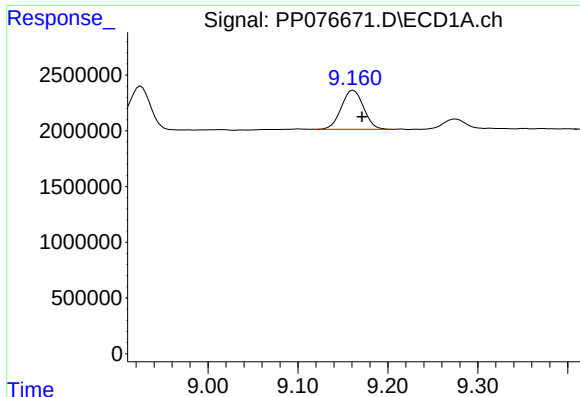


#43 AR-1268-3

R.T.: 9.162 min
Delta R.T.: -0.010 min
Response: 6029736
Conc: 36.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

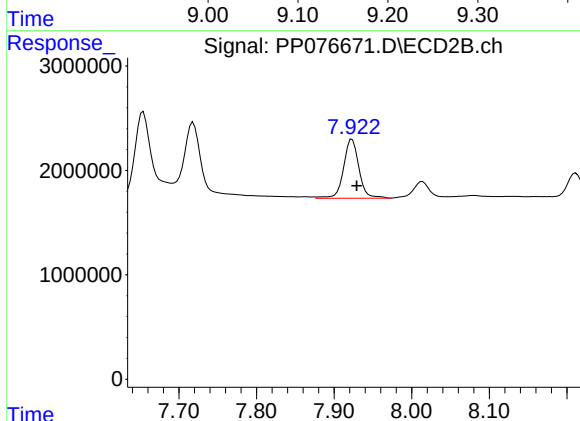


#43 AR-1268-3

R.T.: 7.923 min
Delta R.T.: -0.006 min
Response: 7794765
Conc: 37.76 ng/ml

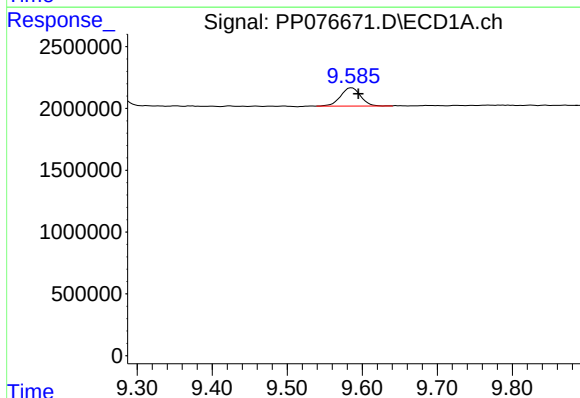


#44 AR-1268-4

R.T.: 9.586 min
Delta R.T.: -0.009 min
Response: 2769311
Conc: 33.25 ng/ml

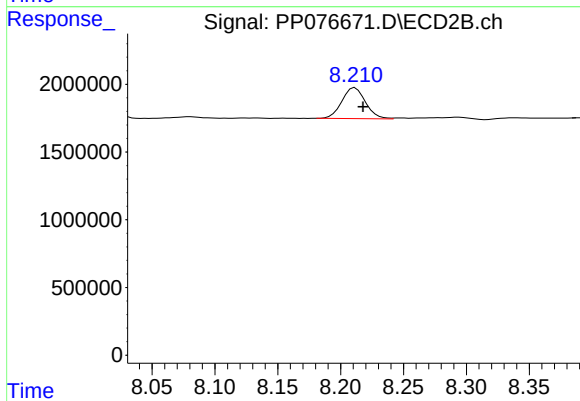

#44 AR-1268-4

R.T.: 8.211 min
Delta R.T.: -0.006 min
Response: 2982645
Conc: 31.76 ng/ml

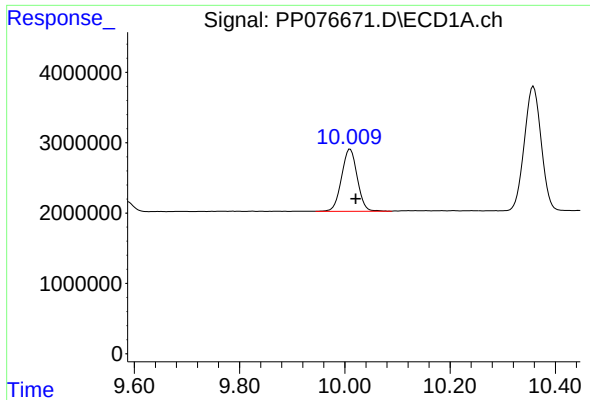


#45 AR-1268-5

R.T.: 10.010 min
Delta R.T.: -0.010 min
Response: 18344318
Conc: 36.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

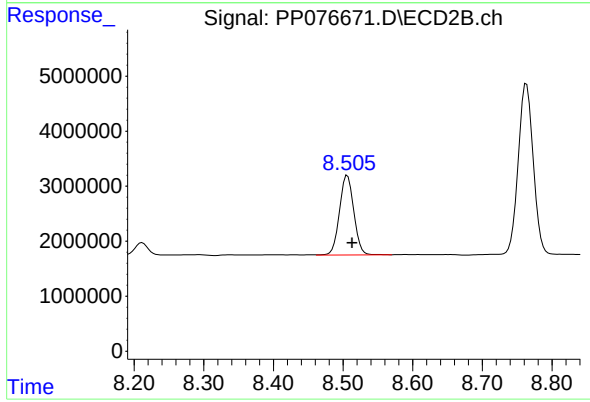

#45 AR-1268-5

R.T.: 8.506 min
Delta R.T.: -0.007 min
Response: 20784678
Conc: 32.65 ng/ml