

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031785.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 12:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 13:28:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.797	4.061	1173424	1073510	24.233	22.403
2)	SA Decachlor...	10.671	9.367	779478	839970	22.950	22.685
Target Compounds							
7)	L1 AR-1016-5	0.000	5.838f	0	14975	N.D.	13.166 #
9)	L2 AR-1221-2	0.000	4.413	0	11798	N.D.	30.585 #
24)	L5 AR-1248-4	0.000	5.838f	0	14975	N.D.	9.774 #
30)	L6 AR-1254-5	0.000	7.430	0	1525	N.D.	0.565 #
32)	L7 AR-1260-2	0.000	7.073f	0	10934	N.D.	4.490 #
35)	L7 AR-1260-5	0.000	7.983	0	1066	N.D.	0.235 #
36)	L8 AR-1262-1	0.000	7.448f	0	341	N.D.	0.123 #
37)	L8 AR-1262-2	0.000	7.983	0	1066	N.D.	0.220 #
38)	L8 AR-1262-3	0.000	8.272	0	1354	N.D.	0.688 #
39)	L8 AR-1262-4	0.000	8.329	0	718	N.D.	0.198 #
40)	L8 AR-1262-5	0.000	8.827	0	1713	N.D.	1.055 #
41)	L9 AR-1268-1	0.000	8.272	0	1354	N.D.	0.245 #
42)	L9 AR-1268-2	0.000	8.329	0	718	N.D.	0.133 #
44)	L9 AR-1268-4	0.000	8.827	0	1713	N.D.	0.940 #
45)	L9 AR-1268-5	0.000	9.119	0	7613	N.D.	0.550 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031785.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 12:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 13:28:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

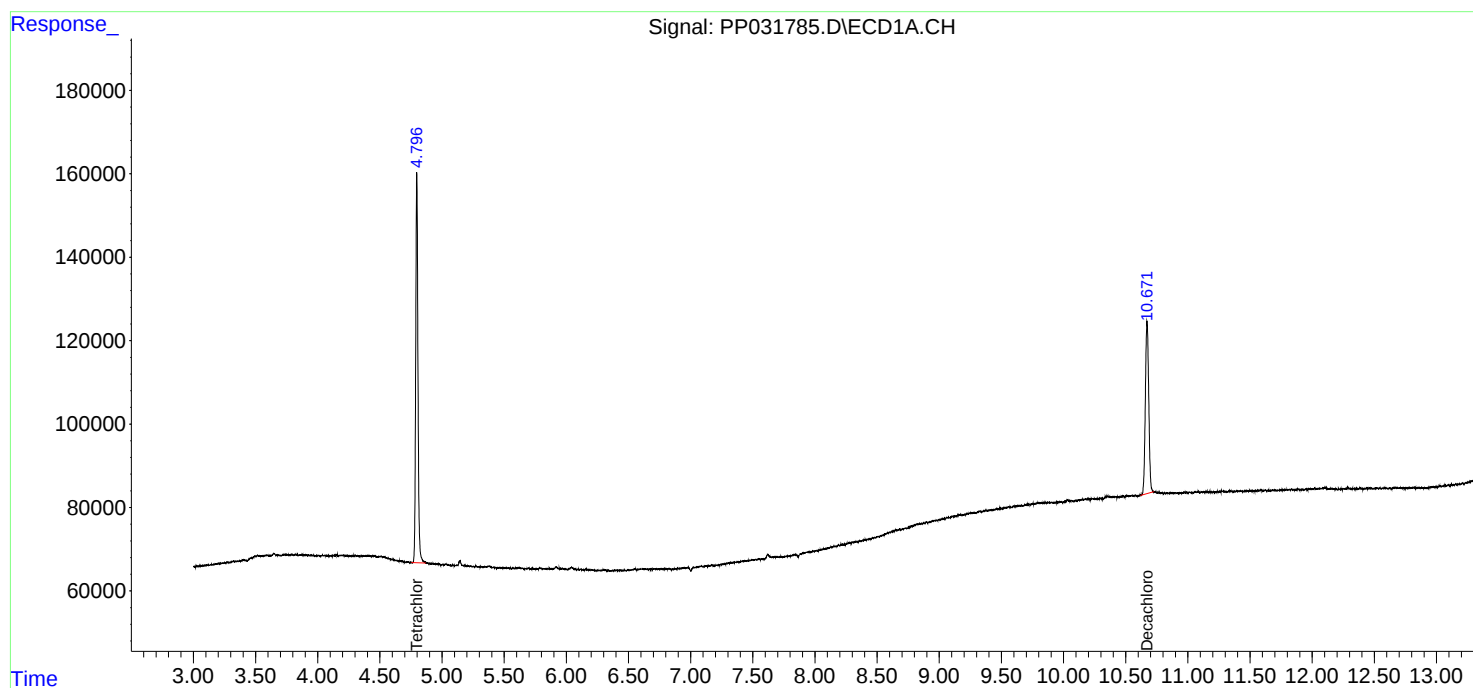


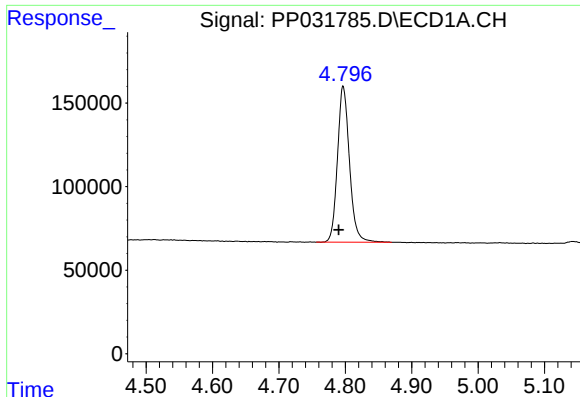

#1 Tetrachloro-m-xylene


R.T.: 4.797 min
Delta R.T.: 0.007 min
Response: 1173424
Conc: 24.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

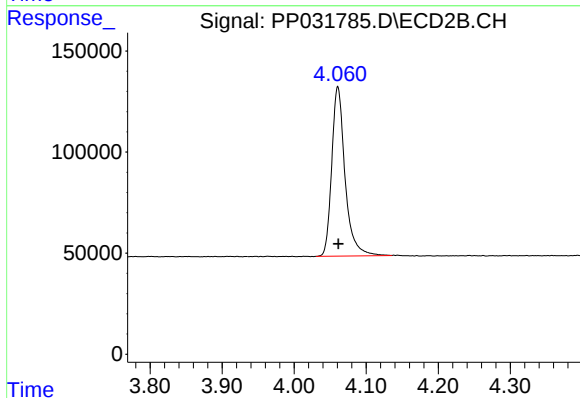


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1073510
Conc: 22.40 ng/ml

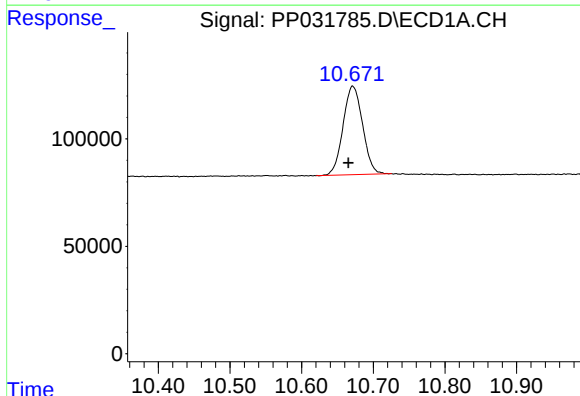


#2 Decachlorobiphenyl

R.T.: 10.671 min
Delta R.T.: 0.006 min
Response: 779478
Conc: 22.95 ng/ml

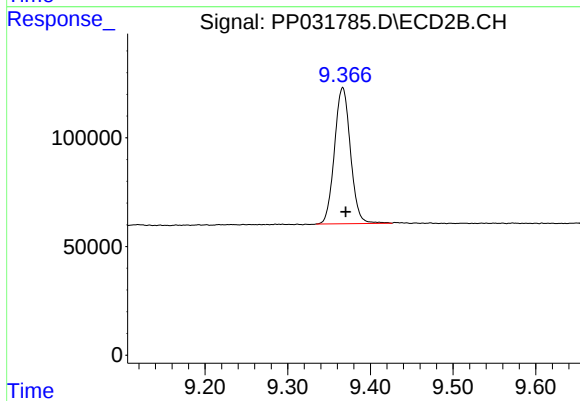

#2 Decachlorobiphenyl


R.T.: 9.367 min
Delta R.T.: -0.004 min
Response: 839970
Conc: 22.69 ng/ml

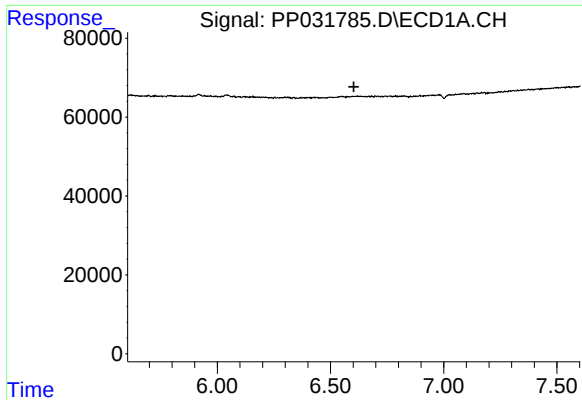

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

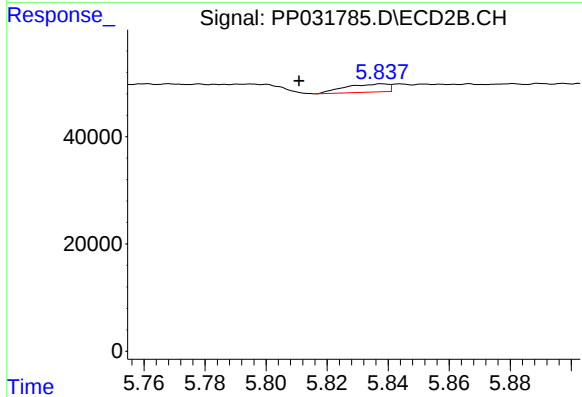


#7 AR-1016-5

R.T.: 5.838 min
Delta R.T.: 0.027 min
Response: 14975
Conc: 13.17 ng/ml

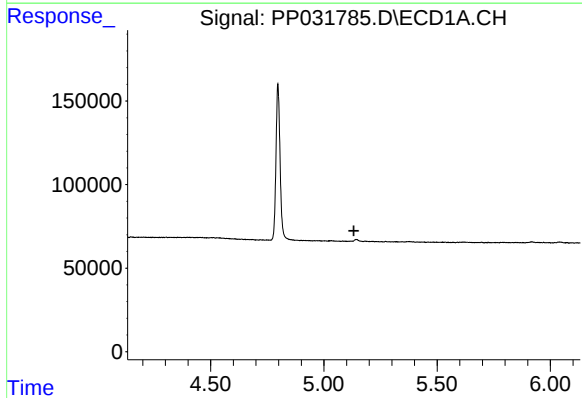


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

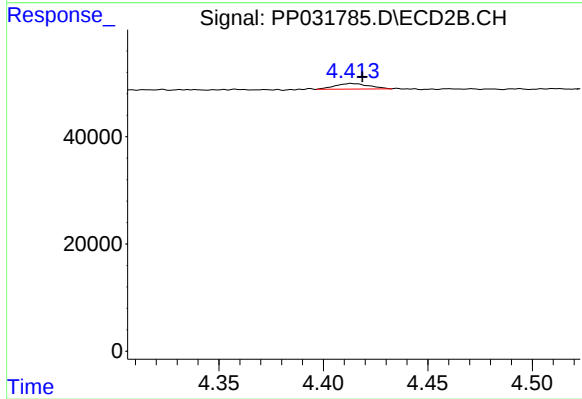

#9 AR-1221-2


R.T.: 4.413 min
Delta R.T.: -0.005 min
Response: 11798
Conc: 30.59 ng/ml

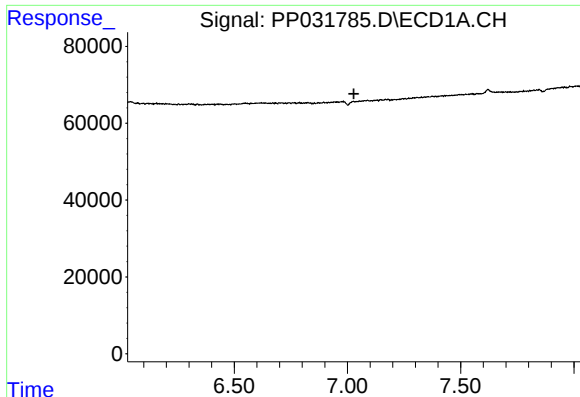

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

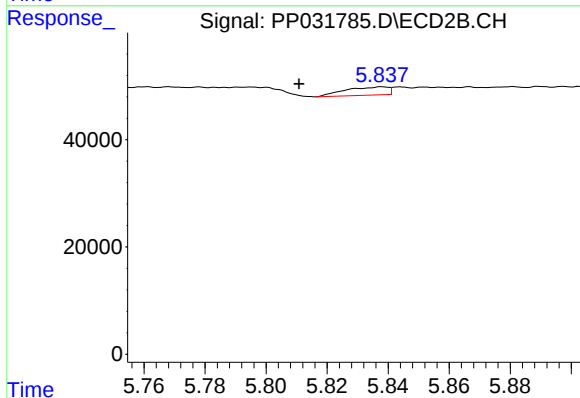


#24 AR-1248-4

R.T.: 5.838 min
Delta R.T.: 0.027 min
Response: 14975
Conc: 9.77 ng/ml

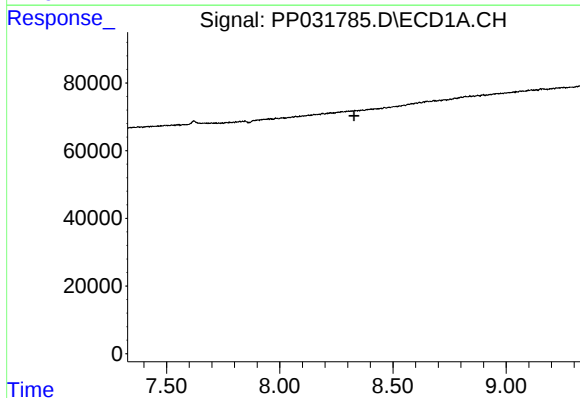


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 8.328 min
Response: 0
Conc: N.D.

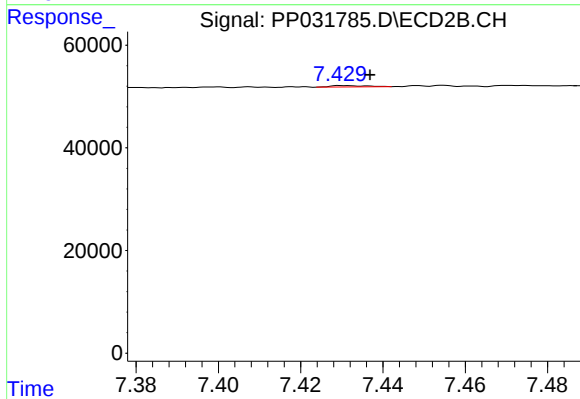

#30 AR-1254-5


R.T.: 7.430 min
Delta R.T.: -0.007 min
Response: 1525
Conc: 0.56 ng/ml

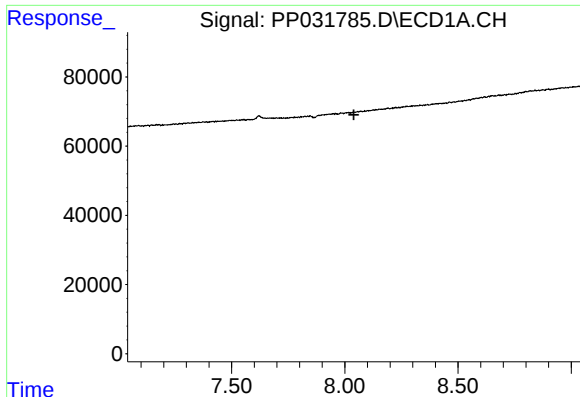

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

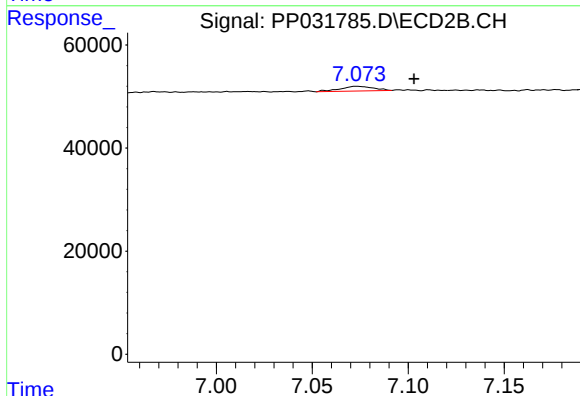


#32 AR-1260-2

R.T.: 7.073 min
Delta R.T.: -0.030 min
Response: 10934
Conc: 4.49 ng/ml

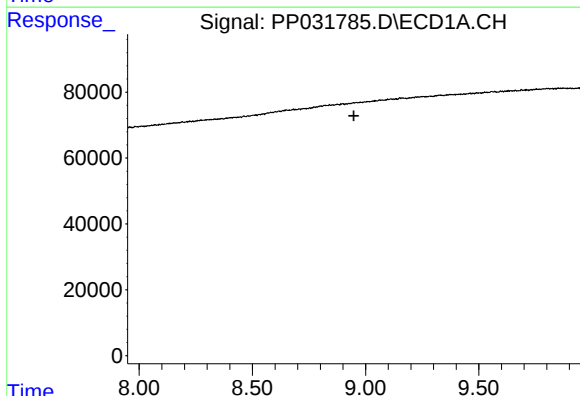


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.948 min
Response: 0
Conc: N.D.

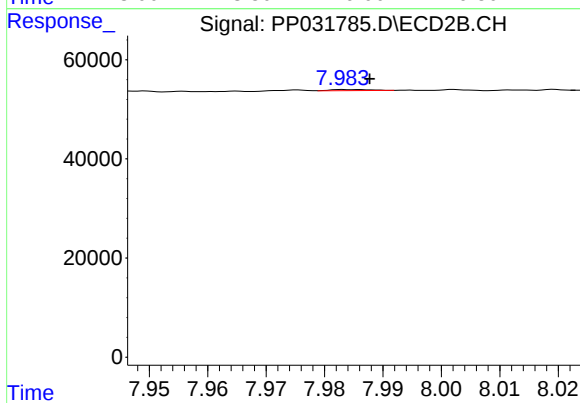

#35 AR-1260-5


R.T.: 7.983 min
Delta R.T.: -0.005 min
Response: 1066
Conc: 0.23 ng/ml

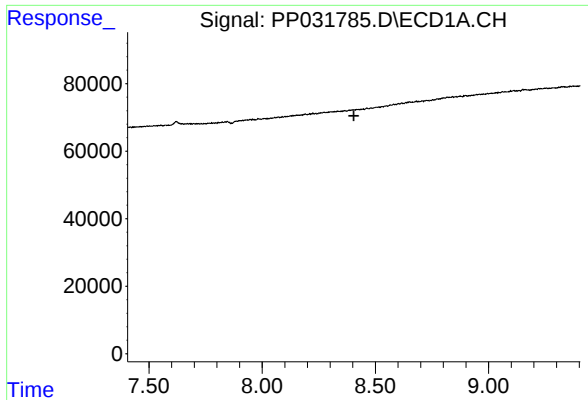

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

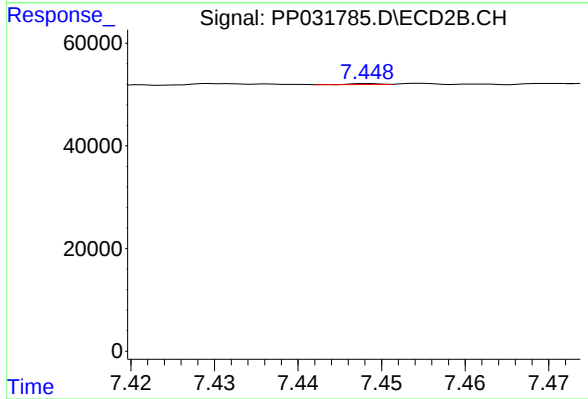


#36 AR-1262-1

R.T.: 7.448 min
Delta R.T.: -0.029 min
Response: 341
Conc: 0.12 ng/ml

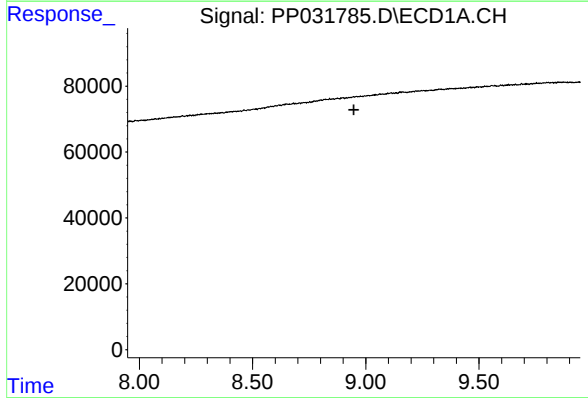


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.948 min
Response: 0
Conc: N.D.

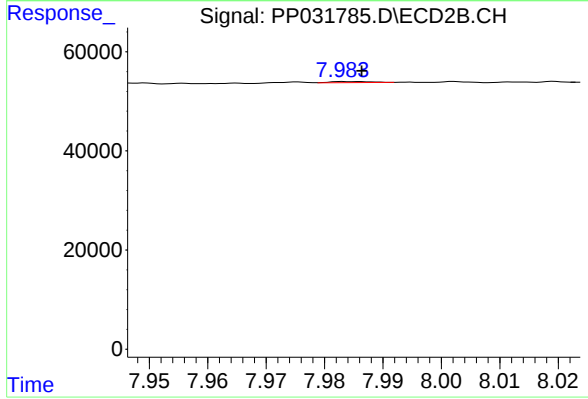

#37 AR-1262-2


R.T.: 7.983 min
Delta R.T.: -0.003 min
Response: 1066
Conc: 0.22 ng/ml

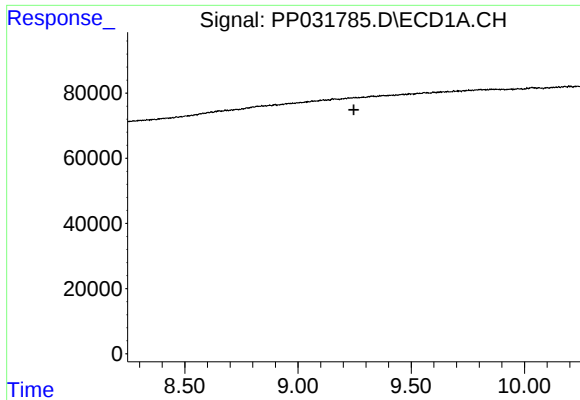

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

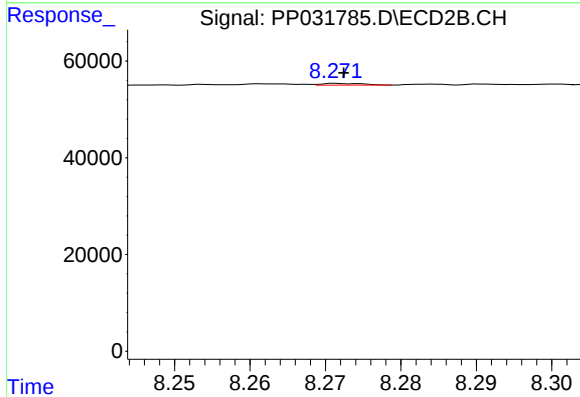


#38 AR-1262-3

R.T.: 8.272 min
Delta R.T.: 0.000 min
Response: 1354
Conc: 0.69 ng/ml

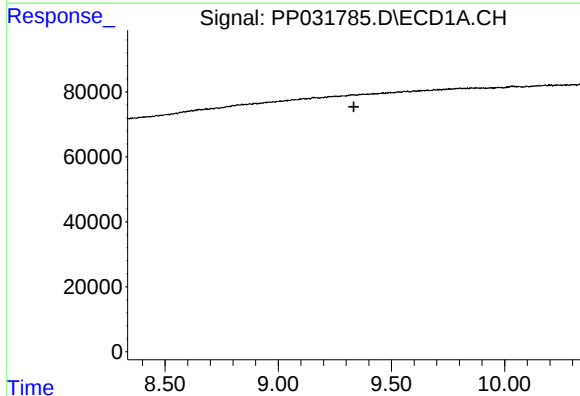


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.334 min
Response: 0
Conc: N.D.

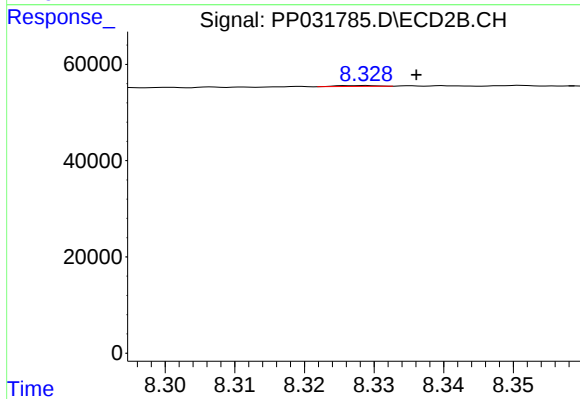

#39 AR-1262-4


R.T.: 8.329 min
Delta R.T.: -0.007 min
Response: 718
Conc: 0.20 ng/ml

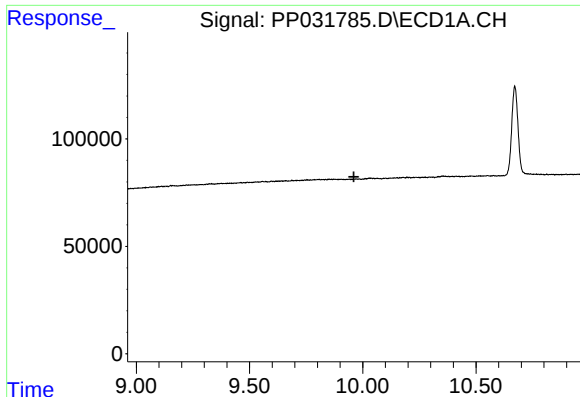

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

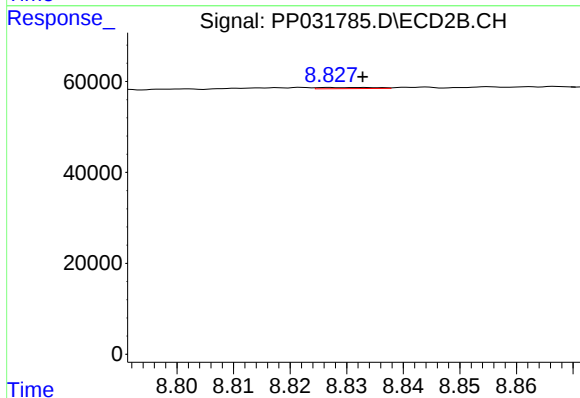


#40 AR-1262-5

R.T.: 8.827 min
Delta R.T.: -0.006 min
Response: 1713
Conc: 1.06 ng/ml

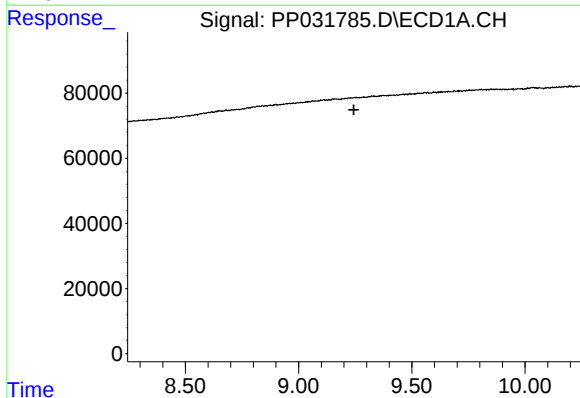


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

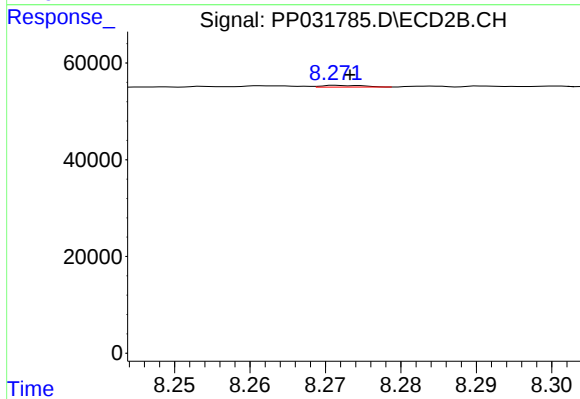

#41 AR-1268-1


R.T.: 8.272 min
Delta R.T.: -0.002 min
Response: 1354
Conc: 0.24 ng/ml

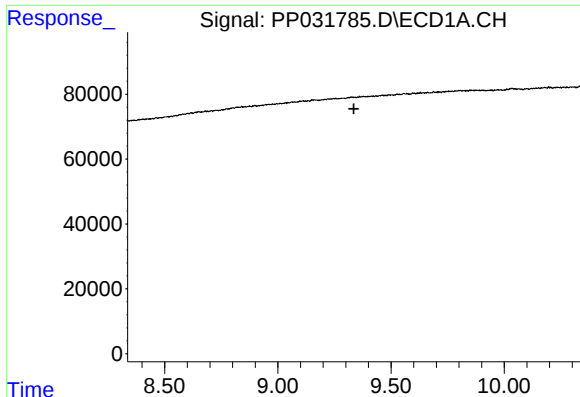

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

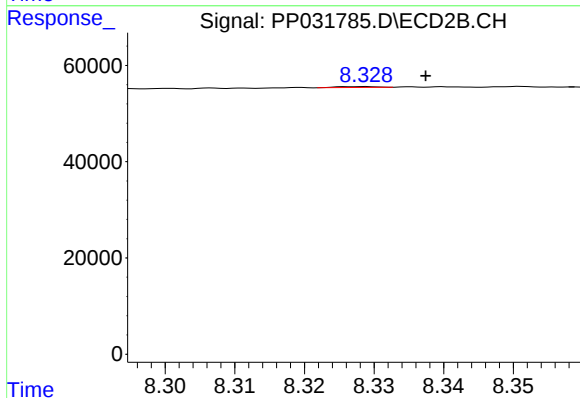


#42 AR-1268-2

R.T.: 8.329 min
Delta R.T.: -0.009 min
Response: 718
Conc: 0.13 ng/ml

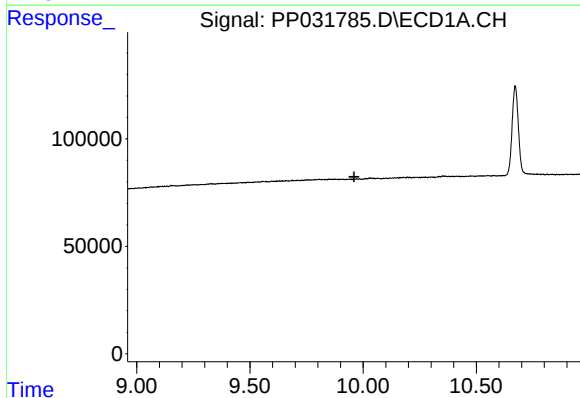


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.960 min
Response: 0
Conc: N.D.

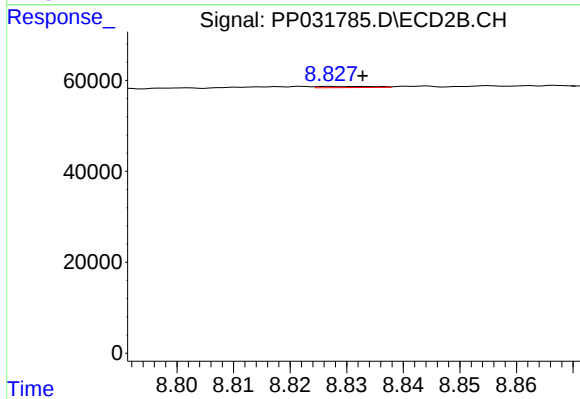

#44 AR-1268-4


R.T.: 8.827 min
Delta R.T.: -0.006 min
Response: 1713
Conc: 0.94 ng/ml

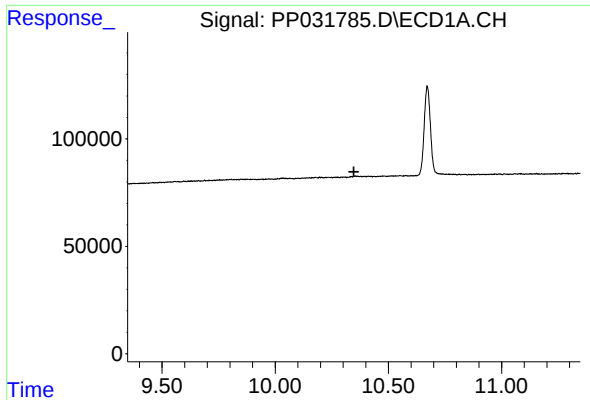

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

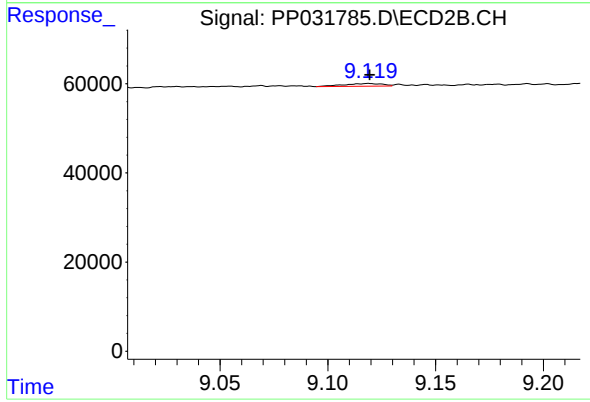

#45 AR-1268-5

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 7613
Conc: 0.55 ng/ml