

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031797.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 15:57
 Operator : DD\AJ
 Sample : PB133349BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 17:20:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.787	4.060	1153197	1055408	23.815	22.025
2)	SA Decachlor...	10.660	9.362	775497	822843	22.833	22.223
Target Compounds							
9)	L2 AR-1221-2	0.000	4.414	0	19802	N.D.	51.334 #
30)	L6 AR-1254-5	0.000	7.431	0	1717	N.D.	0.636 #
32)	L7 AR-1260-2	0.000	7.078f	0	2381	N.D.	0.978 #
39)	L8 AR-1262-4	0.000	8.347	0	1265	N.D.	0.349 #
40)	L8 AR-1262-5	0.000	8.831	0	3463	N.D.	2.133 #
42)	L9 AR-1268-2	0.000	8.347	0	1265	N.D.	0.234 #
44)	L9 AR-1268-4	0.000	8.831	0	3463	N.D.	1.900 #
45)	L9 AR-1268-5	0.000	9.111	0	1143	N.D.	0.083 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031797.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 15:57
Operator : DD\AJ
Sample : PB133349BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 17:20:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

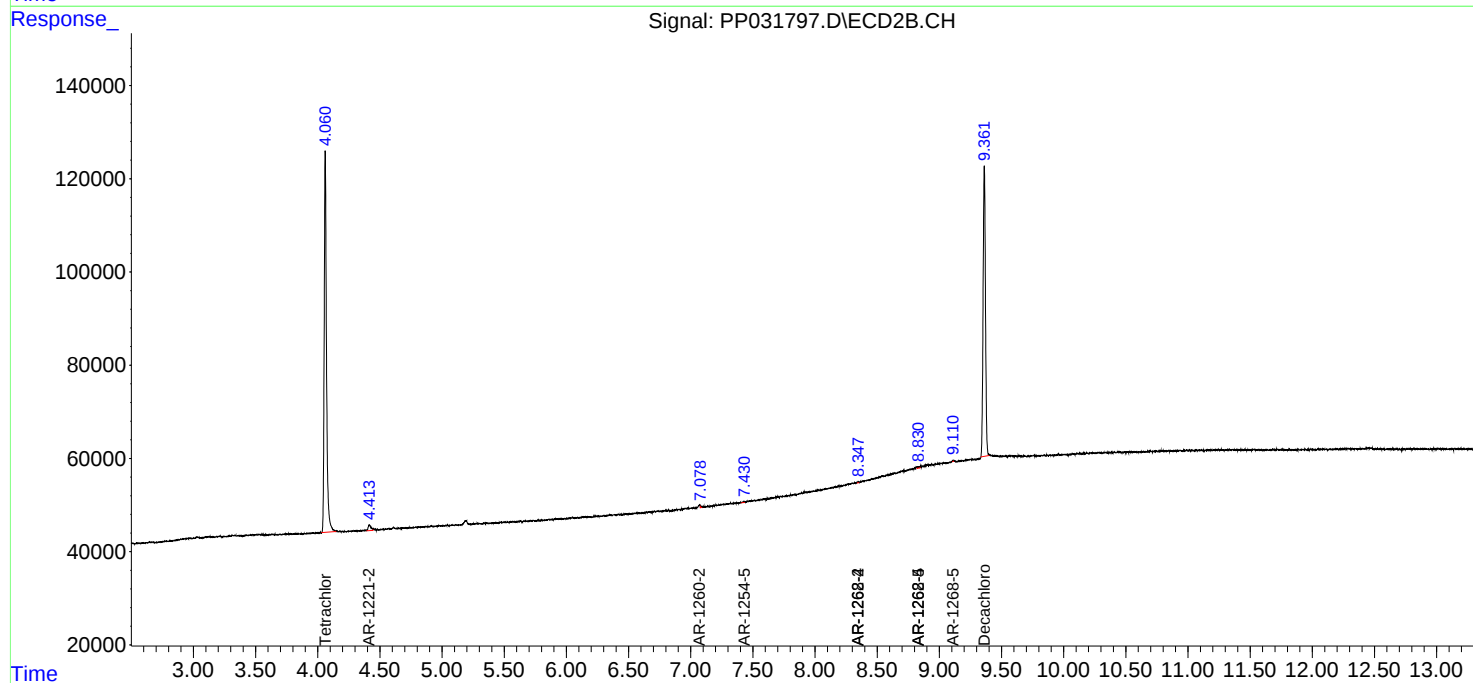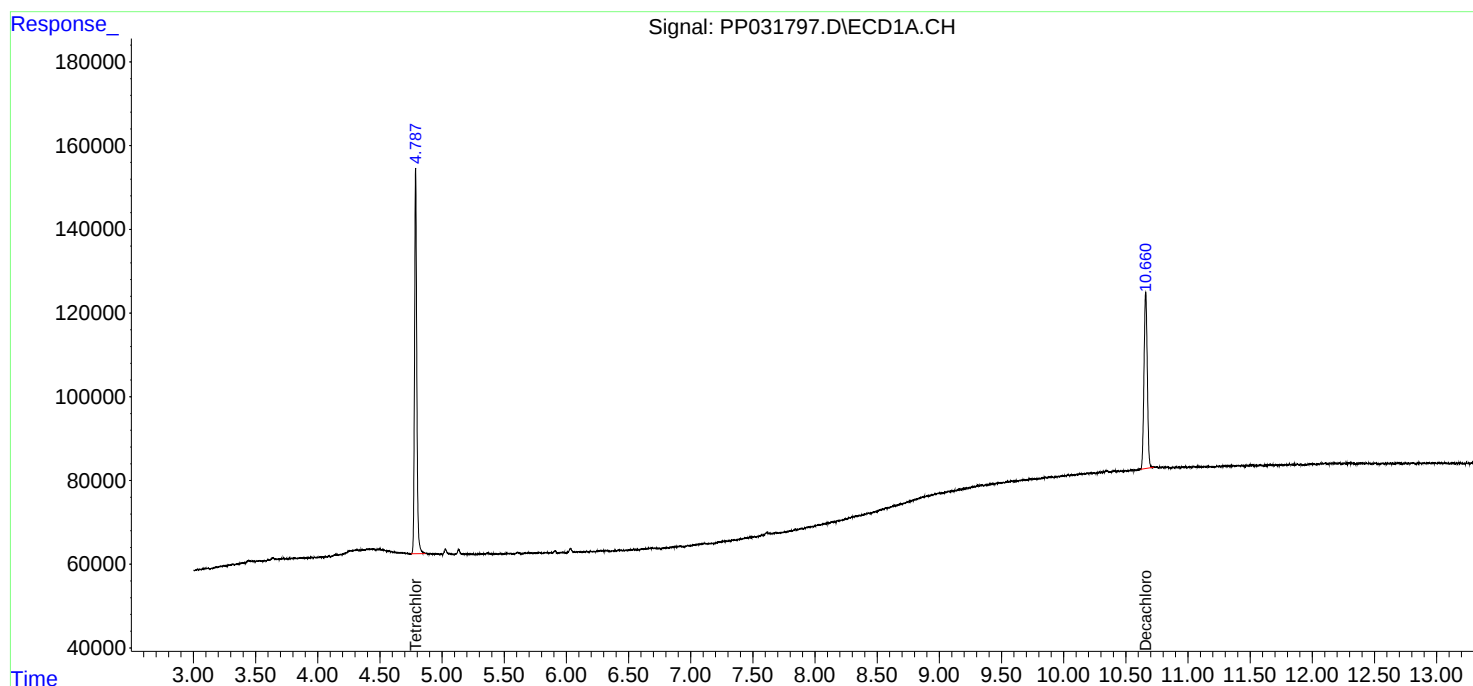


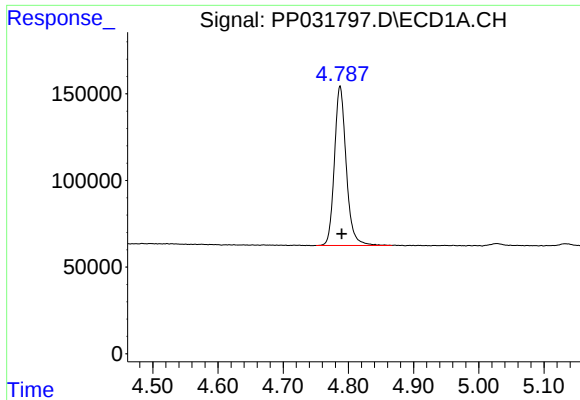

#1 Tetrachloro-m-xylene


R.T.: 4.787 min
Delta R.T.: -0.003 min
Response: 1153197
Conc: 23.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

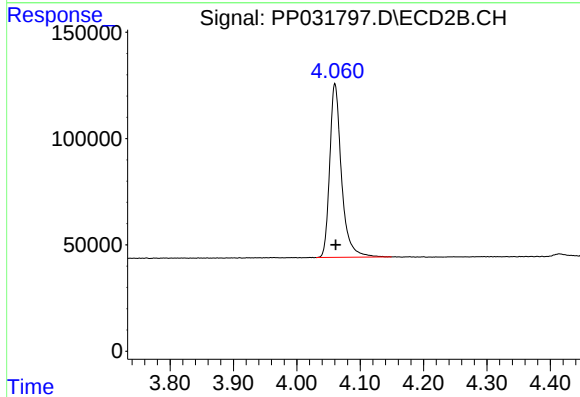


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.001 min
Response: 1055408
Conc: 22.03 ng/ml

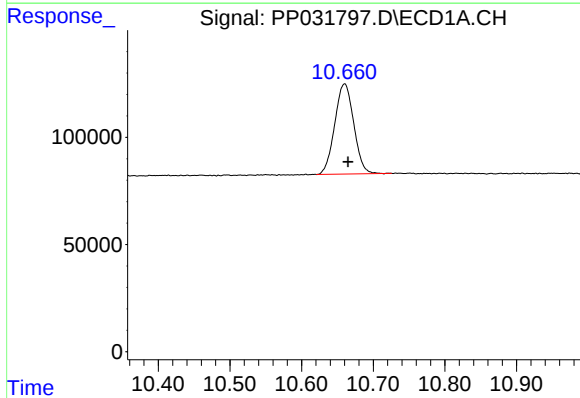


#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.005 min
Response: 775497
Conc: 22.83 ng/ml

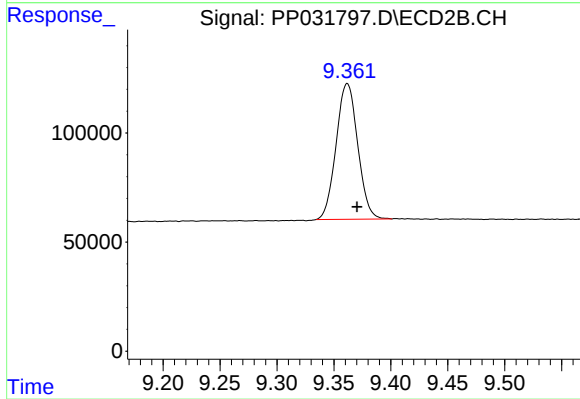

#2 Decachlorobiphenyl


R.T.: 9.362 min
Delta R.T.: -0.009 min
Response: 822843
Conc: 22.22 ng/ml

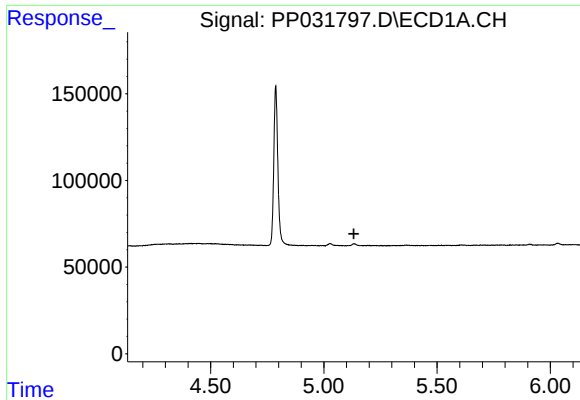

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

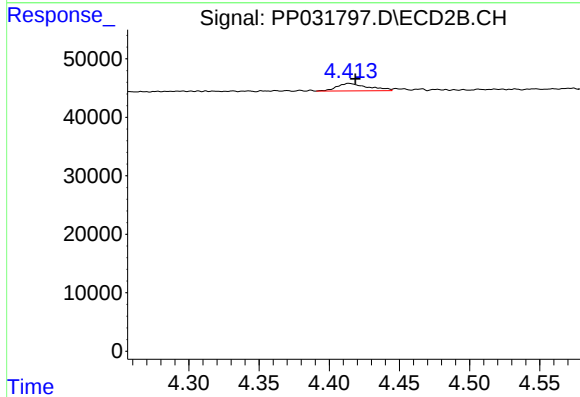


#9 AR-1221-2

R.T.: 4.414 min
Delta R.T.: -0.005 min
Response: 19802
Conc: 51.33 ng/ml

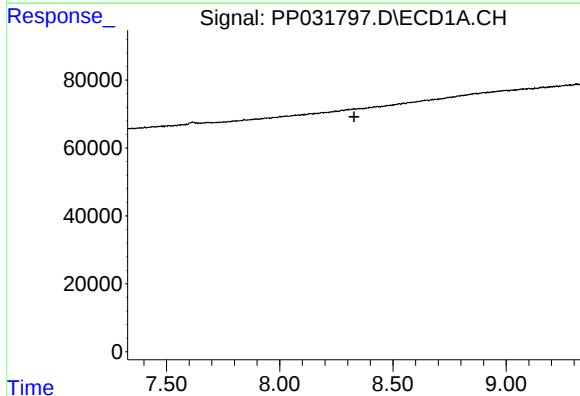


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 8.328 min
Response: 0
Conc: N.D.

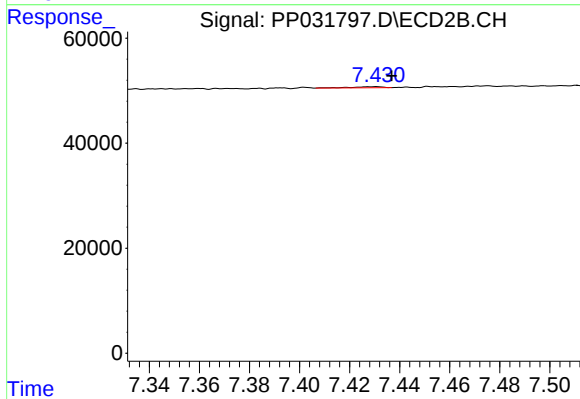

#30 AR-1254-5


R.T.: 7.431 min
Delta R.T.: -0.006 min
Response: 1717
Conc: 0.64 ng/ml

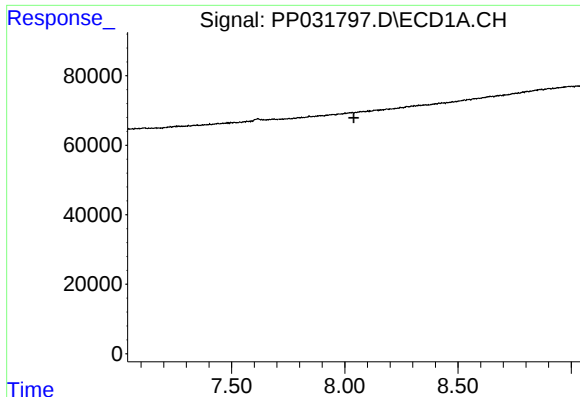

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

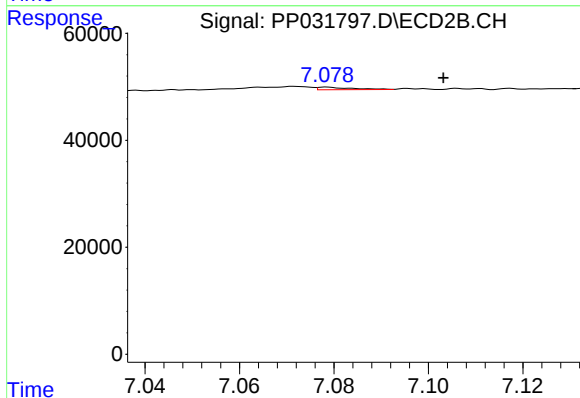


#32 AR-1260-2

R.T.: 7.078 min
Delta R.T.: -0.025 min
Response: 2381
Conc: 0.98 ng/ml

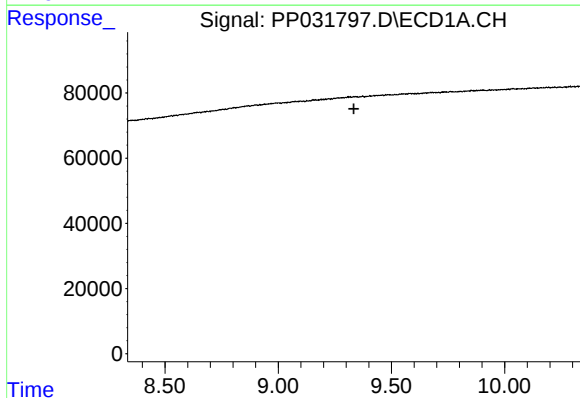


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.334 min
Response: 0
Conc: N.D.

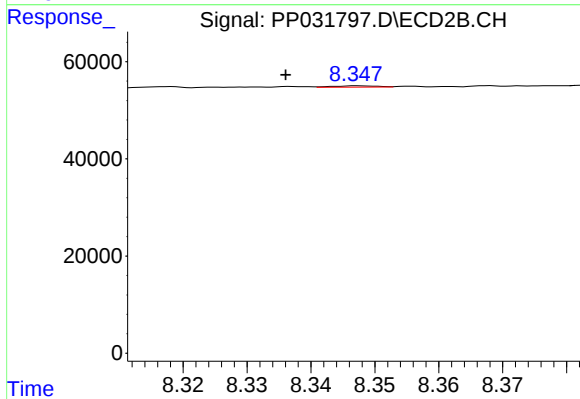

#39 AR-1262-4


R.T.: 8.347 min
Delta R.T.: 0.011 min
Response: 1265
Conc: 0.35 ng/ml

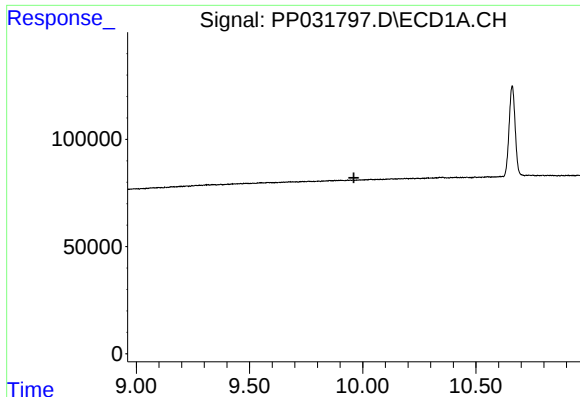

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.961 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

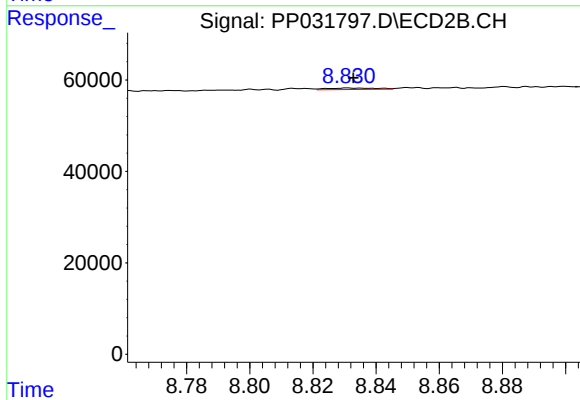


#40 AR-1262-5

R.T.: 8.831 min
Delta R.T.: -0.002 min
Response: 3463
Conc: 2.13 ng/ml

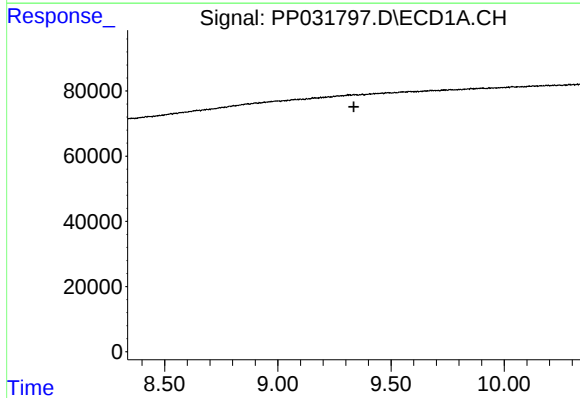


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.336 min
Response: 0
Conc: N.D.

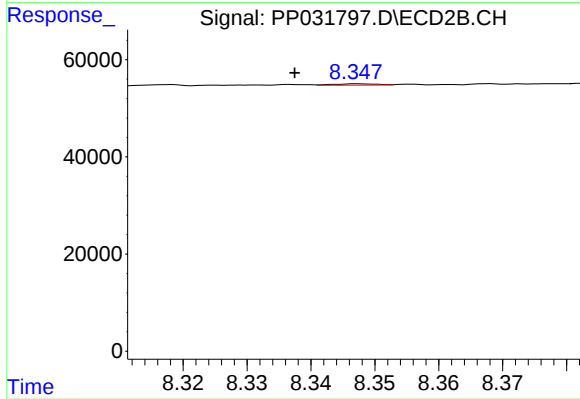

#42 AR-1268-2


R.T.: 8.347 min
Delta R.T.: 0.010 min
Response: 1265
Conc: 0.23 ng/ml

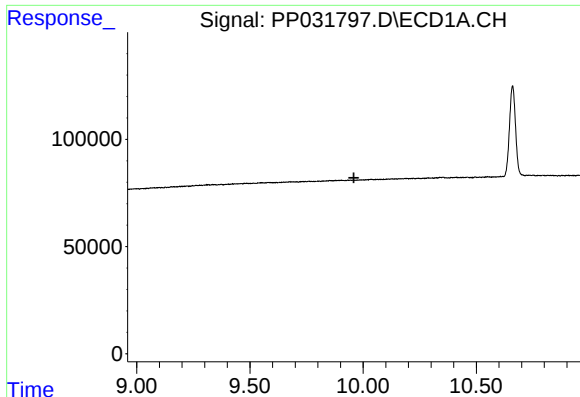

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

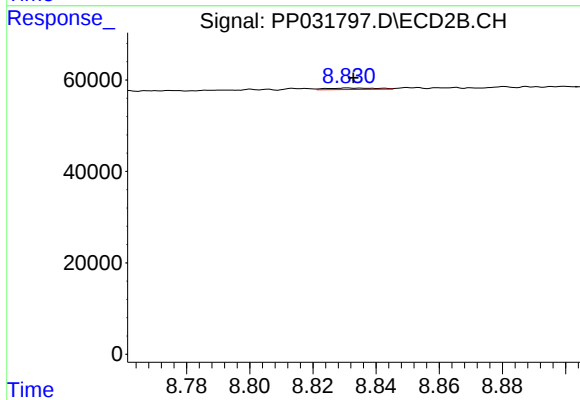


#44 AR-1268-4

R.T.: 8.831 min
Delta R.T.: -0.002 min
Response: 3463
Conc: 1.90 ng/ml

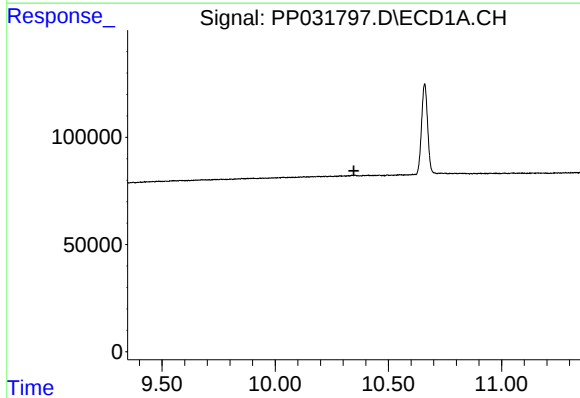

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.347 min
Response: 0
Conc: N.D.

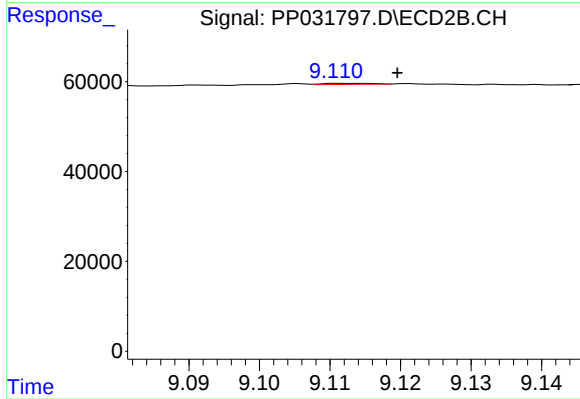

#45 AR-1268-5

R.T.: 9.111 min
Delta R.T.: -0.008 min
Response: 1143
Conc: 0.08 ng/ml