

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 13:27
 Operator : DD\AJ
 Sample : L4911-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SK-12-1-SPA

Manual Integrations
 APPROVED

Ankita
 12/3/2020 10:24:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 13:48:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.787	4.060	1162711	1057529	24.011	22.069
2) SA Decachlor...	10.660	9.361	556790	594747	16.393	16.062m
Target Compounds						
31) L7 AR-1260-1	7.773	6.902	74379	108198	42.501m	54.754 #
32) L7 AR-1260-2	8.037	7.098	103594	133394	50.417	54.777
33) L7 AR-1260-3	8.403	7.252	75014	99028	45.992	43.364
34) L7 AR-1260-4	8.629	7.735	120061	88183	65.203m	46.409 #
35) L7 AR-1260-5	8.946	7.982	176013	214419	47.736	47.250

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 13:27
Operator : DD\AJ
Sample : L4911-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SK-12-1-SPA


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 13:48:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

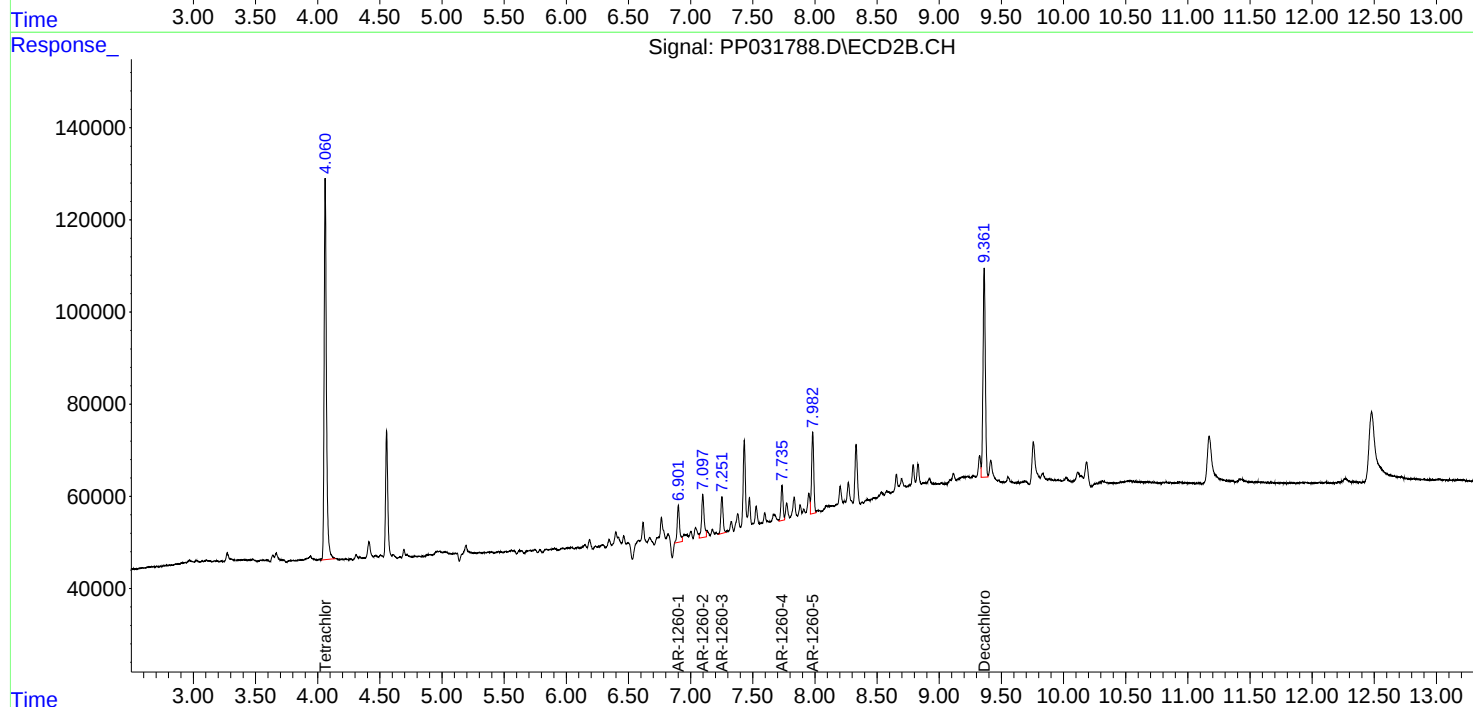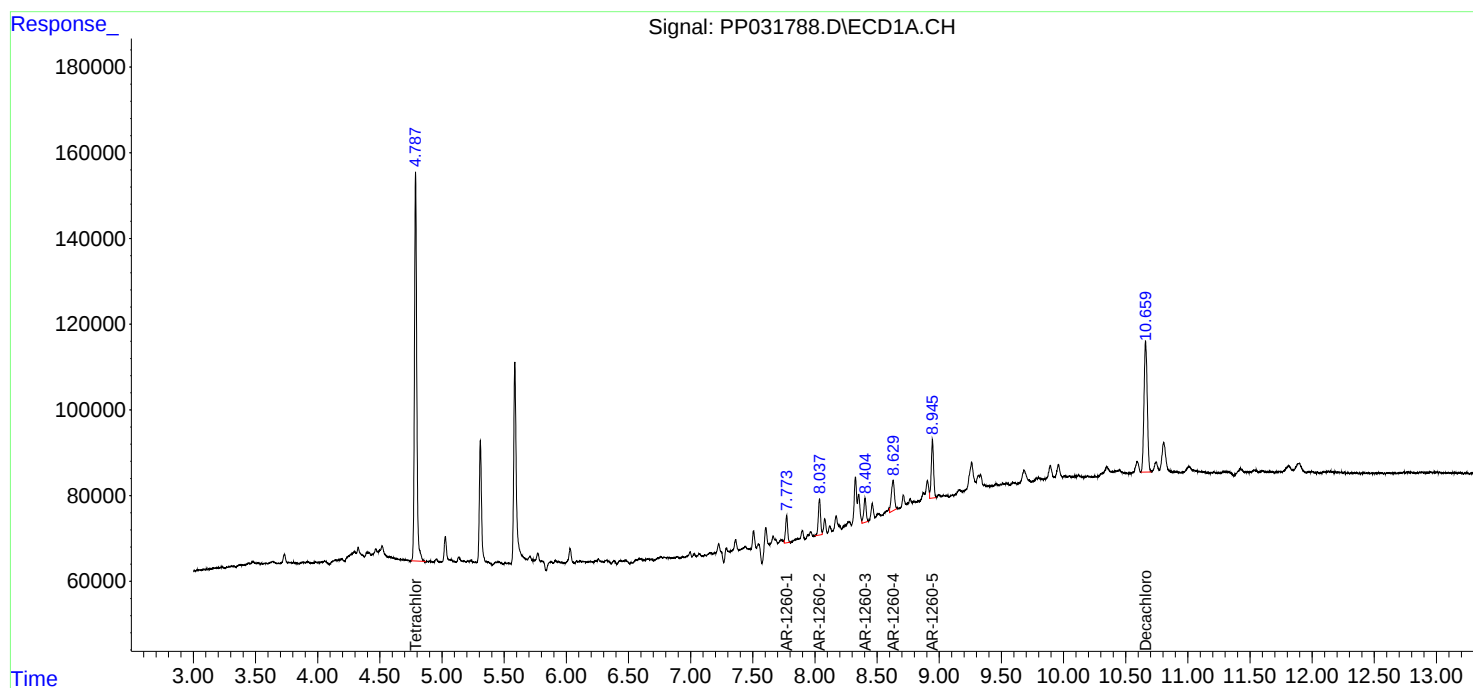

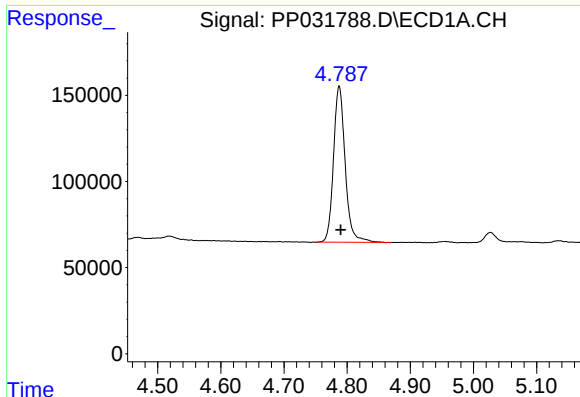


#1 Tetrachloro-m-xylene

R.T.: 4.787 min
Delta R.T.: -0.003 min
Response: 1162711
Conc: 24.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPA


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:03 AM

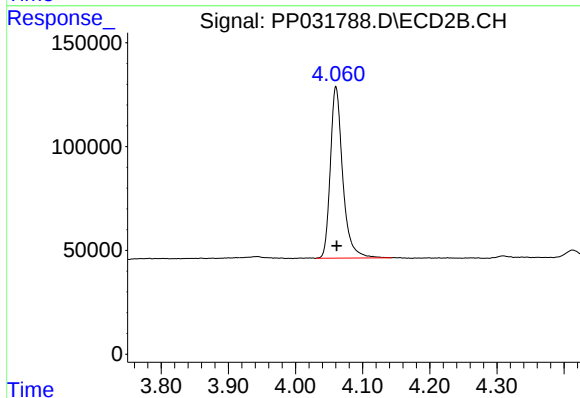


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.001 min
Response: 1057529
Conc: 22.07 ng/ml

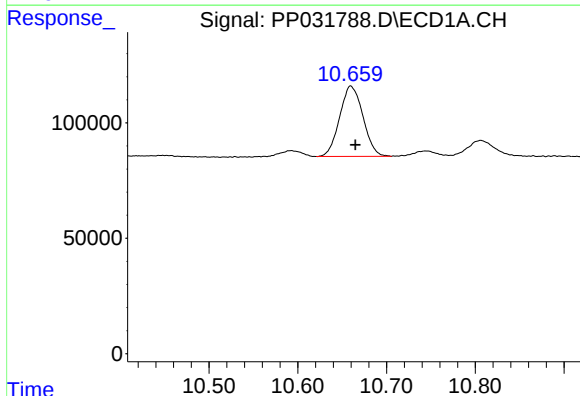


#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.005 min
Response: 556790
Conc: 16.39 ng/ml

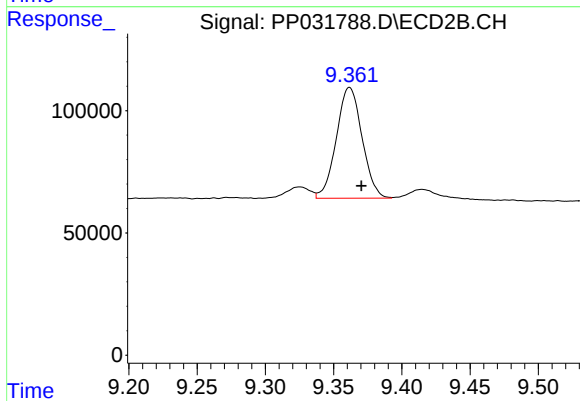

#2 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: -0.009 min
Response: 594747
Conc: 16.06 ng/ml m

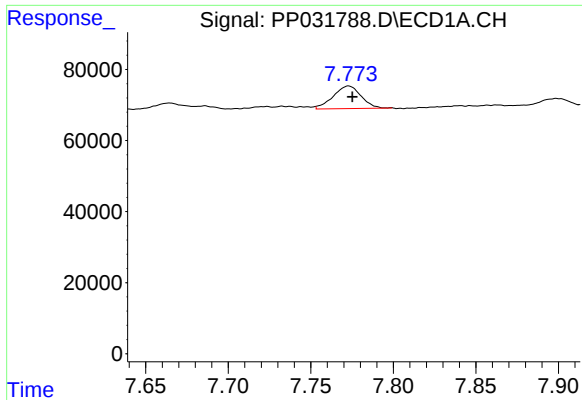


#31 AR-1260-1

R.T.: 7.773 min
Delta R.T.: -0.003 min
Response: 74379
Conc: 42.50 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPA


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:03 AM

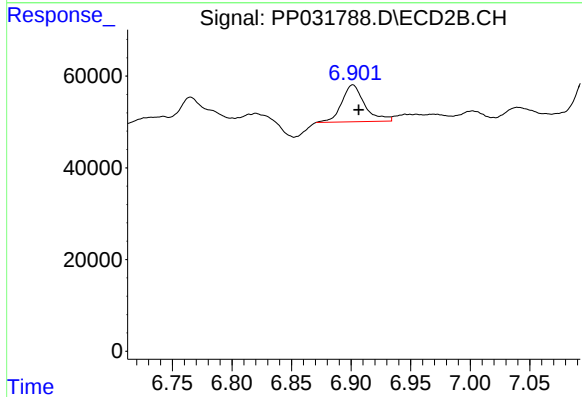


#31 AR-1260-1

R.T.: 6.902 min
Delta R.T.: -0.005 min
Response: 108198
Conc: 54.75 ng/ml

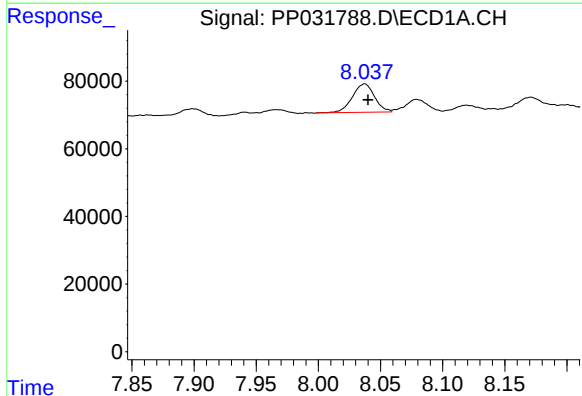


#32 AR-1260-2

R.T.: 8.037 min
Delta R.T.: -0.003 min
Response: 103594
Conc: 50.42 ng/ml

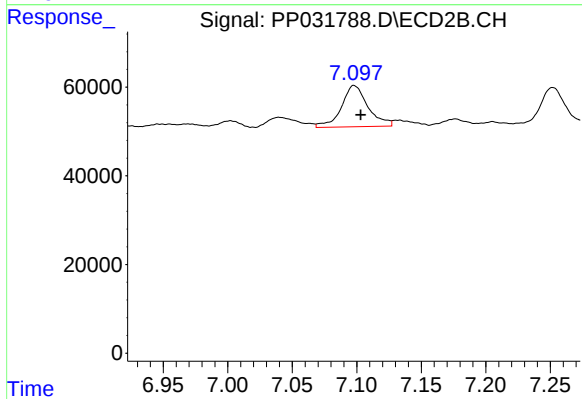

#32 AR-1260-2

R.T.: 7.098 min
Delta R.T.: -0.005 min
Response: 133394
Conc: 54.78 ng/ml

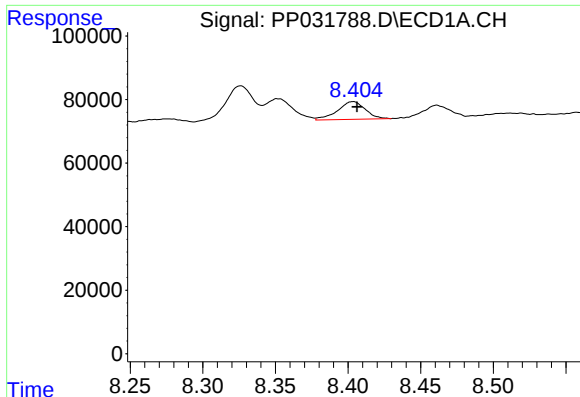


#33 AR-1260-3

R.T.: 8.403 min
Delta R.T.: -0.003 min
Response: 75014
Conc: 45.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPA


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:03 AM

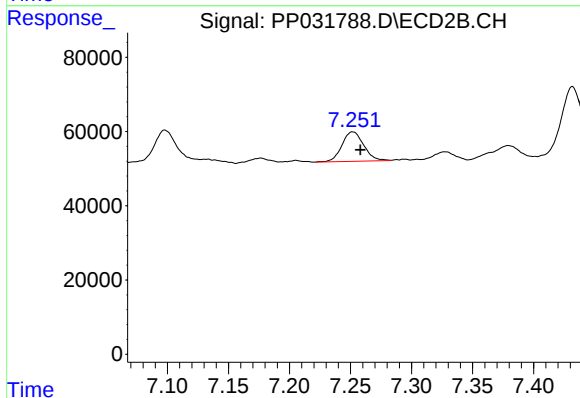


#33 AR-1260-3

R.T.: 7.252 min
Delta R.T.: -0.006 min
Response: 99028
Conc: 43.36 ng/ml

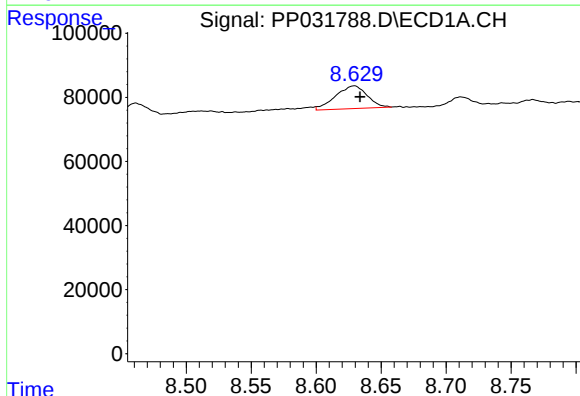


#34 AR-1260-4

R.T.: 8.629 min
Delta R.T.: -0.005 min
Response: 120061
Conc: 65.20 ng/ml m

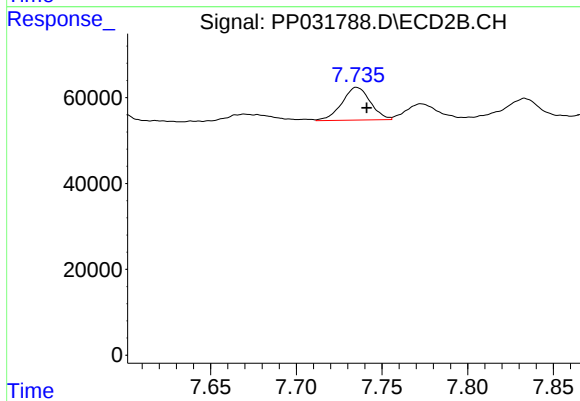

#34 AR-1260-4

R.T.: 7.735 min
Delta R.T.: -0.006 min
Response: 88183
Conc: 46.41 ng/ml

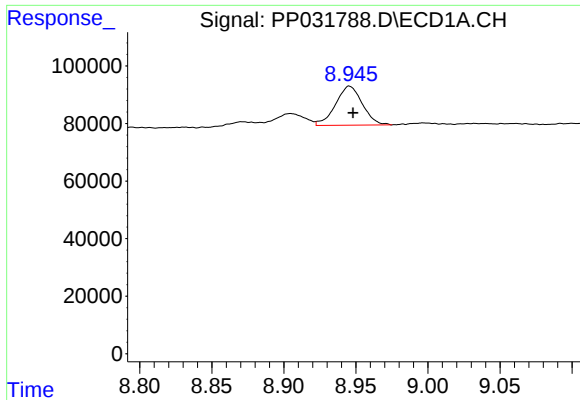


#35 AR-1260-5

R.T.: 8.946 min
Delta R.T.: -0.002 min
Response: 176013
Conc: 47.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPA

Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:03 AM

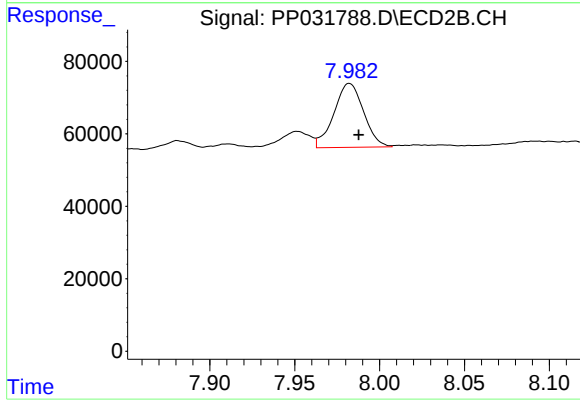

#35 AR-1260-5

R.T.: 7.982 min
Delta R.T.: -0.005 min
Response: 214419
Conc: 47.25 ng/ml