

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031789.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 13:44
 Operator : DD\AJ
 Sample : L4911-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SK-12-1-SPB

Manual Integrations
 APPROVED

Ankita
 12/3/2020 10:24:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 15:46:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.788	4.061	1136616	1028893	23.472	21.472
2) SA Decachlor...	10.663	9.363	563086	609488	16.579	16.461m
Target Compounds						
31) L7 AR-1260-1	7.773	6.902	162948	176138	93.111m	89.135
32) L7 AR-1260-2	8.039	7.100	146045	194124	71.077	79.714
33) L7 AR-1260-3	8.405	7.254	118530	156579	72.672	68.565
34) L7 AR-1260-4	8.630	7.737	217231	135983	117.974	71.565 #
35) L7 AR-1260-5	8.947	7.984	283702	353728	76.942	77.949

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031789.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 13:44
Operator : DD\AJ
Sample : L4911-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SK-12-1-SPB


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 15:46:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

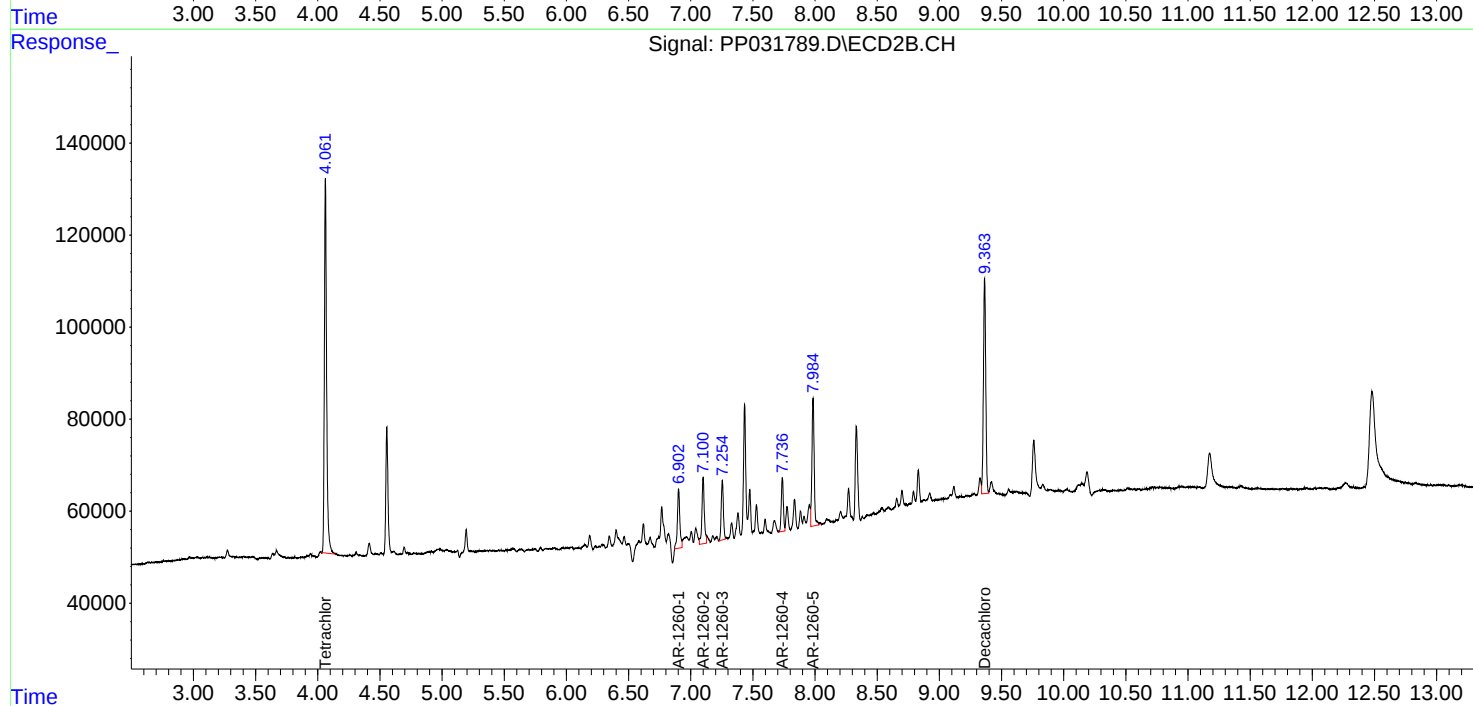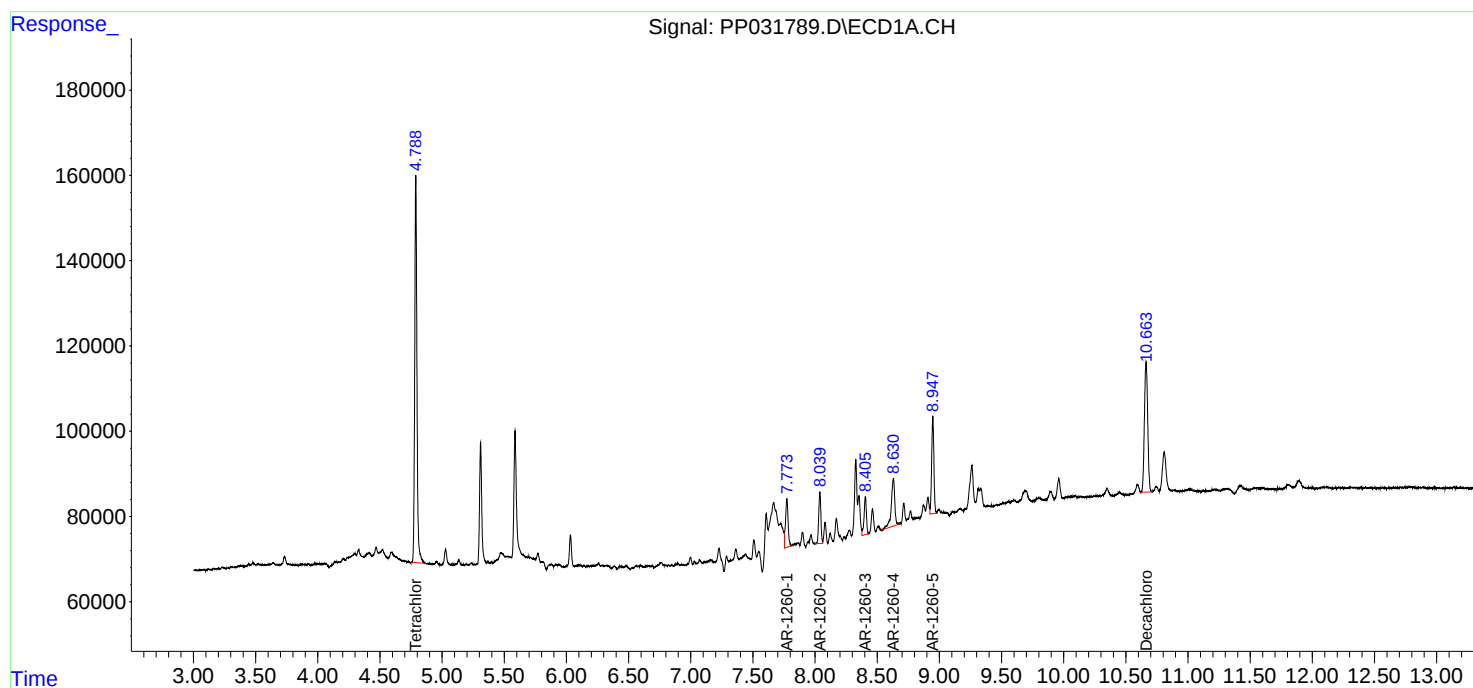

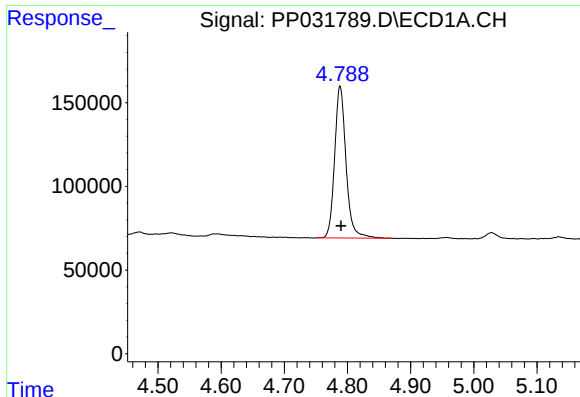


#1 Tetrachloro-m-xylene

R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 1136616
Conc: 23.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPB


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:05 AM

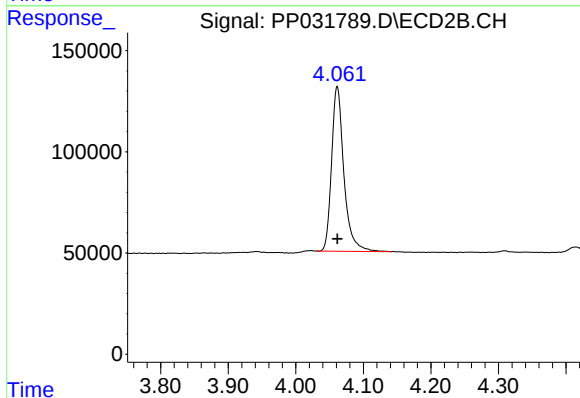


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1028893
Conc: 21.47 ng/ml

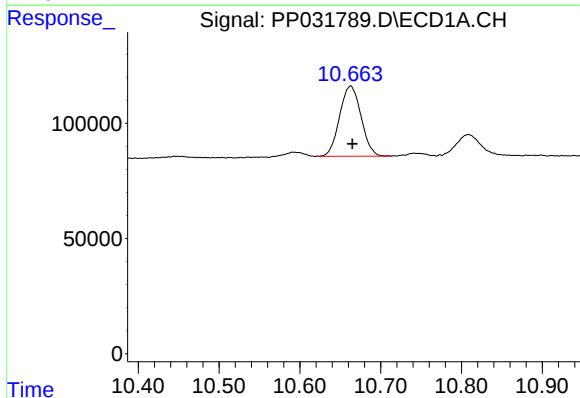


#2 Decachlorobiphenyl

R.T.: 10.663 min
Delta R.T.: -0.002 min
Response: 563086
Conc: 16.58 ng/ml

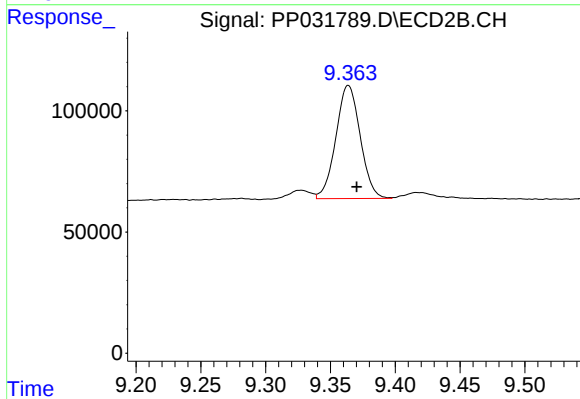

#2 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.007 min
Response: 609488
Conc: 16.46 ng/ml m

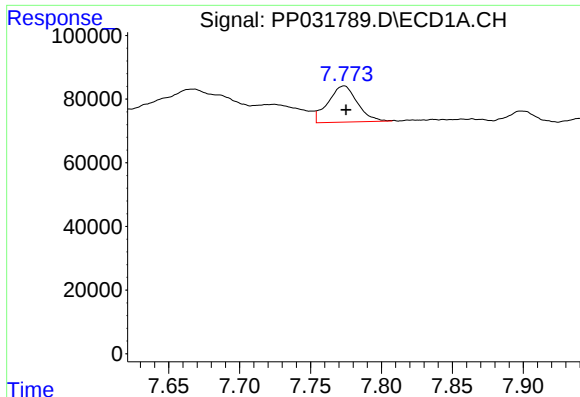


#31 AR-1260-1

R.T.: 7.773 min
Delta R.T.: -0.002 min
Response: 162948
Conc: 93.11 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPB


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:05 AM

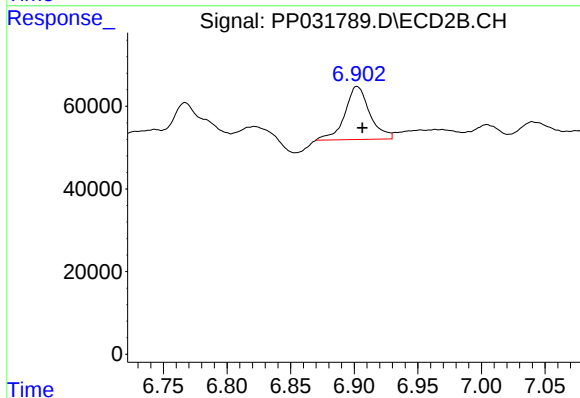


#31 AR-1260-1

R.T.: 6.902 min
Delta R.T.: -0.005 min
Response: 176138
Conc: 89.13 ng/ml

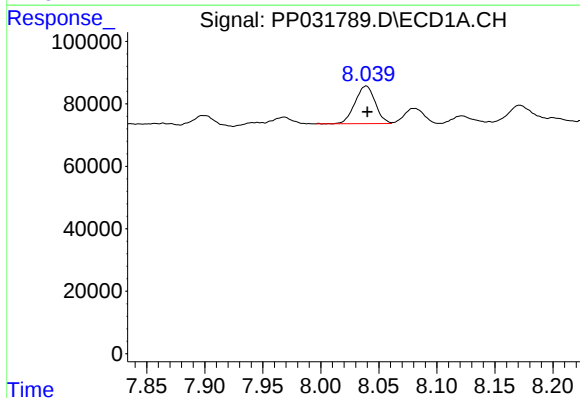


#32 AR-1260-2

R.T.: 8.039 min
Delta R.T.: 0.000 min
Response: 146045
Conc: 71.08 ng/ml

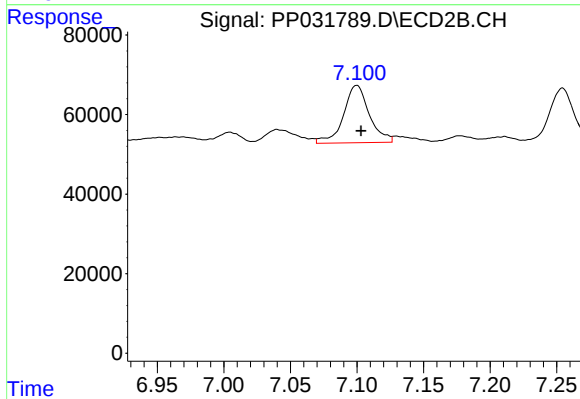

#32 AR-1260-2

R.T.: 7.100 min
Delta R.T.: -0.003 min
Response: 194124
Conc: 79.71 ng/ml

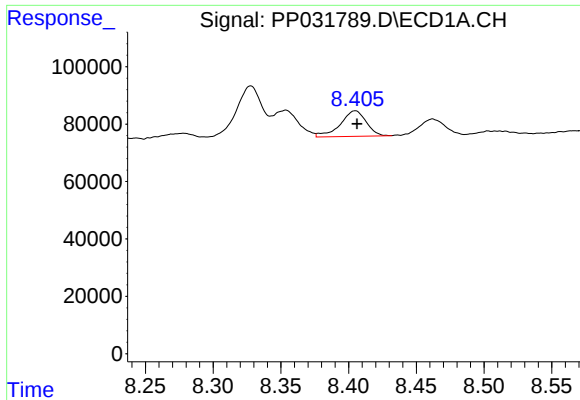


#33 AR-1260-3

R.T.: 8.405 min
Delta R.T.: -0.001 min
Response: 118530
Conc: 72.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPB


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:05 AM

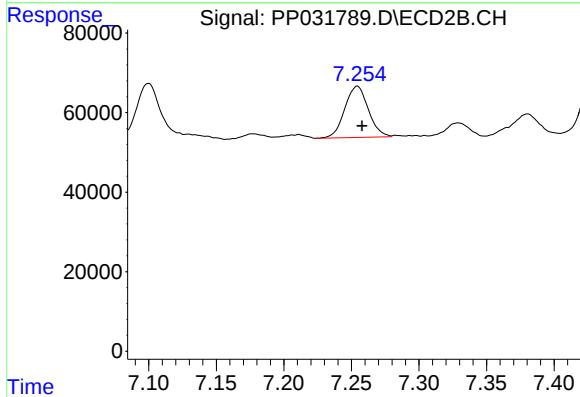


#33 AR-1260-3

R.T.: 7.254 min
Delta R.T.: -0.004 min
Response: 156579
Conc: 68.57 ng/ml

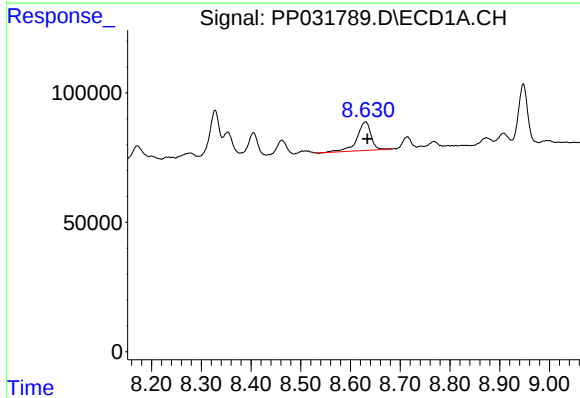


#34 AR-1260-4

R.T.: 8.630 min
Delta R.T.: -0.004 min
Response: 217231
Conc: 117.97 ng/ml

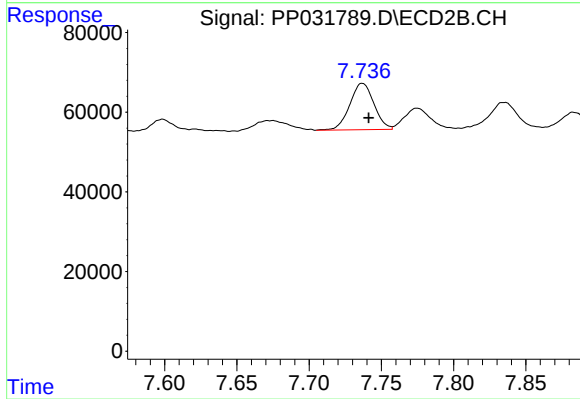

#34 AR-1260-4

R.T.: 7.737 min
Delta R.T.: -0.004 min
Response: 135983
Conc: 71.57 ng/ml

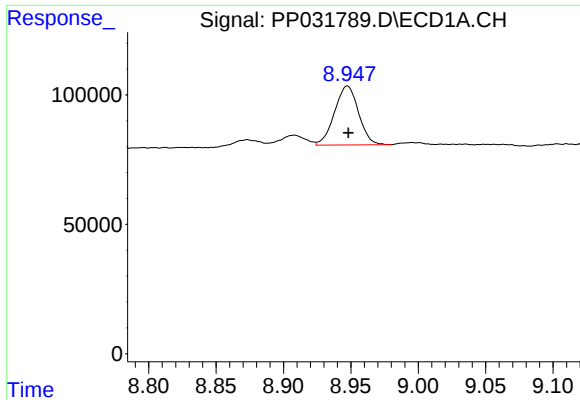


#35 AR-1260-5

R.T.: 8.947 min
Delta R.T.: 0.000 min
Response: 283702
Conc: 76.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPB

Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:05 AM

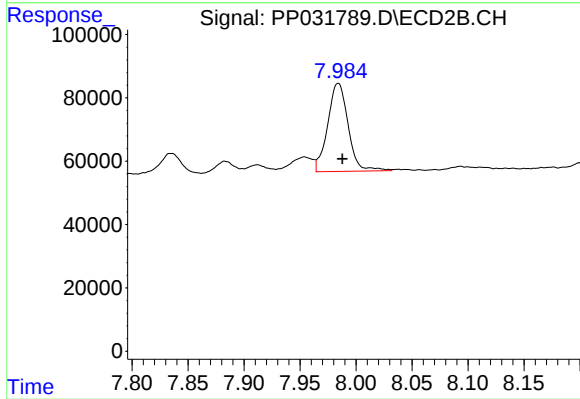

#35 AR-1260-5

R.T.: 7.984 min
Delta R.T.: -0.004 min
Response: 353728
Conc: 77.95 ng/ml