

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031790.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 14:01
 Operator : DD\AJ
 Sample : L4911-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SK-12-1-SPC

Manual Integrations
 APPROVED

Ankita
 12/3/2020 10:24:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 15:47:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.788	4.060	1128590	1014653	23.307	21.175
2) SA Decachlor...	10.663	9.363	523054	575463	15.400	15.542m
Target Compounds						
31) L7 AR-1260-1	7.773	6.901	134688	92825	76.963m	46.974 #
32) L7 AR-1260-2	8.038	7.098	72847	143698	35.453	59.008 #
33) L7 AR-1260-3	8.404	7.252	58520	89666	35.879	39.265
34) L7 AR-1260-4	8.629	7.736	118400	71478	64.300	37.618 #
35) L7 AR-1260-5	8.945	7.982	142065	186265	38.529	41.046

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031790.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 14:01
Operator : DD\AJ
Sample : L4911-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPC


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 15:47:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

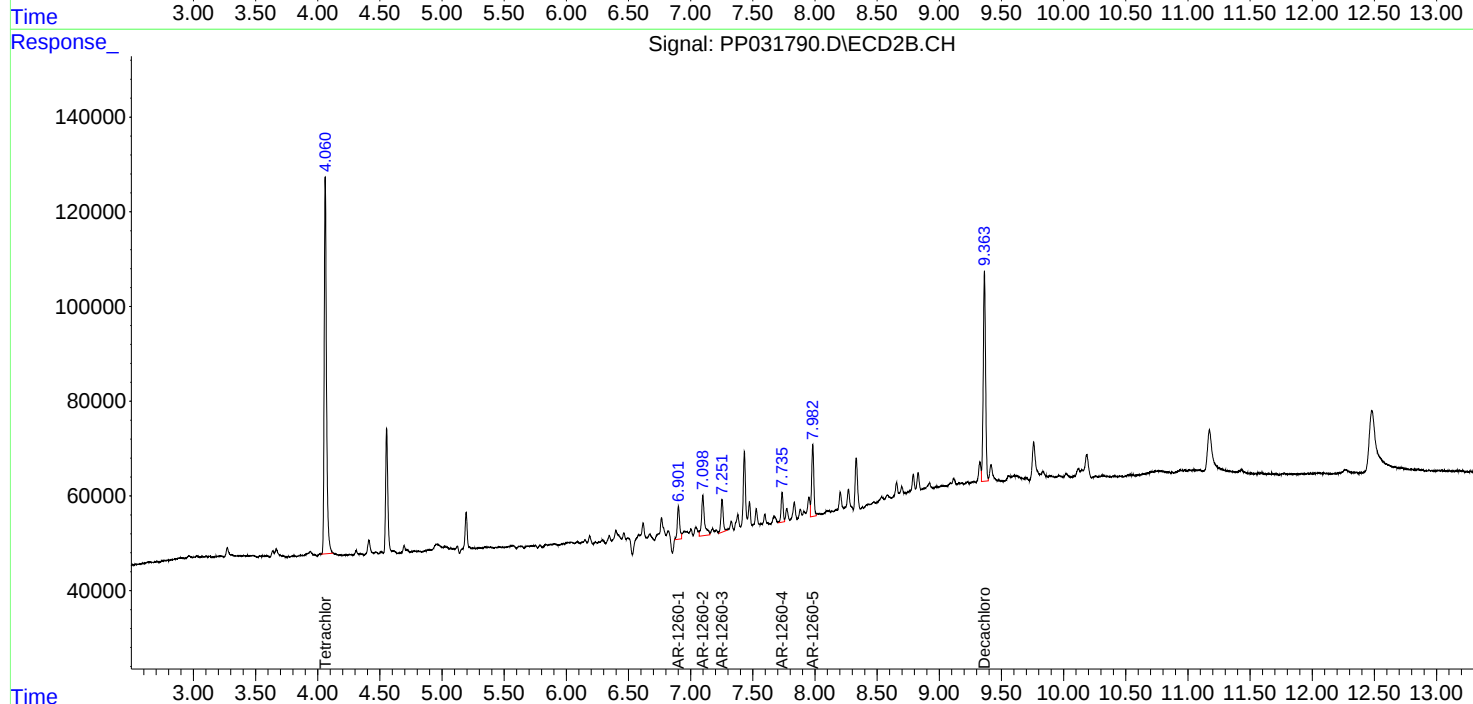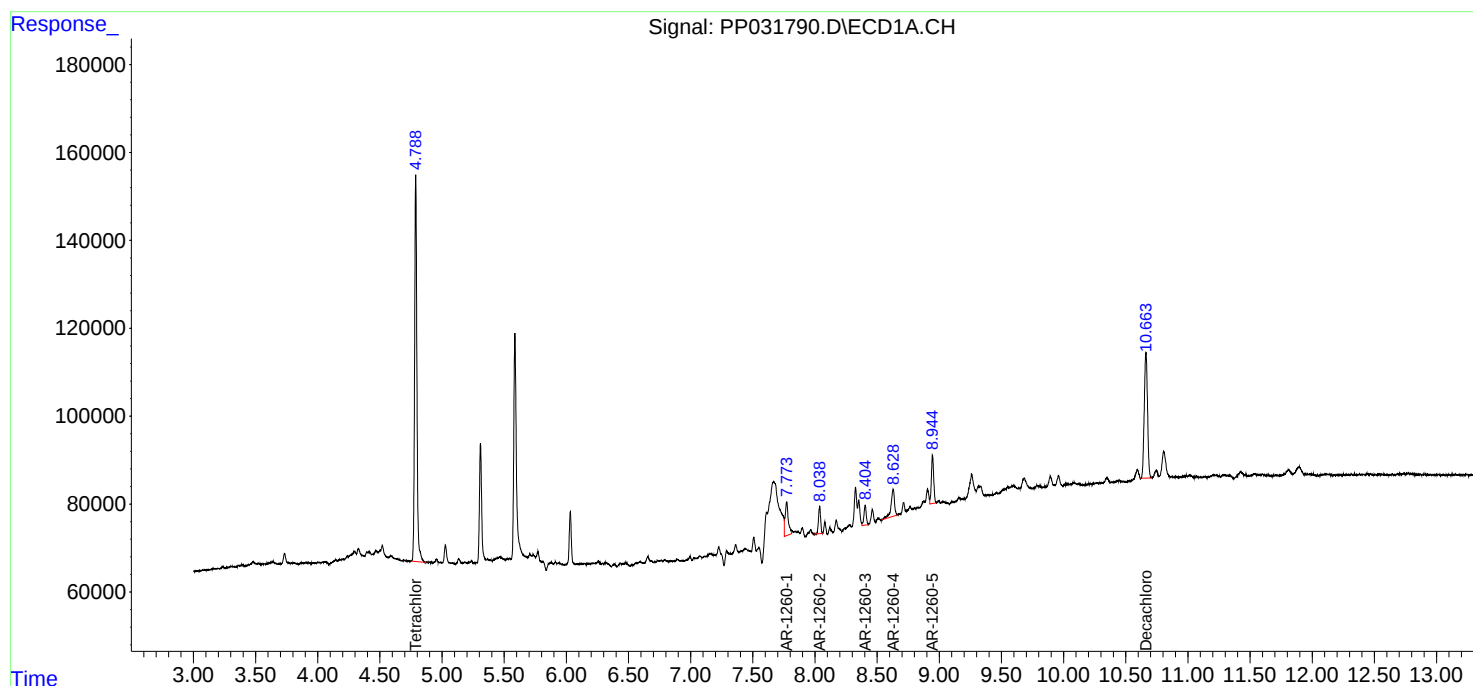

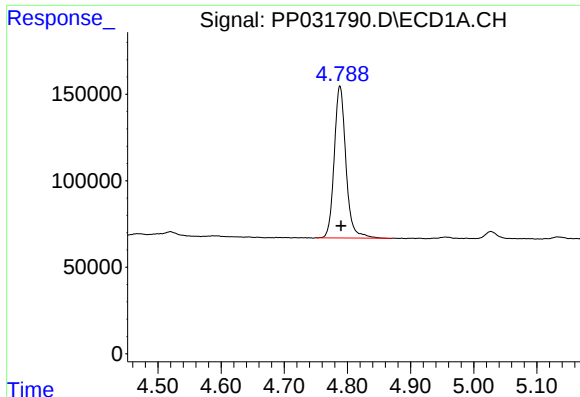


#1 Tetrachloro-m-xylene

R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 1128590
Conc: 23.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPC


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:06 AM

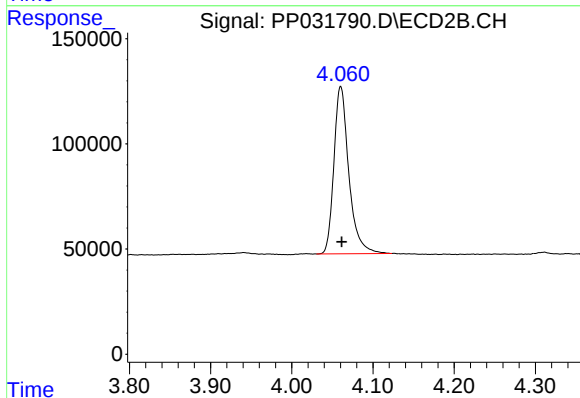


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.001 min
Response: 1014653
Conc: 21.17 ng/ml

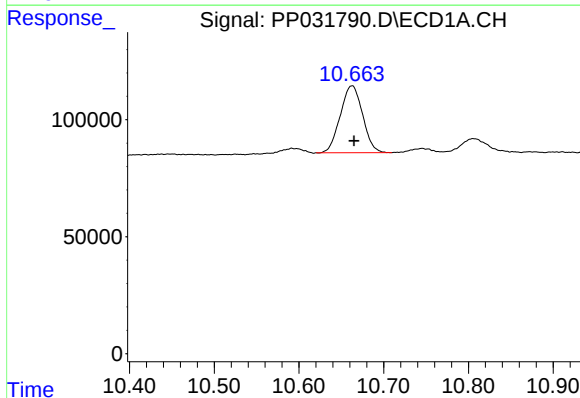


#2 Decachlorobiphenyl

R.T.: 10.663 min
Delta R.T.: -0.002 min
Response: 523054
Conc: 15.40 ng/ml

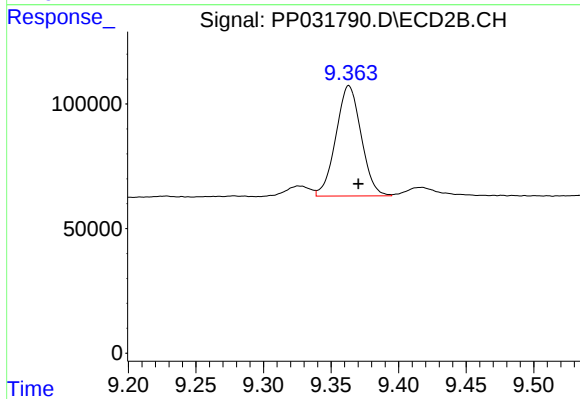

#2 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.008 min
Response: 575463
Conc: 15.54 ng/ml m

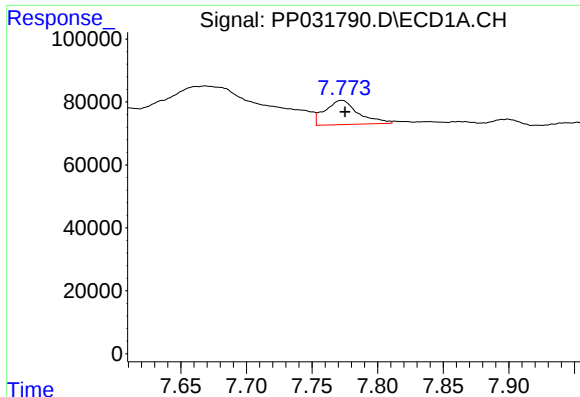


#31 AR-1260-1

R.T.: 7.773 min
Delta R.T.: -0.003 min
Response: 134688
Conc: 76.96 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPC


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:06 AM

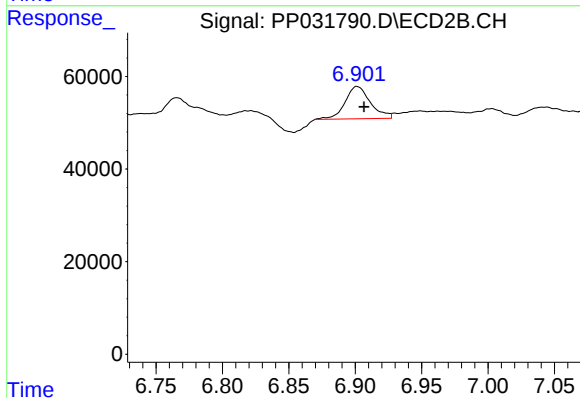


#31 AR-1260-1

R.T.: 6.901 min
Delta R.T.: -0.005 min
Response: 92825
Conc: 46.97 ng/ml

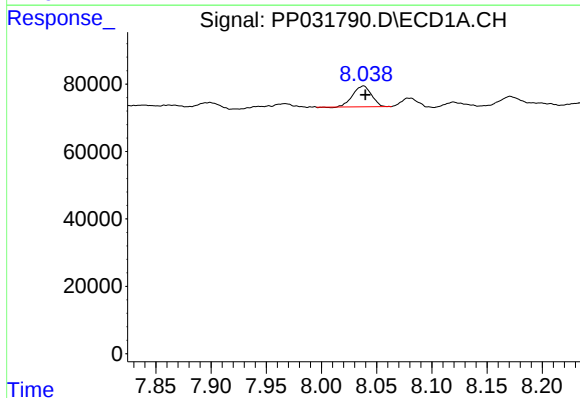


#32 AR-1260-2

R.T.: 8.038 min
Delta R.T.: -0.002 min
Response: 72847
Conc: 35.45 ng/ml

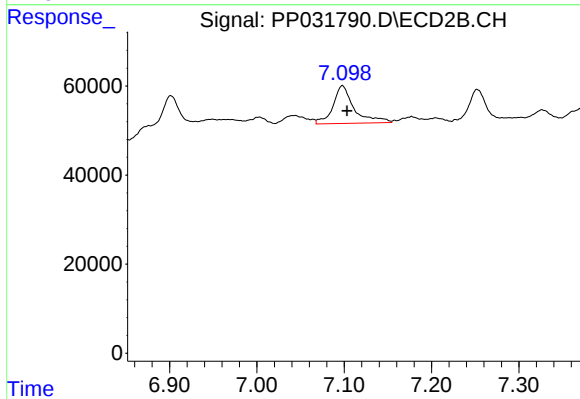

#32 AR-1260-2

R.T.: 7.098 min
Delta R.T.: -0.005 min
Response: 143698
Conc: 59.01 ng/ml

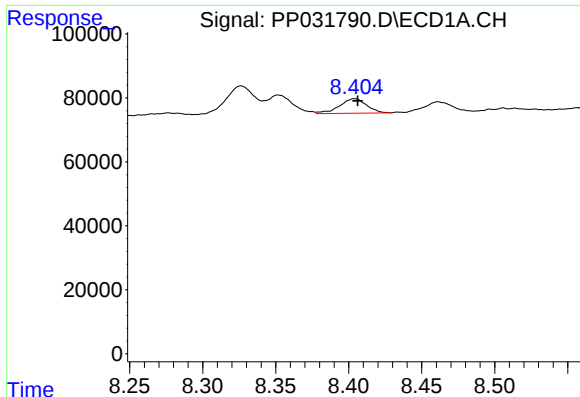


#33 AR-1260-3

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 58520
Conc: 35.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPC


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:06 AM

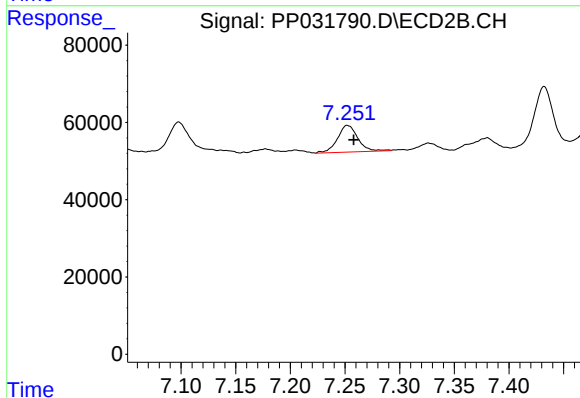


#33 AR-1260-3

R.T.: 7.252 min
Delta R.T.: -0.006 min
Response: 89666
Conc: 39.26 ng/ml

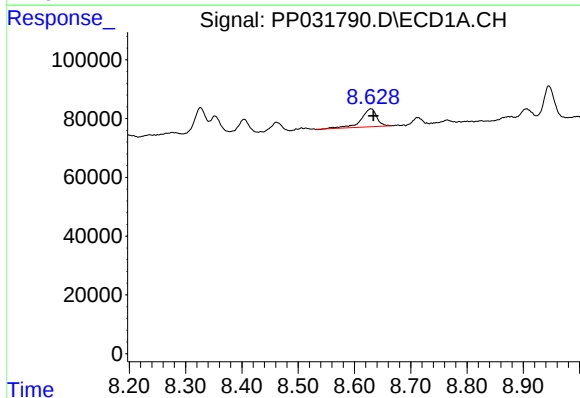


#34 AR-1260-4

R.T.: 8.629 min
Delta R.T.: -0.004 min
Response: 118400
Conc: 64.30 ng/ml

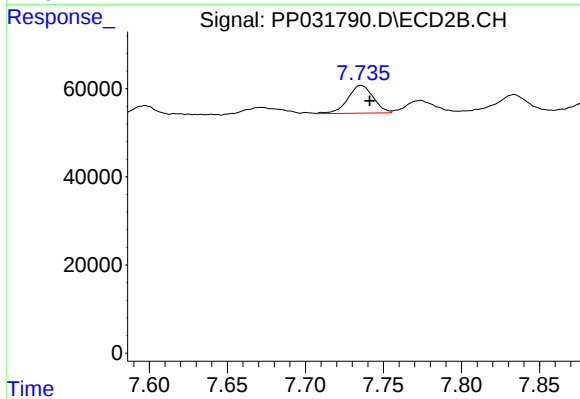

#34 AR-1260-4

R.T.: 7.736 min
Delta R.T.: -0.005 min
Response: 71478
Conc: 37.62 ng/ml

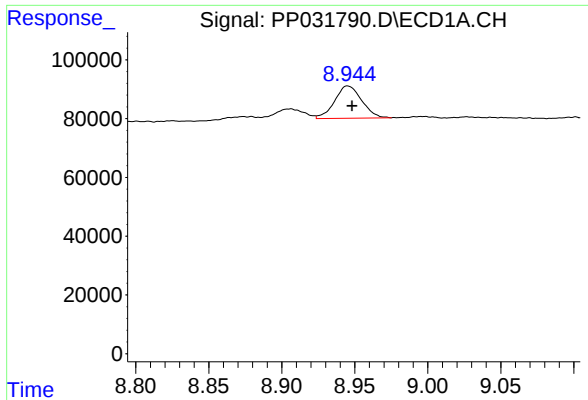


#35 AR-1260-5

R.T.: 8.945 min
Delta R.T.: -0.003 min
Response: 142065
Conc: 38.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPC

Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:06 AM

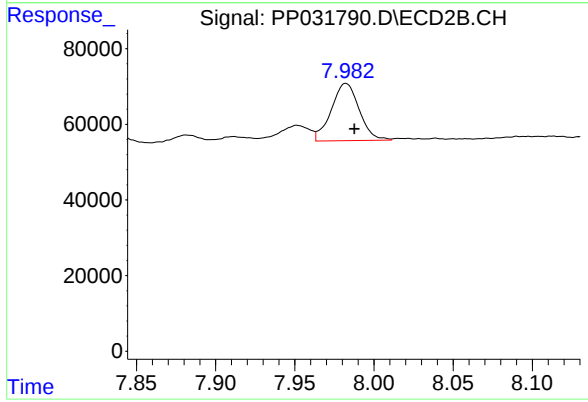

#35 AR-1260-5

R.T.: 7.982 min
Delta R.T.: -0.005 min
Response: 186265
Conc: 41.05 ng/ml