

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031791.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 14:17
 Operator : DD\AJ
 Sample : L4911-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SK-12-1-SPD

Manual Integrations
 APPROVED

Ankita
 12/3/2020 10:24:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 15:47:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.788	4.061	1143788	1031506	23.621	21.526
2) SA Decachlor...	10.661	9.362	619551	674426	18.241	18.214m
Target Compounds						
31) L7 AR-1260-1	7.772	6.901	131992	130143	75.422m	65.859
32) L7 AR-1260-2	8.037	7.098	122705	172196	59.718	70.710
33) L7 AR-1260-3	8.404	7.252	86990	120848	53.334	52.919
34) L7 AR-1260-4	8.630	7.735	150771	100379	81.881m	52.828 #
35) L7 AR-1260-5	8.947	7.983	221319	261305	60.023	57.582

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031791.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 14:17
Operator : DD\AJ
Sample : L4911-04
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SK-12-1-SPD


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 15:47:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

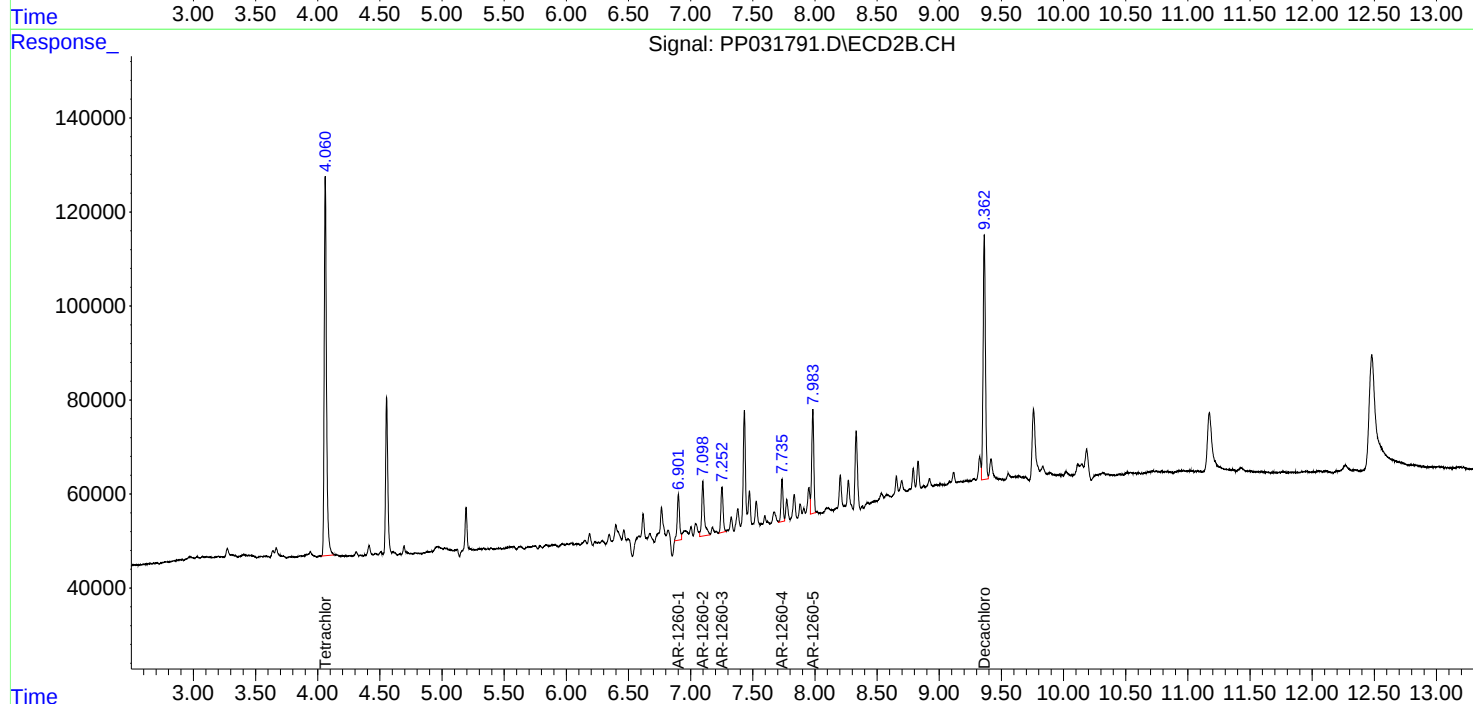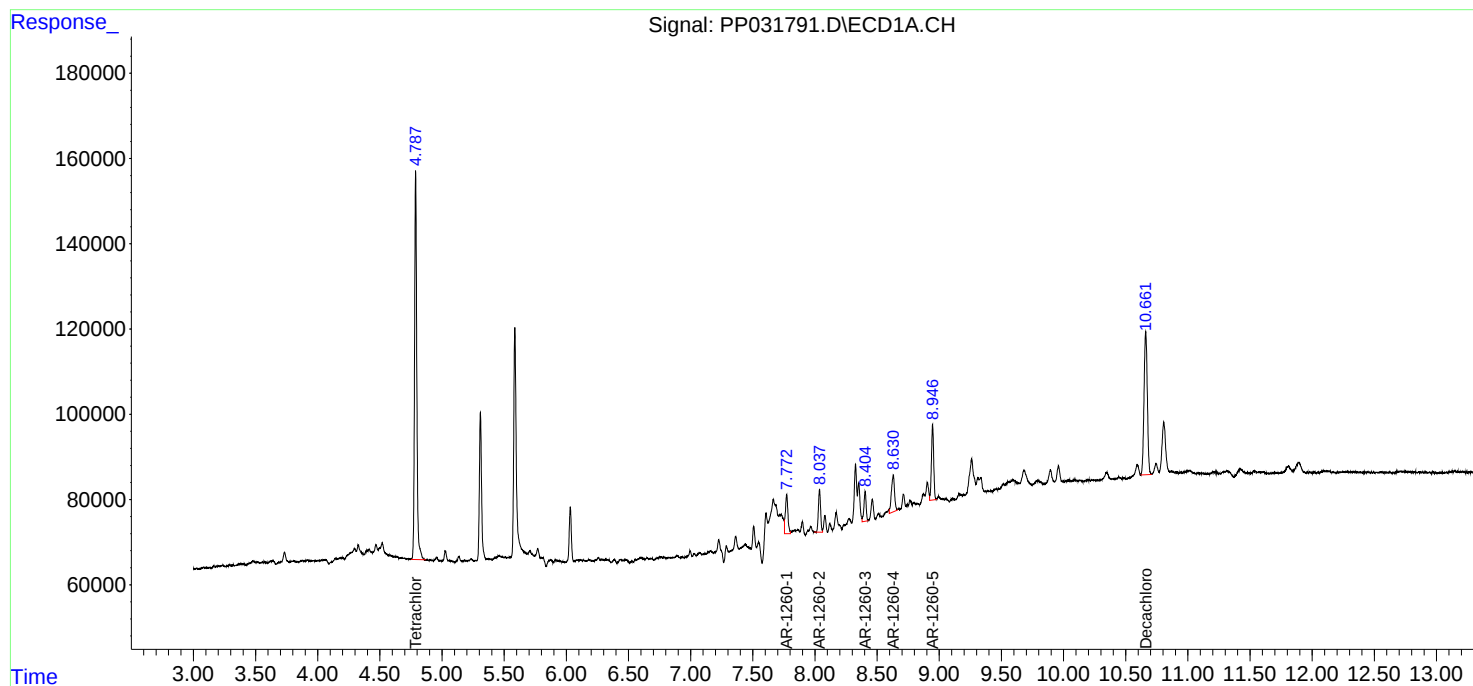

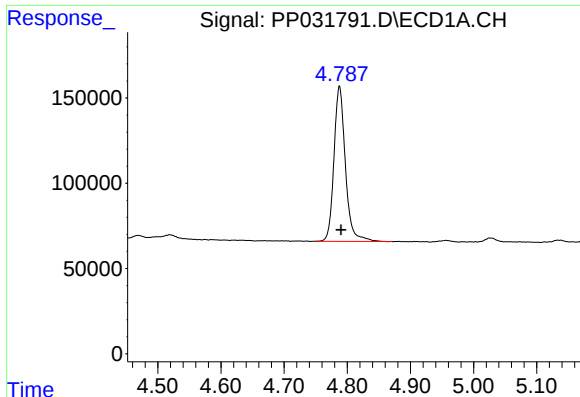


#1 Tetrachloro-m-xylene

R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 1143788
Conc: 23.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPD


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:08 AM

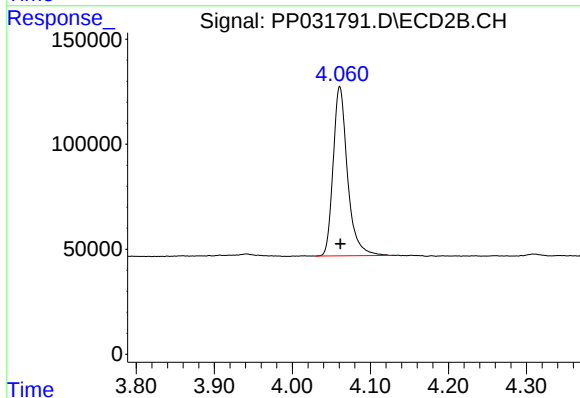


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1031506
Conc: 21.53 ng/ml

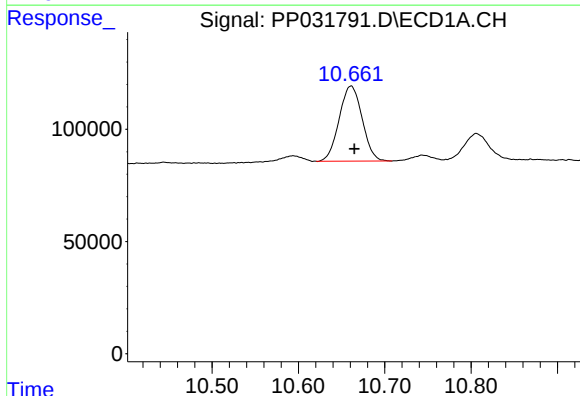


#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: -0.004 min
Response: 619551
Conc: 18.24 ng/ml

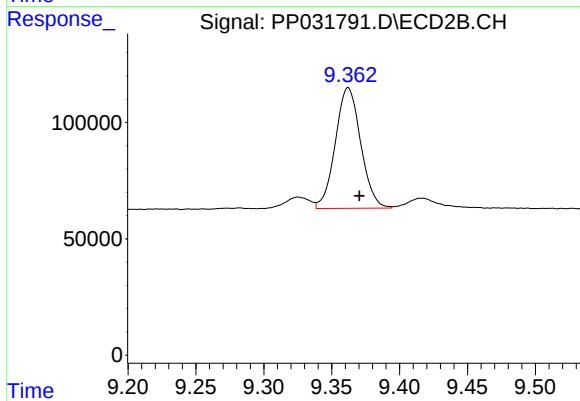

#2 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.009 min
Response: 674426
Conc: 18.21 ng/ml m

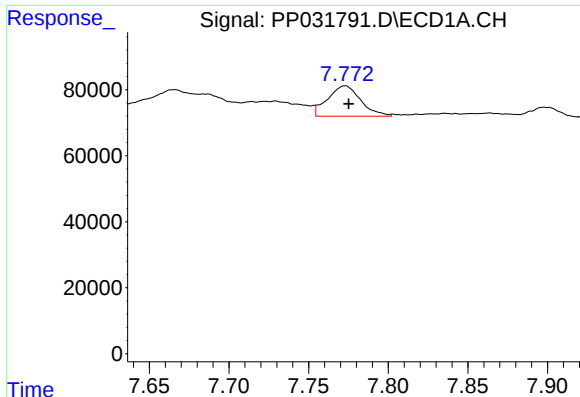


#31 AR-1260-1

R.T.: 7.772 min
Delta R.T.: -0.003 min
Response: 131992
Conc: 75.42 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPD


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:08 AM

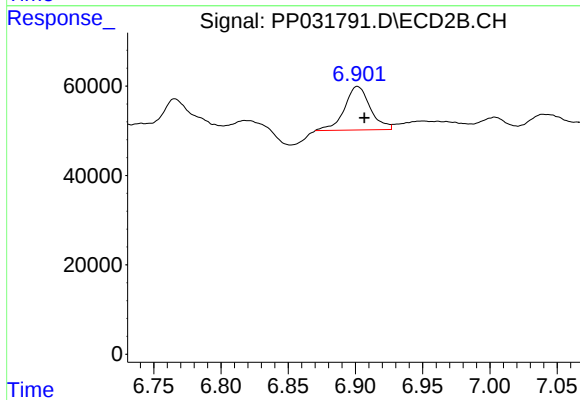


#31 AR-1260-1

R.T.: 6.901 min
Delta R.T.: -0.005 min
Response: 130143
Conc: 65.86 ng/ml

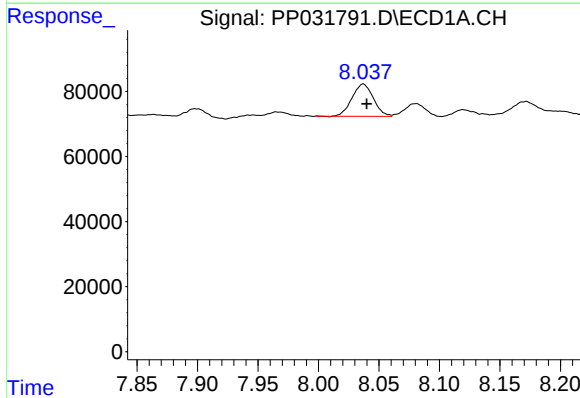


#32 AR-1260-2

R.T.: 8.037 min
Delta R.T.: -0.003 min
Response: 122705
Conc: 59.72 ng/ml

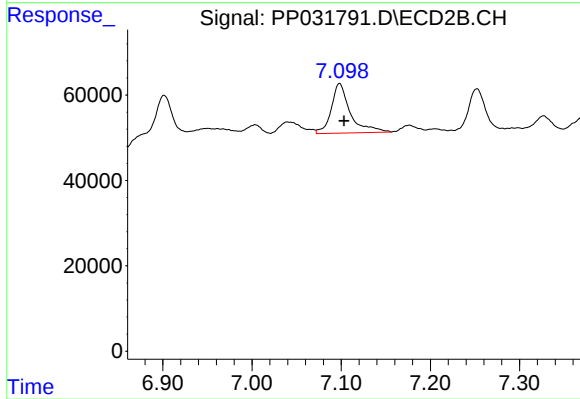

#32 AR-1260-2

R.T.: 7.098 min
Delta R.T.: -0.005 min
Response: 172196
Conc: 70.71 ng/ml

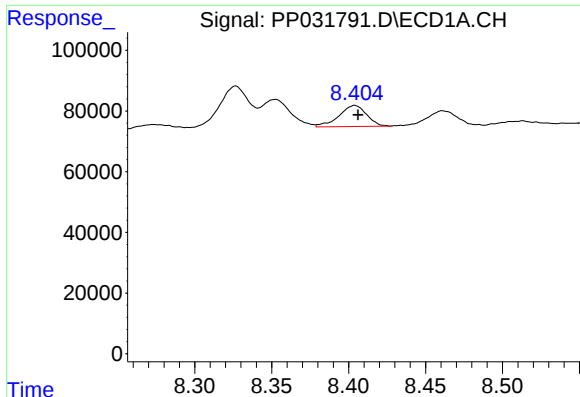


#33 AR-1260-3

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 86990
Conc: 53.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPD


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:08 AM

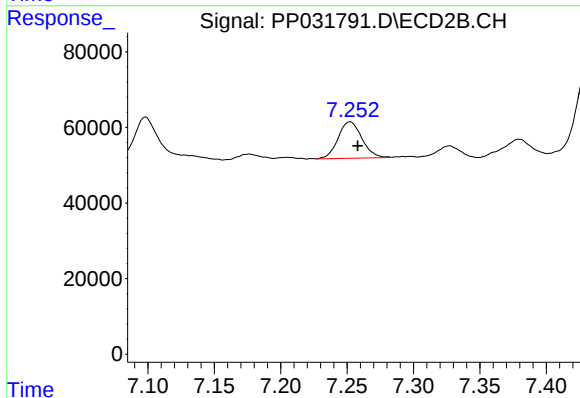


#33 AR-1260-3

R.T.: 7.252 min
Delta R.T.: -0.006 min
Response: 120848
Conc: 52.92 ng/ml

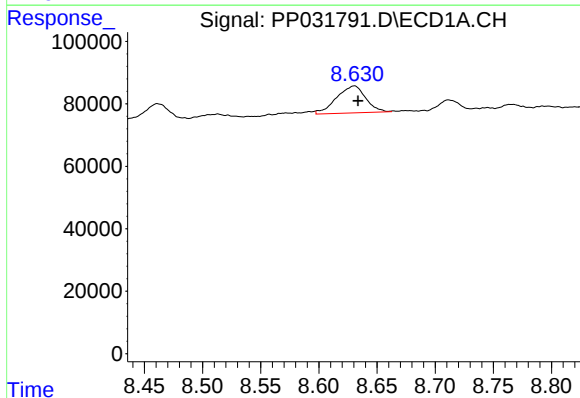


#34 AR-1260-4

R.T.: 8.630 min
Delta R.T.: -0.003 min
Response: 150771
Conc: 81.88 ng/ml m

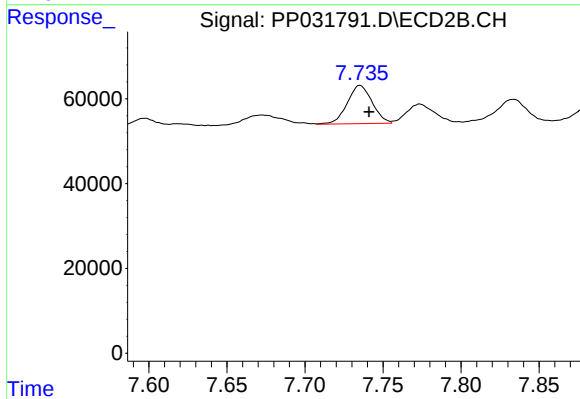

#34 AR-1260-4

R.T.: 7.735 min
Delta R.T.: -0.006 min
Response: 100379
Conc: 52.83 ng/ml

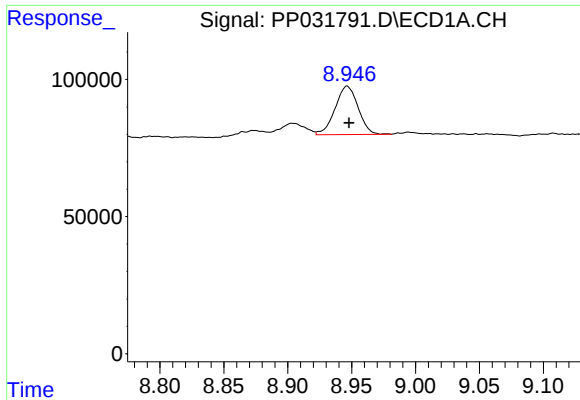


#35 AR-1260-5

R.T.: 8.947 min
Delta R.T.: -0.002 min
Response: 221319
Conc: 60.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPD

Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:08 AM

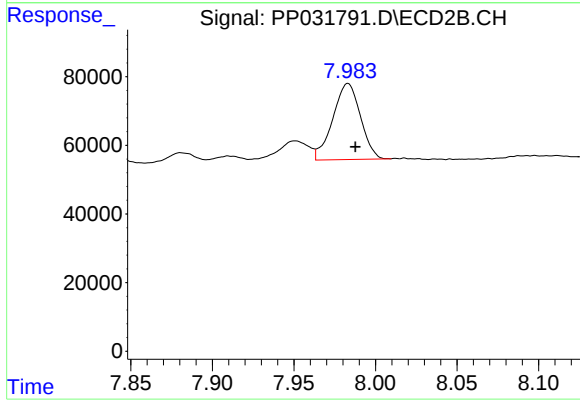

#35 AR-1260-5

R.T.: 7.983 min
Delta R.T.: -0.005 min
Response: 261305
Conc: 57.58 ng/ml