

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031794.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 15:08
 Operator : DD\AJ
 Sample : L4911-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SK-12-1-SPE

Manual Integrations
 APPROVED

Ankita
 12/3/2020 10:24:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 15:48:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.788	4.061	1114867	1008136	23.023	21.039
2) SA Decachlor...	10.662	9.362	606905	648933	17.869	17.526m
Target Compounds						
31) L7 AR-1260-1	7.774	6.901	36529	61121	20.873m	30.930 #
32) L7 AR-1260-2	8.036	7.099	65131	92856	31.698	38.130
33) L7 AR-1260-3	8.403	7.253	37000	56971	22.685m	24.948
34) L7 AR-1260-4	8.627	7.735	105407	56154	57.244	29.553 #
35) L7 AR-1260-5	8.947	7.983	135110	178827	36.643	39.407

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031794.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 15:08
Operator : DD\AJ
Sample : L4911-05
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SK-12-1-SPE


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 15:48:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

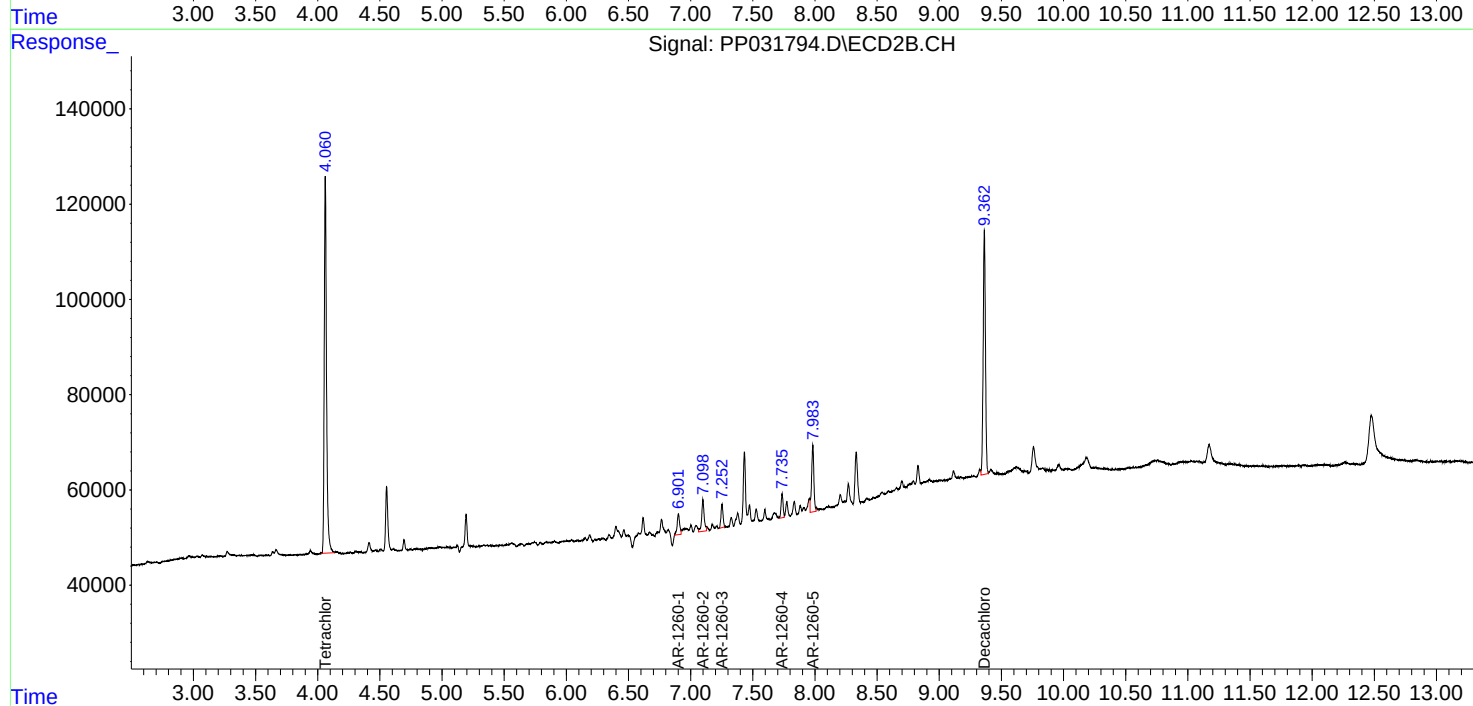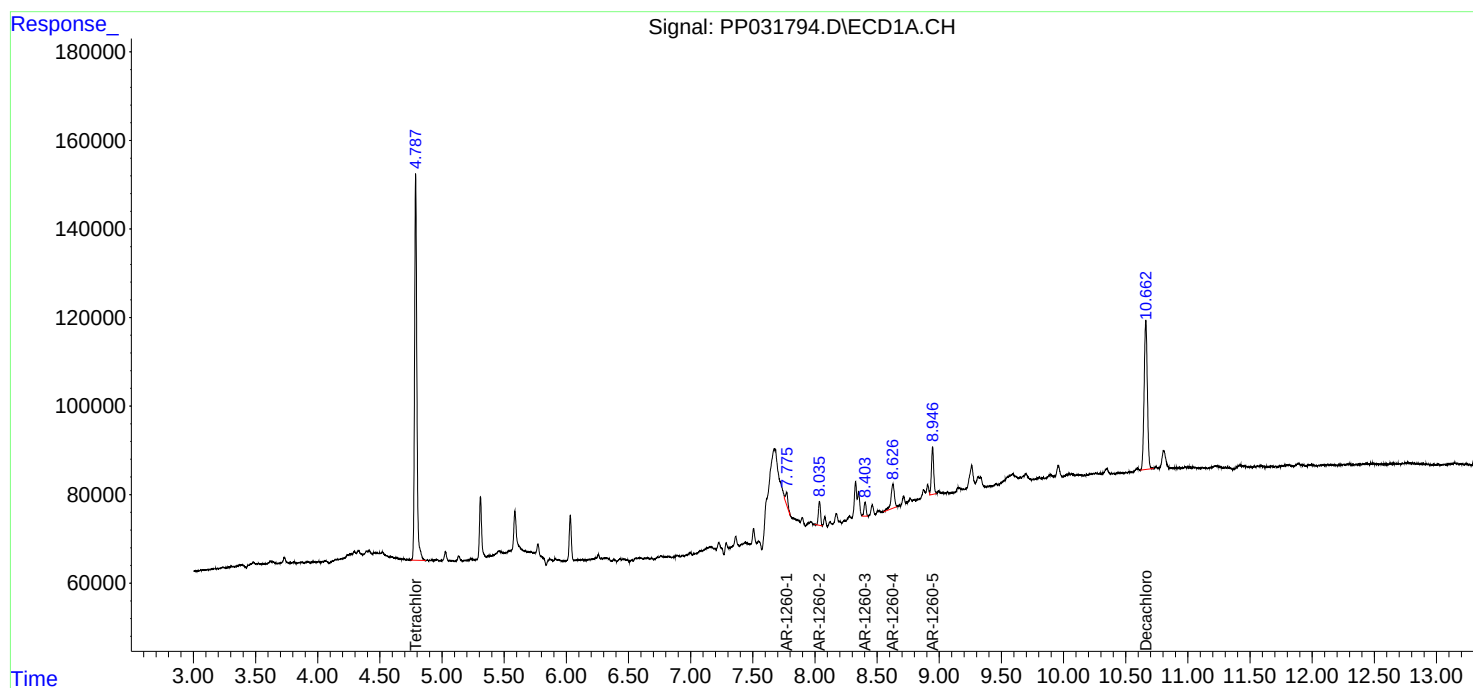

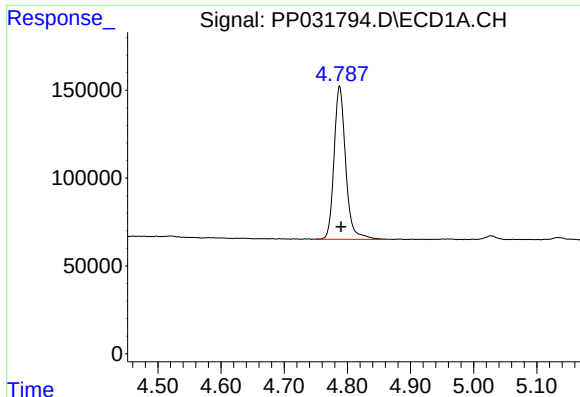


#1 Tetrachloro-m-xylene

R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 1114867
Conc: 23.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPE


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:14 AM

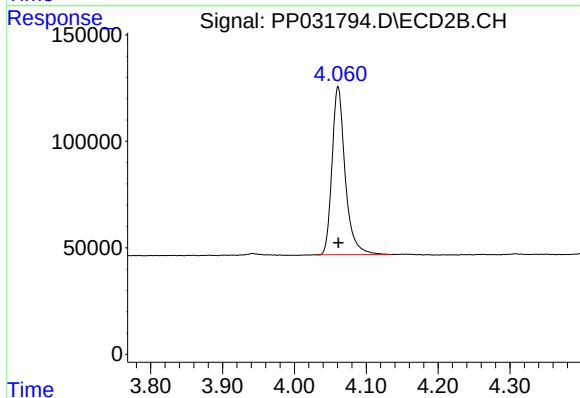


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1008136
Conc: 21.04 ng/ml

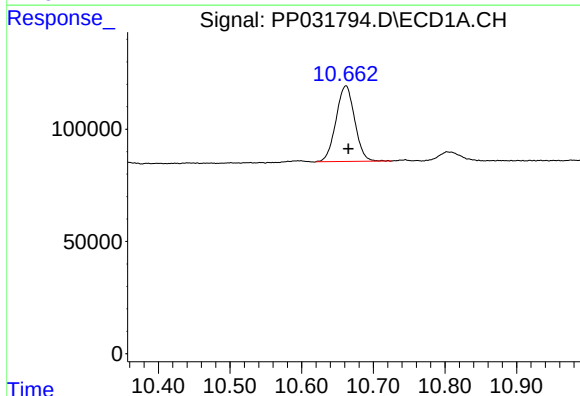


#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.003 min
Response: 606905
Conc: 17.87 ng/ml

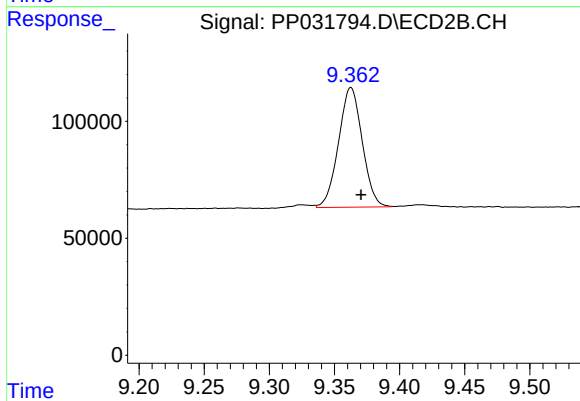

#2 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.008 min
Response: 648933
Conc: 17.53 ng/ml m

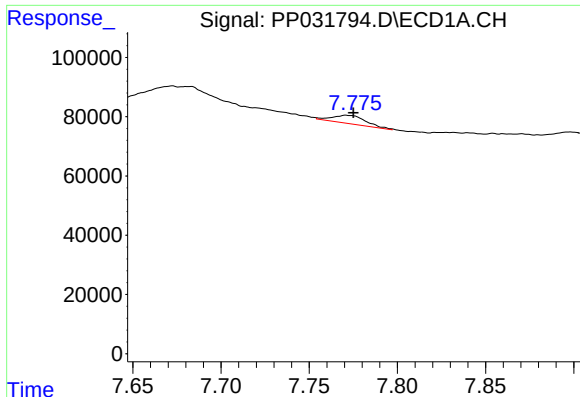


#31 AR-1260-1

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 36529
Conc: 20.87 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPE


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:14 AM

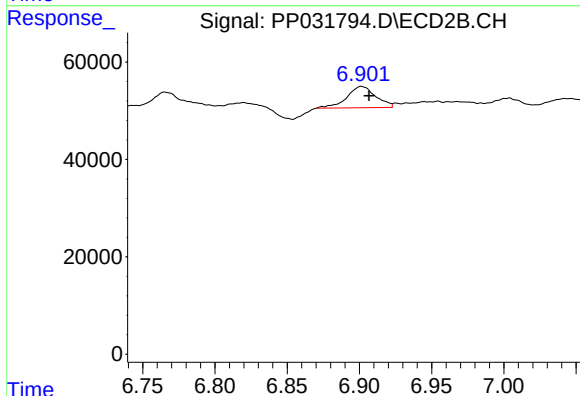


#31 AR-1260-1

R.T.: 6.901 min
Delta R.T.: -0.005 min
Response: 61121
Conc: 30.93 ng/ml

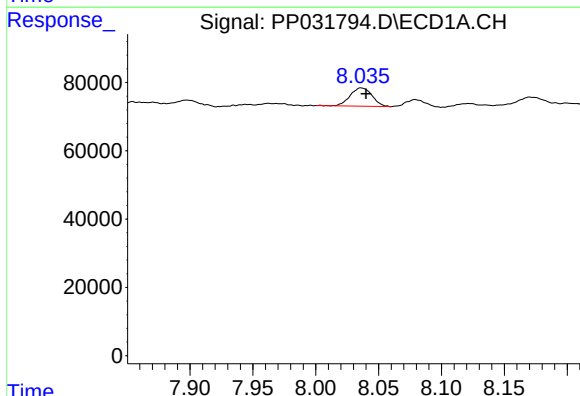


#32 AR-1260-2

R.T.: 8.036 min
Delta R.T.: -0.004 min
Response: 65131
Conc: 31.70 ng/ml

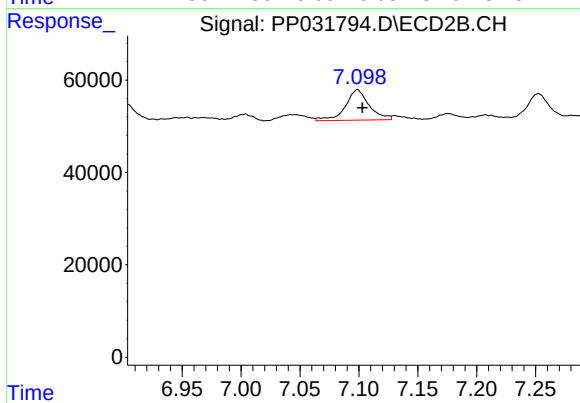

#32 AR-1260-2

R.T.: 7.099 min
Delta R.T.: -0.004 min
Response: 92856
Conc: 38.13 ng/ml

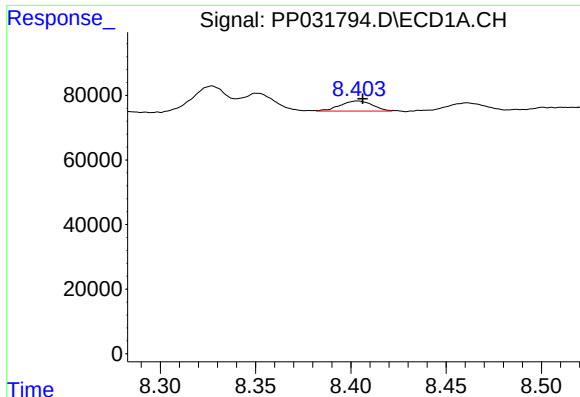


#33 AR-1260-3

R.T.: 8.403 min
Delta R.T.: -0.003 min
Response: 37000
Conc: 22.69 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPE


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:14 AM

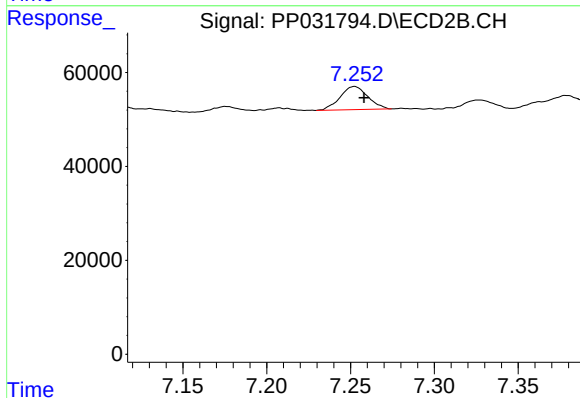


#33 AR-1260-3

R.T.: 7.253 min
Delta R.T.: -0.005 min
Response: 56971
Conc: 24.95 ng/ml

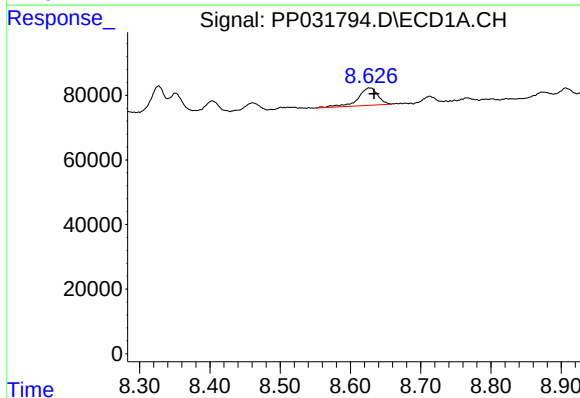


#34 AR-1260-4

R.T.: 8.627 min
Delta R.T.: -0.007 min
Response: 105407
Conc: 57.24 ng/ml

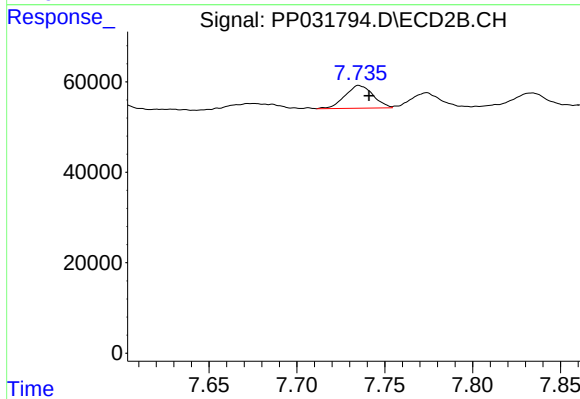

#34 AR-1260-4

R.T.: 7.735 min
Delta R.T.: -0.006 min
Response: 56154
Conc: 29.55 ng/ml

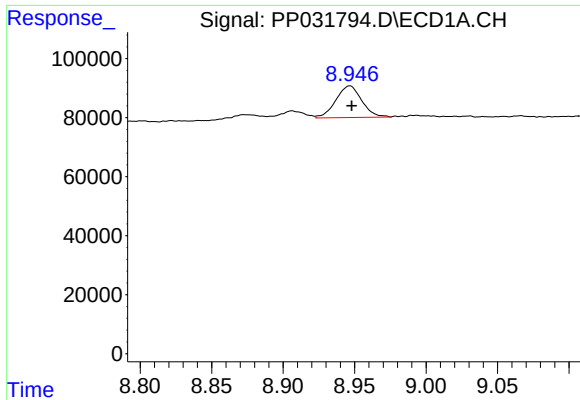


#35 AR-1260-5

R.T.: 8.947 min
Delta R.T.: -0.001 min
Response: 135110
Conc: 36.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
SK-12-1-SPE

Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:14 AM

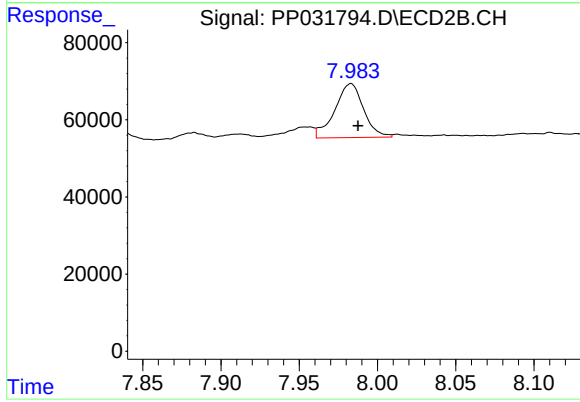

#35 AR-1260-5

R.T.: 7.983 min
Delta R.T.: -0.005 min
Response: 178827
Conc: 39.41 ng/ml