

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
 Data File : PP031801.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2020 17:04
 Operator : DD\AJ
 Sample : L4905-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-11-12-13-14

Manual Integrations
 APPROVED

Ankita
 12/3/2020 10:24:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 18:21:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.788	4.061	922720	1113562	19.055m	23.239
2) SA Decachlor...	10.658	9.360	393417	384885	11.583	10.395m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120220\
Data File : PP031801.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2020 17:04
Operator : DD\AJ
Sample : L4905-08
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-11-12-13-14


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 18:21:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

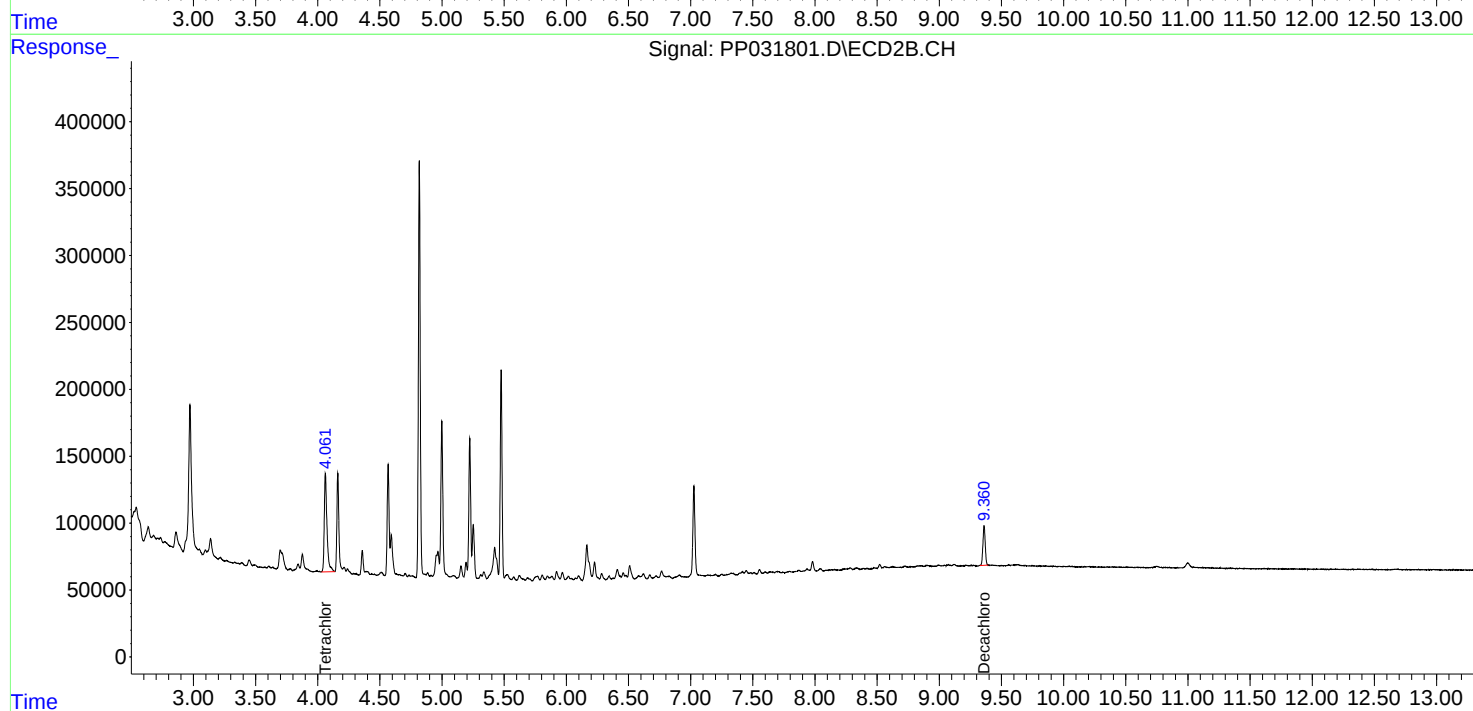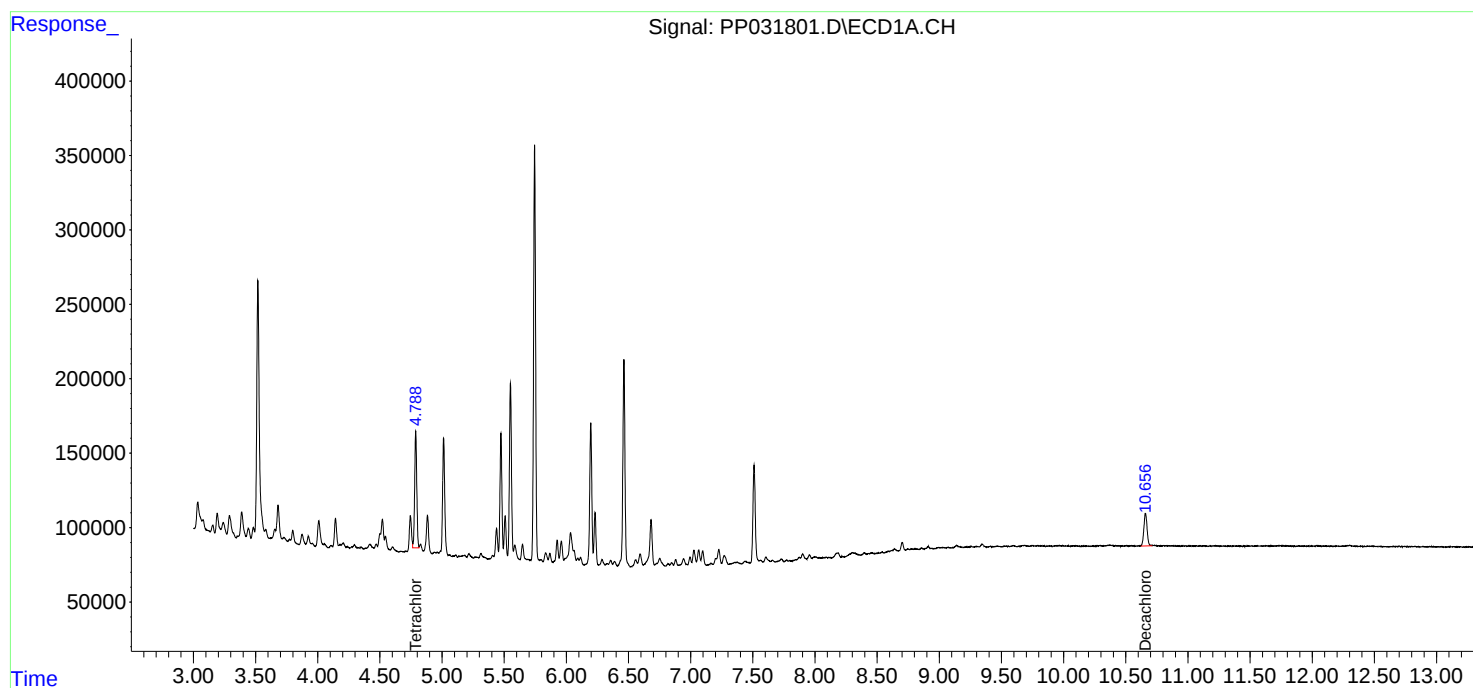

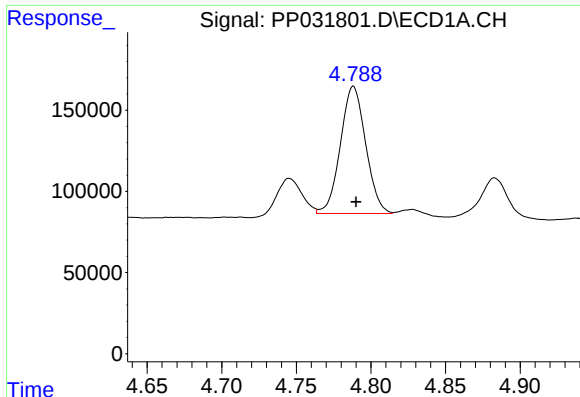


#1 Tetrachloro-m-xylene

R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 922720
Conc: 19.06 ng/ml m

Instrument :
ECD_P
ClientSampleId :
COMP-11-12-13-14


Manual Integrations
APPROVED

Ankita
12/3/2020 10:24:17 AM

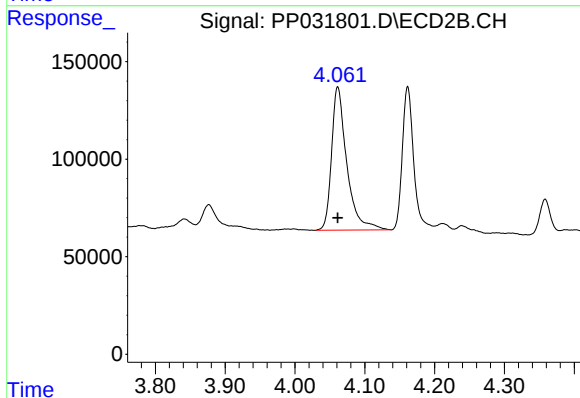


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1113562
Conc: 23.24 ng/ml

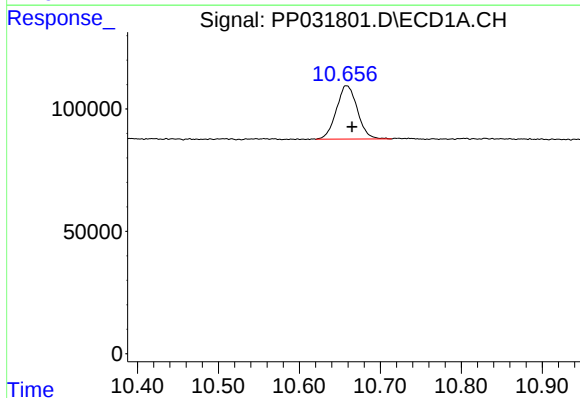

#2 Decachlorobiphenyl

R.T.: 10.658 min
Delta R.T.: -0.007 min
Response: 393417
Conc: 11.58 ng/ml

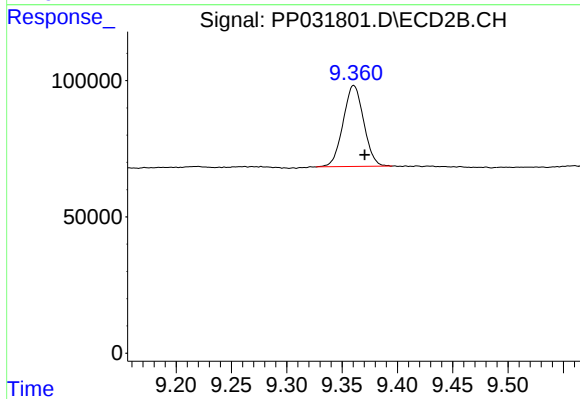

#2 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: -0.010 min
Response: 384885
Conc: 10.39 ng/ml m