

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120221\
 Data File : PP041589.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 18:09
 Operator : AJ\MA
 Sample : M4068-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 22:55:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.749	3.753	516621	727179	22.911	23.939
2) SA Decachlor...	10.646	9.011	526082	367550	24.432	23.782
Target Compounds						
36) L8 AR-1262-1	8.376	7.113	53979	36227	42.509	48.469
37) L8 AR-1262-2	8.921	7.667	100150	105194	44.327	49.859
38) L8 AR-1262-3	9.217	7.951	42757	42625	39.394	47.831m
39) L8 AR-1262-4	9.305	8.016	25354	79172	37.044m	49.298 #
40) L8 AR-1262-5	9.938	8.516	39497	33954	44.145m	46.770



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120221\
Data File : PP041589.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 18:09
Operator : AJ\MA
Sample : M4068-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 22:55:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

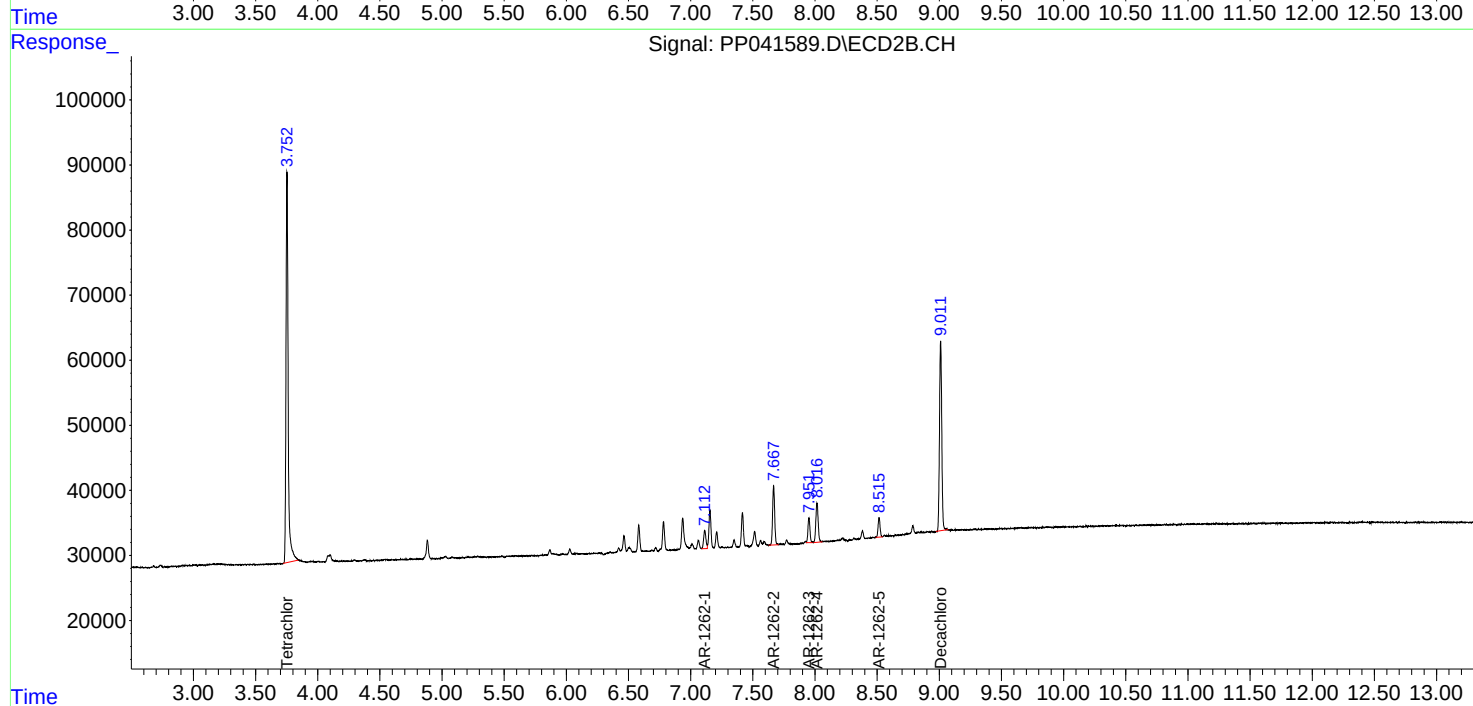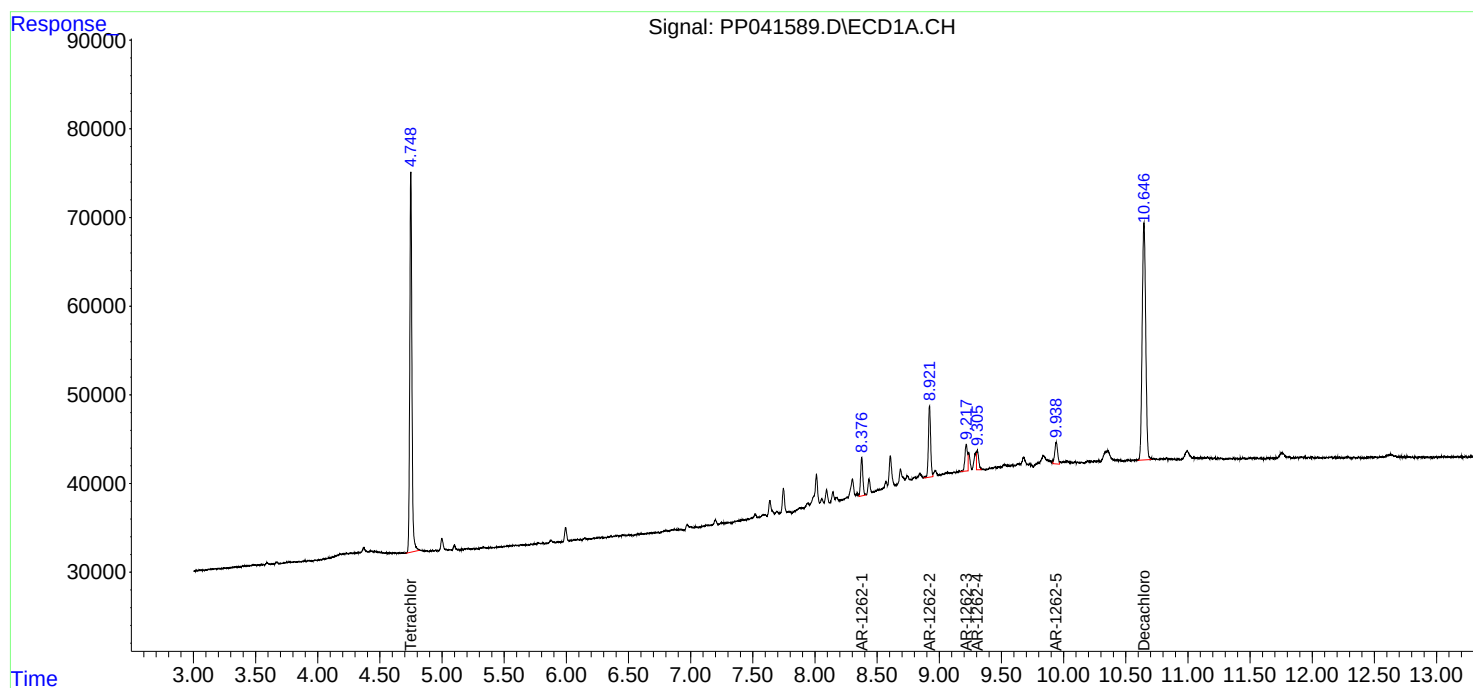


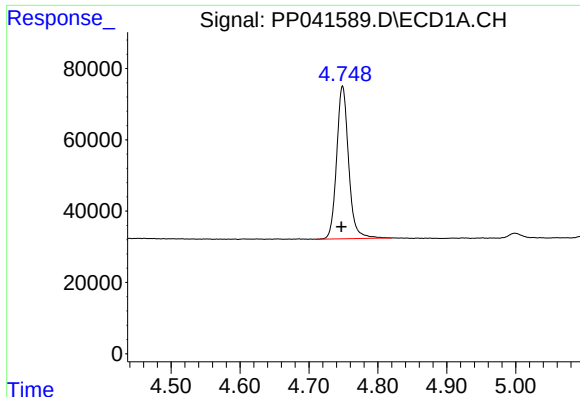

#1 Tetrachloro-m-xylene


R.T.: 4.749 min
Delta R.T.: 0.002 min
Response: 516621
Conc: 22.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

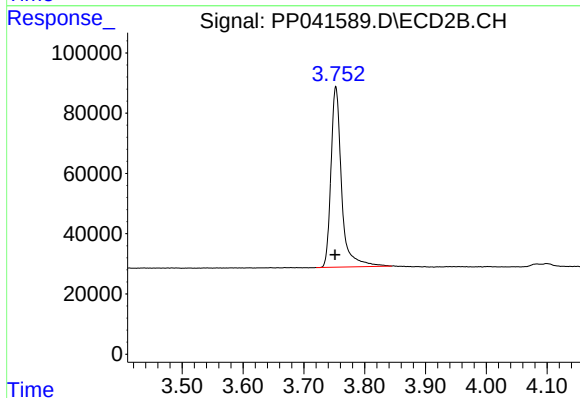


#1 Tetrachloro-m-xylene

R.T.: 3.753 min
Delta R.T.: 0.001 min
Response: 727179
Conc: 23.94 ng/ml

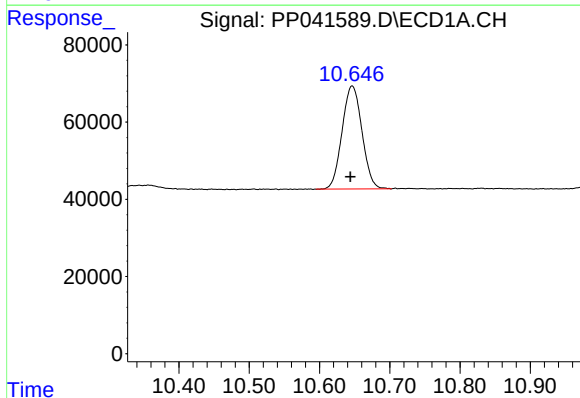


#2 Decachlorobiphenyl

R.T.: 10.646 min
Delta R.T.: 0.002 min
Response: 526082
Conc: 24.43 ng/ml

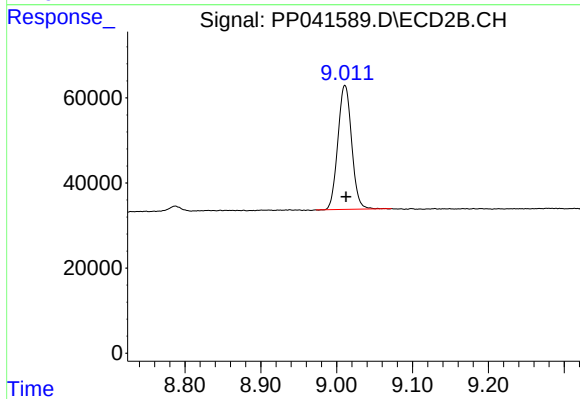

#2 Decachlorobiphenyl


R.T.: 9.011 min
Delta R.T.: -0.001 min
Response: 367550
Conc: 23.78 ng/ml

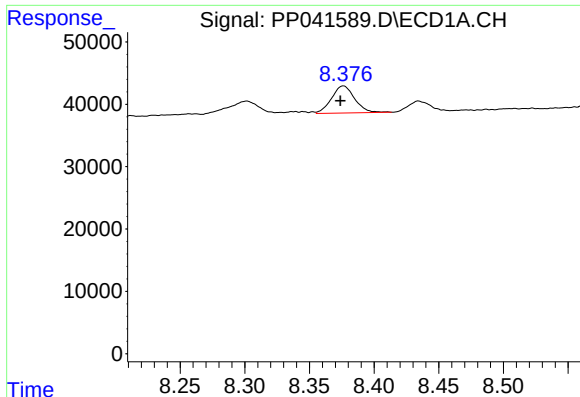

#36 AR-1262-1


R.T.: 8.376 min
Delta R.T.: 0.002 min
Response: 53979
Conc: 42.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

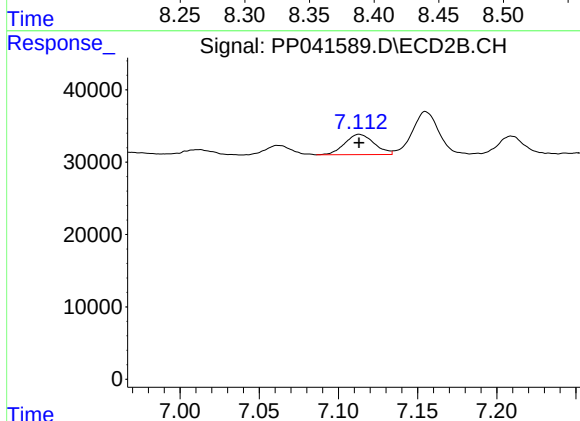


#36 AR-1262-1

R.T.: 7.113 min
Delta R.T.: 0.000 min
Response: 36227
Conc: 48.47 ng/ml

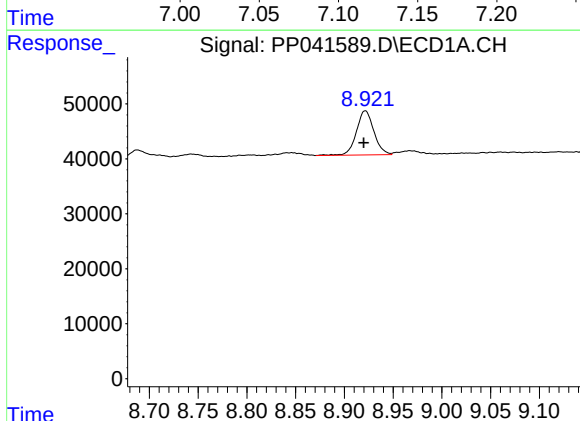


#37 AR-1262-2

R.T.: 8.921 min
Delta R.T.: 0.002 min
Response: 100150
Conc: 44.33 ng/ml

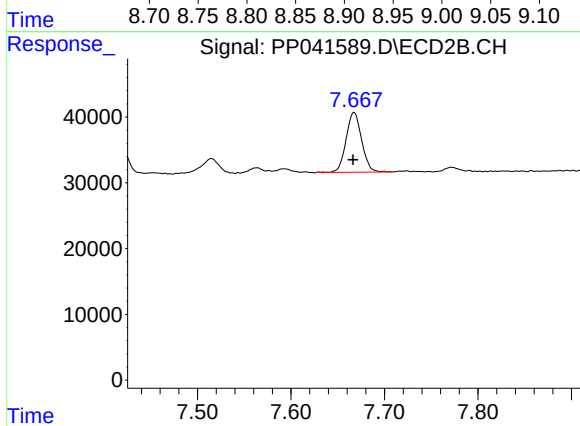

#37 AR-1262-2


R.T.: 7.667 min
Delta R.T.: 0.001 min
Response: 105194
Conc: 49.86 ng/ml

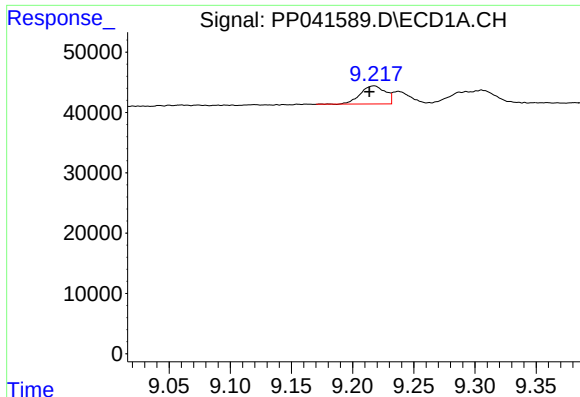

#38 AR-1262-3


R.T.: 9.217 min
Delta R.T.: 0.004 min
Response: 42757
Conc: 39.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

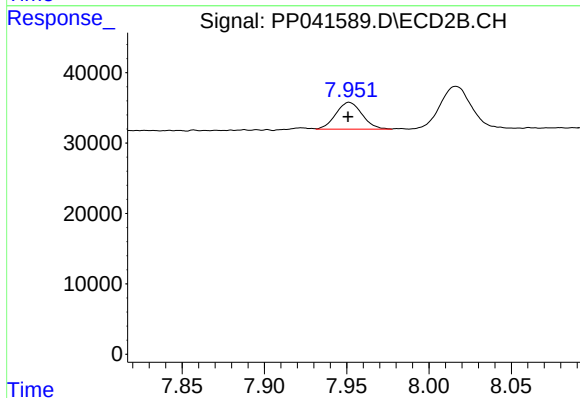


#38 AR-1262-3

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 42625
Conc: 47.83 ng/ml m

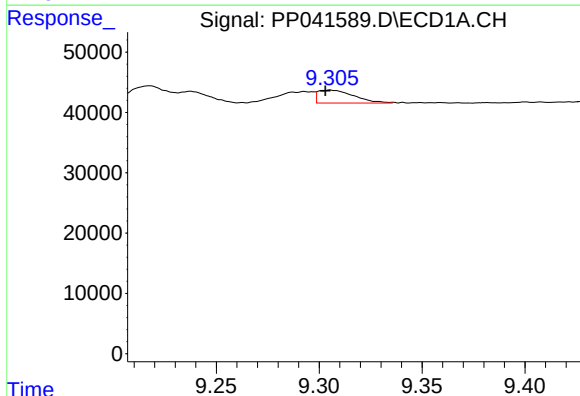


#39 AR-1262-4

R.T.: 9.305 min
Delta R.T.: 0.002 min
Response: 25354
Conc: 37.04 ng/ml m

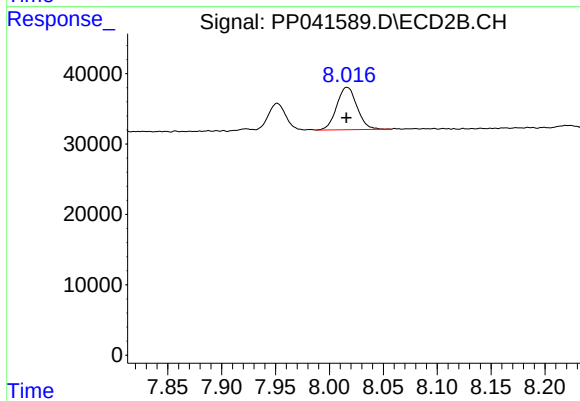

#39 AR-1262-4


R.T.: 8.016 min
Delta R.T.: 0.000 min
Response: 79172
Conc: 49.30 ng/ml

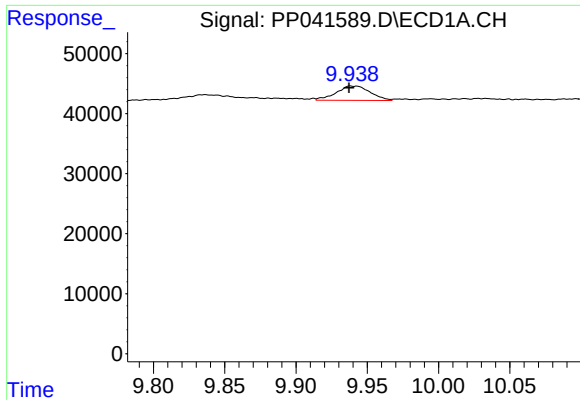

#40 AR-1262-5

R.T.: 9.938 min
Delta R.T.: 0.000 min
Response: 39497
Conc: 44.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2021

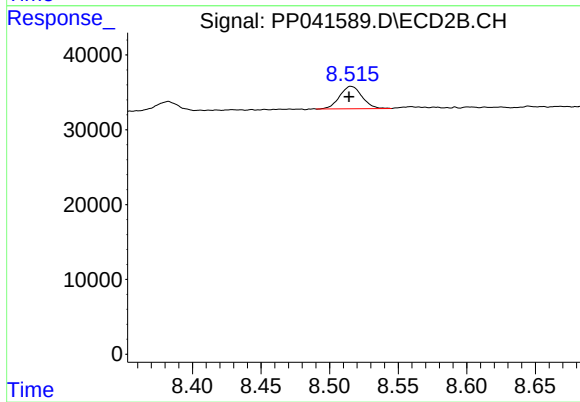

#40 AR-1262-5

R.T.: 8.516 min
Delta R.T.: 0.001 min
Response: 33954
Conc: 46.77 ng/ml