

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120225\
 Data File : PP076727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 17:53
 Operator : YP\AJ
 Sample : Q3530-07
 Misc : (Sig #1); LOD-MDL-1262-SOIL-25 PPB-QT4-2025 (Sig #2)
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 07:10:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.620	3.776	33213951	34853083	18.095	16.733
2) SA Decachlor...	10.374	8.771	28404099	30996343	18.953	17.566
Target Compounds						
36) L8 AR-1262-1	8.201	6.880	2603641	3284841	26.311	24.640
37) L8 AR-1262-2	8.524	7.137	4733819	3027003	27.450	25.242
38) L8 AR-1262-3	8.848	7.680	3236586	32604590	25.744	330.960 #
39) L8 AR-1262-4	8.935	7.719	2402525	23413965	24.215	134.189 #
40) L8 AR-1262-5	9.600	8.219	1913105	1769201	26.930	22.017



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120225\
Data File : PP076727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 17:53
Operator : YP\AJ
Sample : Q3530-07
Misc : (Sig #1); LOD-MDL-1262-SOIL-25 PPB-QT4-2025 (Sig #2)
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 07:10:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

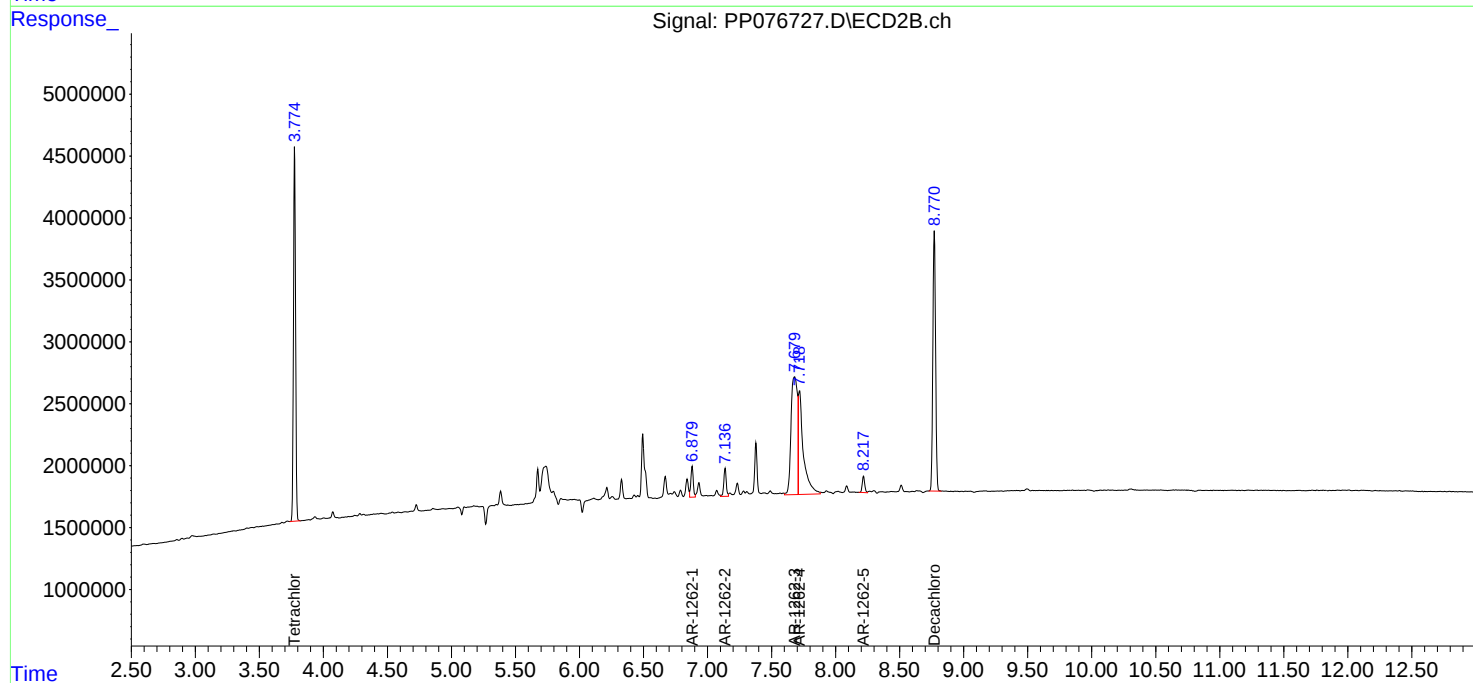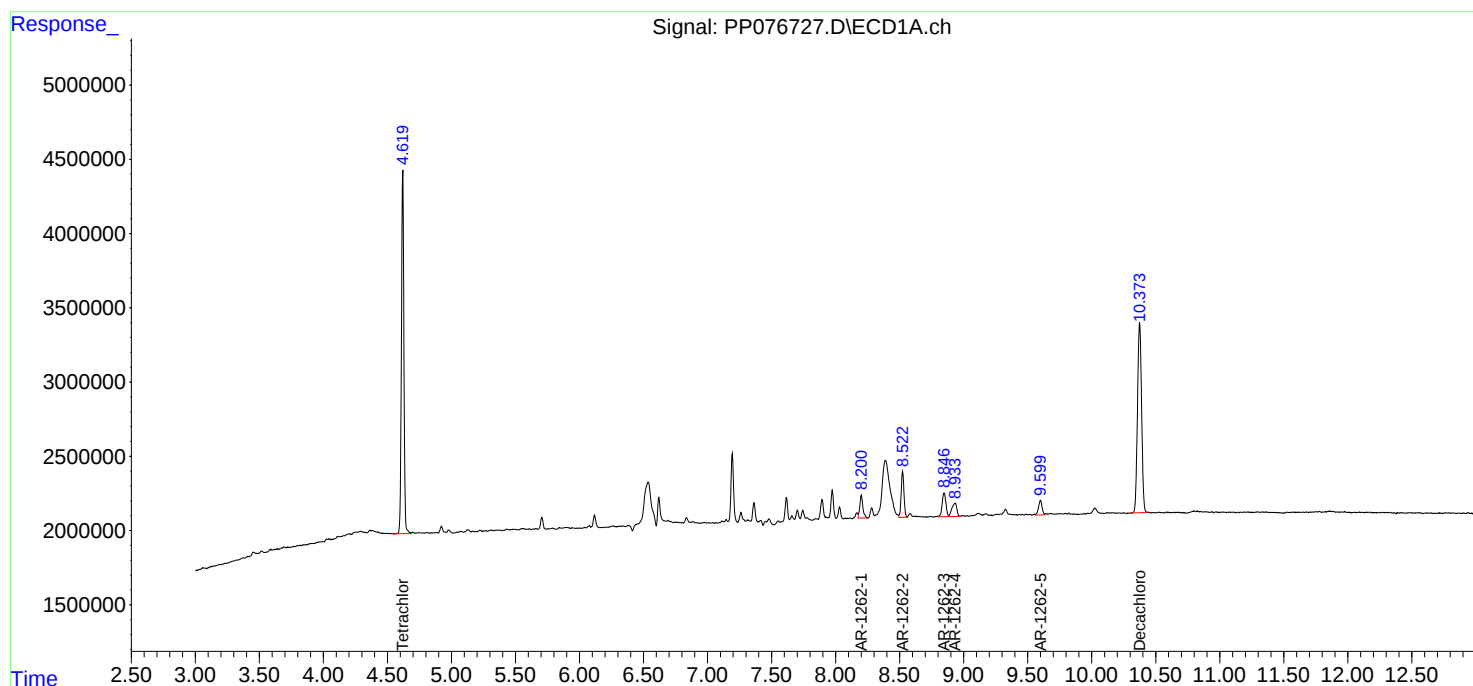


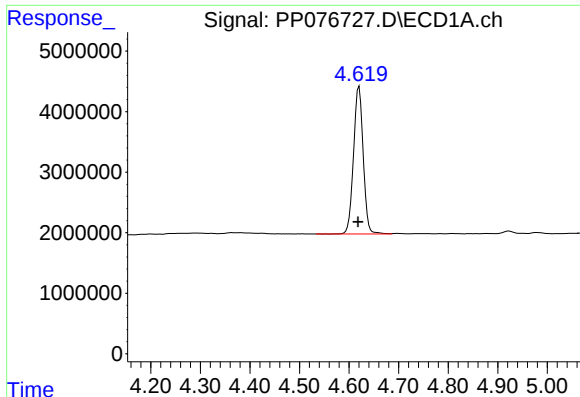

#1 Tetrachloro-m-xylene


R.T.: 4.620 min
Delta R.T.: 0.002 min
Response: 33213951
Conc: 18.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

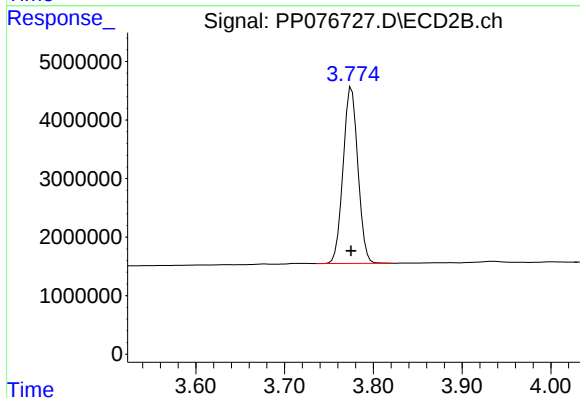


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 34853083
Conc: 16.73 ng/ml

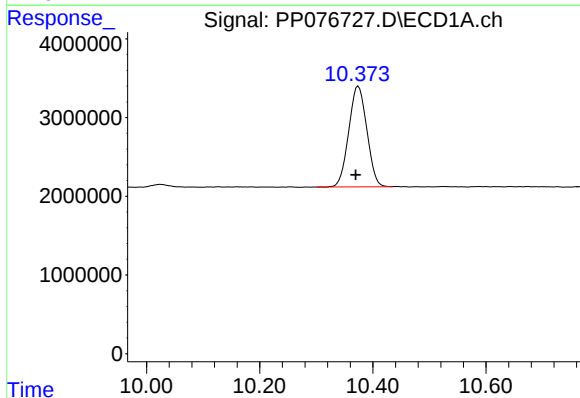


#2 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: 0.005 min
Response: 28404099
Conc: 18.95 ng/ml

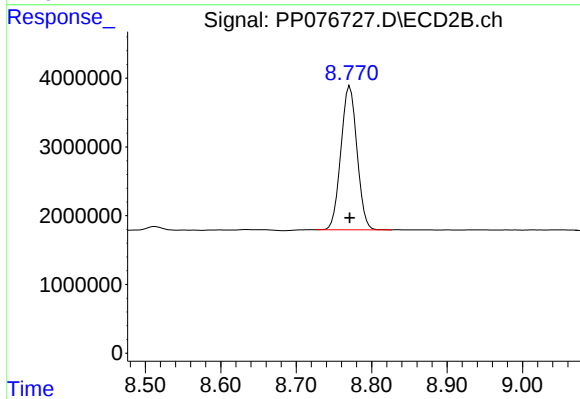

#2 Decachlorobiphenyl


R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 30996343
Conc: 17.57 ng/ml

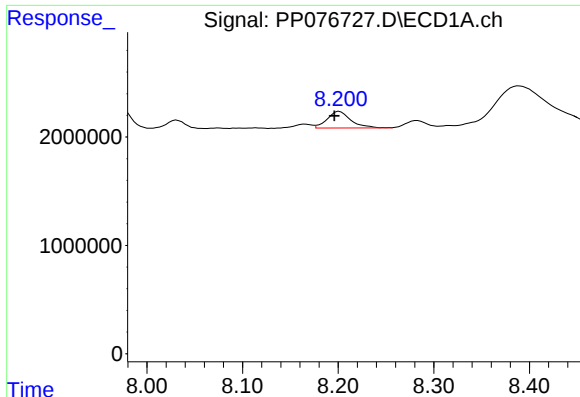

#36 AR-1262-1


R.T.: 8.201 min
Delta R.T.: 0.005 min
Response: 2603641
Conc: 26.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

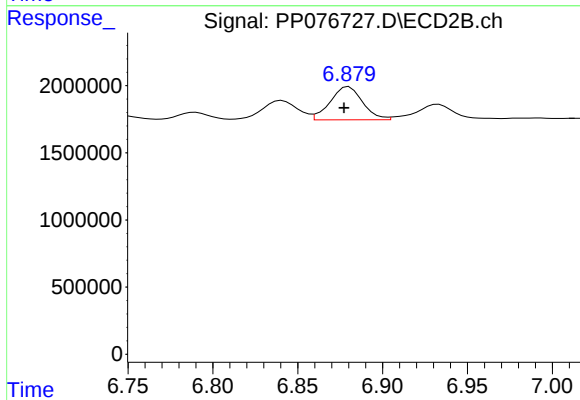


#36 AR-1262-1

R.T.: 6.880 min
Delta R.T.: 0.003 min
Response: 3284841
Conc: 24.64 ng/ml

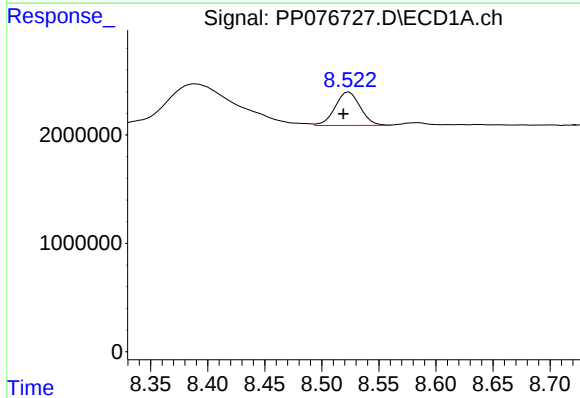


#37 AR-1262-2

R.T.: 8.524 min
Delta R.T.: 0.005 min
Response: 4733819
Conc: 27.45 ng/ml

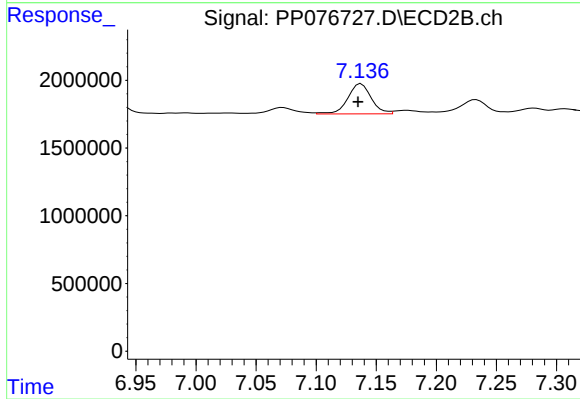

#37 AR-1262-2


R.T.: 7.137 min
Delta R.T.: 0.003 min
Response: 3027003
Conc: 25.24 ng/ml

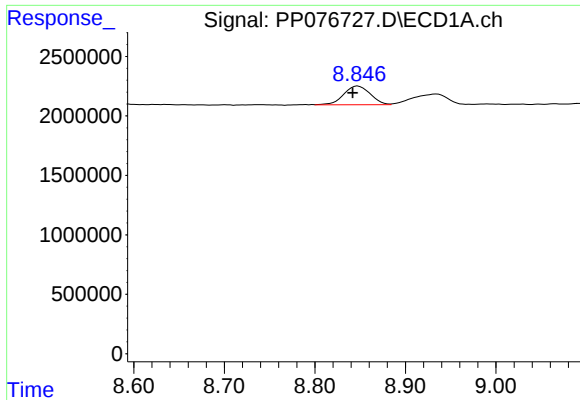

#38 AR-1262-3


R.T.: 8.848 min
Delta R.T.: 0.006 min
Response: 3236586
Conc: 25.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

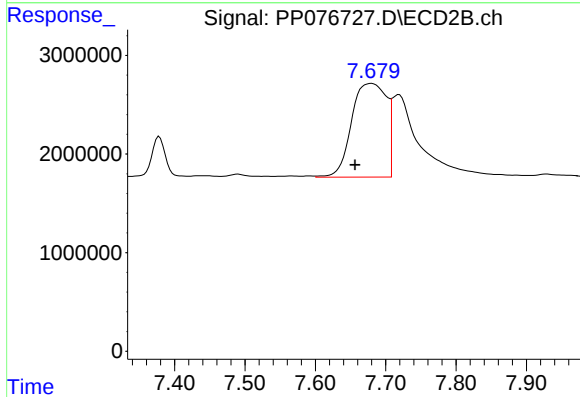


#38 AR-1262-3

R.T.: 7.680 min
Delta R.T.: 0.023 min
Response: 32604590
Conc: 330.96 ng/ml

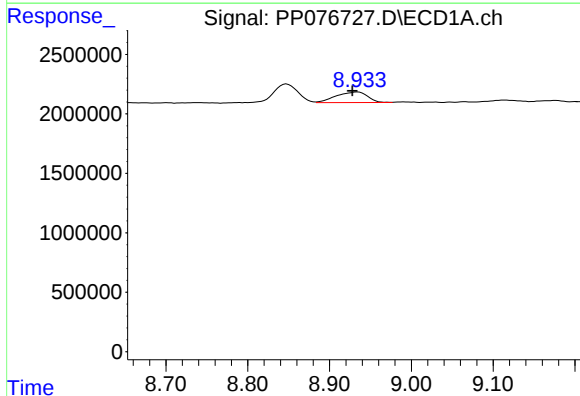


#39 AR-1262-4

R.T.: 8.935 min
Delta R.T.: 0.007 min
Response: 2402525
Conc: 24.21 ng/ml

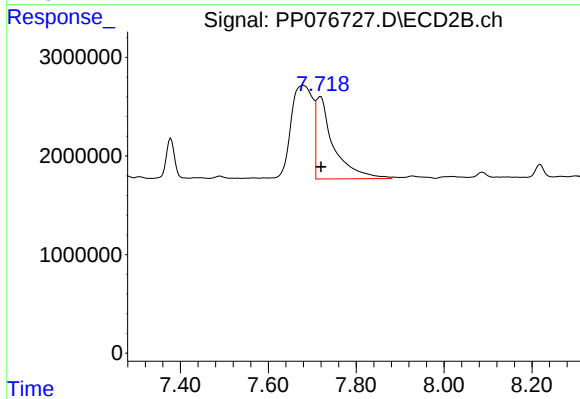

#39 AR-1262-4


R.T.: 7.719 min
Delta R.T.: 0.000 min
Response: 23413965
Conc: 134.19 ng/ml

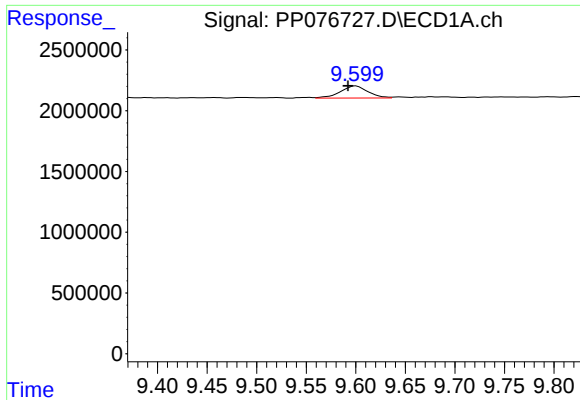

#40 AR-1262-5

R.T.: 9.600 min
Delta R.T.: 0.008 min
Response: 1913105
Conc: 26.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

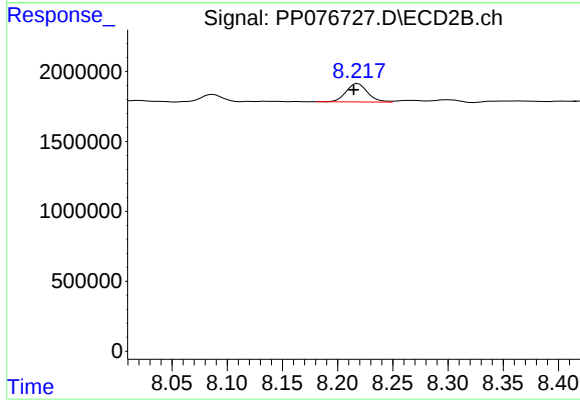

#40 AR-1262-5

R.T.: 8.219 min
Delta R.T.: 0.004 min
Response: 1769201
Conc: 22.02 ng/ml