

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120225\
 Data File : PP076728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 18:09
 Operator : YP\AJ
 Sample : Q3530-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 07:11:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.620	3.775	46549070	50033479	25.360	24.021
2) SA Decachlor...	10.375	8.771	41314700	45815195	27.567	25.965
Target Compounds						
41) L9 AR-1268-1	8.843	7.662	5277538	19192267	24.556	68.218 #
42) L9 AR-1268-2	8.937	7.724	4793255	15715382	23.819	61.744 #
43) L9 AR-1268-3	9.174	7.929	3823633	5385698	23.013	26.091
44) L9 AR-1268-4	9.598	8.218	2070675	1935147	24.858	20.605
45) L9 AR-1268-5	10.025	8.513	12580796	14009990	24.946	22.010



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120225\
Data File : PP076728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 18:09
Operator : YP\AJ
Sample : Q3530-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 07:11:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

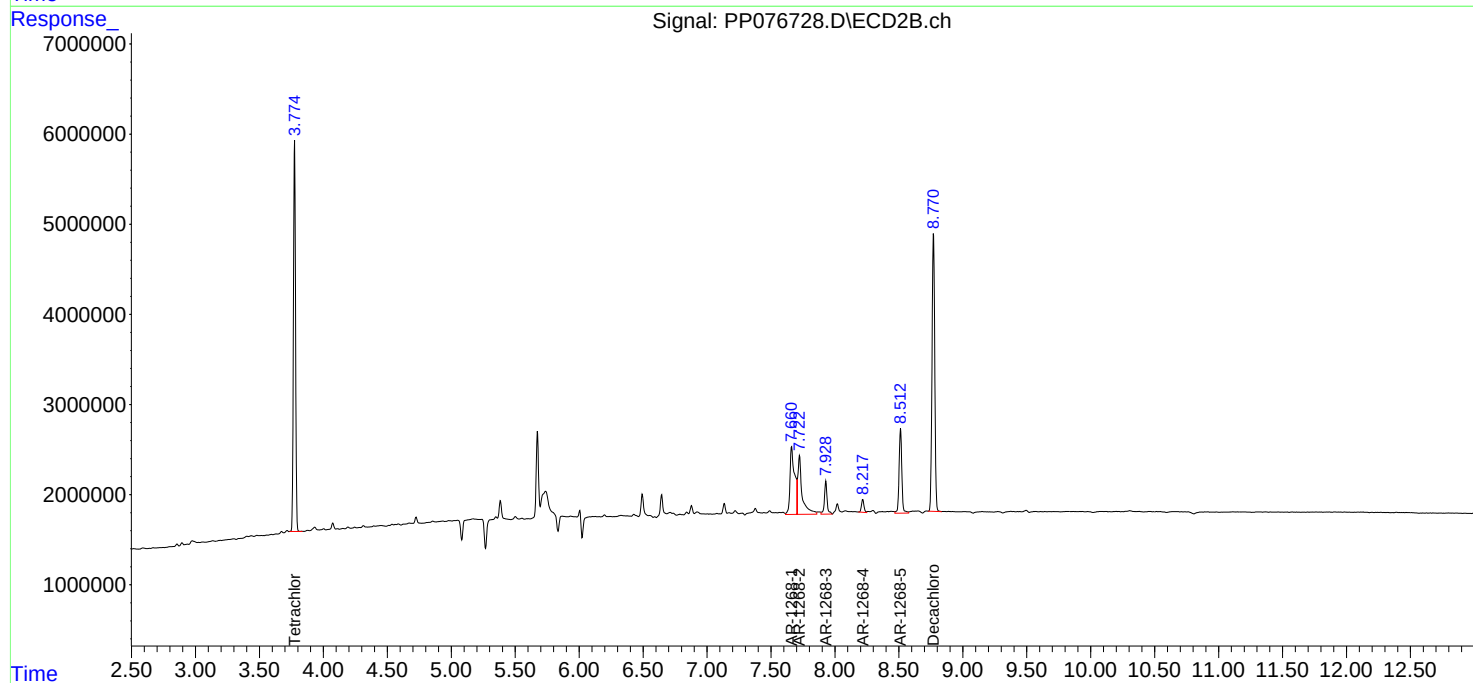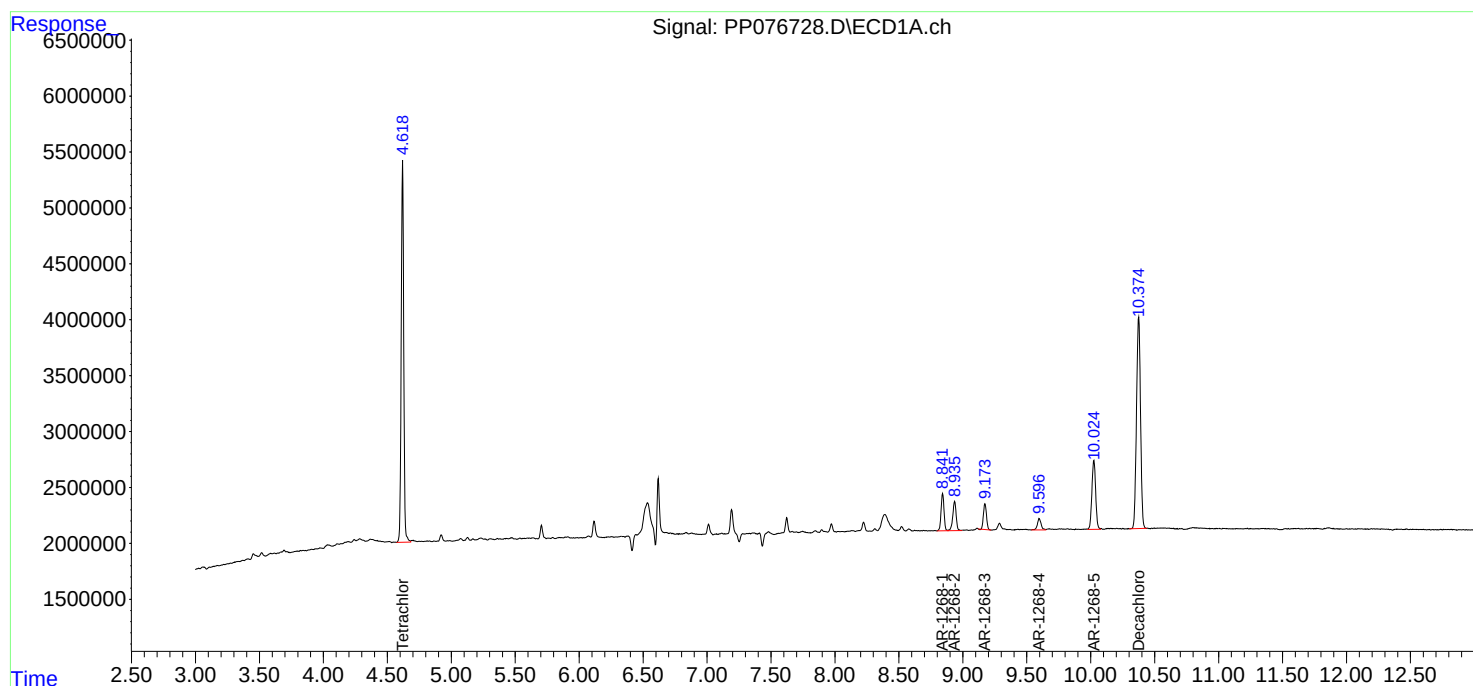


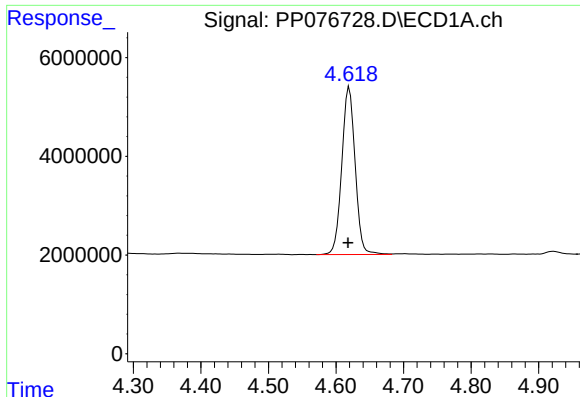

#1 Tetrachloro-m-xylene


R.T.: 4.620 min
Delta R.T.: 0.002 min
Response: 46549070
Conc: 25.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

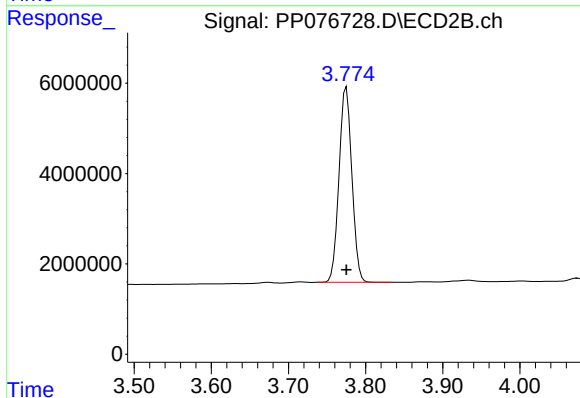


#1 Tetrachloro-m-xylene

R.T.: 3.775 min
Delta R.T.: 0.000 min
Response: 50033479
Conc: 24.02 ng/ml

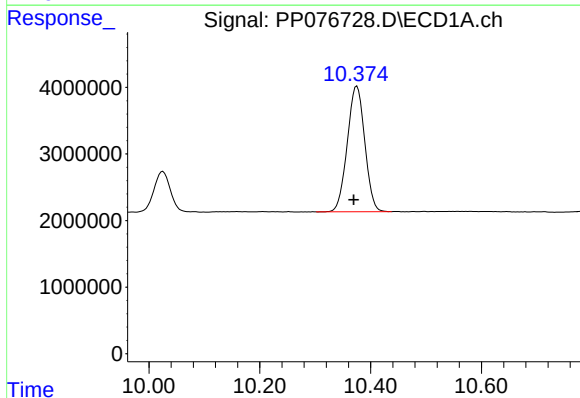


#2 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.006 min
Response: 41314700
Conc: 27.57 ng/ml

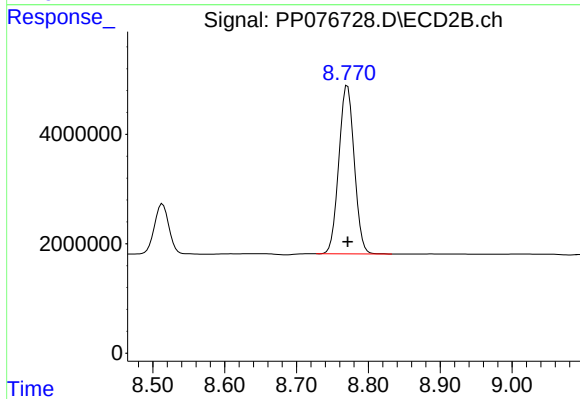

#2 Decachlorobiphenyl


R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 45815195
Conc: 25.96 ng/ml

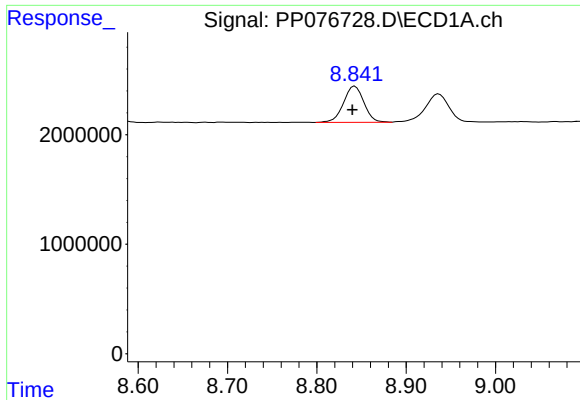

#41 AR-1268-1


R.T.: 8.843 min
Delta R.T.: 0.003 min
Response: 5277538
Conc: 24.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

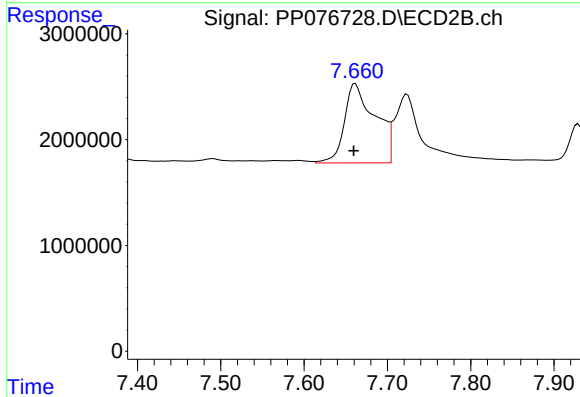


#41 AR-1268-1

R.T.: 7.662 min
Delta R.T.: 0.002 min
Response: 19192267
Conc: 68.22 ng/ml

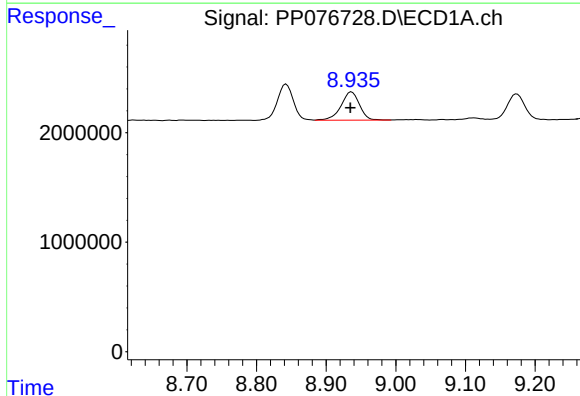


#42 AR-1268-2

R.T.: 8.937 min
Delta R.T.: 0.002 min
Response: 4793255
Conc: 23.82 ng/ml

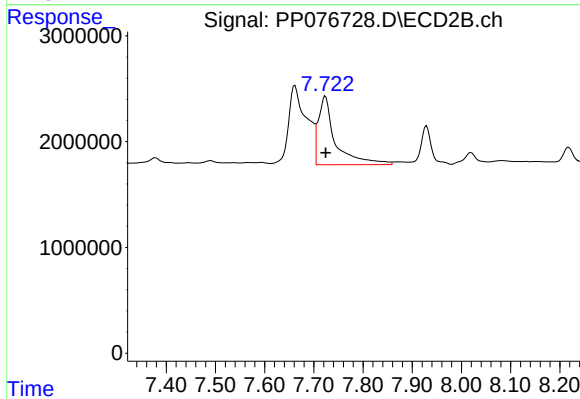

#42 AR-1268-2


R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 15715382
Conc: 61.74 ng/ml

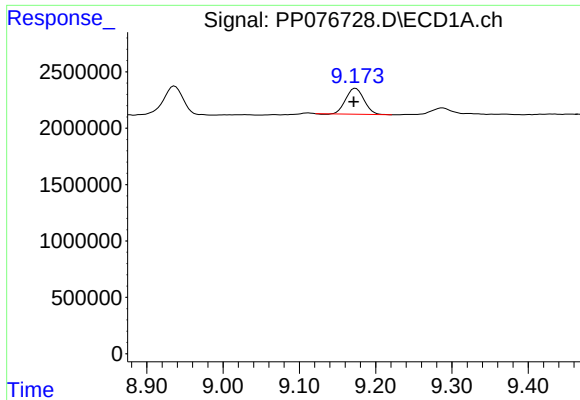

#43 AR-1268-3


R.T.: 9.174 min
Delta R.T.: 0.003 min
Response: 3823633
Conc: 23.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

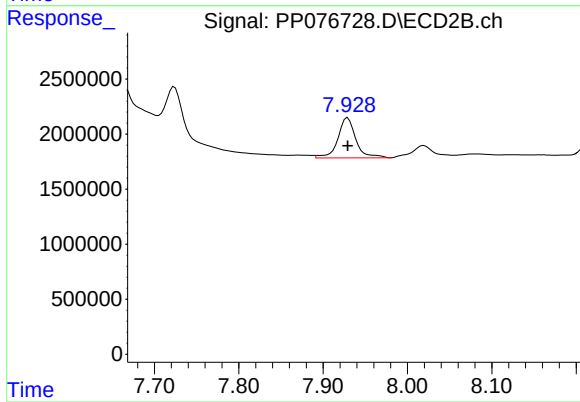


#43 AR-1268-3

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 5385698
Conc: 26.09 ng/ml

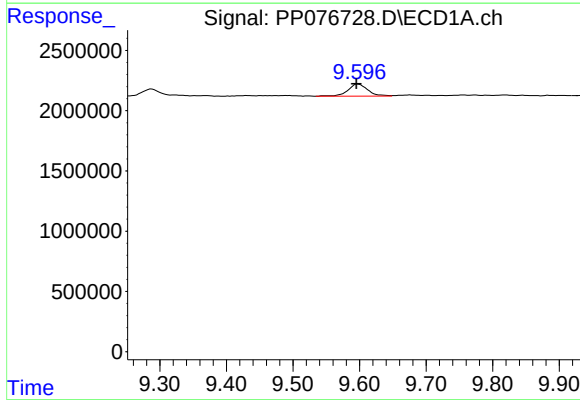


#44 AR-1268-4

R.T.: 9.598 min
Delta R.T.: 0.003 min
Response: 2070675
Conc: 24.86 ng/ml

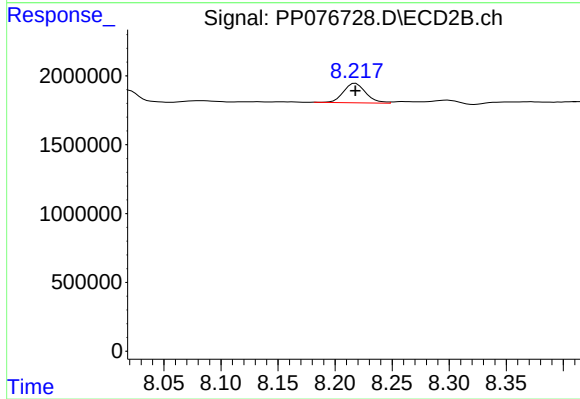

#44 AR-1268-4


R.T.: 8.218 min
Delta R.T.: 0.000 min
Response: 1935147
Conc: 20.60 ng/ml

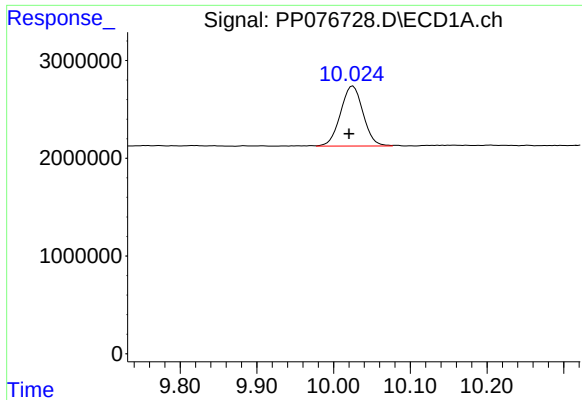

#45 AR-1268-5

R.T.: 10.025 min
Delta R.T.: 0.005 min
Response: 12580796
Conc: 24.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

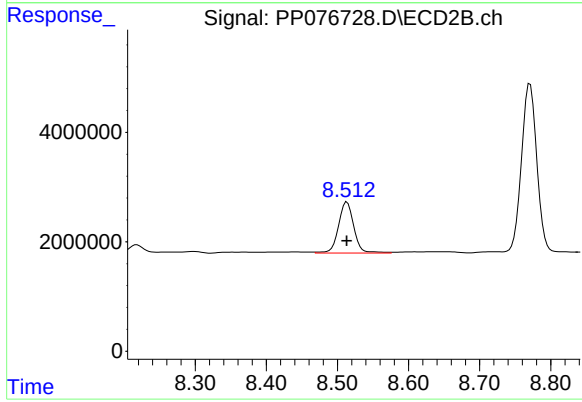

#45 AR-1268-5

R.T.: 8.513 min
Delta R.T.: 0.000 min
Response: 14009990
Conc: 22.01 ng/ml