

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
 Data File : PP031805.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2020 9:07
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 05:54:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.800	4.060	39747	27240	0.821	0.568 #
2)	SA Decachlor...	0.000	9.364	0	38854	N.D.	1.049 #
Target Compounds							
8)	L2 AR-1221-1	0.000	4.321	0	3697	N.D.	7.287 #
9)	L2 AR-1221-2	0.000	4.416	0	8614	N.D.	22.330 #
10)	L2 AR-1221-3	0.000	4.513	0	12458	N.D.	10.328 #
11)	L3 AR-1232-1	0.000	4.513	0	12458	N.D.	11.991 #
20)	L4 AR-1242-5	7.045f	0.000	127054	0	138.685	N.D. #
24)	L5 AR-1248-4	7.045f	0.000	127054	0	81.019	N.D. #
25)	L5 AR-1248-5	7.045f	0.000	127054	0	80.035	N.D. #
28)	L6 AR-1254-3	7.625f	0.000	47936	0	18.975	N.D. #
30)	L6 AR-1254-5	0.000	7.432	0	125060	N.D.	46.326 #
32)	L7 AR-1260-2	0.000	7.080f	0	119754	N.D.	49.175 #
35)	L7 AR-1260-5	0.000	7.983	0	133898	N.D.	29.506 #
37)	L8 AR-1262-2	0.000	7.983	0	133898	N.D.	27.566 #
38)	L8 AR-1262-3	0.000	8.259	0	5102	N.D.	2.594 #
41)	L9 AR-1268-1	0.000	8.259	0	5102	N.D.	0.922 #
43)	L9 AR-1268-3	0.000	8.573f	0	18358	N.D.	4.002 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
Data File : PP031805.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2020 9:07
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 05:54:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

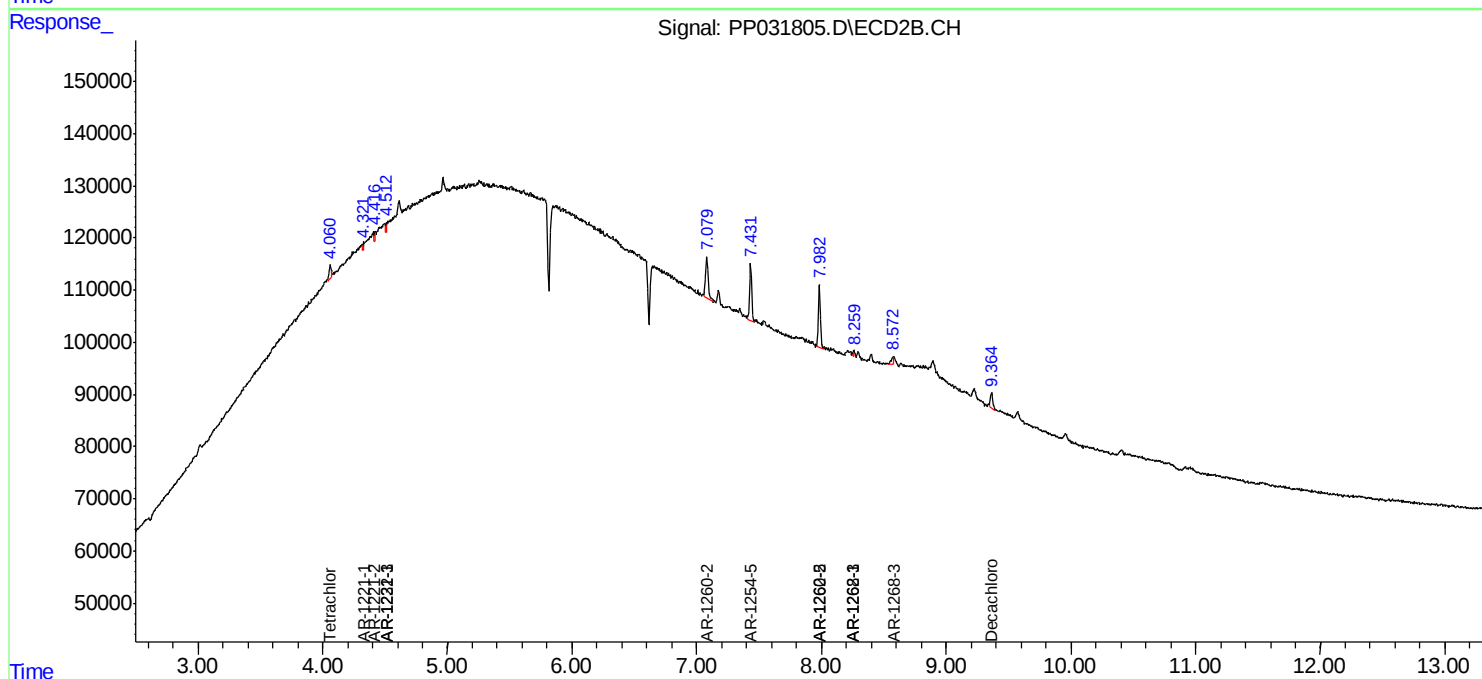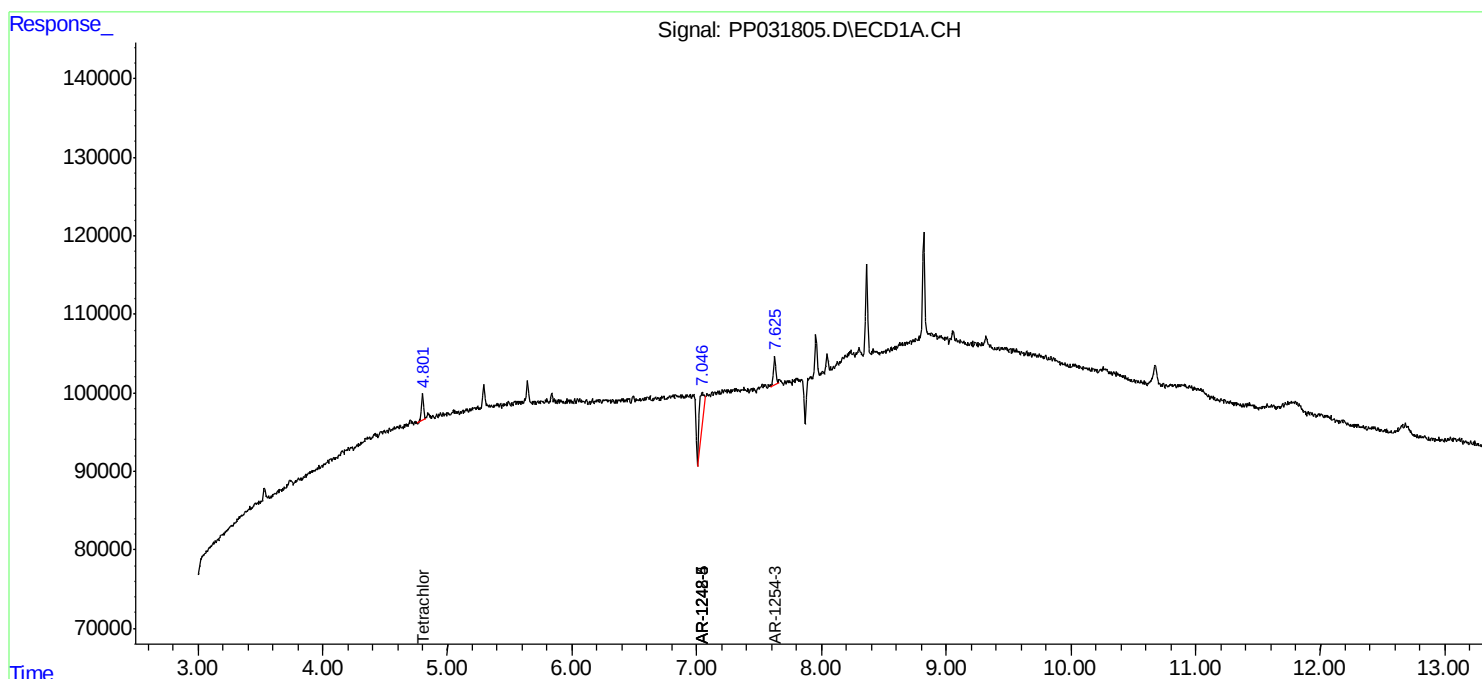


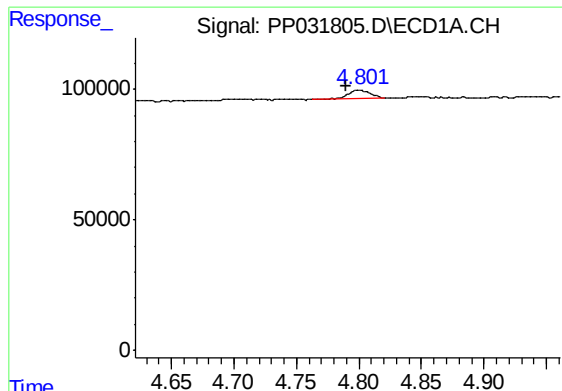

#1 Tetrachloro-m-xylene


R.T.: 4.800 min
Delta R.T.: 0.010 min
Response: 39747
Conc: 0.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

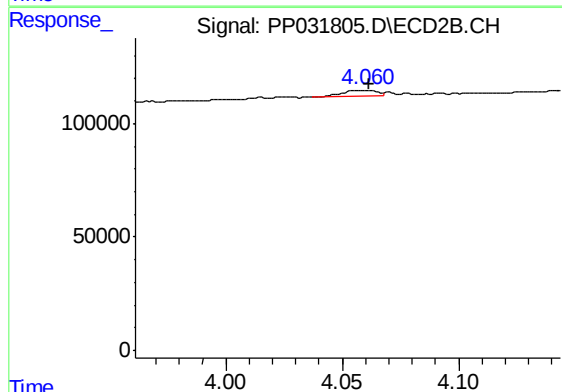


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.002 min
Response: 27240
Conc: 0.57 ng/ml

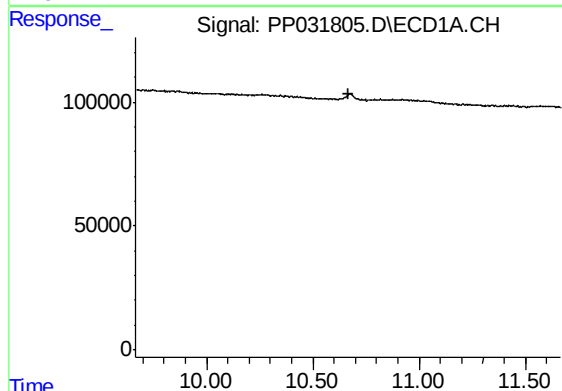


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.665 min
Response: 0
Conc: N.D.

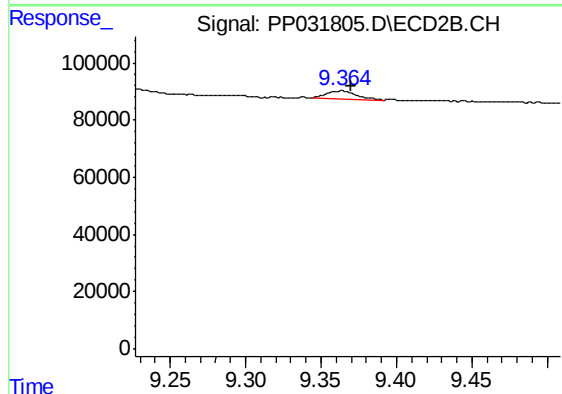

#2 Decachlorobiphenyl


R.T.: 9.364 min
Delta R.T.: -0.006 min
Response: 38854
Conc: 1.05 ng/ml

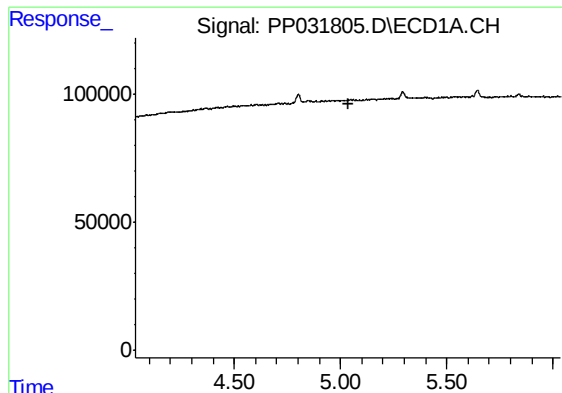

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 5.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

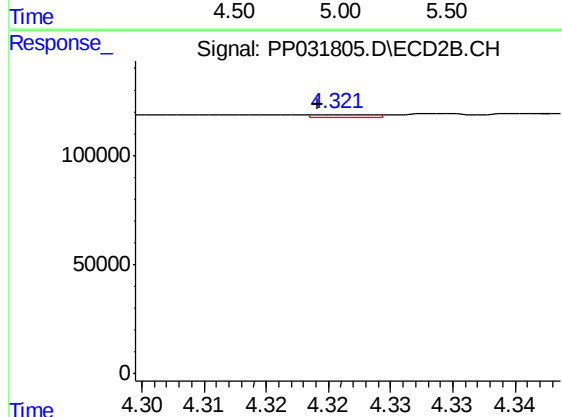


#8 AR-1221-1

R.T.: 4.321 min
Delta R.T.: 0.002 min
Response: 3697
Conc: 7.29 ng/ml

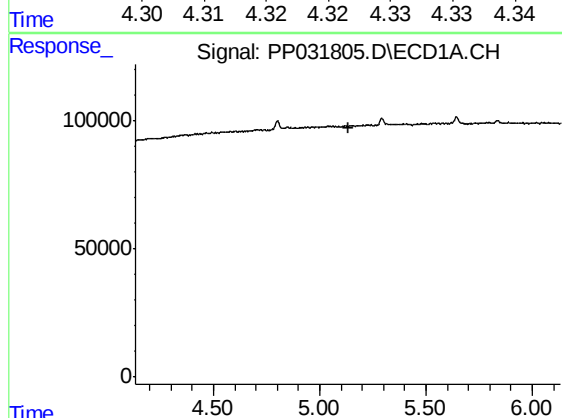


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

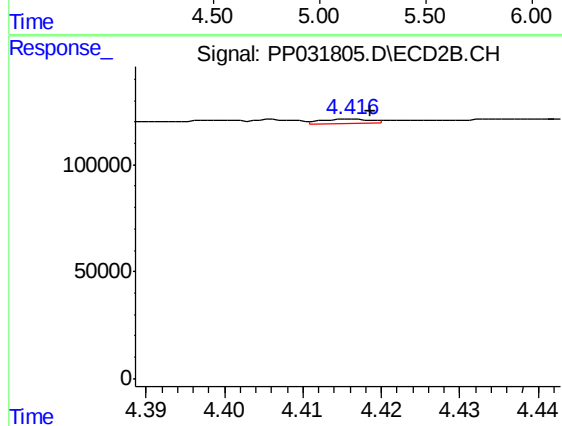

#9 AR-1221-2


R.T.: 4.416 min
Delta R.T.: -0.002 min
Response: 8614
Conc: 22.33 ng/ml

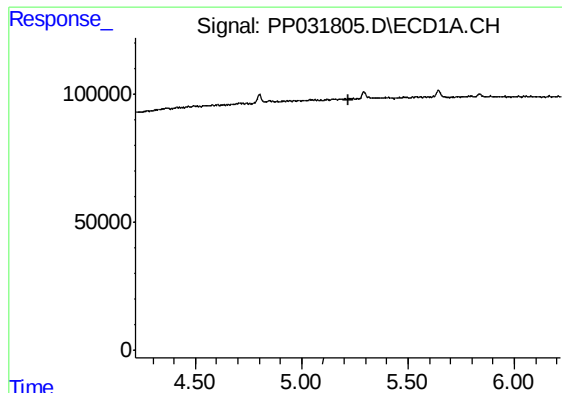

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

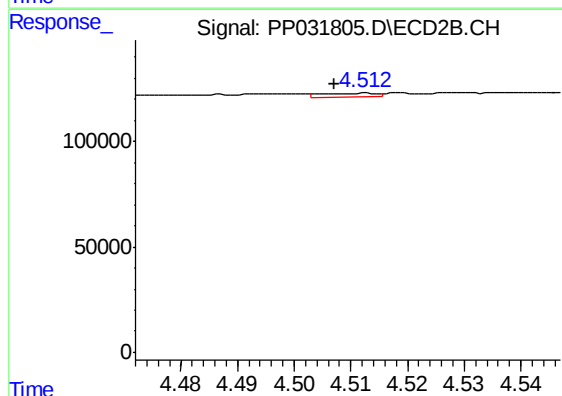


#10 AR-1221-3

R.T.: 4.513 min
Delta R.T.: 0.006 min
Response: 12458
Conc: 10.33 ng/ml

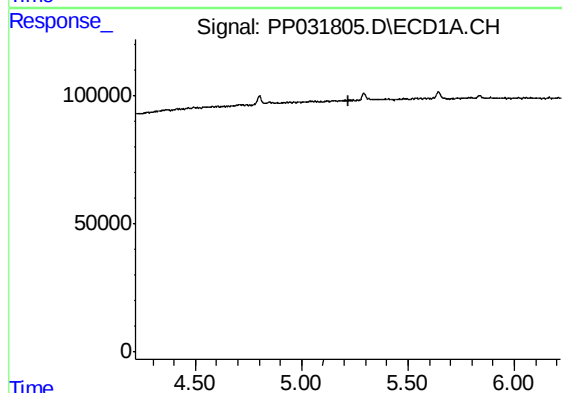


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.218 min
Response: 0
Conc: N.D.

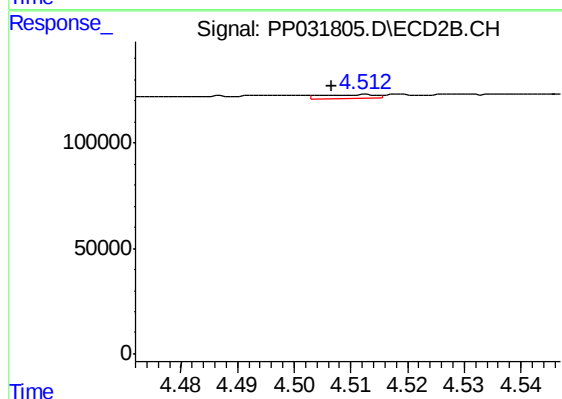

#11 AR-1232-1


R.T.: 4.513 min
Delta R.T.: 0.006 min
Response: 12458
Conc: 11.99 ng/ml

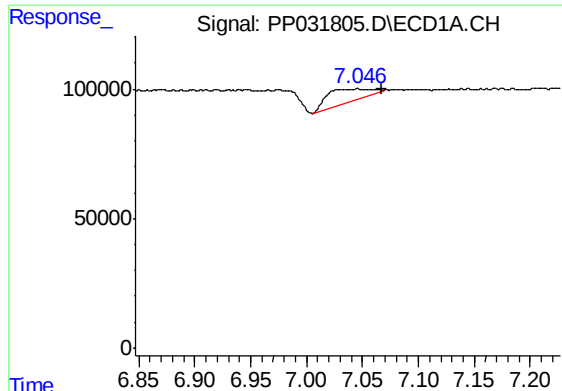

#20 AR-1242-5


R.T.: 7.045 min
Delta R.T.: -0.022 min
Response: 127054
Conc: 138.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

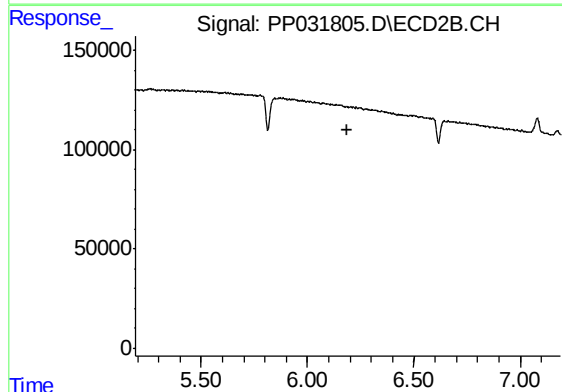


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.190 min
Response: 0
Conc: N.D.

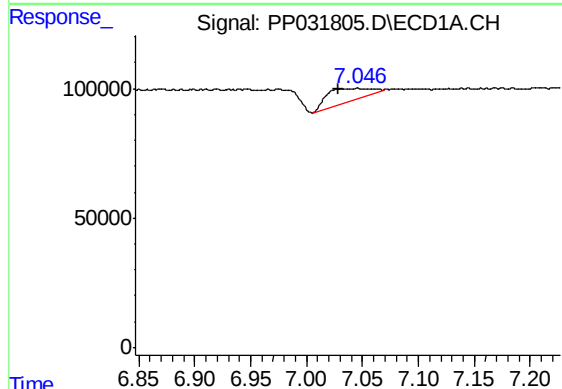


#24 AR-1248-4

R.T.: 7.045 min
Delta R.T.: 0.017 min
Response: 127054
Conc: 81.02 ng/ml

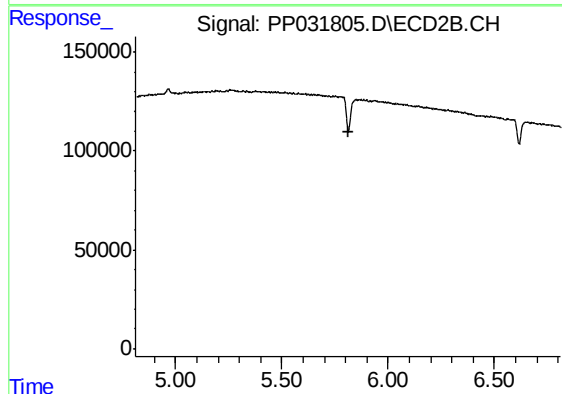

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.811 min
Response: 0
Conc: N.D.

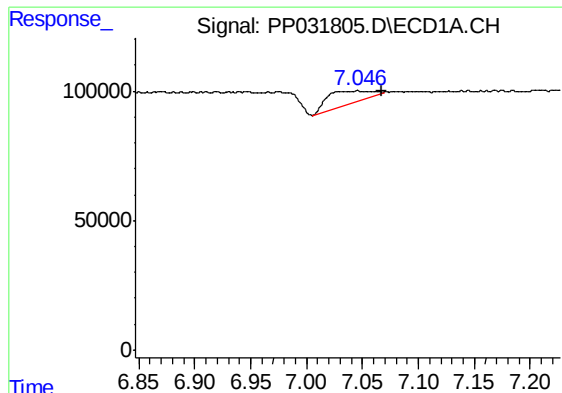

#25 AR-1248-5


R.T.: 7.045 min
Delta R.T.: -0.022 min
Response: 127054
Conc: 80.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

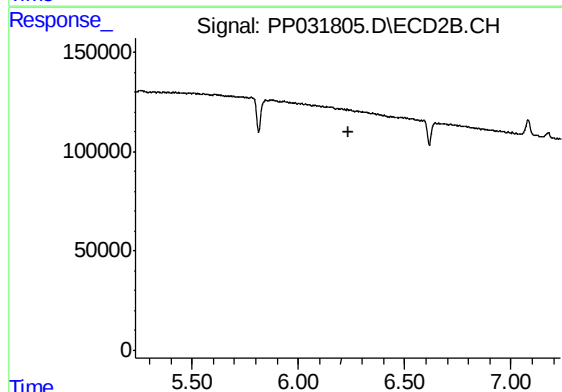


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

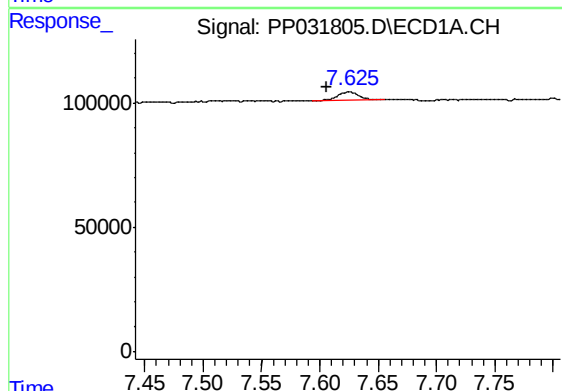


#28 AR-1254-3

R.T.: 7.625 min
Delta R.T.: 0.019 min
Response: 47936
Conc: 18.97 ng/ml

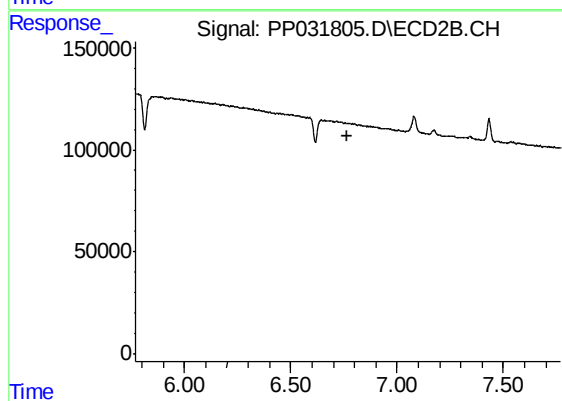

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

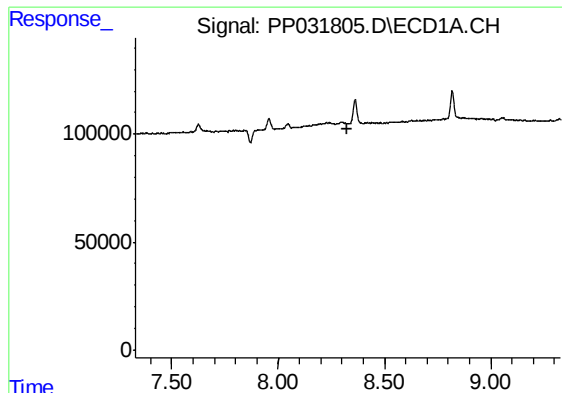

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 8.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

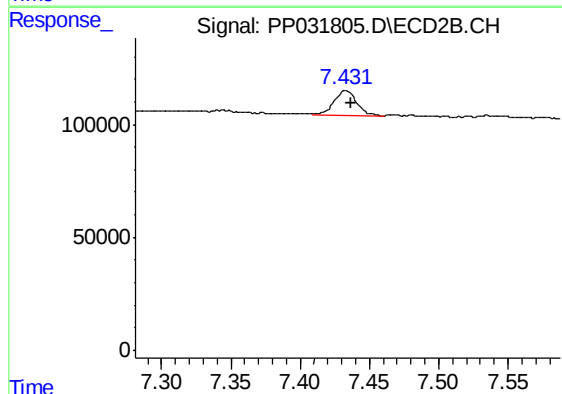


#30 AR-1254-5

R.T.: 7.432 min
Delta R.T.: -0.005 min
Response: 125060
Conc: 46.33 ng/ml

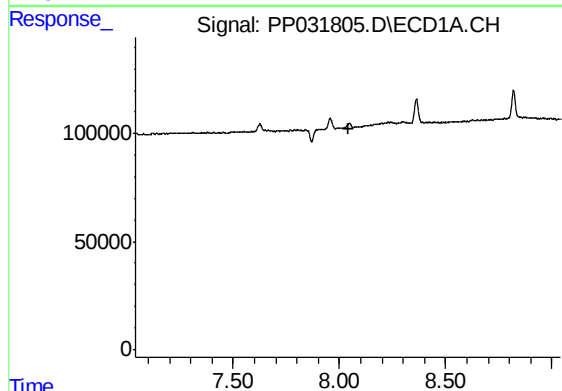


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

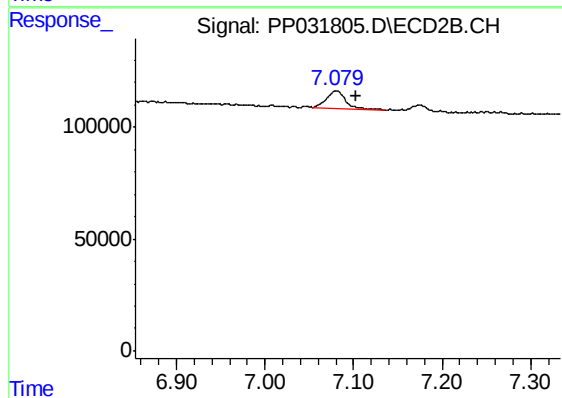

#32 AR-1260-2


R.T.: 7.080 min
Delta R.T.: -0.024 min
Response: 119754
Conc: 49.18 ng/ml

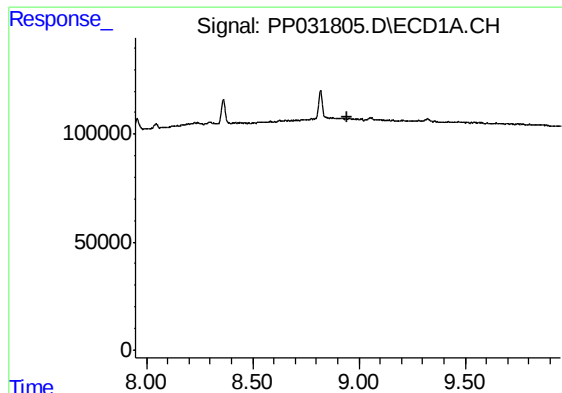

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

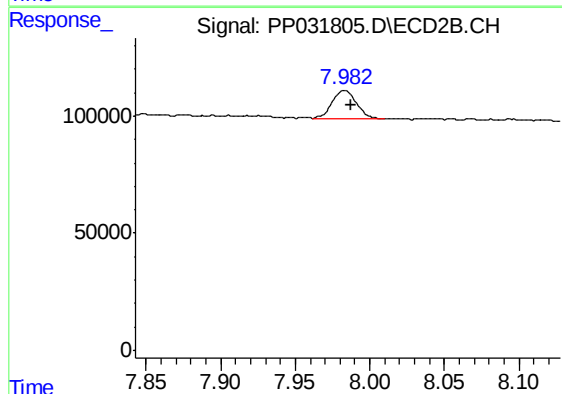


#35 AR-1260-5

R.T.: 7.983 min
Delta R.T.: -0.005 min
Response: 133898
Conc: 29.51 ng/ml

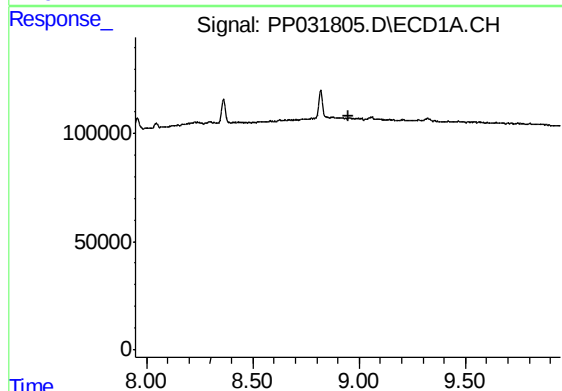


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

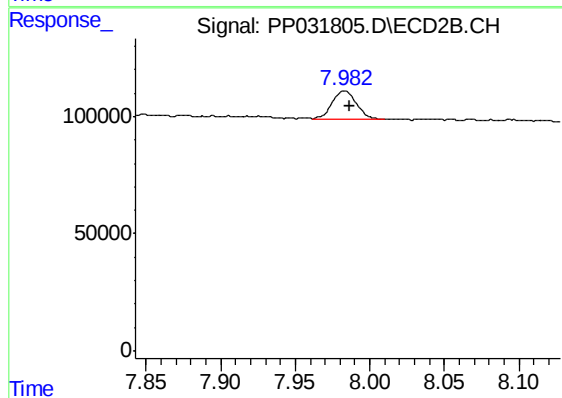

#37 AR-1262-2


R.T.: 7.983 min
Delta R.T.: -0.004 min
Response: 133898
Conc: 27.57 ng/ml

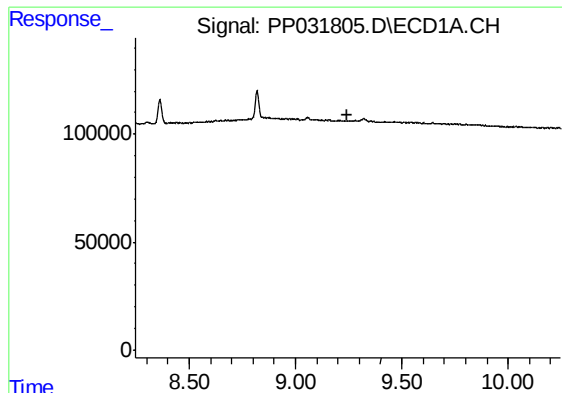

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

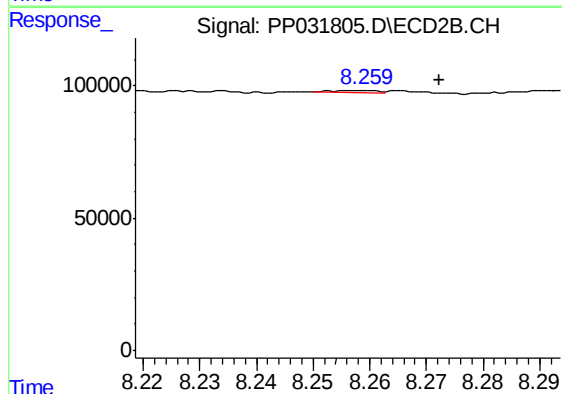


#38 AR-1262-3

R.T.: 8.259 min
Delta R.T.: -0.013 min
Response: 5102
Conc: 2.59 ng/ml

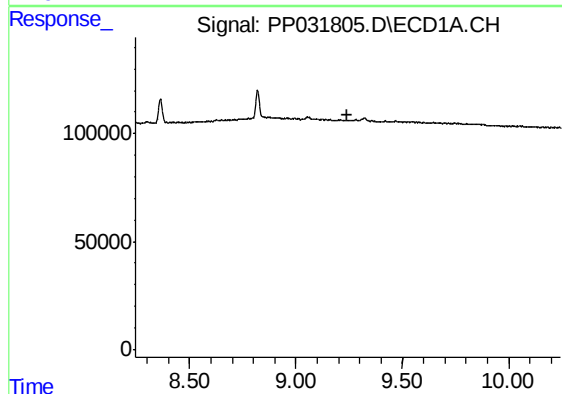


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

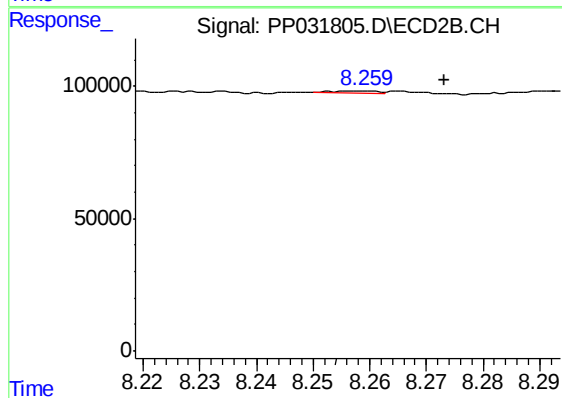

#41 AR-1268-1


R.T.: 8.259 min
Delta R.T.: -0.014 min
Response: 5102
Conc: 0.92 ng/ml

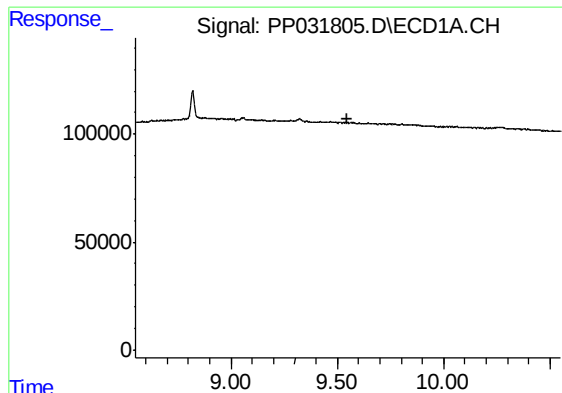

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

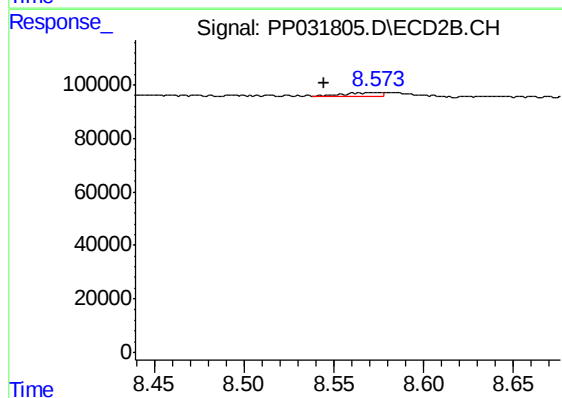

#43 AR-1268-3

R.T.: 8.573 min
Delta R.T.: 0.028 min
Response: 18358
Conc: 4.00 ng/ml