

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
 Data File : PP031819.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2020 15:05
 Operator : DD\AJ
 Sample : L4931-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 R-LA-33-1-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 06:06:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.787	4.060	978771	972416	20.213	20.293
2)	SA Decachlor...	10.657	9.359	632905	634115	18.635	17.126
Target Compounds							
35)	L7 AR-1260-5	0.000	7.972f	0	3884	N.D.	0.856 #
37)	L8 AR-1262-2	0.000	7.972	0	3884	N.D.	0.800 #
38)	L8 AR-1262-3	0.000	8.266	0	80193	N.D.	40.771 #
39)	L8 AR-1262-4	0.000	8.344	0	12255	N.D.	3.381 #
40)	L8 AR-1262-5	0.000	8.840	0	1446	N.D.	0.891 #
41)	L9 AR-1268-1	0.000	8.266	0	80193	N.D.	14.493 #
42)	L9 AR-1268-2	0.000	8.344	0	12255	N.D.	2.267 #
44)	L9 AR-1268-4	0.000	8.840	0	1446	N.D.	0.793 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
Data File : PP031819.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2020 15:05
Operator : DD\AJ
Sample : L4931-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
R-LA-33-1-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 06:06:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

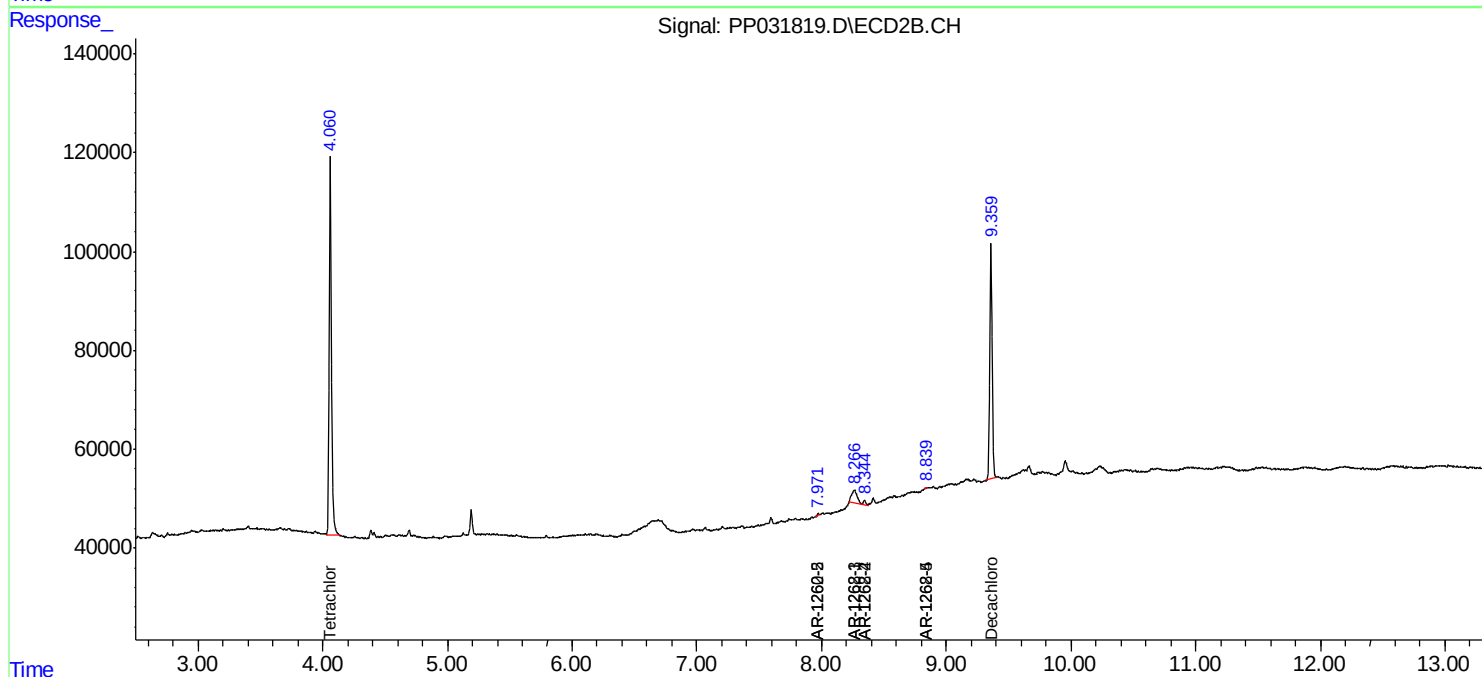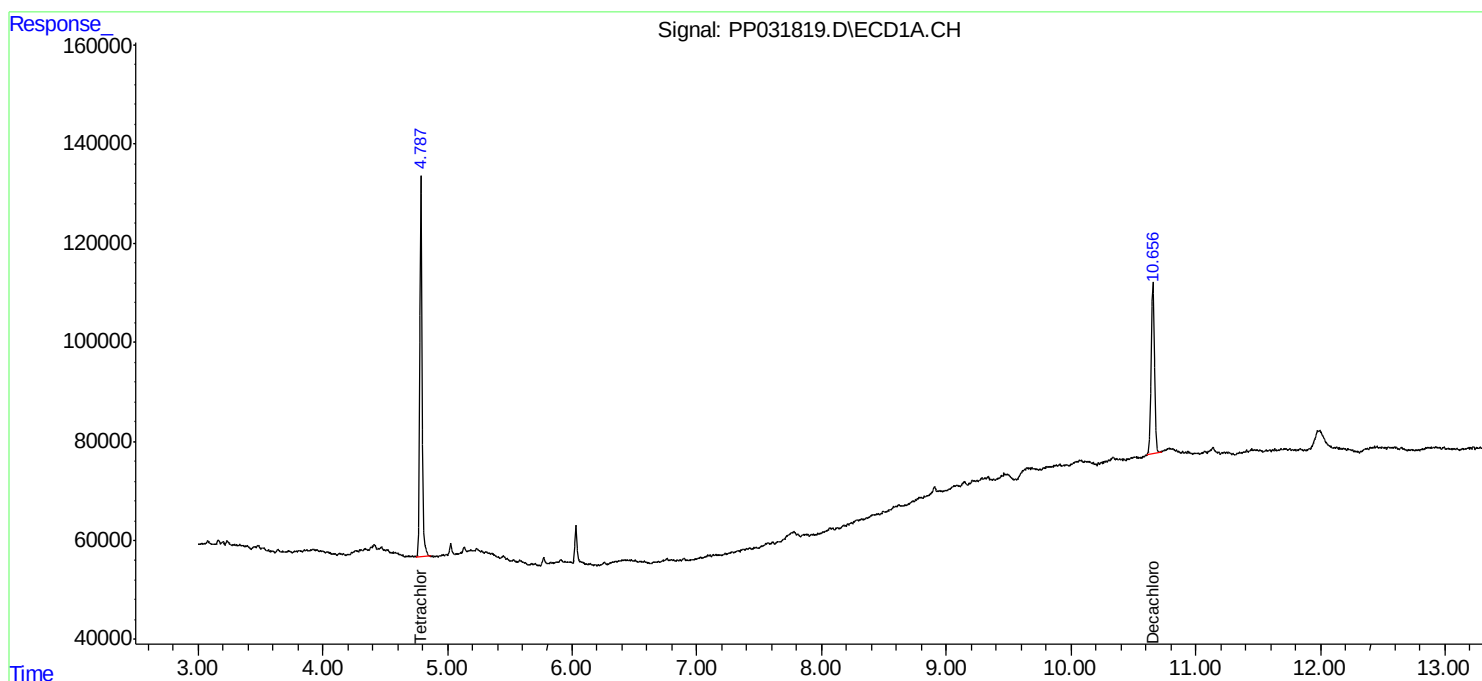


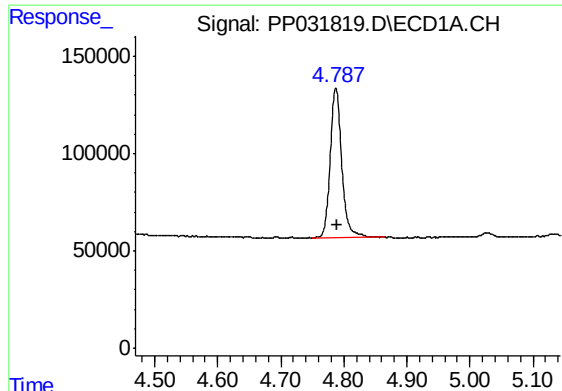

#1 Tetrachloro-m-xylene


R.T.: 4.787 min
Delta R.T.: -0.003 min
Response: 978771
Conc: 20.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
R-LA-33-1-WC

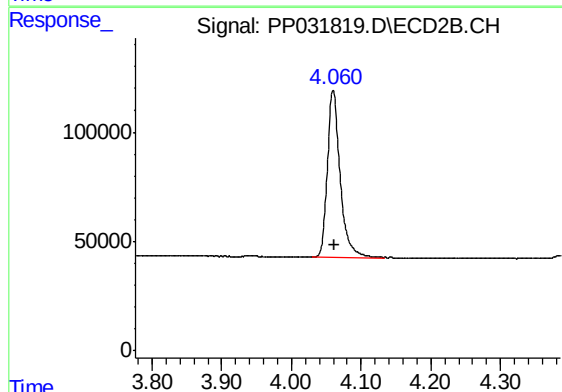


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.002 min
Response: 972416
Conc: 20.29 ng/ml

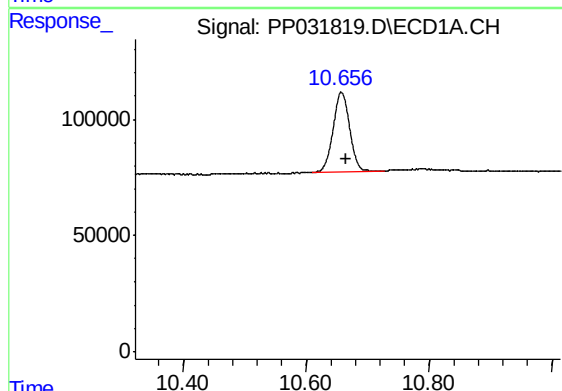


#2 Decachlorobiphenyl

R.T.: 10.657 min
Delta R.T.: -0.008 min
Response: 632905
Conc: 18.63 ng/ml

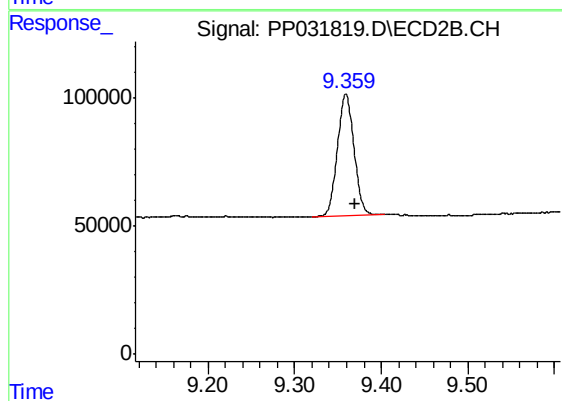

#2 Decachlorobiphenyl


R.T.: 9.359 min
Delta R.T.: -0.011 min
Response: 634115
Conc: 17.13 ng/ml

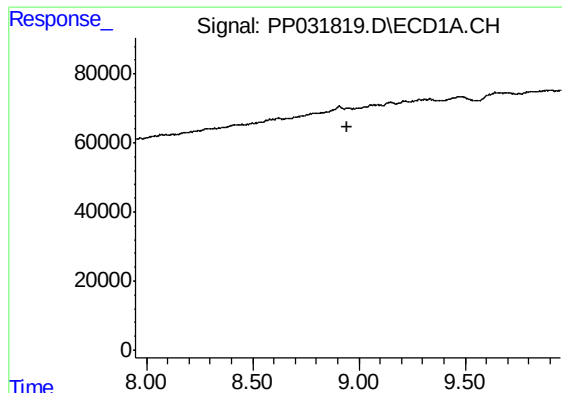

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
R-LA-33-1-WC

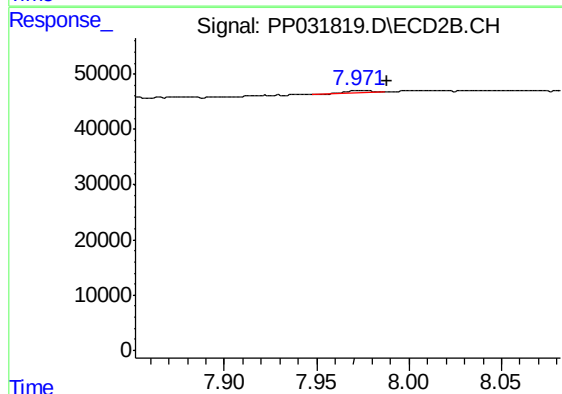


#35 AR-1260-5

R.T.: 7.972 min
Delta R.T.: -0.016 min
Response: 3884
Conc: 0.86 ng/ml

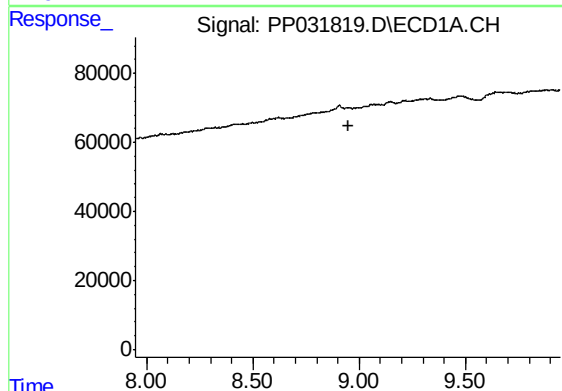


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

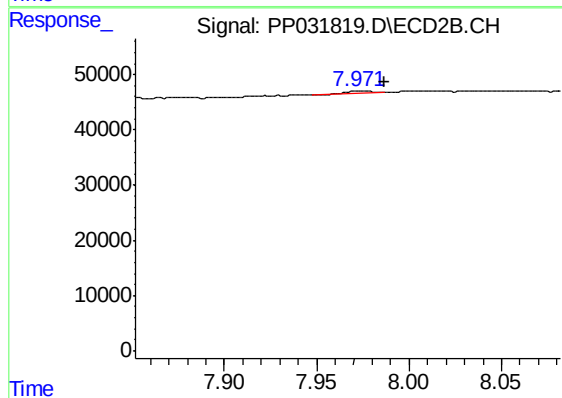

#37 AR-1262-2


R.T.: 7.972 min
Delta R.T.: -0.015 min
Response: 3884
Conc: 0.80 ng/ml

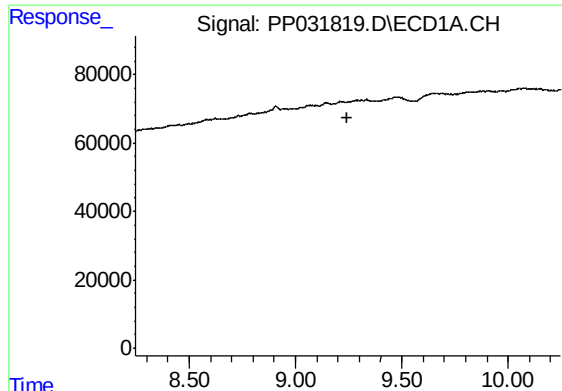

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
R-LA-33-1-WC

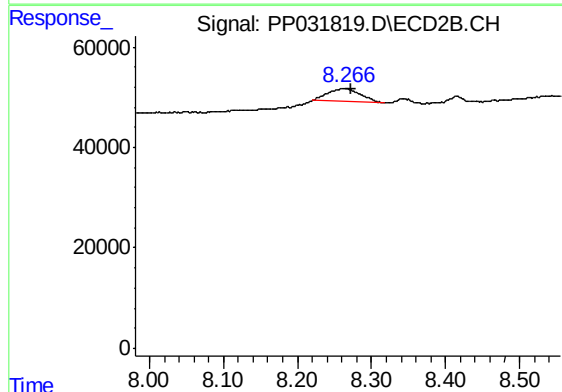


#38 AR-1262-3

R.T.: 8.266 min
Delta R.T.: -0.007 min
Response: 80193
Conc: 40.77 ng/ml

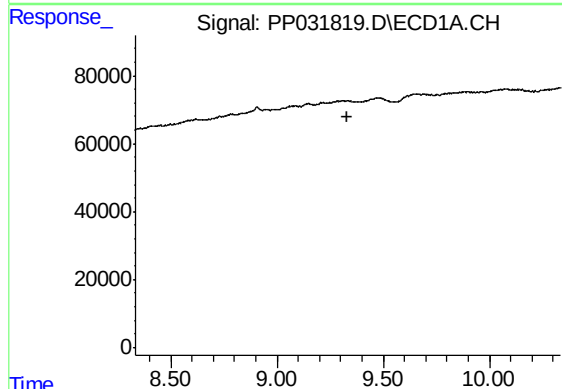


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

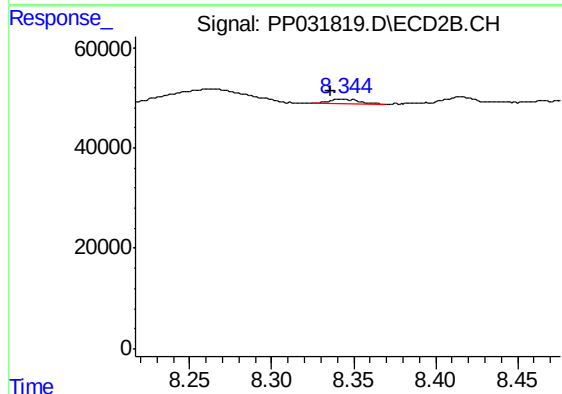

#39 AR-1262-4


R.T.: 8.344 min
Delta R.T.: 0.008 min
Response: 12255
Conc: 3.38 ng/ml

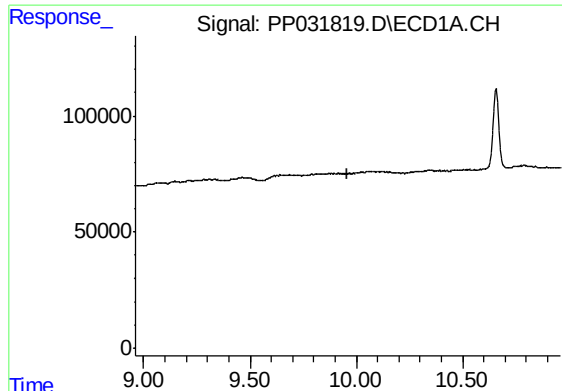

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
R-LA-33-1-WC

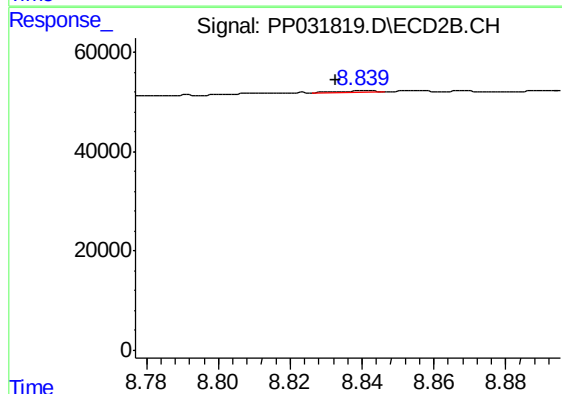


#40 AR-1262-5

R.T.: 8.840 min
Delta R.T.: 0.007 min
Response: 1446
Conc: 0.89 ng/ml

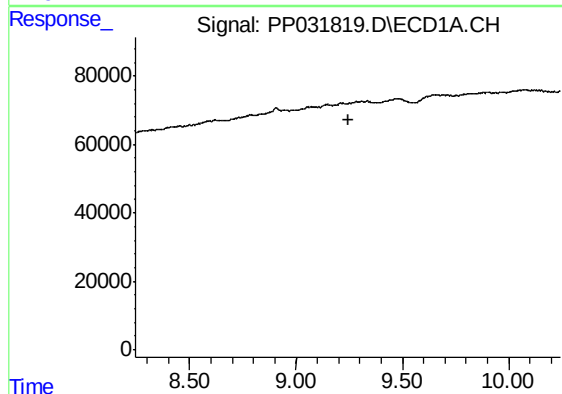


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

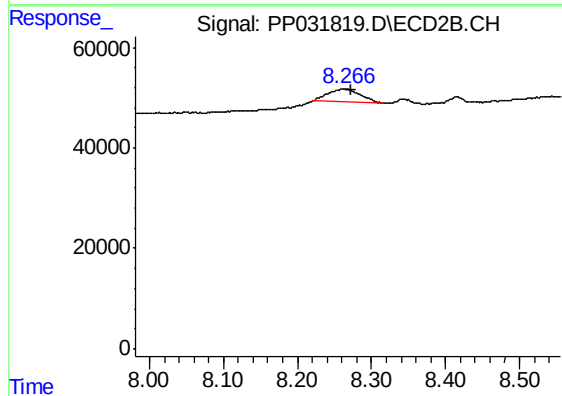

#41 AR-1268-1


R.T.: 8.266 min
Delta R.T.: -0.007 min
Response: 80193
Conc: 14.49 ng/ml

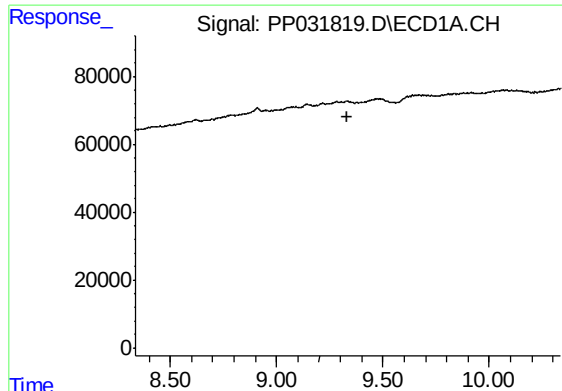

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
R-LA-33-1-WC

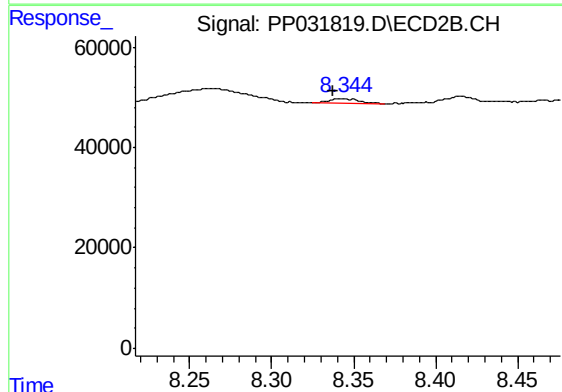


#42 AR-1268-2

R.T.: 8.344 min
Delta R.T.: 0.007 min
Response: 12255
Conc: 2.27 ng/ml

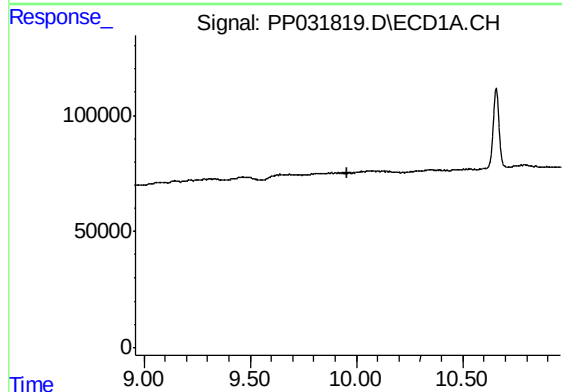

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.960 min
Response: 0
Conc: N.D.

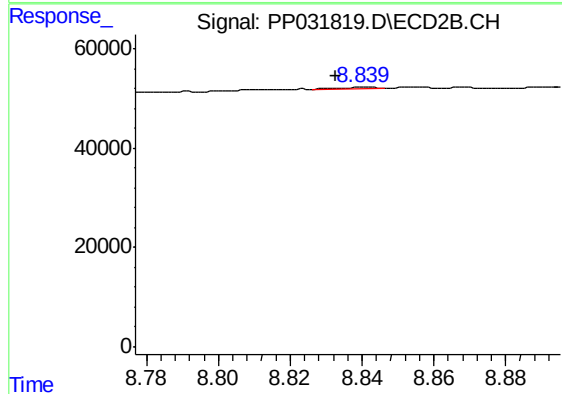

#44 AR-1268-4

R.T.: 8.840 min
Delta R.T.: 0.007 min
Response: 1446
Conc: 0.79 ng/ml