

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
 Data File : PP031818.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2020 14:48
 Operator : DD\AJ
 Sample : L4918-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 16829

Manual Integrations
 APPROVED

mohammad
 12/4/2020 12:34:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 06:05:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.788	4.060	970486	1400931	20.042	29.236m#
2) SA Decachlor...	10.681f	9.375	707840	2163460	20.841	58.429 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
Data File : PP031818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2020 14:48
Operator : DD\AJ
Sample : L4918-06
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
16829


Manual Integrations
APPROVED

mohammad
12/4/2020 12:34:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 06:05:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

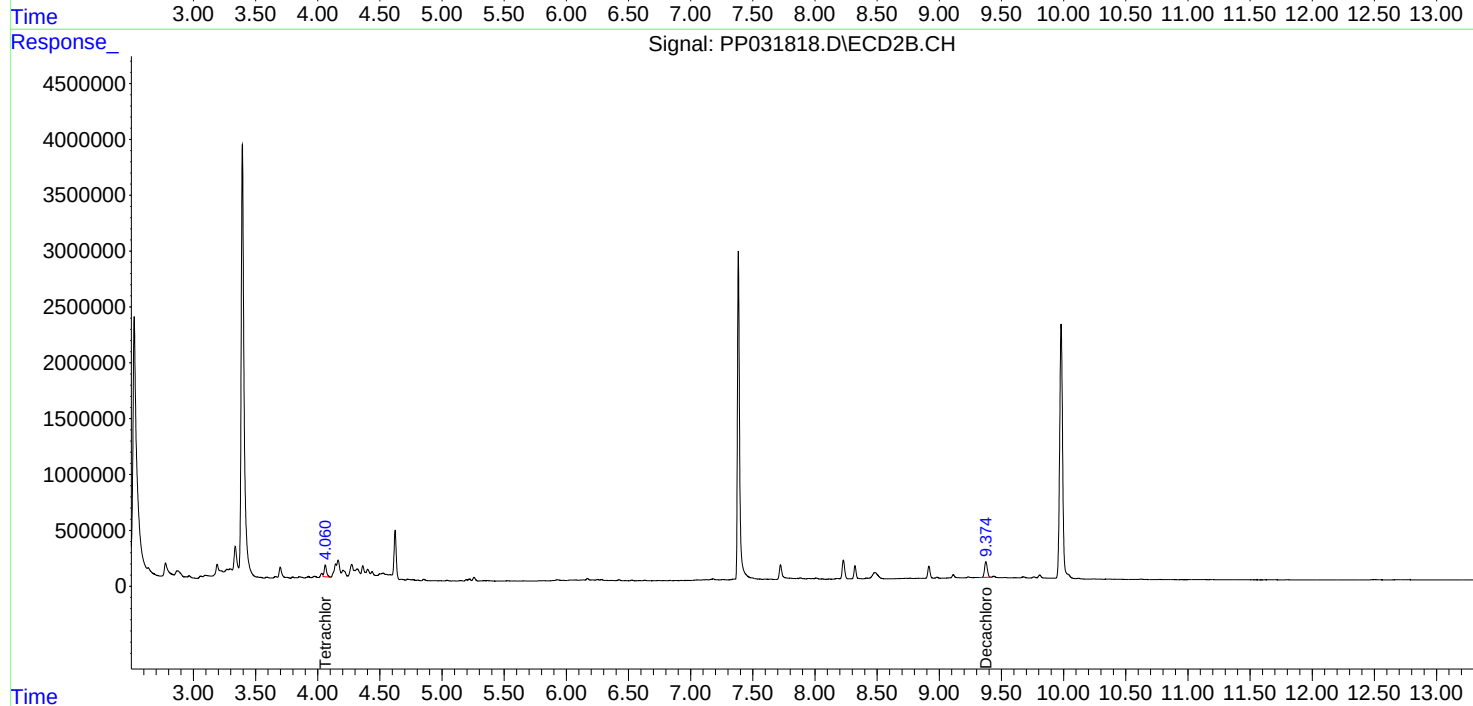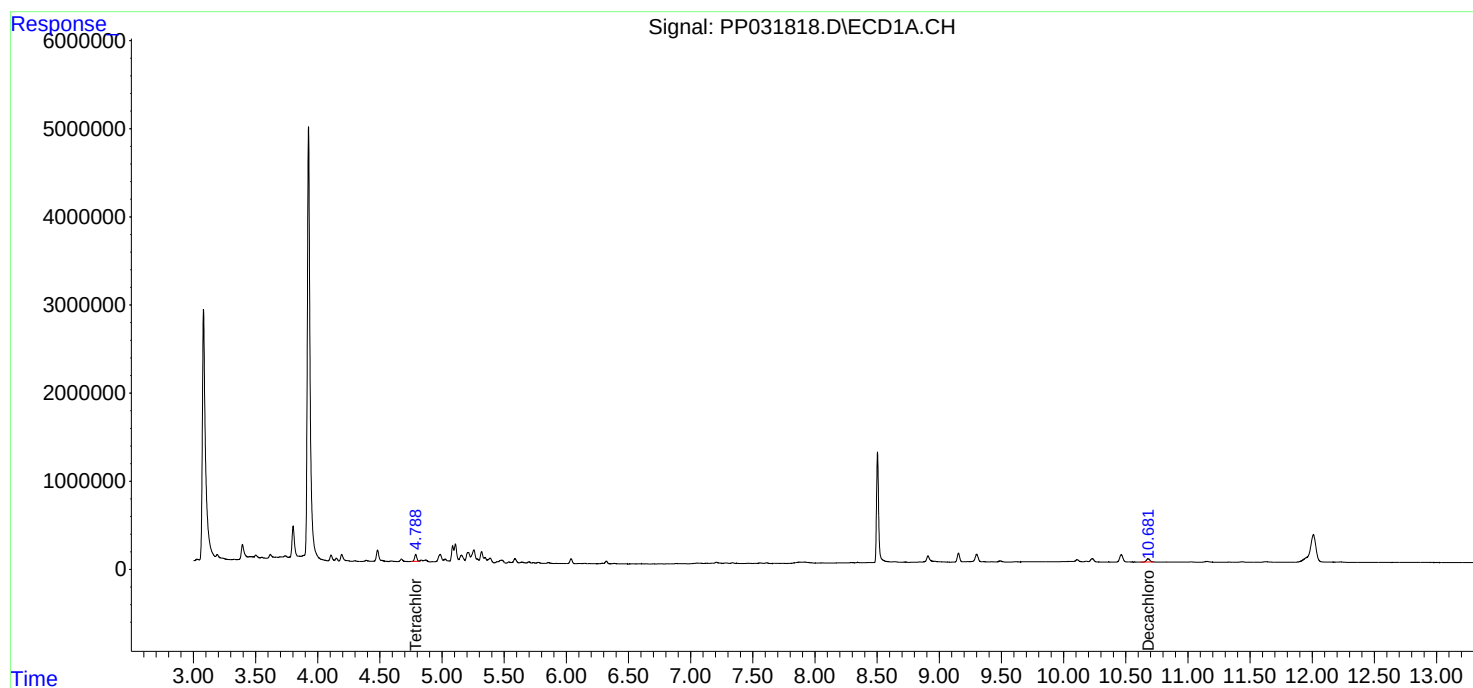

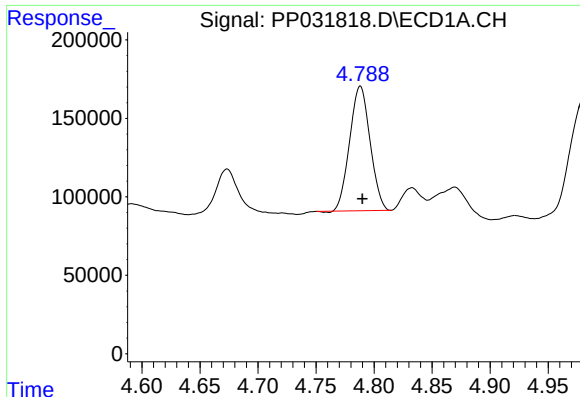


#1 Tetrachloro-m-xylene

R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 970486
Conc: 20.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
16829


Manual Integrations
APPROVED

mohammad
12/4/2020 12:34:47 PM

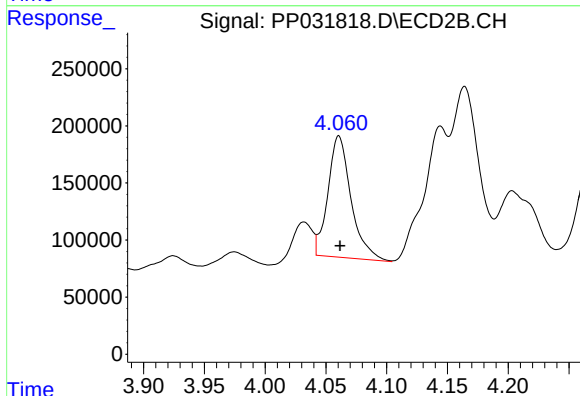


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: -0.001 min
Response: 1400931
Conc: 29.24 ng/ml m

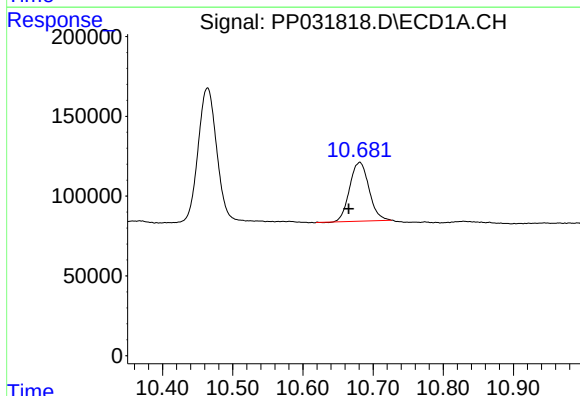

#2 Decachlorobiphenyl

R.T.: 10.681 min
Delta R.T.: 0.016 min
Response: 707840
Conc: 20.84 ng/ml

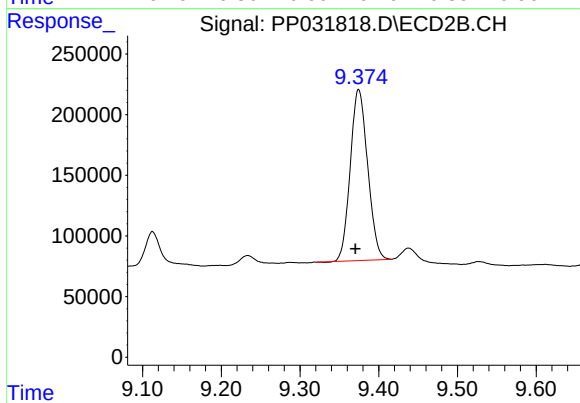

#2 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: 0.004 min
Response: 2163460
Conc: 58.43 ng/ml