

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
 Data File : PP031828.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2020 17:35
 Operator : DD\AJ
 Sample : L4935-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-02-12220

Manual Integrations
 APPROVED

mohammad
 12/4/2020 12:34:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 06:12:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.786	4.059	894104	869331	18.464m	18.142m
2) SA Decachlor...	10.656	9.359	698002	702855	20.551	18.982

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
Data File : PP031828.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2020 17:35
Operator : DD\AJ
Sample : L4935-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OK-02-12220


Manual Integrations
APPROVED

mohammad
12/4/2020 12:34:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 06:12:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

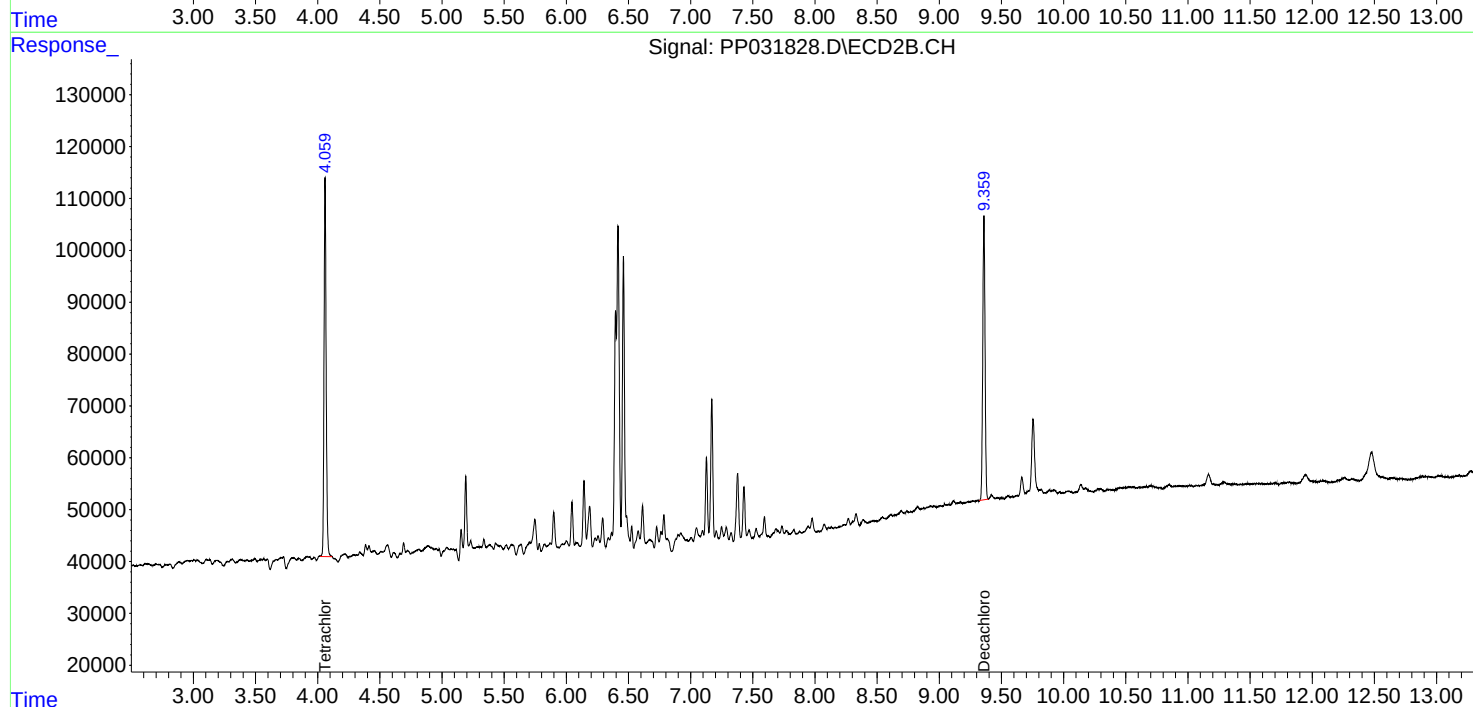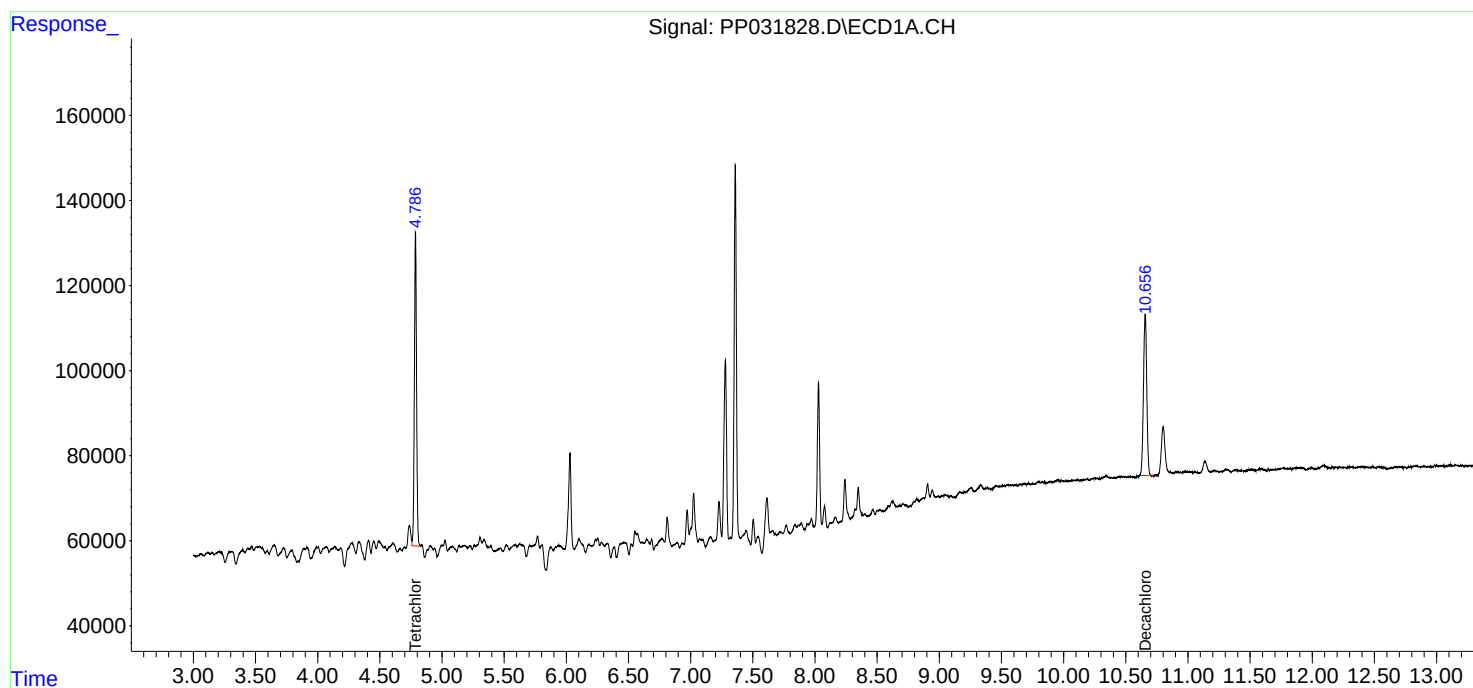

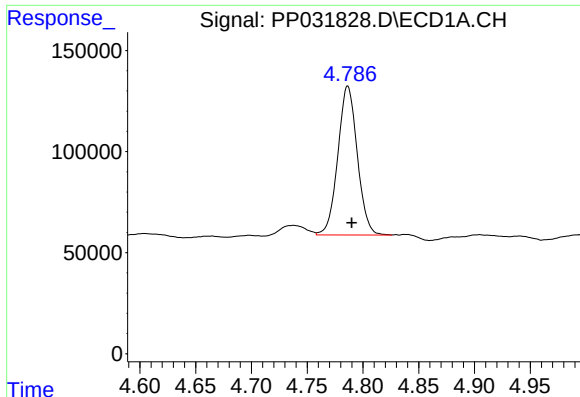


#1 Tetrachloro-m-xylene

R.T.: 4.786 min
Delta R.T.: -0.004 min
Response: 894104
Conc: 18.46 ng/ml m

Instrument :
ECD_P
ClientSampleId :
OK-02-12220


Manual Integrations
APPROVED

mohammad
12/4/2020 12:34:53 PM

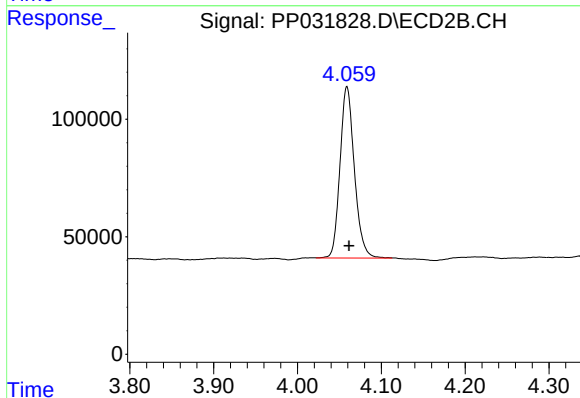


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.003 min
Response: 869331
Conc: 18.14 ng/ml m

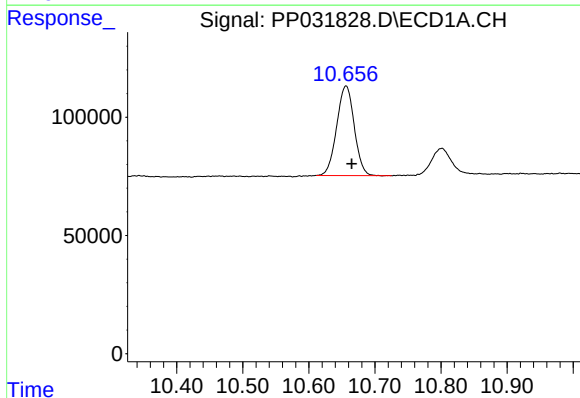

#2 Decachlorobiphenyl

R.T.: 10.656 min
Delta R.T.: -0.009 min
Response: 698002
Conc: 20.55 ng/ml

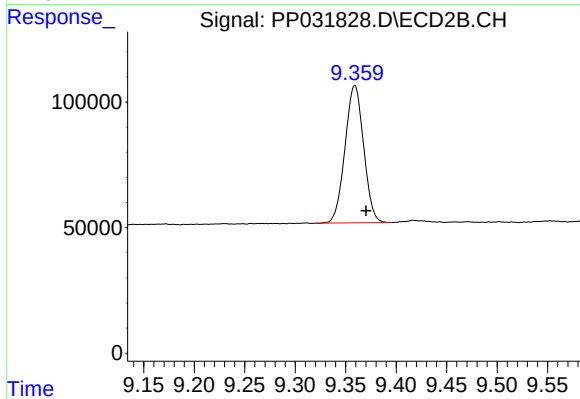

#2 Decachlorobiphenyl

R.T.: 9.359 min
Delta R.T.: -0.011 min
Response: 702855
Conc: 18.98 ng/ml