

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
Data File : PP031830.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2020 18:08
Operator : DD\AJ
Sample : L4940-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LLEXSITUTV-009-001-SO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 06:13:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.787	4.059	1070738	1025104	22.112	21.393
2) SA Decachlor...	10.655	9.358	723085	739608	21.290	19.975

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120320\
Data File : PP031830.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2020 18:08
Operator : DD\AJ
Sample : L4940-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LLEXSITUTV-009-001-SO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 06:13:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

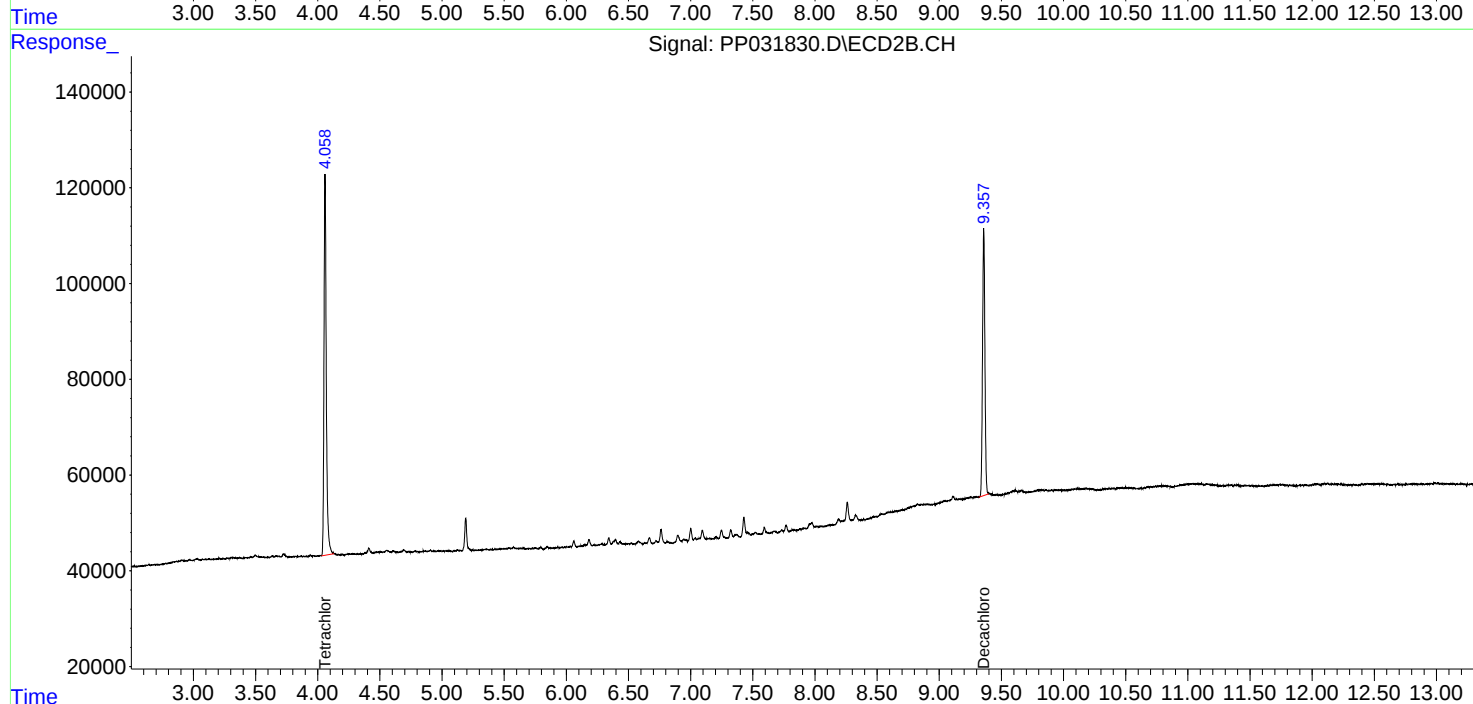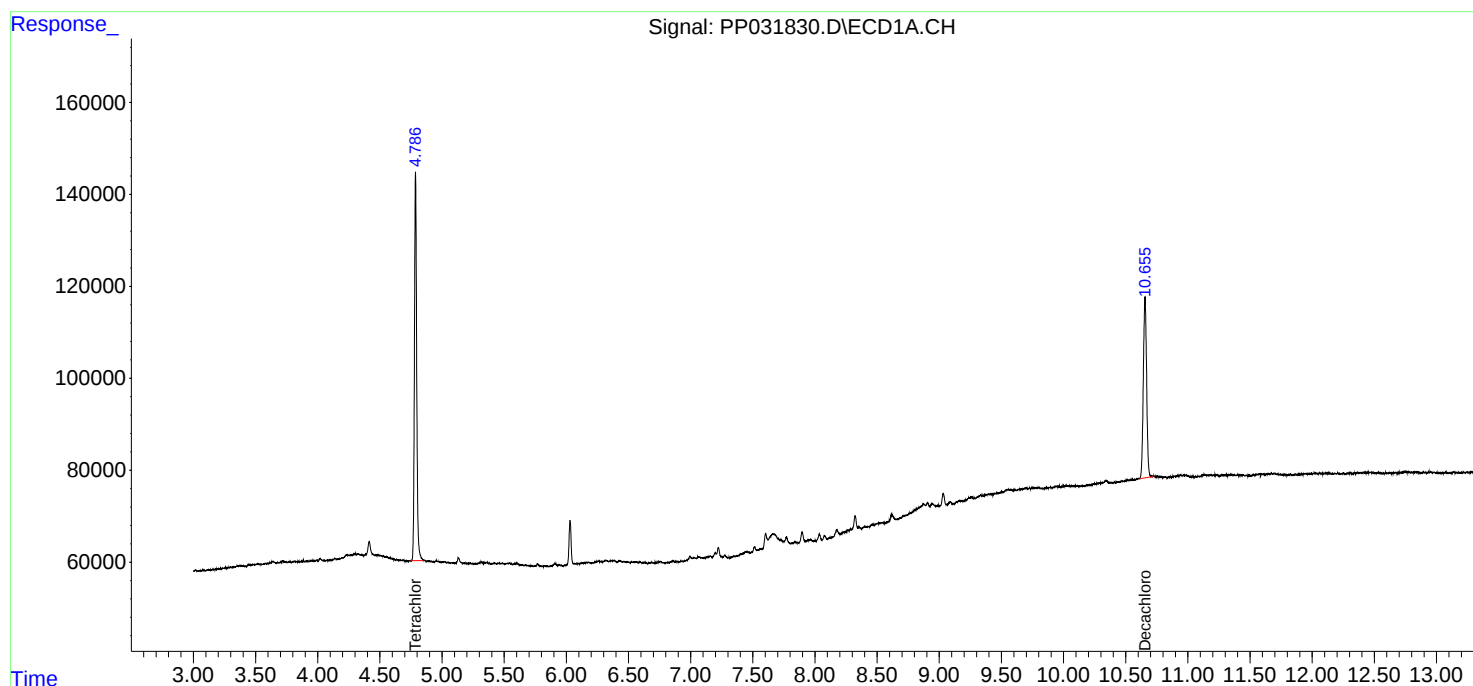


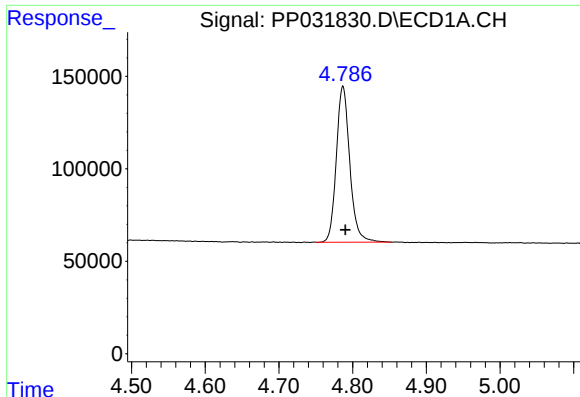

#1 Tetrachloro-m-xylene


R.T.: 4.787 min
Delta R.T.: -0.003 min
Response: 1070738
Conc: 22.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LLEXSITUTV-009-001-SO

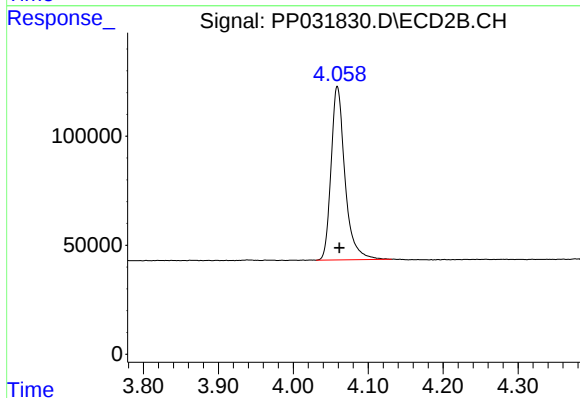


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.003 min
Response: 1025104
Conc: 21.39 ng/ml

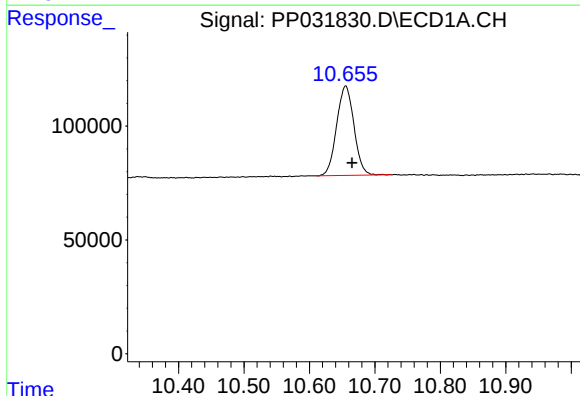

#2 Decachlorobiphenyl

R.T.: 10.655 min
Delta R.T.: -0.010 min
Response: 723085
Conc: 21.29 ng/ml

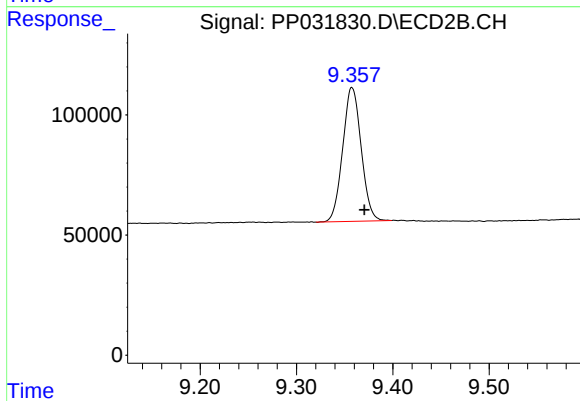

#2 Decachlorobiphenyl

R.T.: 9.358 min
Delta R.T.: -0.013 min
Response: 739608
Conc: 19.97 ng/ml