

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
 Data File : PP041593.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2021 9:52
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 16:20:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
2)	SA Decachlor...	10.627f	0.000	1480	0	0.069	N.D.	#
Target Compounds								
24)	L5 AR-1248-4	6.987	0.000	373	0	0.446	N.D.	#
26)	L6 AR-1254-1	6.987f	0.000	373	0	0.440	N.D.	#
29)	L6 AR-1254-4	7.873	0.000	4000	0	3.855	N.D.	#
30)	L6 AR-1254-5	8.303	0.000	1004	0	0.895	N.D.	#
33)	L7 AR-1260-3	8.369	0.000	1163	0	1.285	N.D.	#
34)	L7 AR-1260-4	8.612	0.000	913	0	0.853	N.D.	#
36)	L8 AR-1262-1	8.369	0.000	1163	0	0.916	N.D.	#
39)	L8 AR-1262-4	9.304	0.000	25563	0	37.348	N.D.	#
42)	L9 AR-1268-2	9.304	0.000	25563	0	9.762	N.D.	#
43)	L9 AR-1268-3	9.544f	0.000	18583	0	8.385	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
Data File : PP041593.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2021 9:52
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 16:20:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

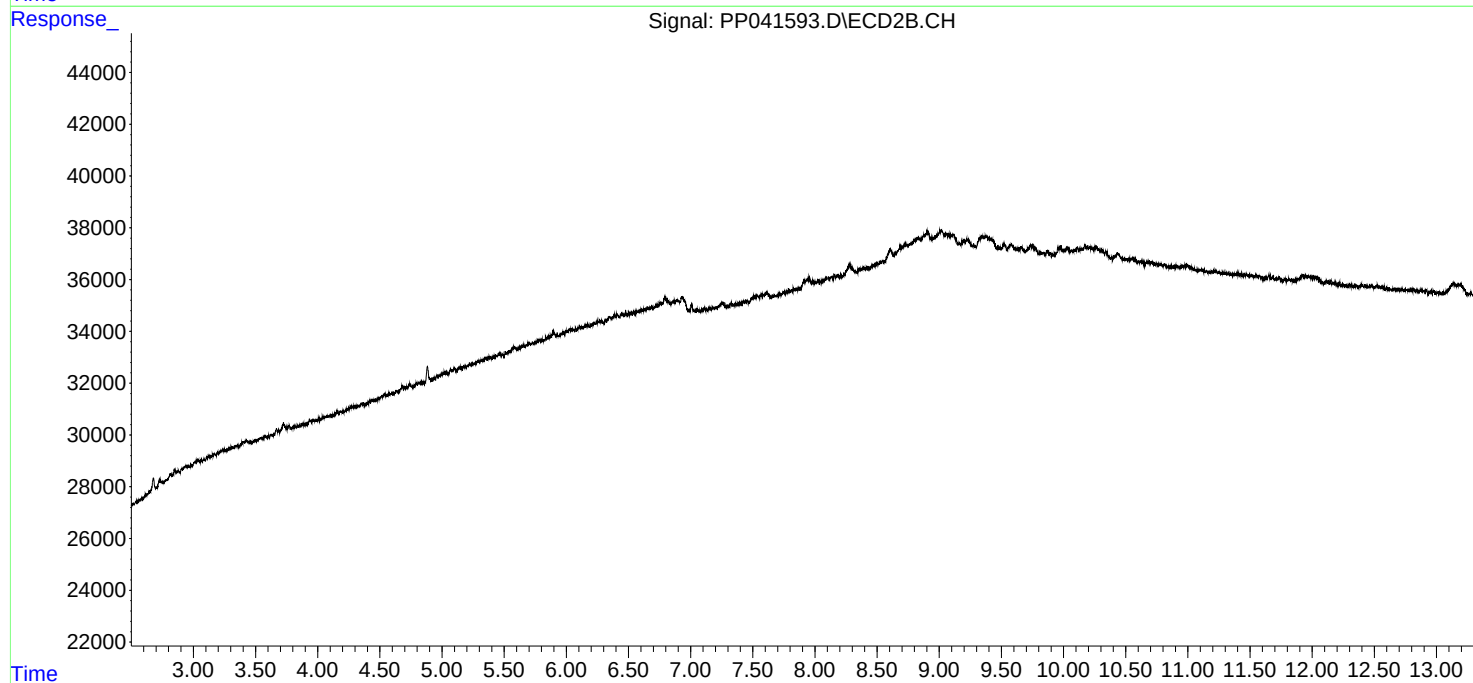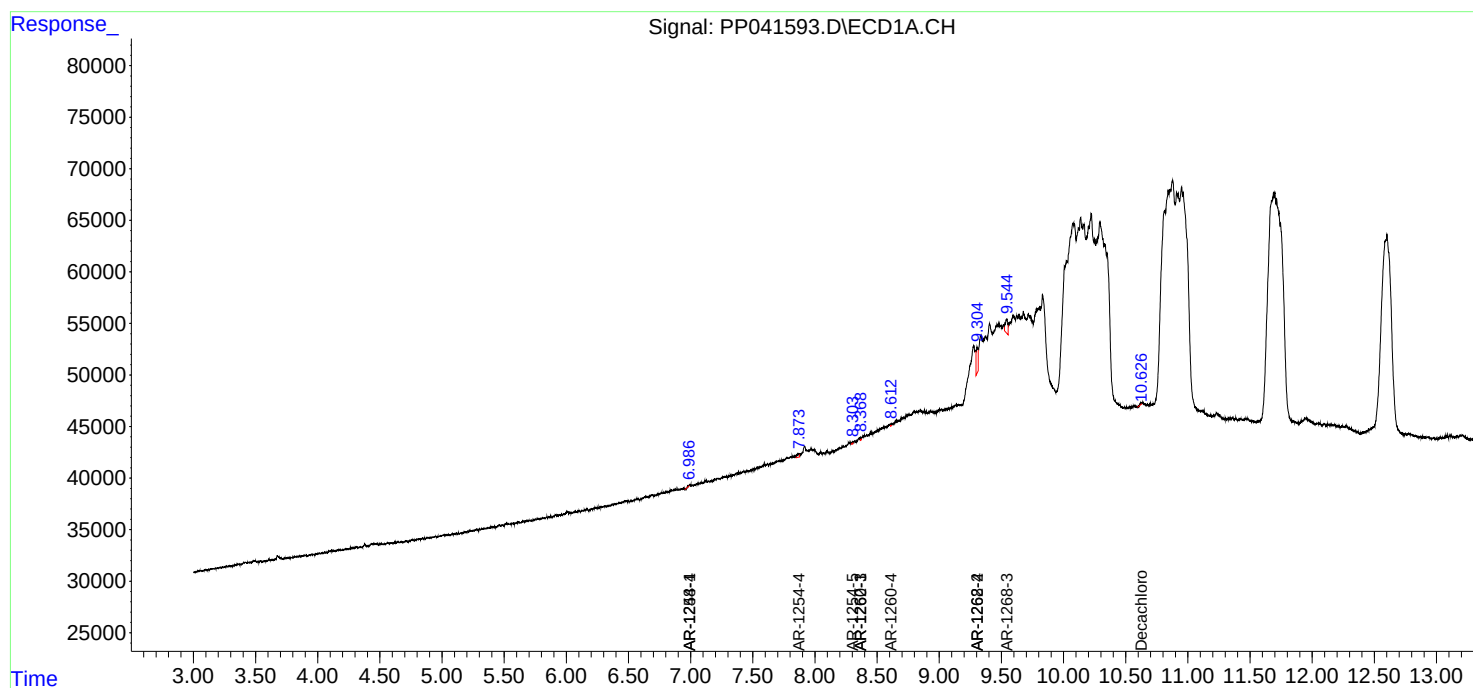


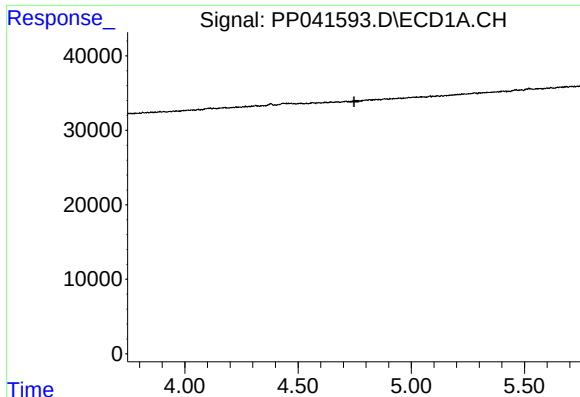

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

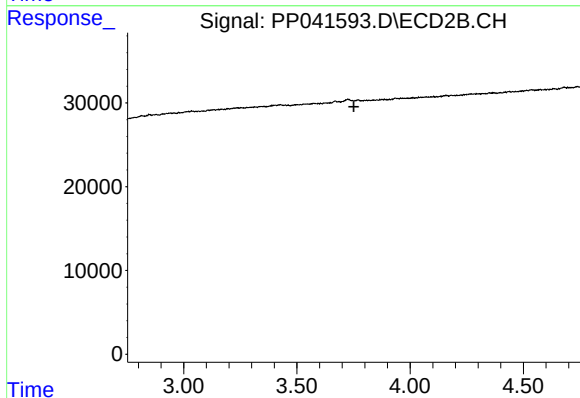


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.751 min
Response: 0
Conc: N.D.

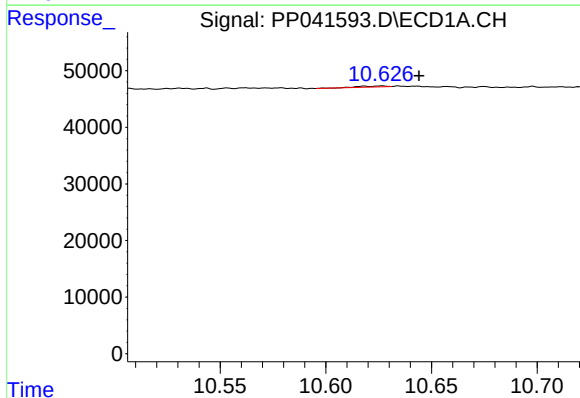


#2 Decachlorobiphenyl

R.T.: 10.627 min
Delta R.T.: -0.017 min
Response: 1480
Conc: 0.07 ng/ml

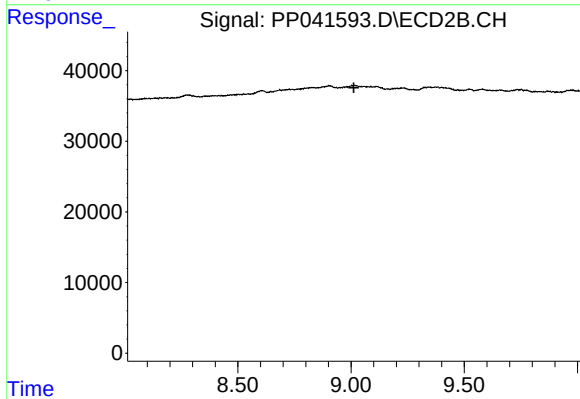

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.012 min
Response: 0
Conc: N.D.

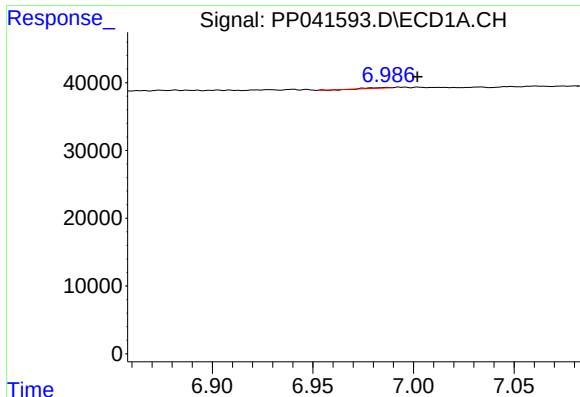

#24 AR-1248-4


R.T.: 6.987 min
Delta R.T.: -0.015 min
Response: 373
Conc: 0.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

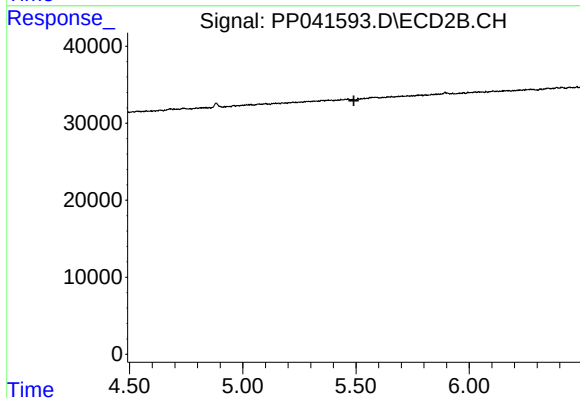


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

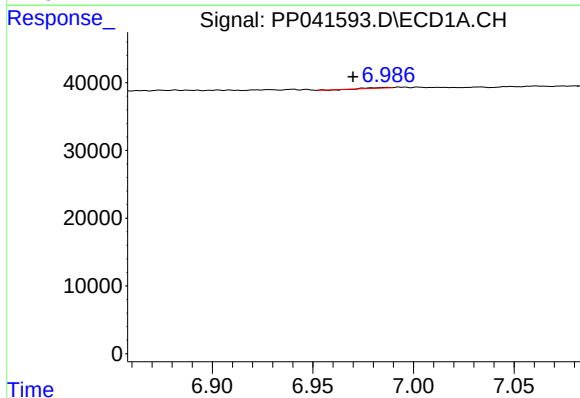


#26 AR-1254-1

R.T.: 6.987 min
Delta R.T.: 0.017 min
Response: 373
Conc: 0.44 ng/ml

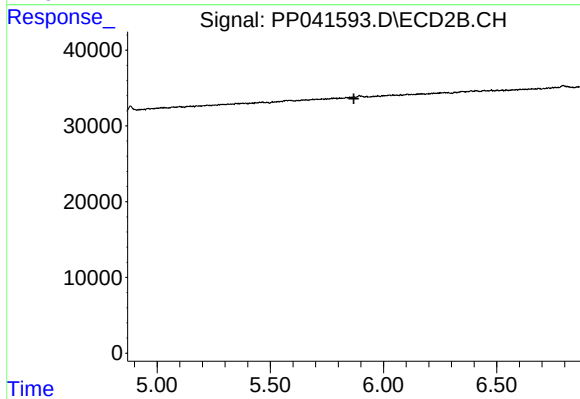

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.869 min
Response: 0
Conc: N.D.

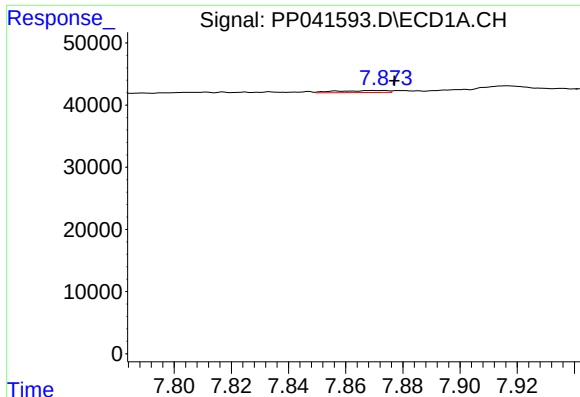

#29 AR-1254-4


R.T.: 7.873 min
Delta R.T.: -0.004 min
Response: 4000
Conc: 3.86 ng/ml

Instrument :
ECD_P
ClientSampleId :

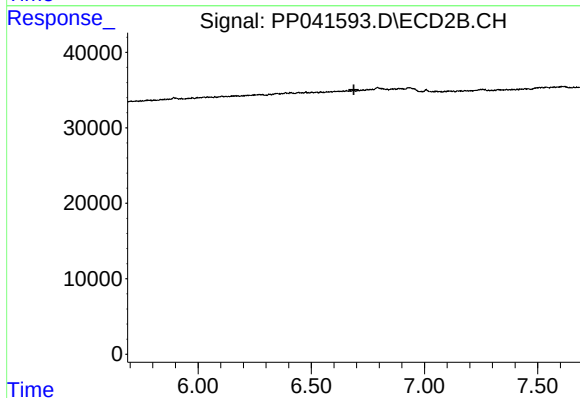


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.688 min
Response: 0
Conc: N.D.

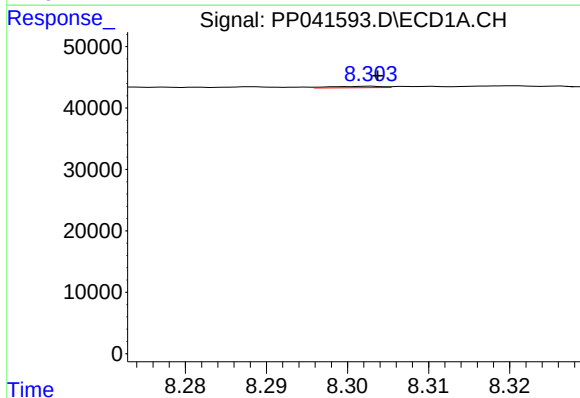


#30 AR-1254-5

R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 1004
Conc: 0.89 ng/ml

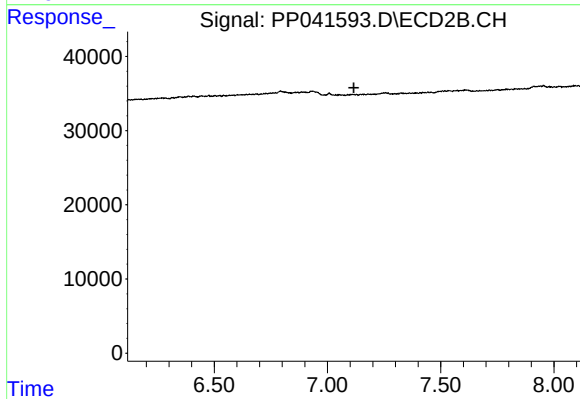

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

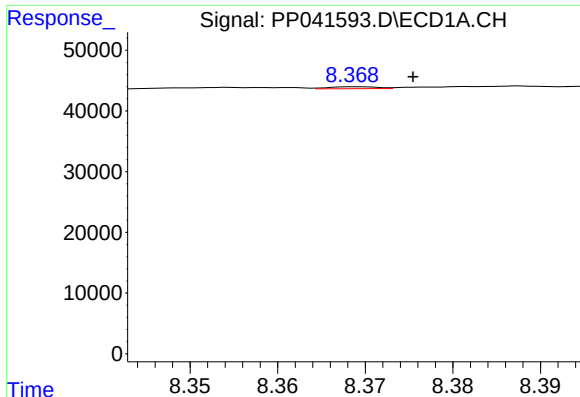

#33 AR-1260-3


R.T.: 8.369 min
Delta R.T.: -0.006 min
Response: 1163
Conc: 1.28 ng/ml

Instrument :
ECD_P
ClientSampleId :

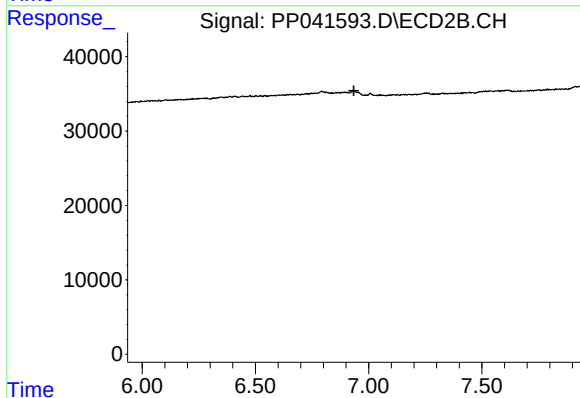


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

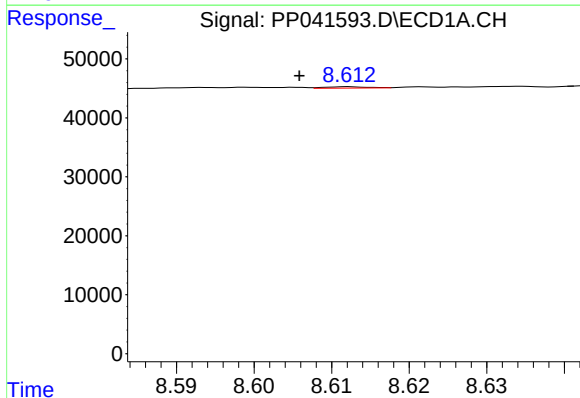


#34 AR-1260-4

R.T.: 8.612 min
Delta R.T.: 0.006 min
Response: 913
Conc: 0.85 ng/ml

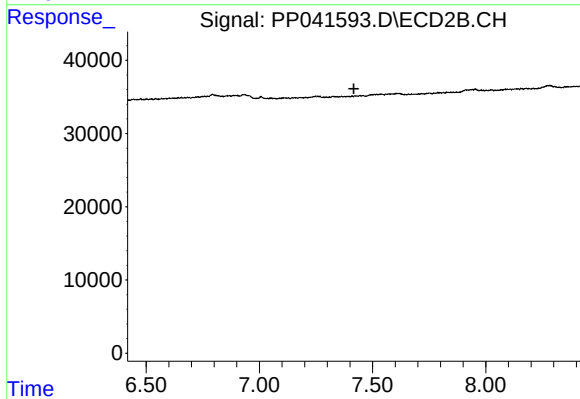

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

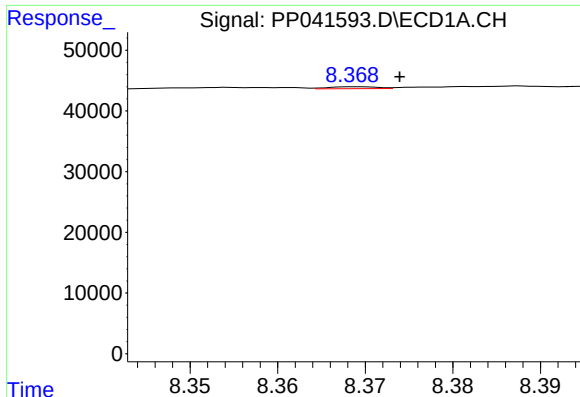

#36 AR-1262-1


R.T.: 8.369 min
Delta R.T.: -0.005 min
Response: 1163
Conc: 0.92 ng/ml

Instrument :
ECD_P
ClientSampleId :

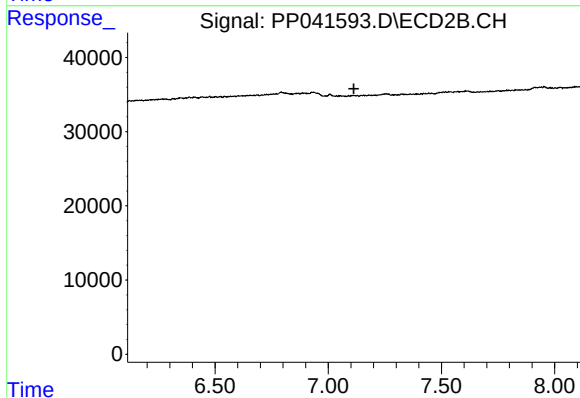


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

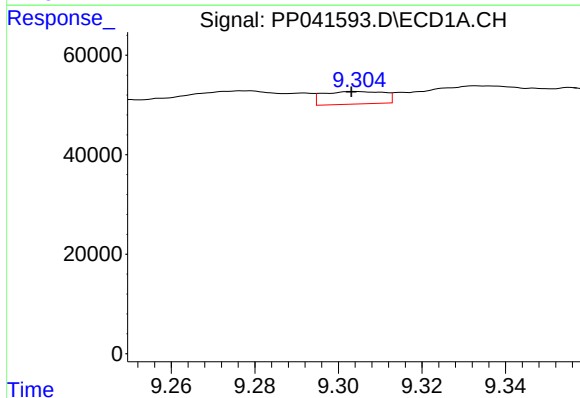


#39 AR-1262-4

R.T.: 9.304 min
Delta R.T.: 0.001 min
Response: 25563
Conc: 37.35 ng/ml

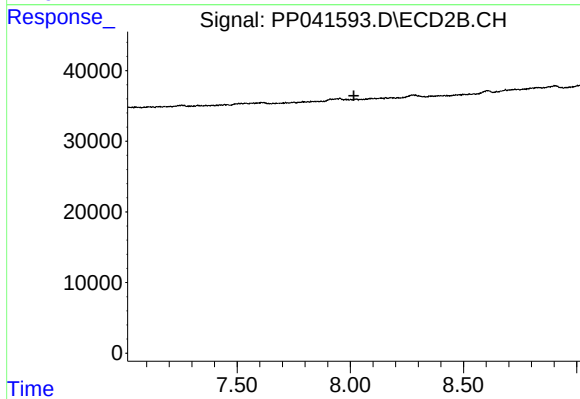

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.016 min
Response: 0
Conc: N.D.

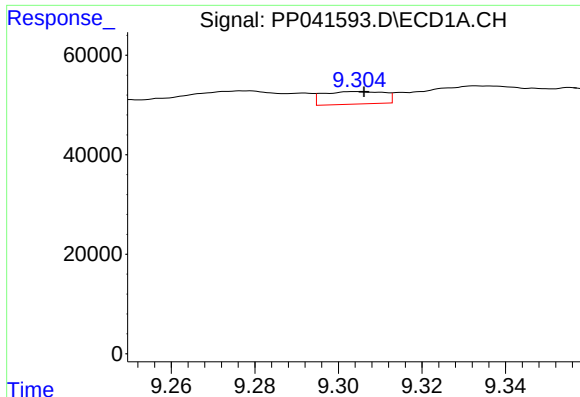

#42 AR-1268-2


R.T.: 9.304 min
Delta R.T.: -0.002 min
Response: 25563
Conc: 9.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

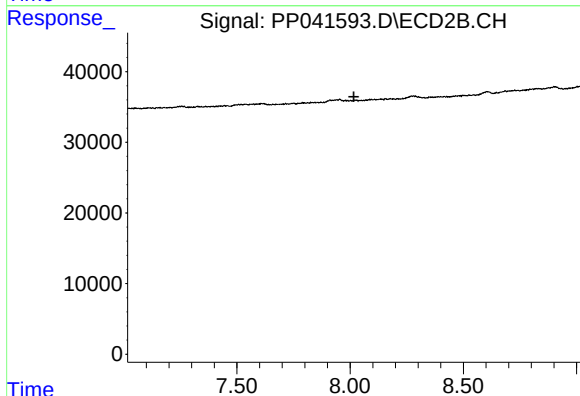


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.017 min
Response: 0
Conc: N.D.

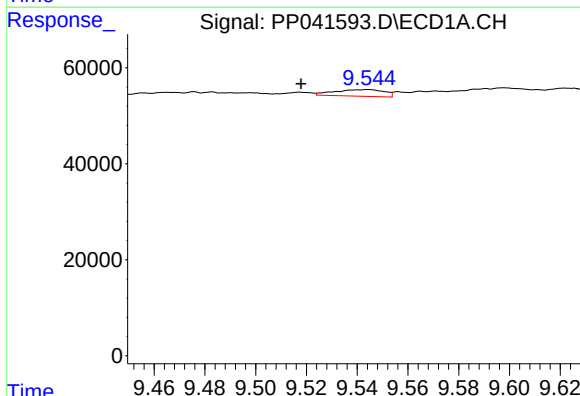

#43 AR-1268-3

R.T.: 9.544 min
Delta R.T.: 0.026 min
Response: 18583
Conc: 8.39 ng/ml

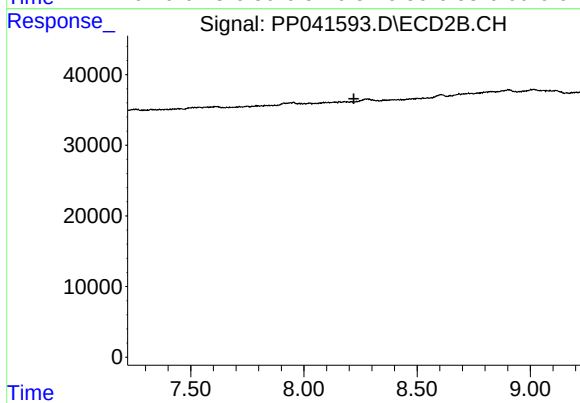

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.220 min
Response: 0
Conc: N.D.