

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
 Data File : PP041598.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2021 12:15
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 16:21:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.746	3.749	483448	700561	21.439	23.063
2)	SA Decachlor...	10.640	9.006	481677	343731	22.370	22.240
Target Compounds							
8)	L2 AR-1221-1	4.983	0.000	13073	0	49.738	N.D. #
9)	L2 AR-1221-2	5.100	4.098	5779	9608	30.835	34.901
10)	L2 AR-1221-3	0.000	4.192	0	31668	N.D.	36.490 #
11)	L3 AR-1232-1	0.000	4.192	0	31668	N.D.	42.751 #
16)	L4 AR-1242-1	6.026f	0.000	946	0	1.577	N.D. #
32)	L7 AR-1260-2	8.035f	0.000	3862	0	3.073	N.D. #
33)	L7 AR-1260-3	0.000	6.934	0	20980	N.D.	15.685 #
45)	L9 AR-1268-5	10.350f	0.000	16287	0	2.253	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
Data File : PP041598.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2021 12:15
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 16:21:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

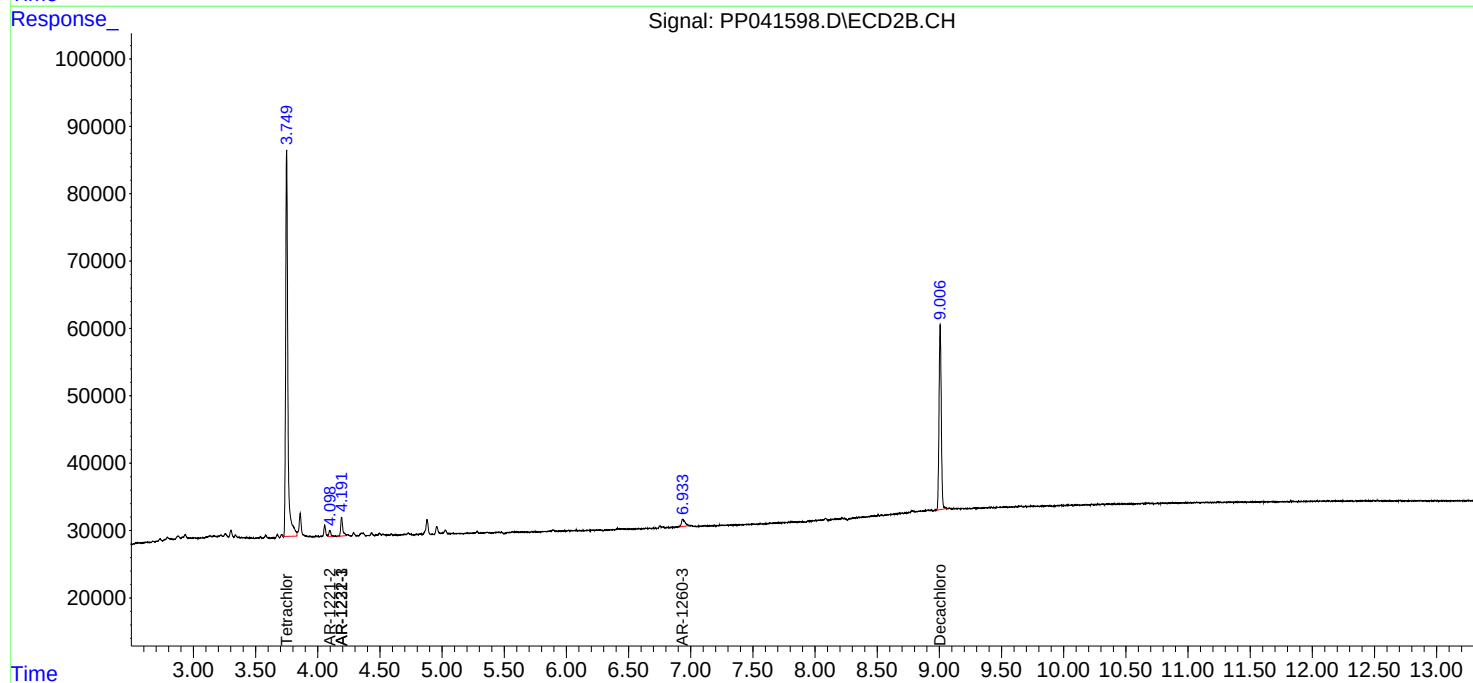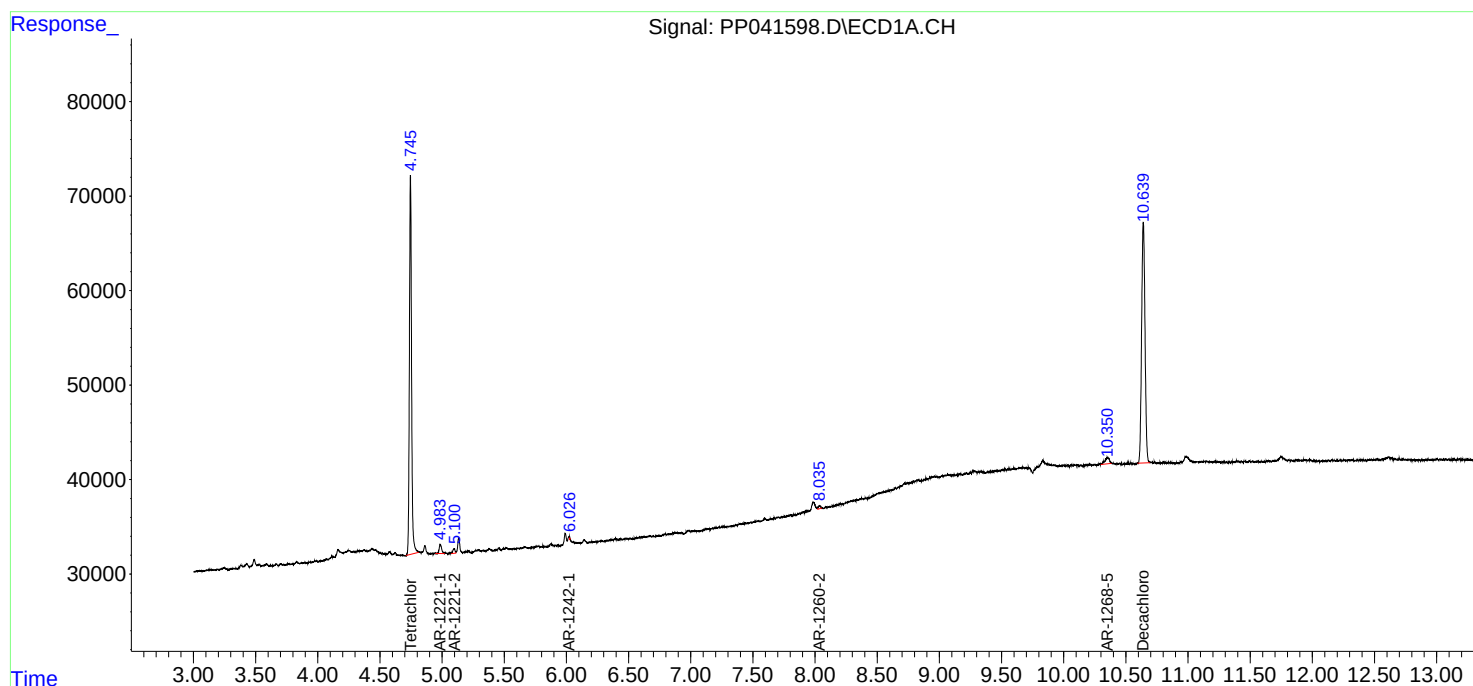


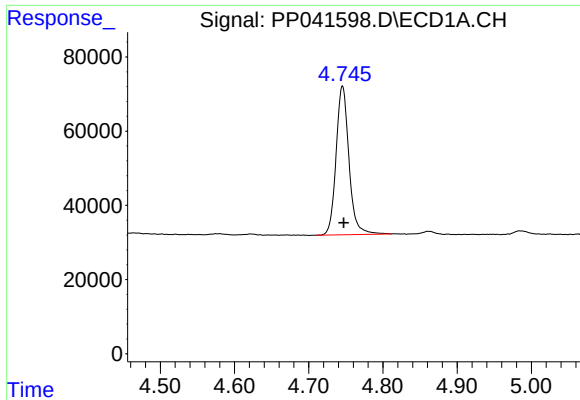

#1 Tetrachloro-m-xylene


R.T.: 4.746 min
Delta R.T.: -0.001 min
Response: 483448
Conc: 21.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

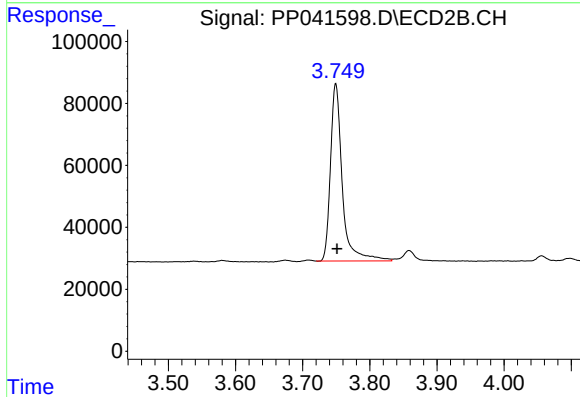


#1 Tetrachloro-m-xylene

R.T.: 3.749 min
Delta R.T.: -0.002 min
Response: 700561
Conc: 23.06 ng/ml

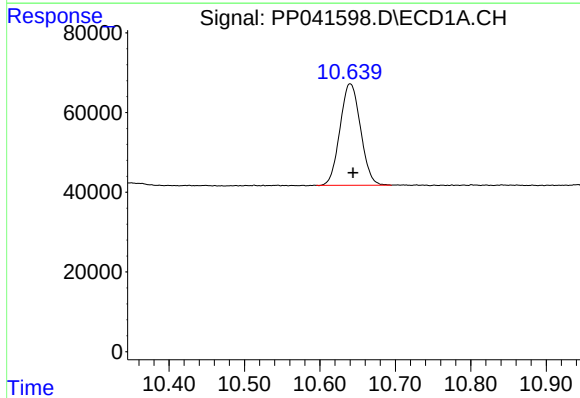


#2 Decachlorobiphenyl

R.T.: 10.640 min
Delta R.T.: -0.004 min
Response: 481677
Conc: 22.37 ng/ml

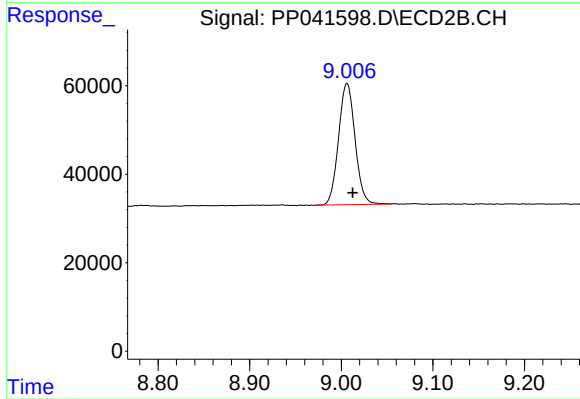

#2 Decachlorobiphenyl


R.T.: 9.006 min
Delta R.T.: -0.006 min
Response: 343731
Conc: 22.24 ng/ml

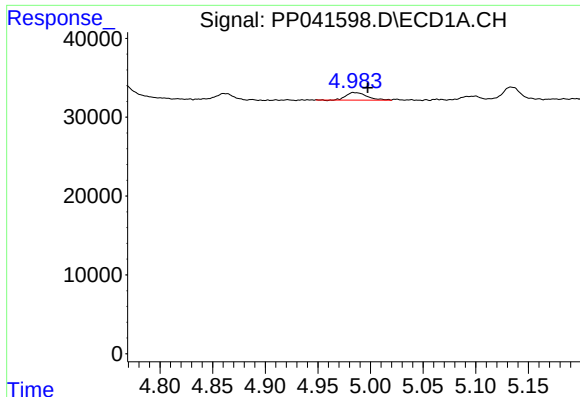

#8 AR-1221-1


R.T.: 4.983 min
Delta R.T.: -0.014 min
Response: 13073
Conc: 49.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

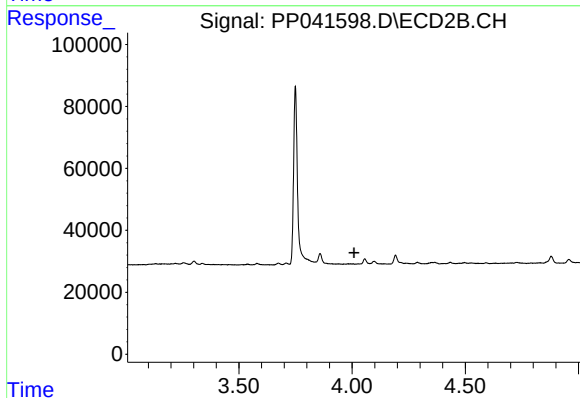


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.008 min
Response: 0
Conc: N.D.

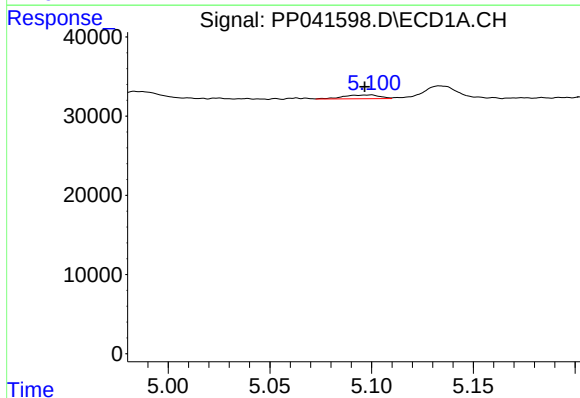


#9 AR-1221-2

R.T.: 5.100 min
Delta R.T.: 0.003 min
Response: 5779
Conc: 30.84 ng/ml

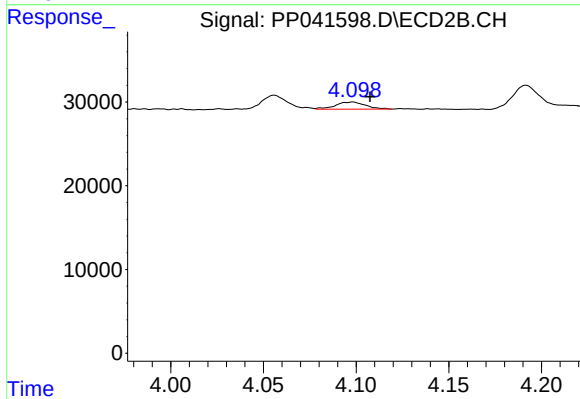

#9 AR-1221-2


R.T.: 4.098 min
Delta R.T.: -0.009 min
Response: 9608
Conc: 34.90 ng/ml

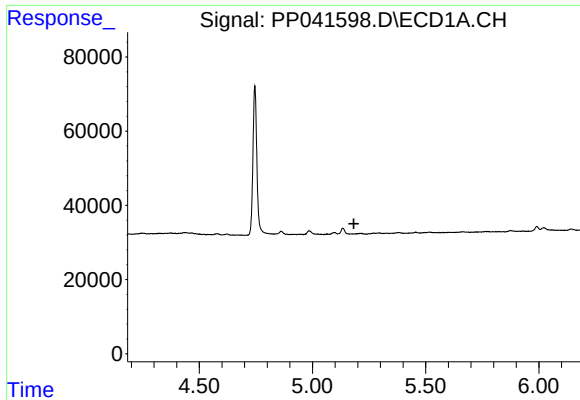

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

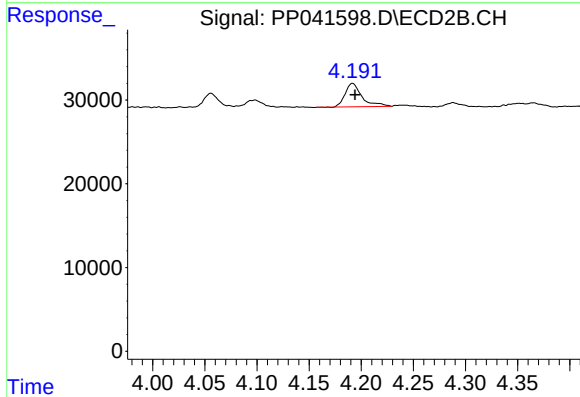


#10 AR-1221-3

R.T.: 4.192 min
Delta R.T.: -0.002 min
Response: 31668
Conc: 36.49 ng/ml

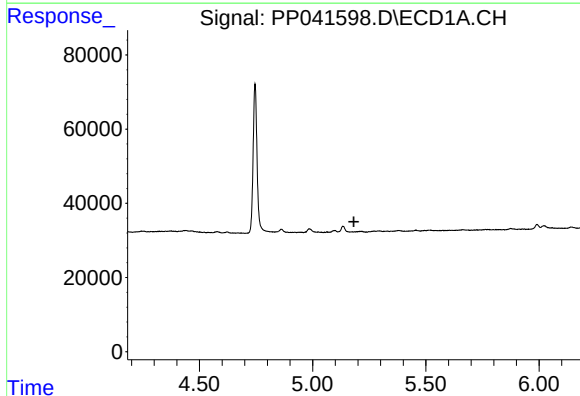


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.182 min
Response: 0
Conc: N.D.

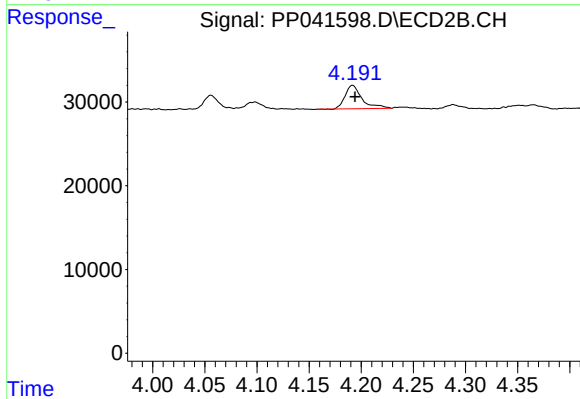

#11 AR-1232-1


R.T.: 4.192 min
Delta R.T.: -0.002 min
Response: 31668
Conc: 42.75 ng/ml

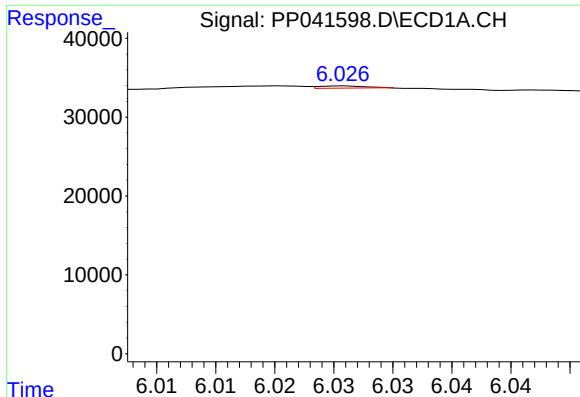

#16 AR-1242-1


R.T.: 6.026 min
Delta R.T.: -0.037 min
Response: 946
Conc: 1.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

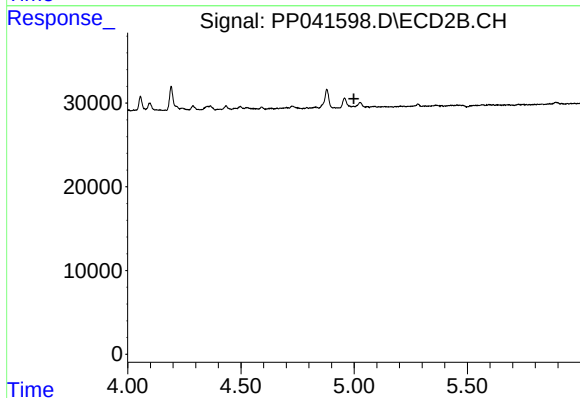


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.999 min
Response: 0
Conc: N.D.

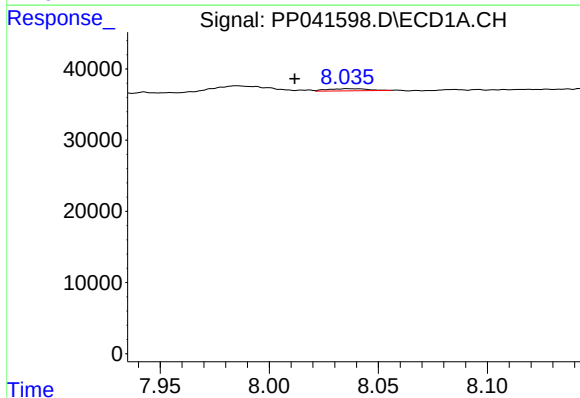


#32 AR-1260-2

R.T.: 8.035 min
Delta R.T.: 0.024 min
Response: 3862
Conc: 3.07 ng/ml

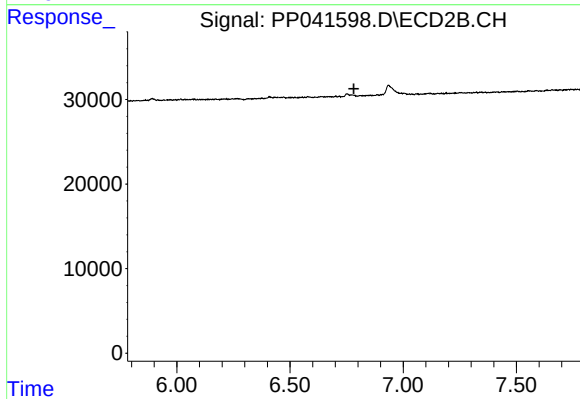

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

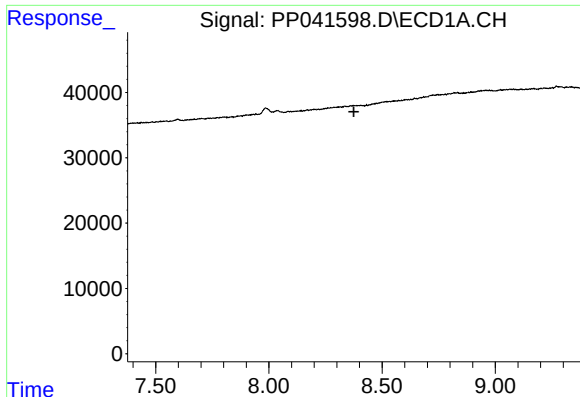

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

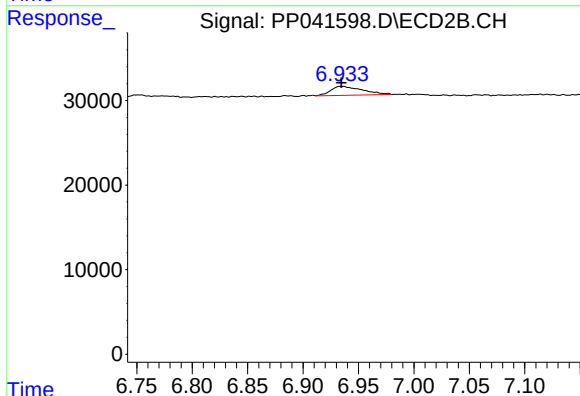


#33 AR-1260-3

R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 20980
Conc: 15.69 ng/ml

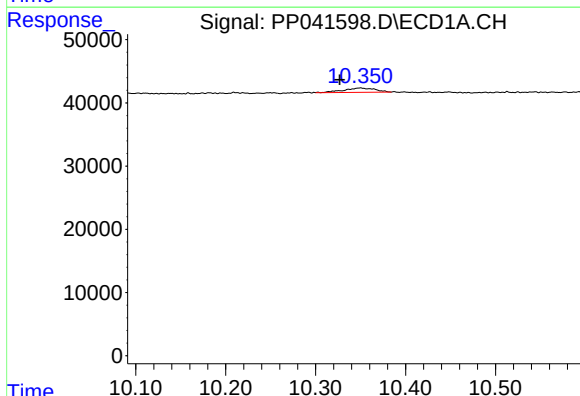

#45 AR-1268-5

R.T.: 10.350 min
Delta R.T.: 0.023 min
Response: 16287
Conc: 2.25 ng/ml

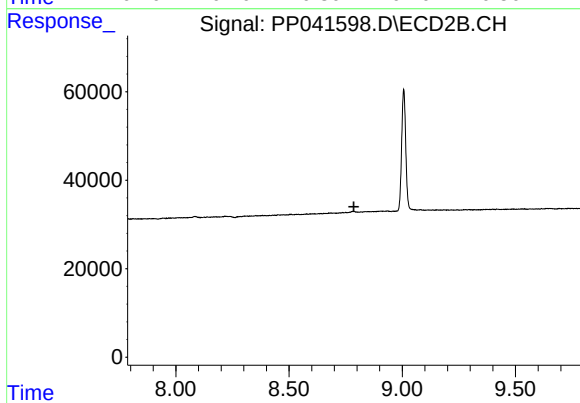

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 8.786 min
Response: 0
Conc: N.D.