

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
 Data File : PP041619.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2021 21:15
 Operator : AJ\MA
 Sample : M4919-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:13:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.745	3.750	475547	656587	21.089	21.615
2)	SA Decachlor...	10.637	9.006	428748	303696	19.912	19.650
Target Compounds							
8)	L2 AR-1221-1	4.996	0.000	20196	0	76.839	N.D. #
9)	L2 AR-1221-2	5.093	0.000	8175	0	43.623	N.D. #
10)	L2 AR-1221-3	5.180	0.000	946	0	1.518	N.D. #
11)	L3 AR-1232-1	5.180	0.000	946	0	1.831	N.D. #
32)	L7 AR-1260-2	8.007	0.000	2521	0	2.006	N.D. #
33)	L7 AR-1260-3	0.000	6.942	0	8351	N.D.	6.244 #
34)	L7 AR-1260-4	8.605	0.000	1580	0	1.476	N.D. #
45)	L9 AR-1268-5	10.341	0.000	4406	0	0.610	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
Data File : PP041619.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2021 21:15
Operator : AJ\MA
Sample : M4919-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:13:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

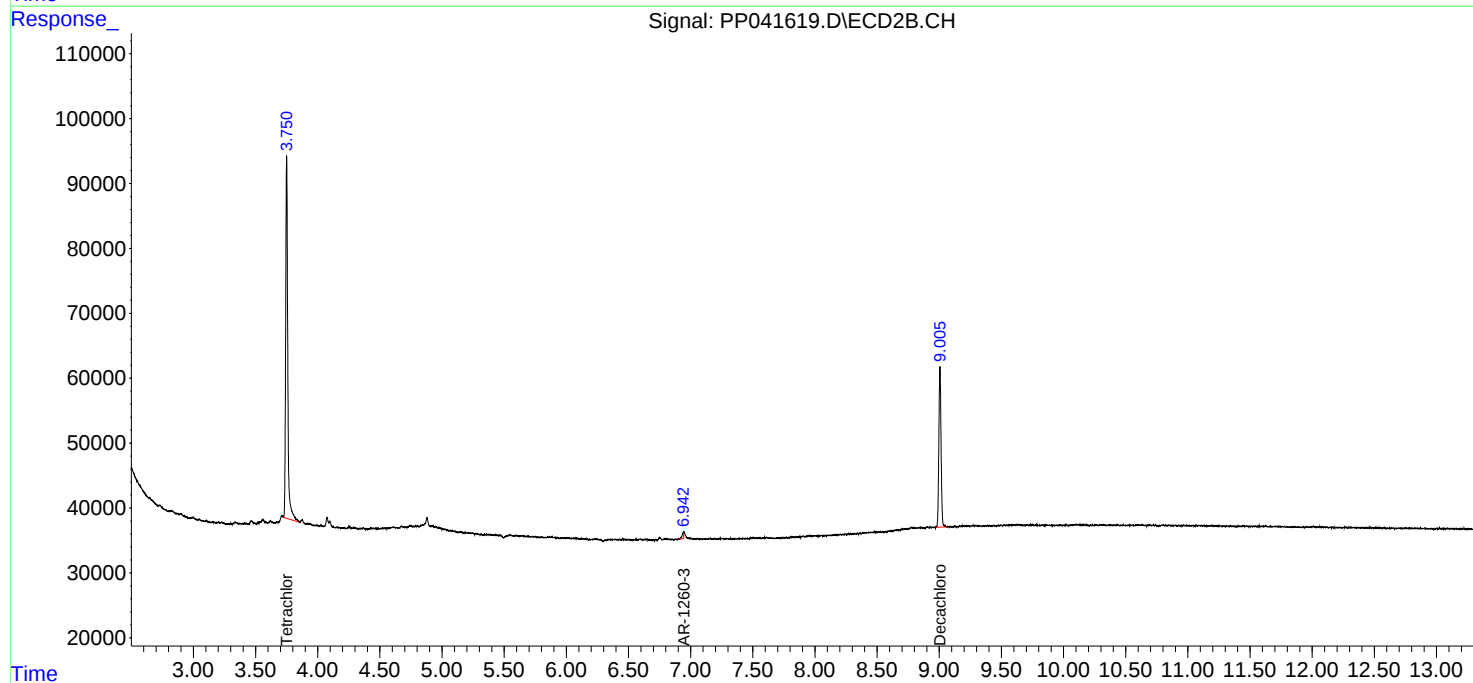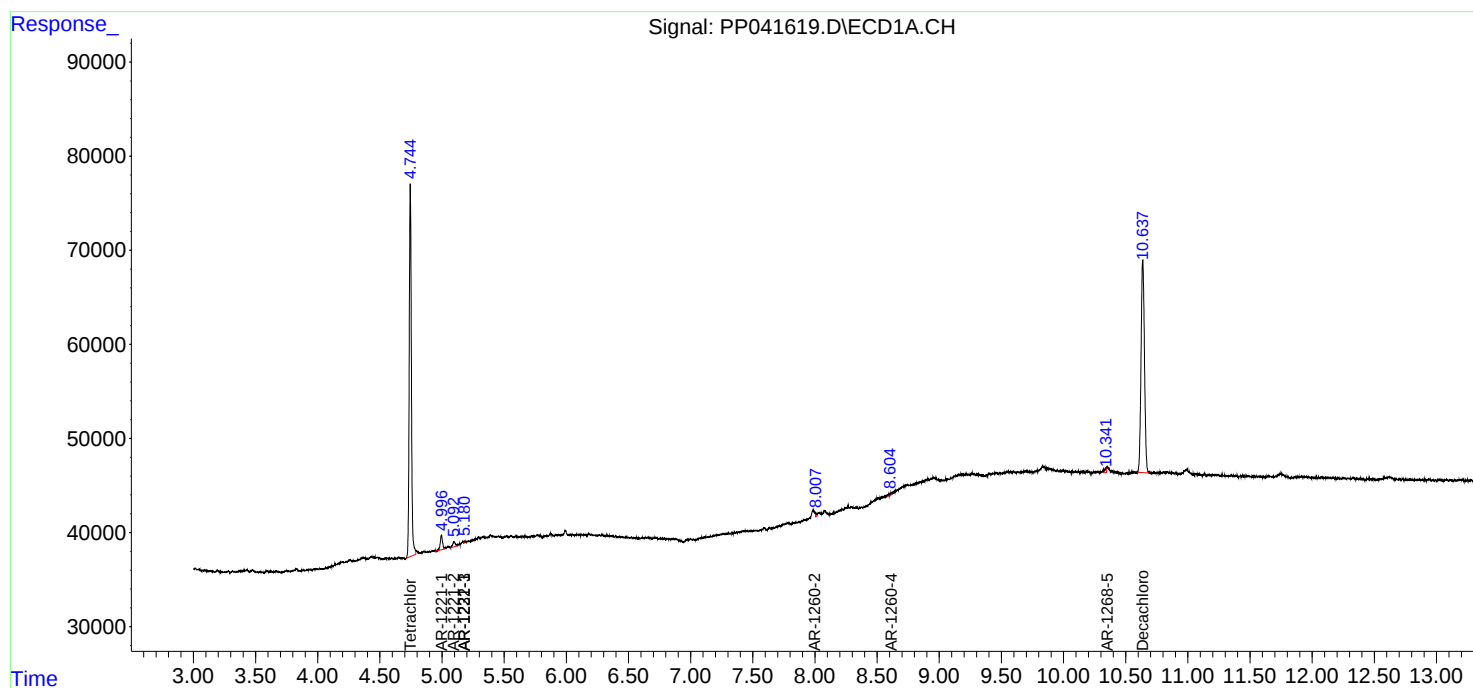


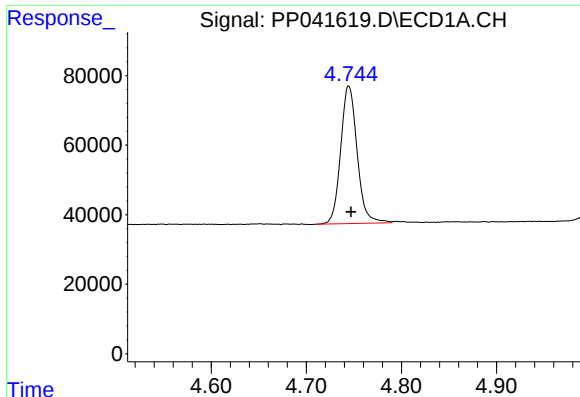

#1 Tetrachloro-m-xylene


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 475547
Conc: 21.09 ng/ml

Instrument :
ECD_P
ClientSampleId :

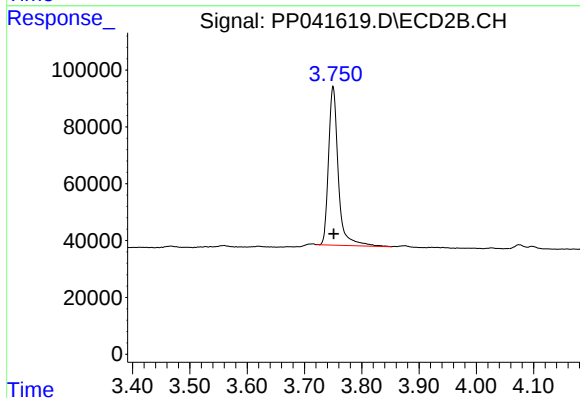


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.001 min
Response: 656587
Conc: 21.62 ng/ml

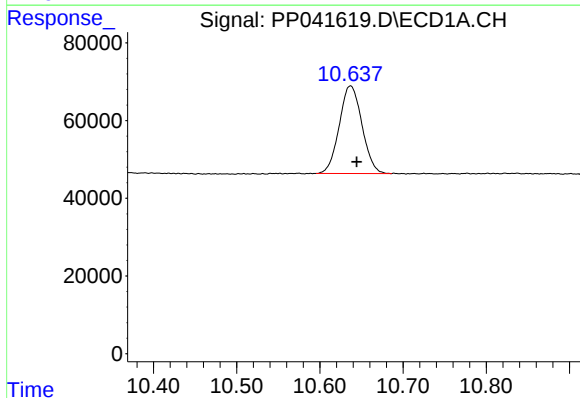


#2 Decachlorobiphenyl

R.T.: 10.637 min
Delta R.T.: -0.007 min
Response: 428748
Conc: 19.91 ng/ml

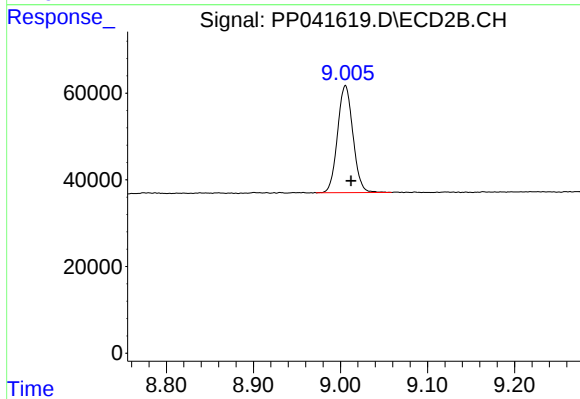

#2 Decachlorobiphenyl


R.T.: 9.006 min
Delta R.T.: -0.007 min
Response: 303696
Conc: 19.65 ng/ml

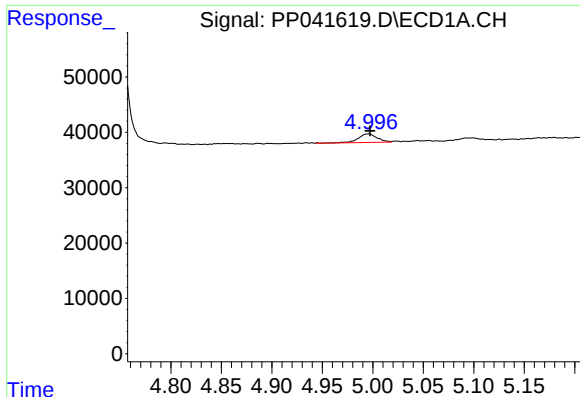

#8 AR-1221-1


R.T.: 4.996 min
Delta R.T.: -0.001 min
Response: 20196
Conc: 76.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

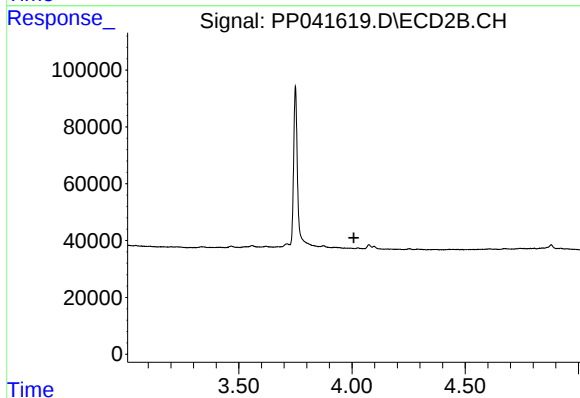


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.008 min
Response: 0
Conc: N.D.

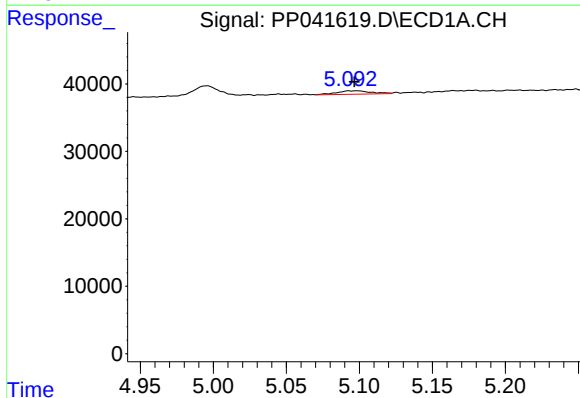


#9 AR-1221-2

R.T.: 5.093 min
Delta R.T.: -0.004 min
Response: 8175
Conc: 43.62 ng/ml

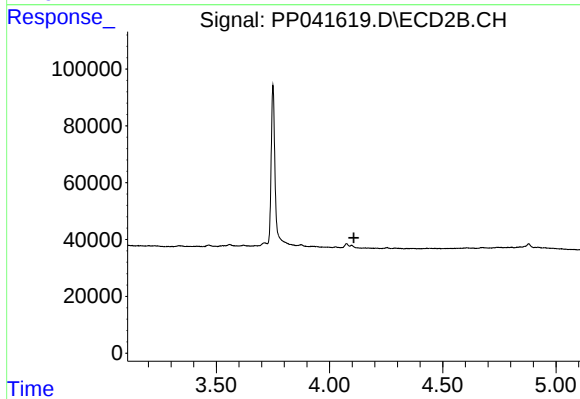

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

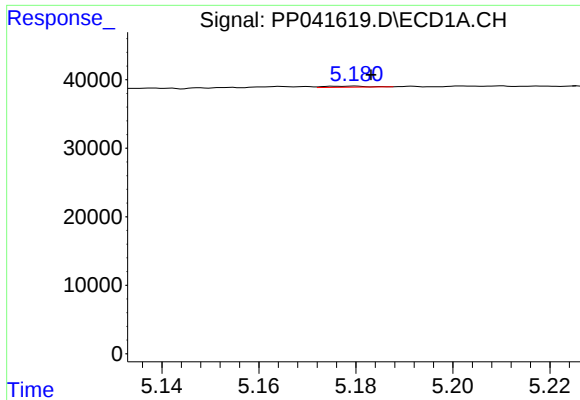

#10 AR-1221-3


R.T.: 5.180 min
Delta R.T.: -0.003 min
Response: 946
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

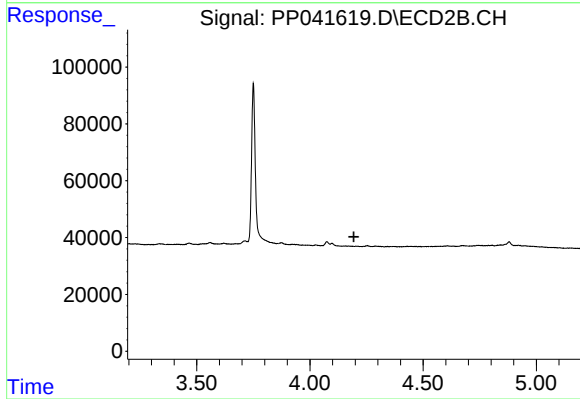


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.194 min
Response: 0
Conc: N.D.

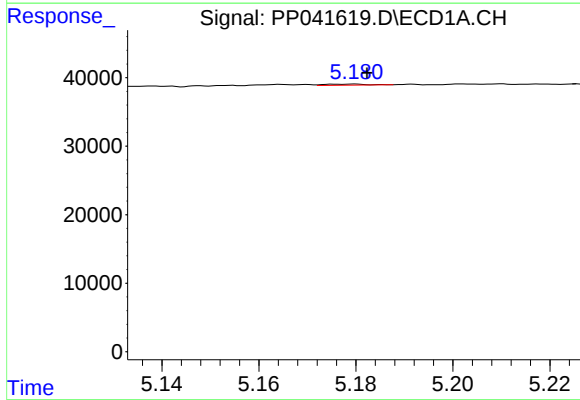


#11 AR-1232-1

R.T.: 5.180 min
Delta R.T.: -0.002 min
Response: 946
Conc: 1.83 ng/ml

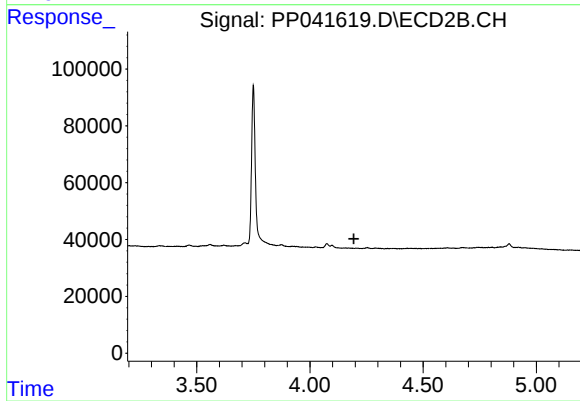

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.194 min
Response: 0
Conc: N.D.

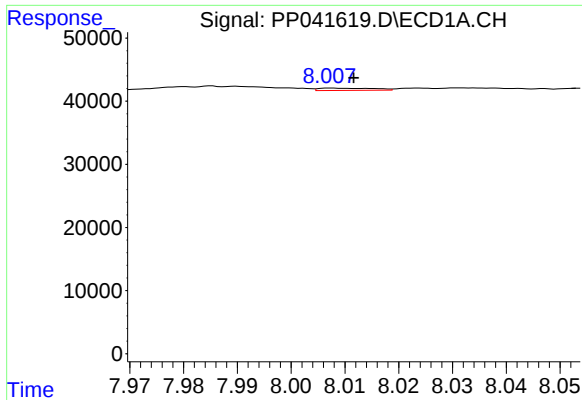

#32 AR-1260-2


R.T.: 8.007 min
Delta R.T.: -0.004 min
Response: 2521
Conc: 2.01 ng/ml

Instrument :
ECD_P
ClientSampleId :

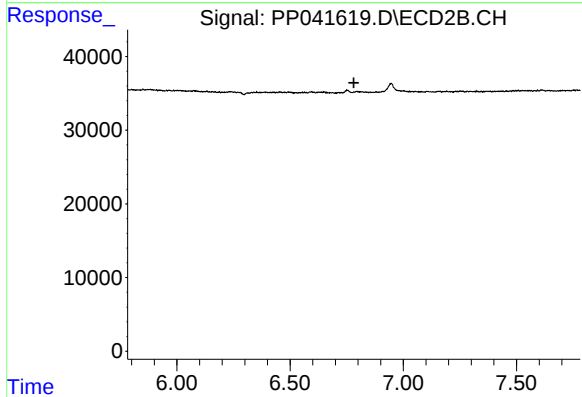


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

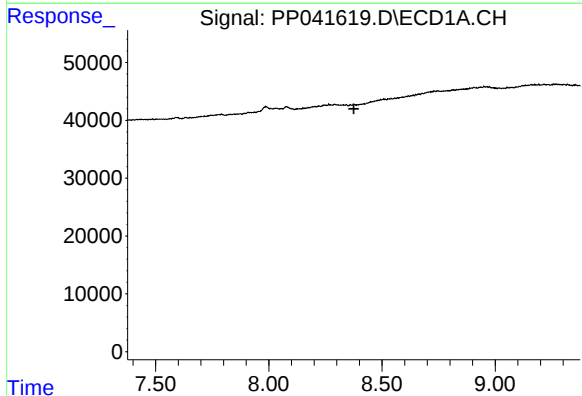


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

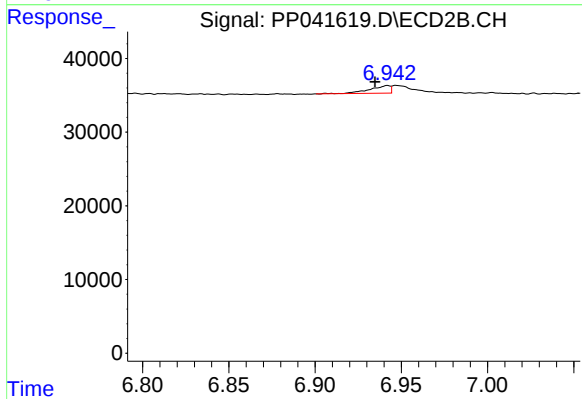

#33 AR-1260-3


R.T.: 6.942 min
Delta R.T.: 0.007 min
Response: 8351
Conc: 6.24 ng/ml

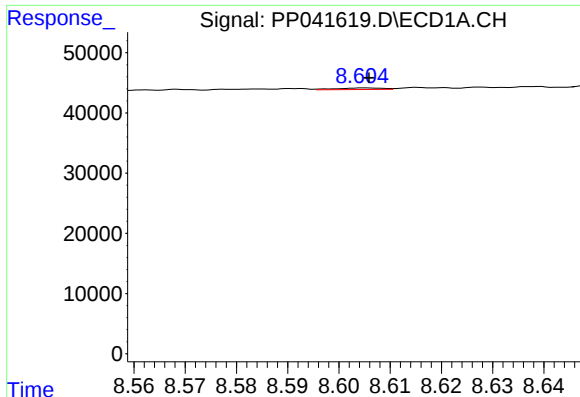

#34 AR-1260-4


R.T.: 8.605 min
Delta R.T.: 0.000 min
Response: 1580
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :

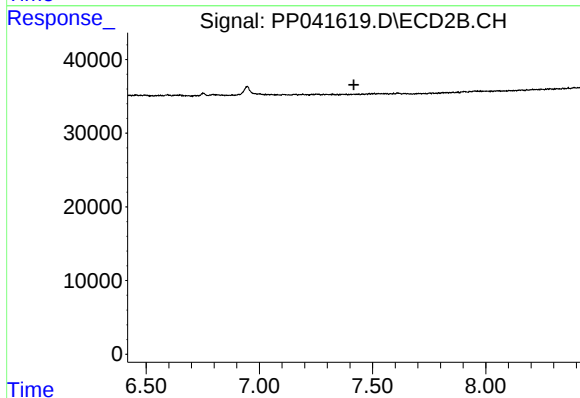


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

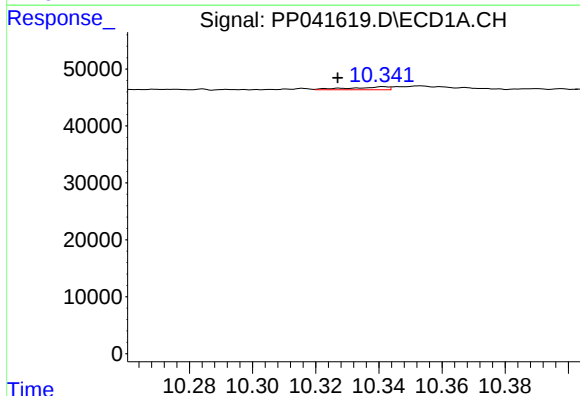

#45 AR-1268-5

R.T.: 10.341 min
Delta R.T.: 0.014 min
Response: 4406
Conc: 0.61 ng/ml

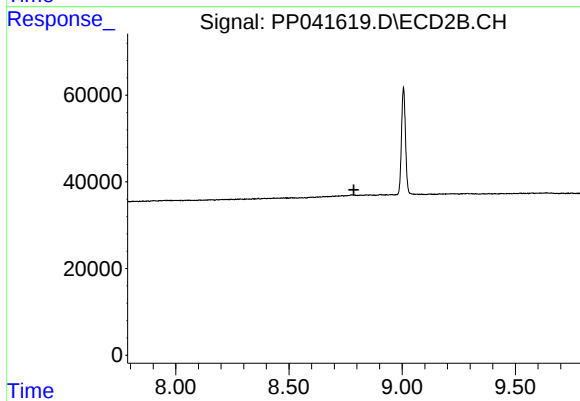

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.786 min
Response: 0
Conc: N.D.