

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
Data File : PP041617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2021 20:42
Operator : AJ\MA
Sample : M4919-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FDR-MW-2-20211202

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:12:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.745	3.751	459917	682291	20.396	22.462
2) SA Decachlor...	10.639	9.005	392574	277950	18.232	17.984

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
Data File : PP041617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2021 20:42
Operator : AJ\MA
Sample : M4919-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FDR-MW-2-20211202

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:12:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

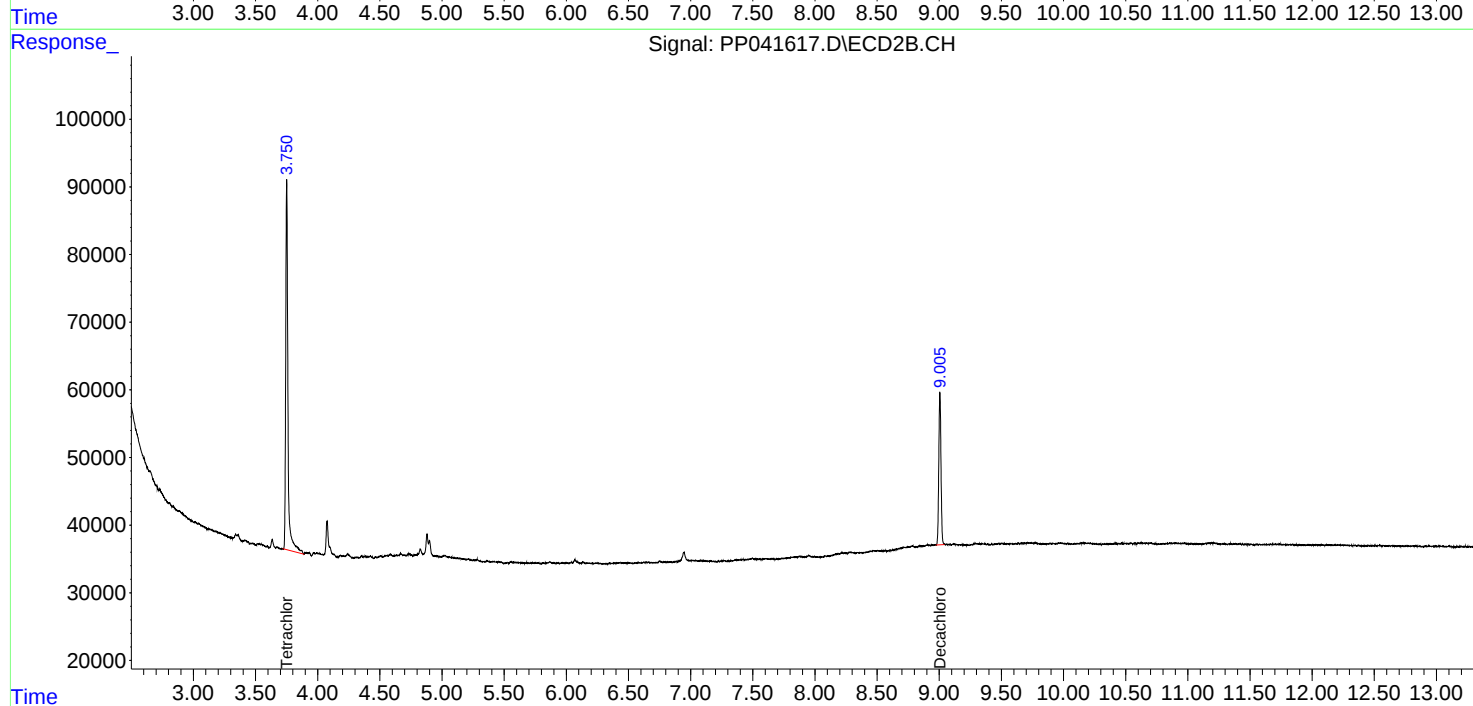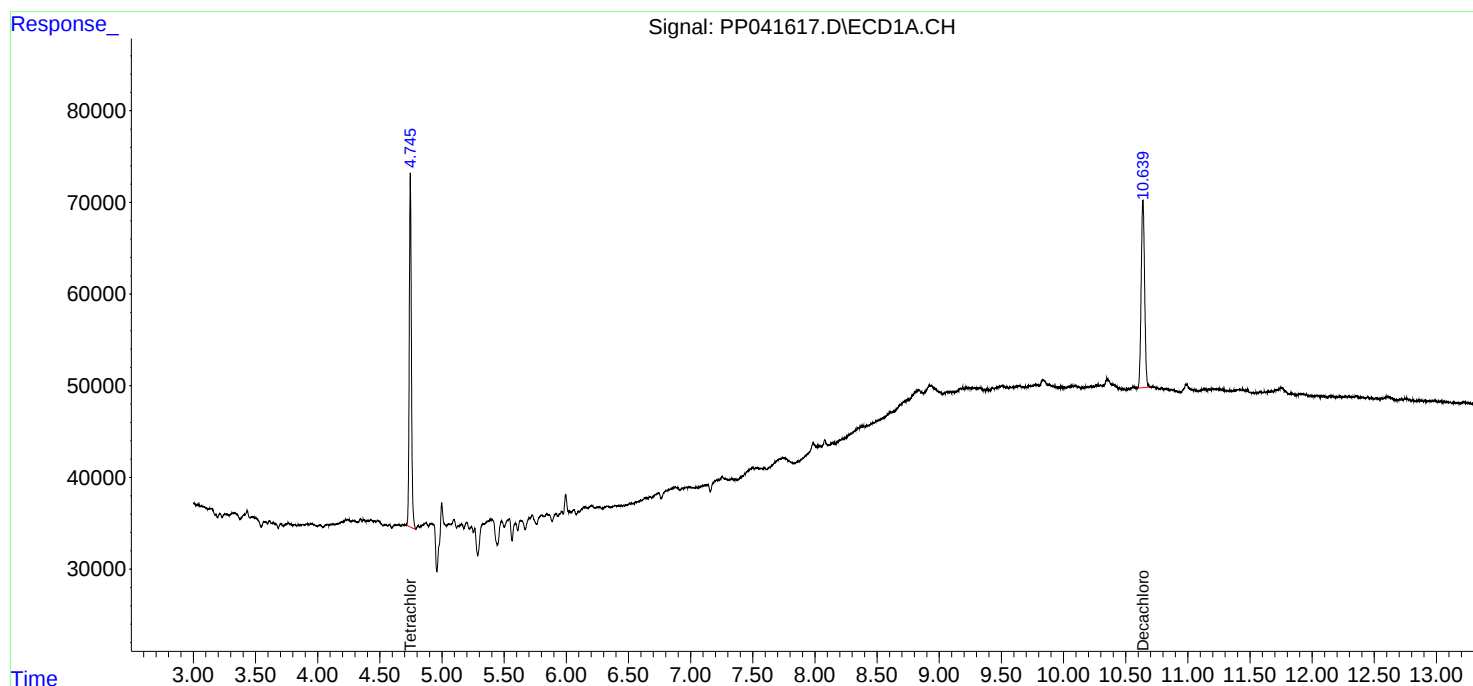


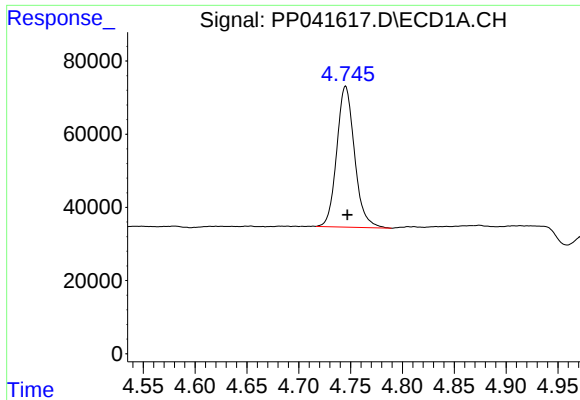

#1 Tetrachloro-m-xylene


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 459917
Conc: 20.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDR-MW-2-20211202

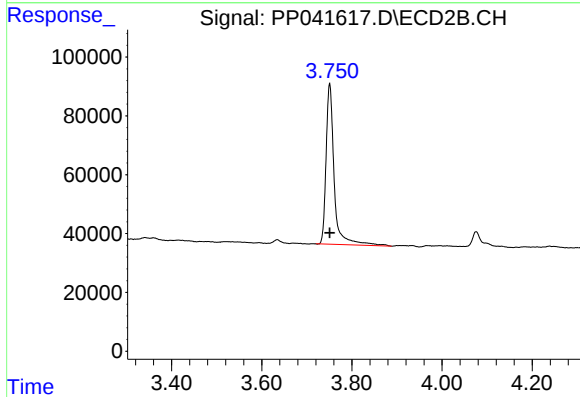


#1 Tetrachloro-m-xylene

R.T.: 3.751 min
Delta R.T.: 0.000 min
Response: 682291
Conc: 22.46 ng/ml

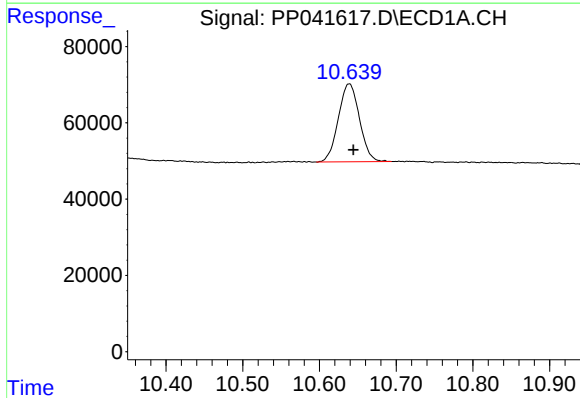

#2 Decachlorobiphenyl

R.T.: 10.639 min
Delta R.T.: -0.005 min
Response: 392574
Conc: 18.23 ng/ml

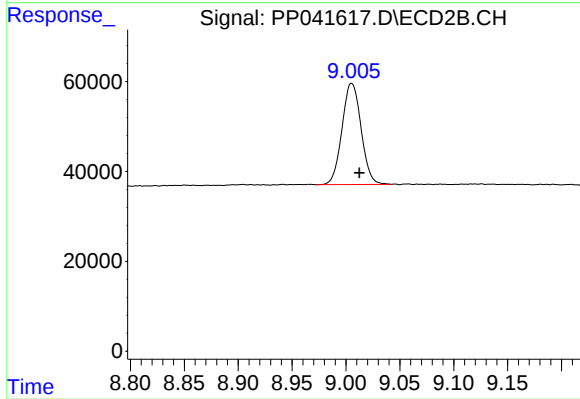

#2 Decachlorobiphenyl

R.T.: 9.005 min
Delta R.T.: -0.007 min
Response: 277950
Conc: 17.98 ng/ml