

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
 Data File : PP041623.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2021 22:22
 Operator : AJ\MA
 Sample : M4919-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EB-20211202

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:14:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.745	3.750	483407	680797	21.438	22.412
2)	SA Decachlor...	10.638	9.005	458415	319285	21.289	20.659

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120321\
Data File : PP041623.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2021 22:22
Operator : AJ\MA
Sample : M4919-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
EB-20211202

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:14:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

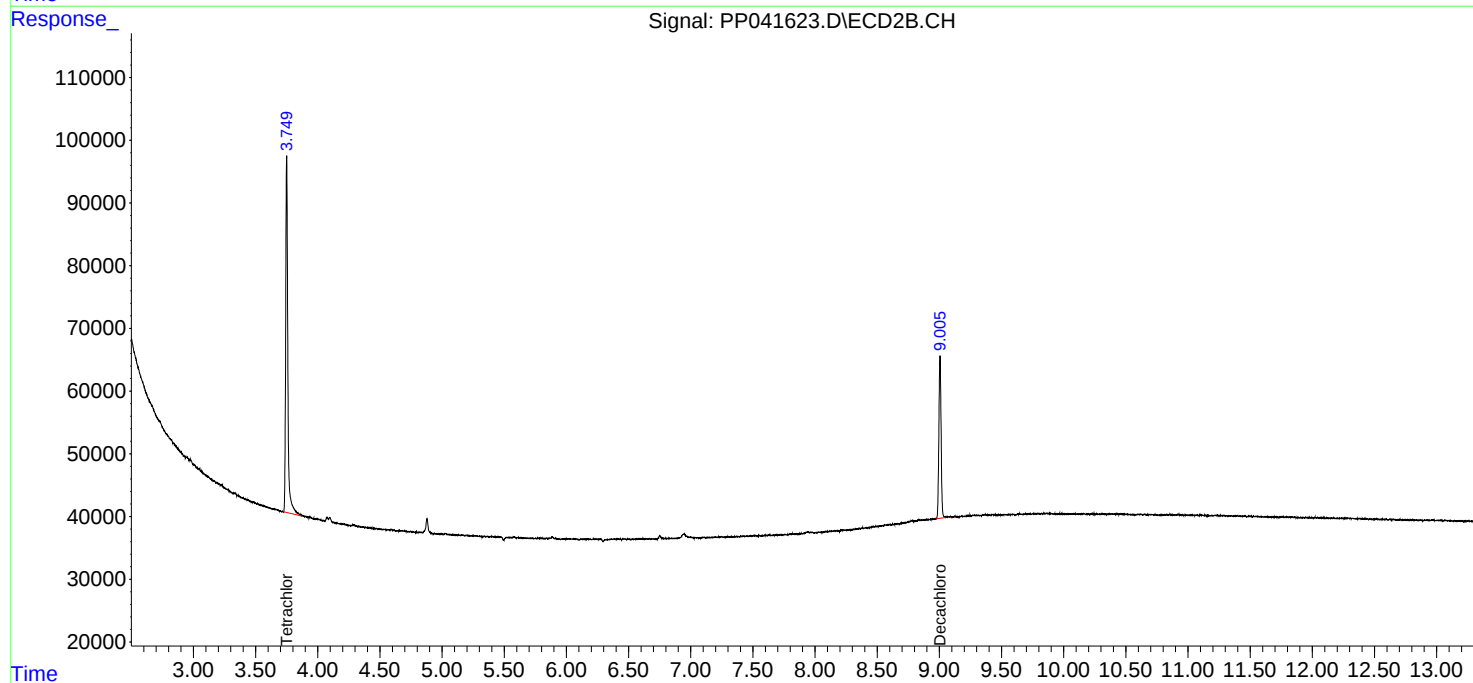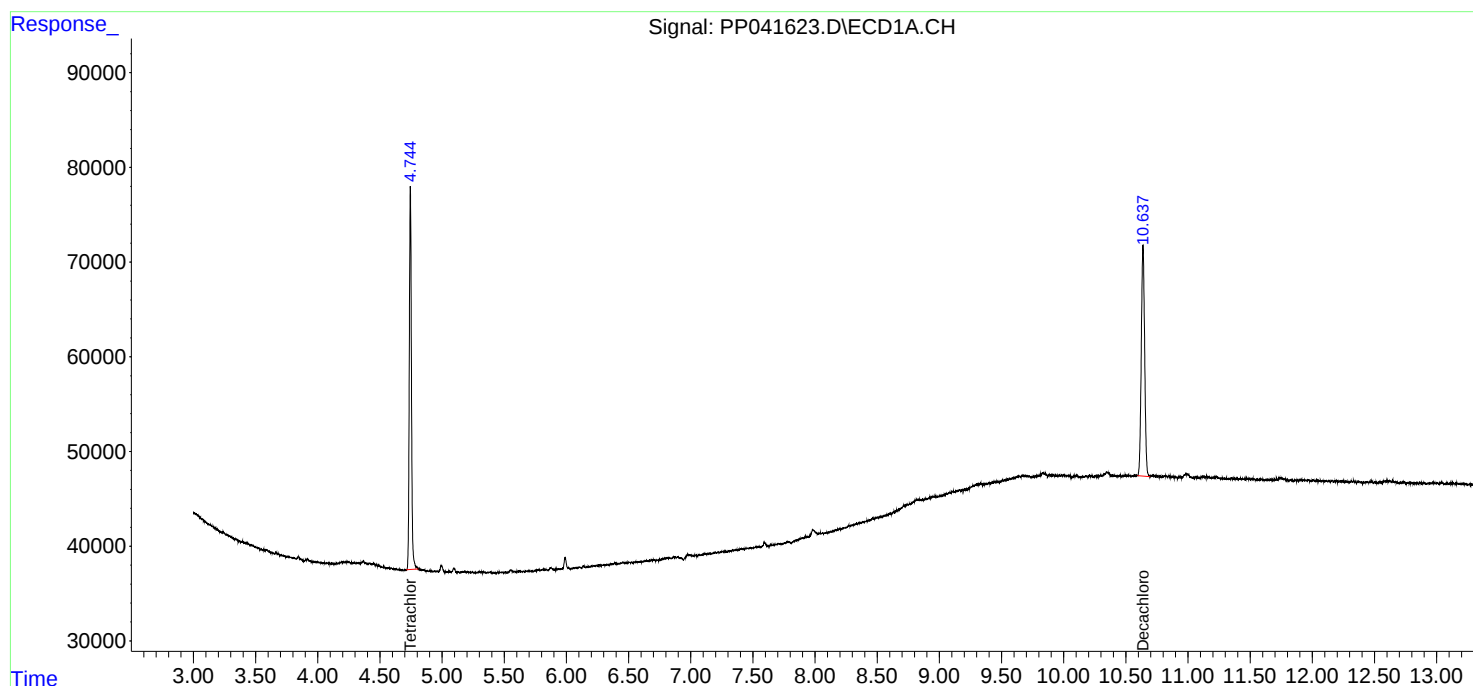


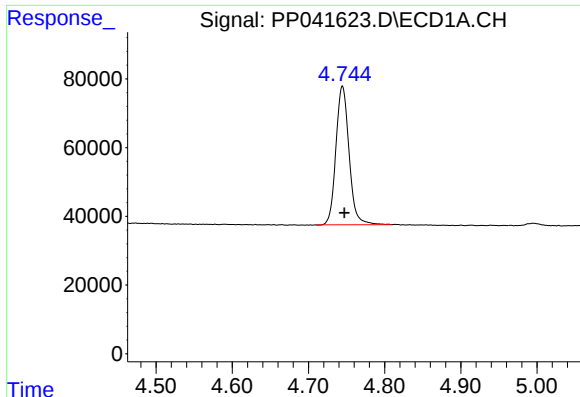

#1 Tetrachloro-m-xylene


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 483407
Conc: 21.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
EB-20211202

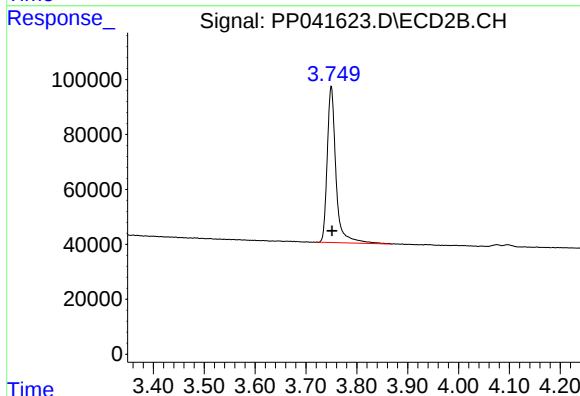


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.001 min
Response: 680797
Conc: 22.41 ng/ml

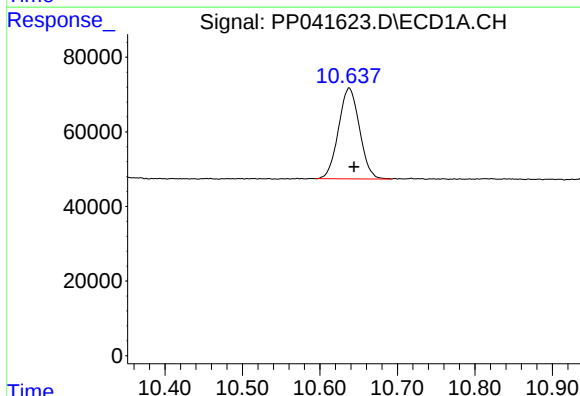

#2 Decachlorobiphenyl

R.T.: 10.638 min
Delta R.T.: -0.006 min
Response: 458415
Conc: 21.29 ng/ml

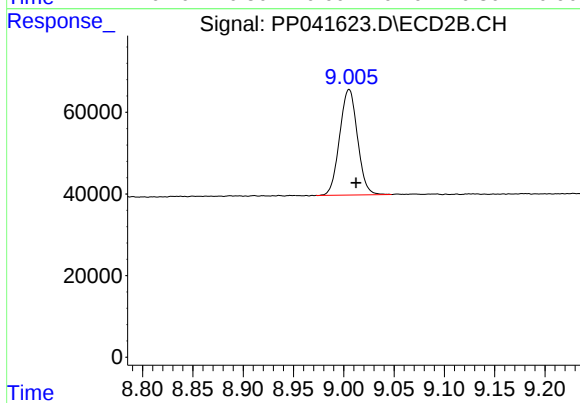

#2 Decachlorobiphenyl

R.T.: 9.005 min
Delta R.T.: -0.007 min
Response: 319285
Conc: 20.66 ng/ml