

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120325\
 Data File : PP076755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2025 15:09
 Operator : YP\AJ
 Sample : Q3749-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-25-0204

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/04/2025
 Supervised By :mohammad ahmed 12/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:58:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.613	3.770	3289484	4994403	1.792m	2.398m#
2) SA Decachlor...	10.365	8.766	2202968	2468311	1.470	1.399

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120325\
Data File : PP076755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2025 15:09
Operator : YP\AJ
Sample : Q3749-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-25-0204


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/04/2025
Supervised By :mohammad ahmed 12/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:58:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

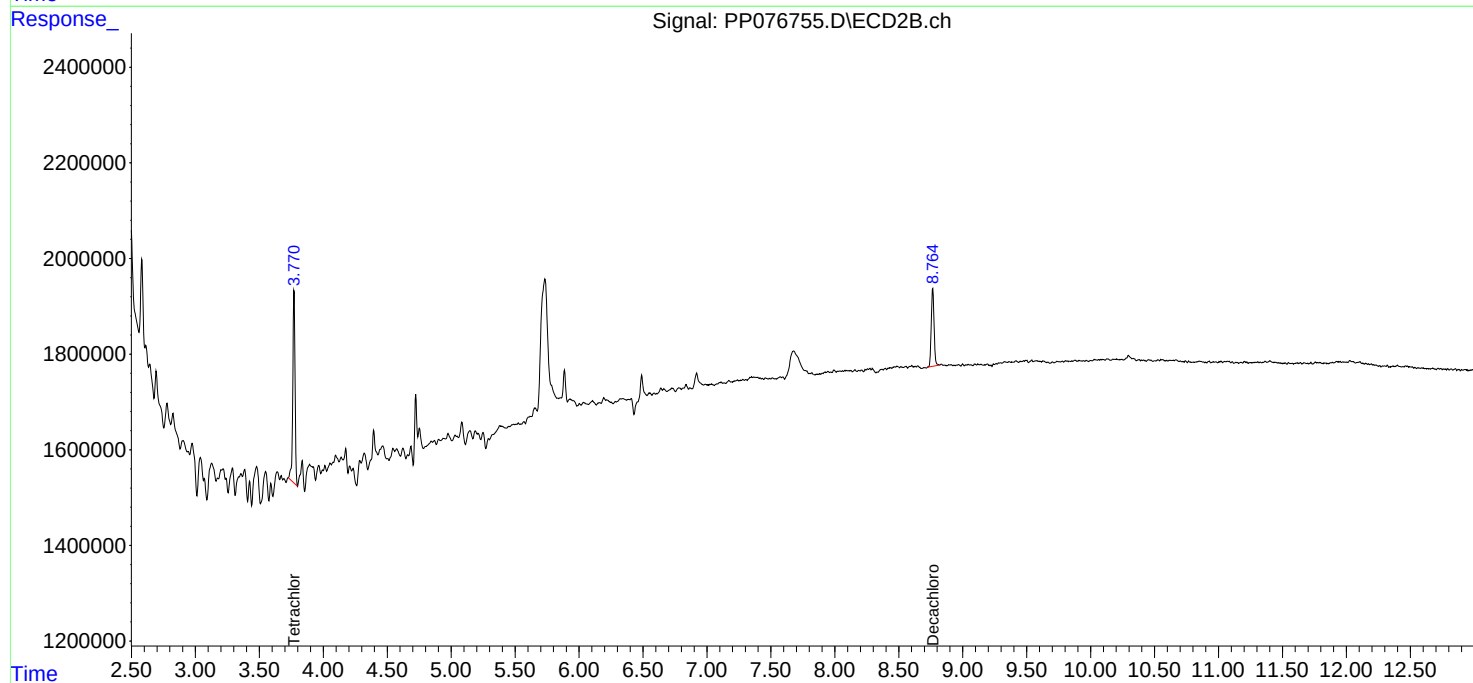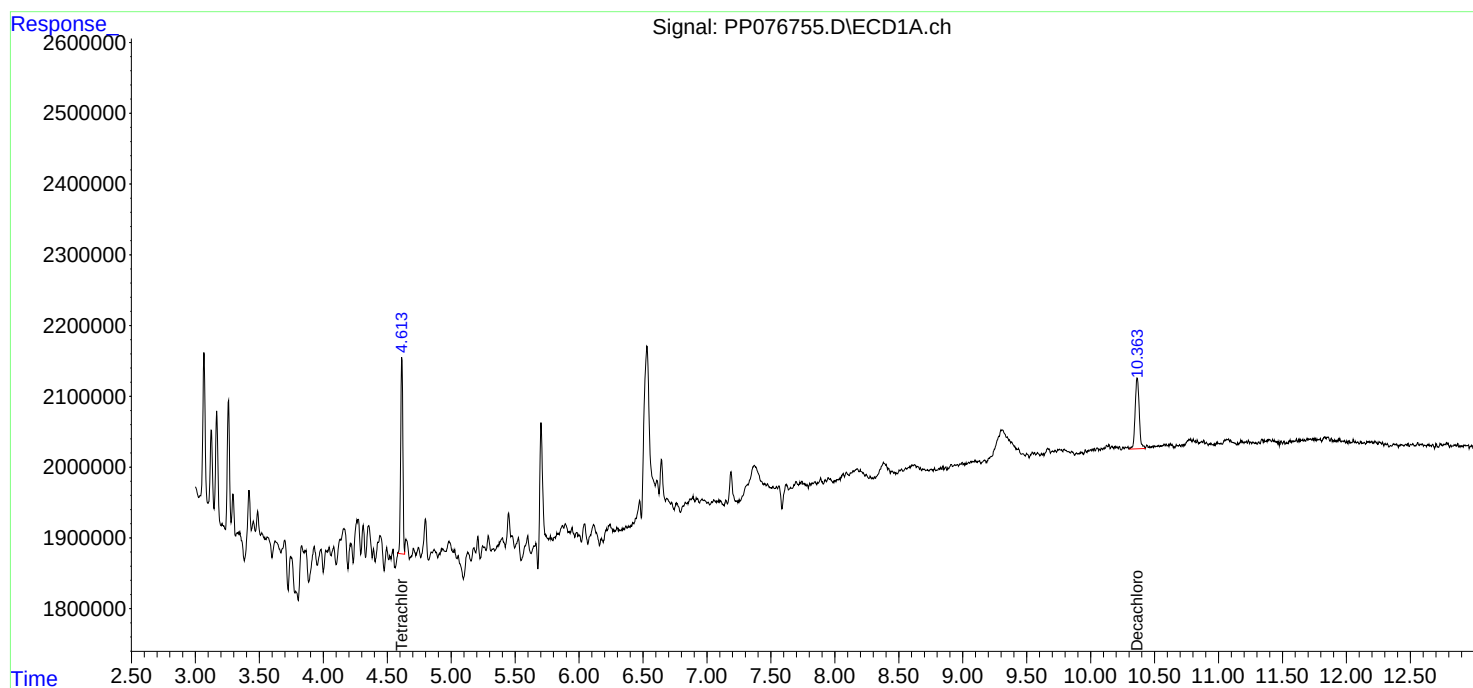

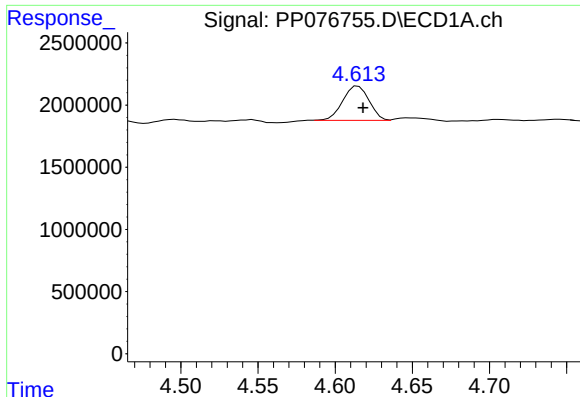


#1 Tetrachloro-m-xylene

R.T.: 4.613 min
Delta R.T.: -0.005 min
Response: 3289484
Conc: 1.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-25-0204


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/04/2025
Supervised By :mohammad ahmed 12/05/2025

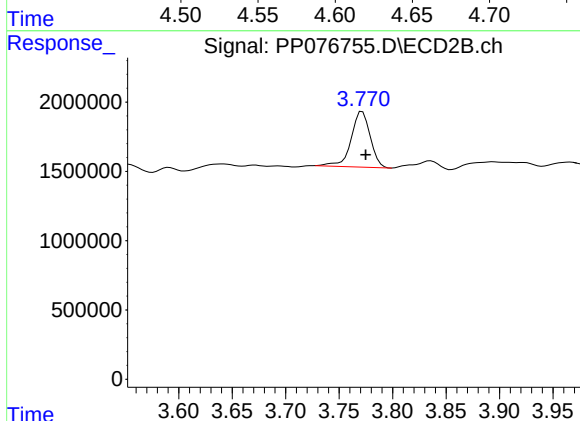


#1 Tetrachloro-m-xylene

R.T.: 3.770 min
Delta R.T.: -0.005 min
Response: 4994403
Conc: 2.40 ng/ml m

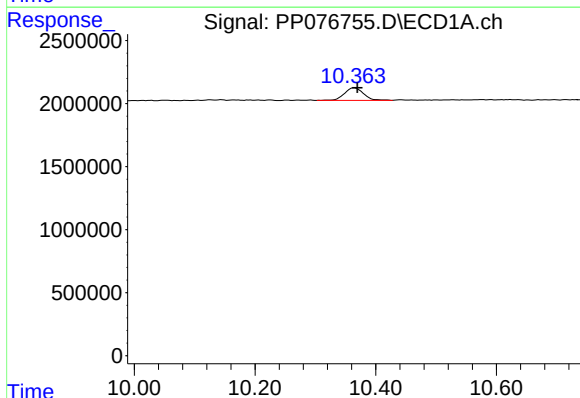

#2 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: -0.005 min
Response: 2202968
Conc: 1.47 ng/ml

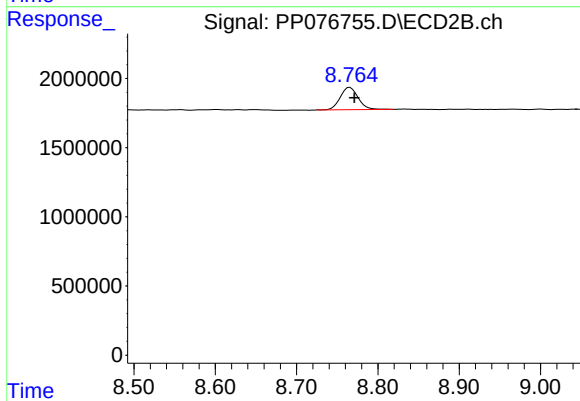

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.006 min
Response: 2468311
Conc: 1.40 ng/ml