

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120523\
 Data File : PP062154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 14:48
 Operator : YP\AJ
 Sample : 05606-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-111723-103-25

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/06/2023
 Supervised By :Ankita Jodhani 12/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:24:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.721	32020990	40272327	24.324	22.381
2) SA Decachlor...	10.240	8.843	26174939	47639232	25.363	23.082

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120523\
Data File : PP062154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2023 14:48
Operator : YP\AJ
Sample : 05606-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-111723-103-25


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/06/2023
Supervised By :Ankita Jodhani 12/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:24:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

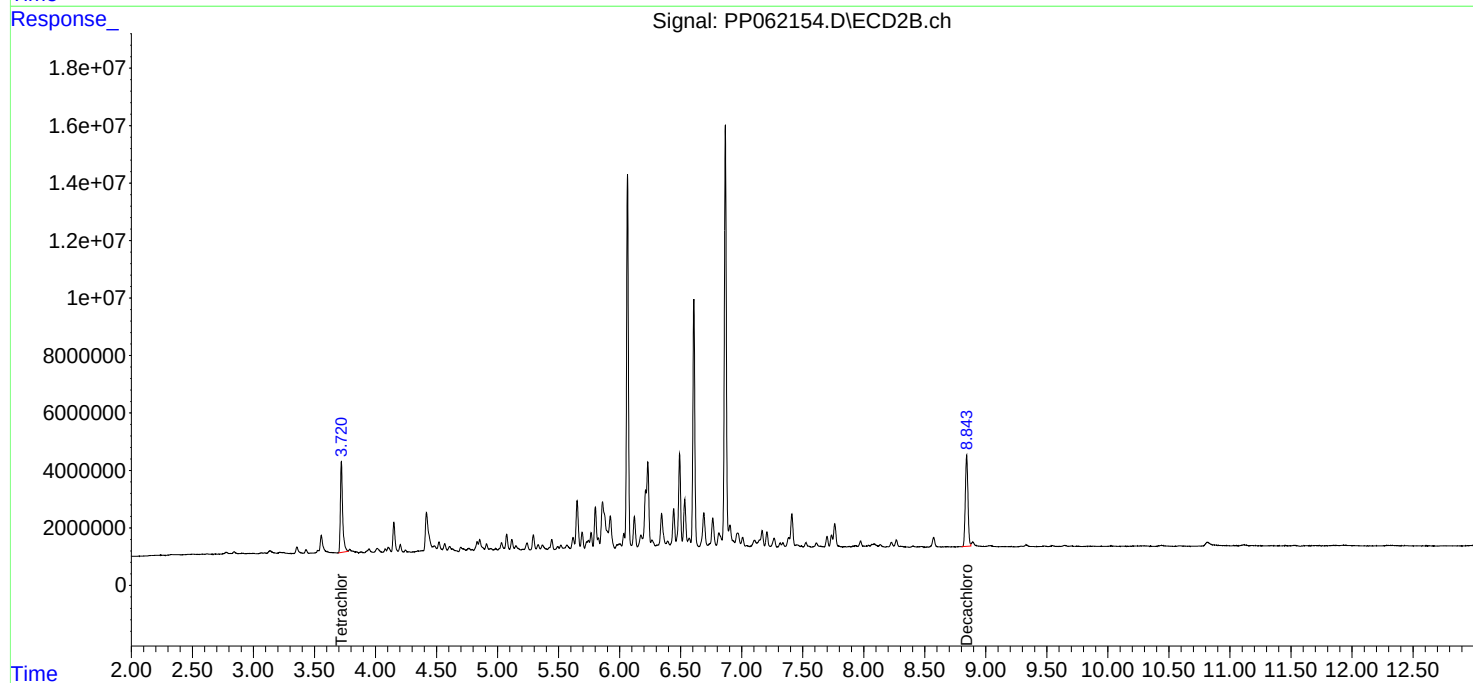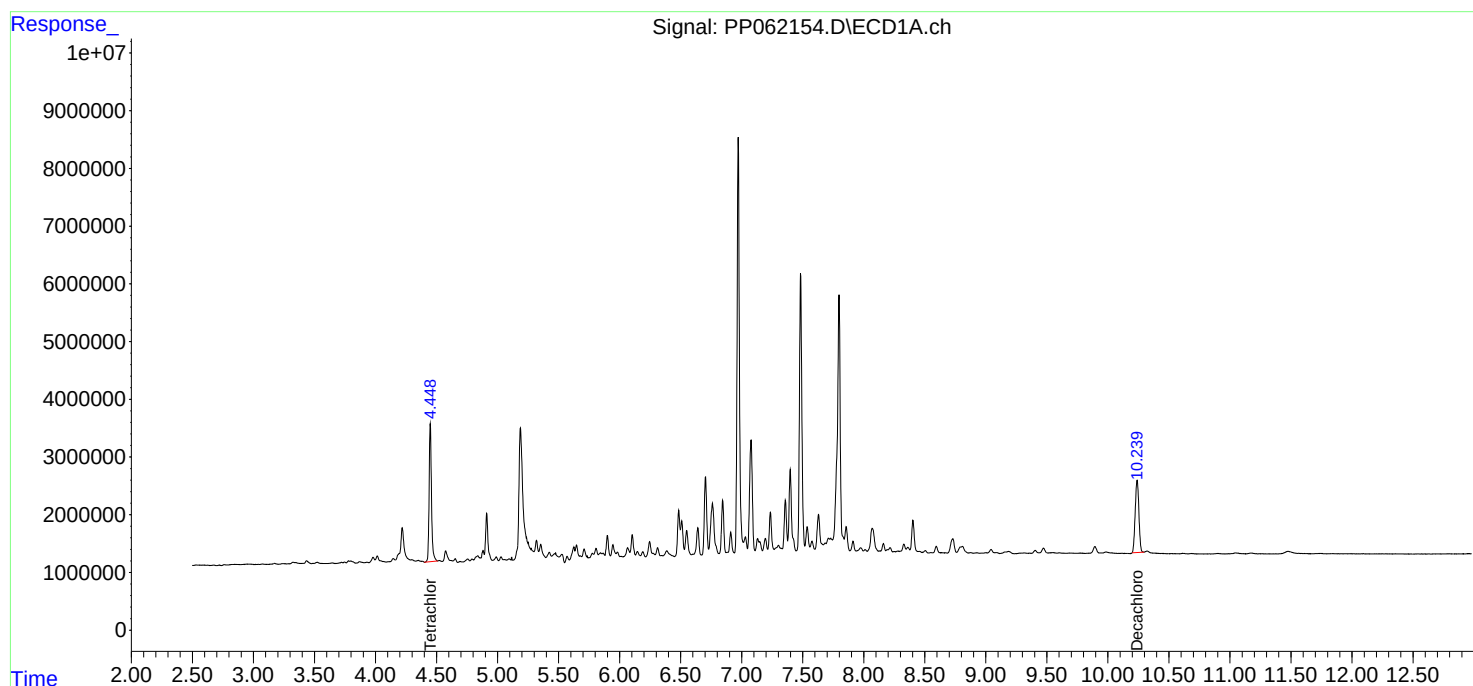

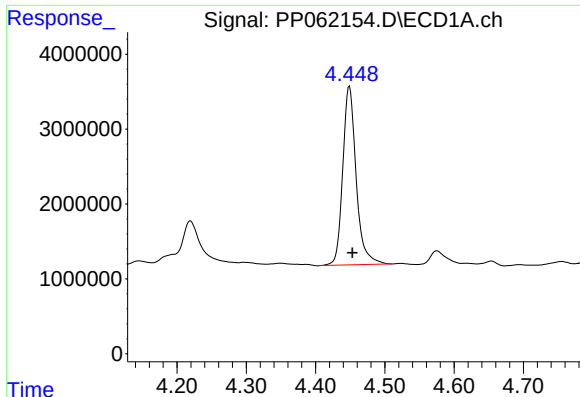


#1 Tetrachloro-m-xylene

R.T.: 4.449 min
Delta R.T.: -0.004 min
Response: 32020990
Conc: 24.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-111723-103-25


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/06/2023
Supervised By :Ankita Jodhani 12/06/2023

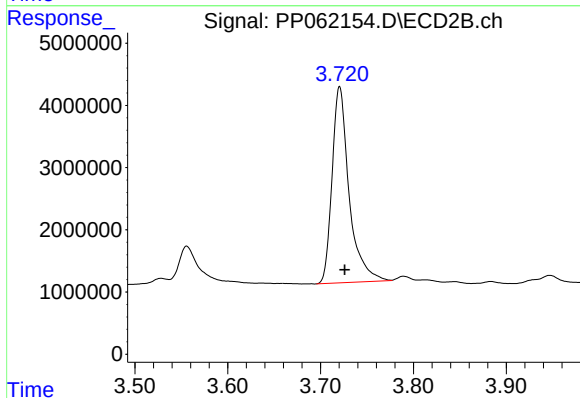


#1 Tetrachloro-m-xylene

R.T.: 3.721 min
Delta R.T.: -0.005 min
Response: 40272327
Conc: 22.38 ng/ml

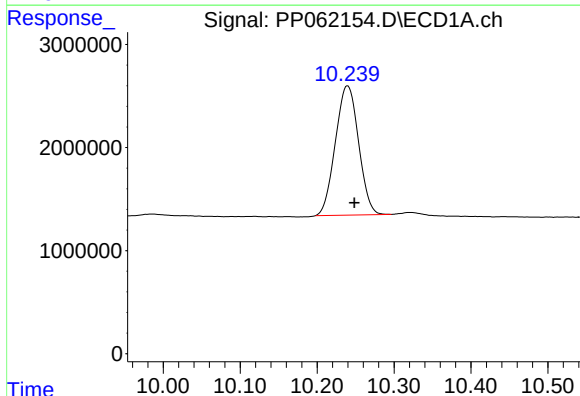

#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: -0.009 min
Response: 26174939
Conc: 25.36 ng/ml

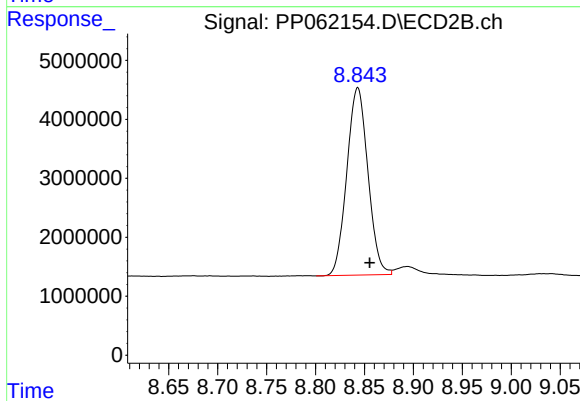

#2 Decachlorobiphenyl

R.T.: 8.843 min
Delta R.T.: -0.012 min
Response: 47639232
Conc: 23.08 ng/ml