

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120524\
 Data File : PP068828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 02:32
 Operator : YP\AJ
 Sample : P5102-05 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC247637-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/09/2024
 Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:51:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.759	4.047	1509262	1668576	1.555m	1.723m
2) SA Decachlor...	10.677	9.203	2266816	2048138	1.811	1.811m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120524\
Data File : PP068828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 02:32
Operator : YP\AJ
Sample : P5102-05 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC247637-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:51:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

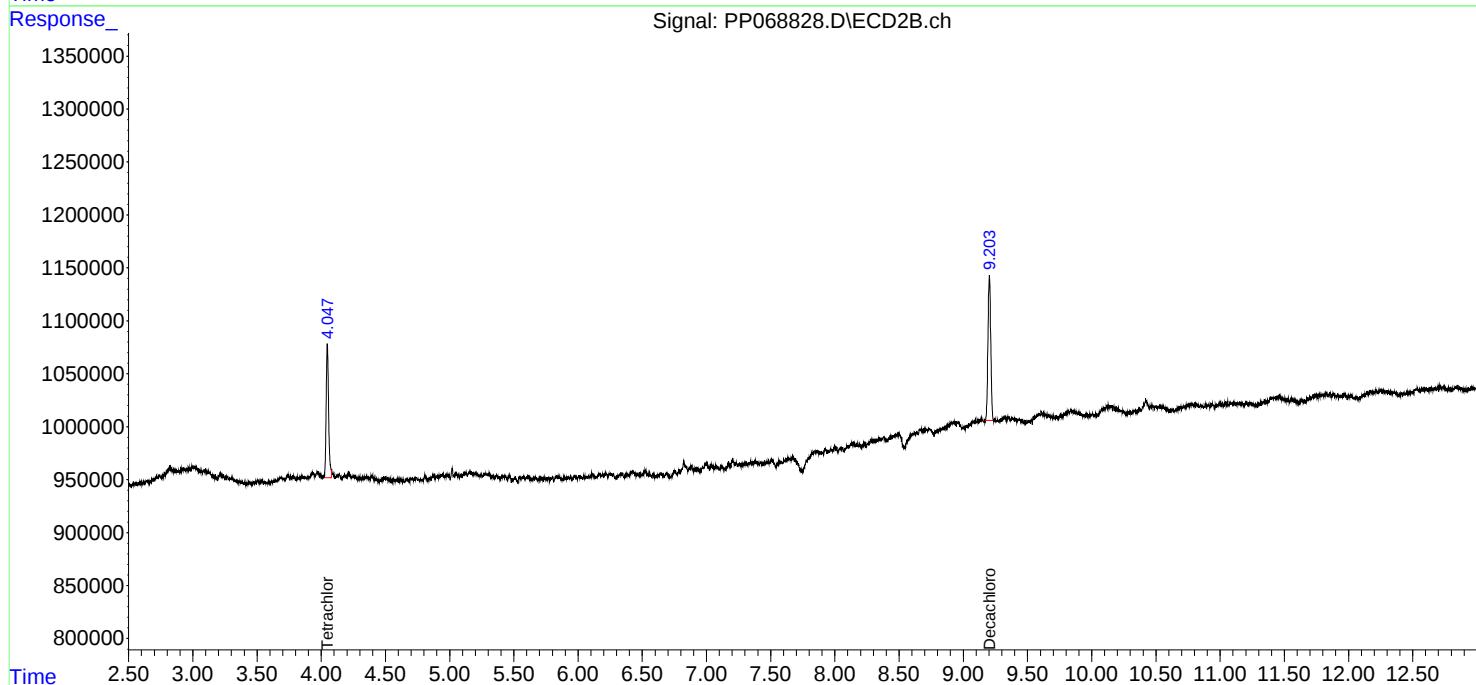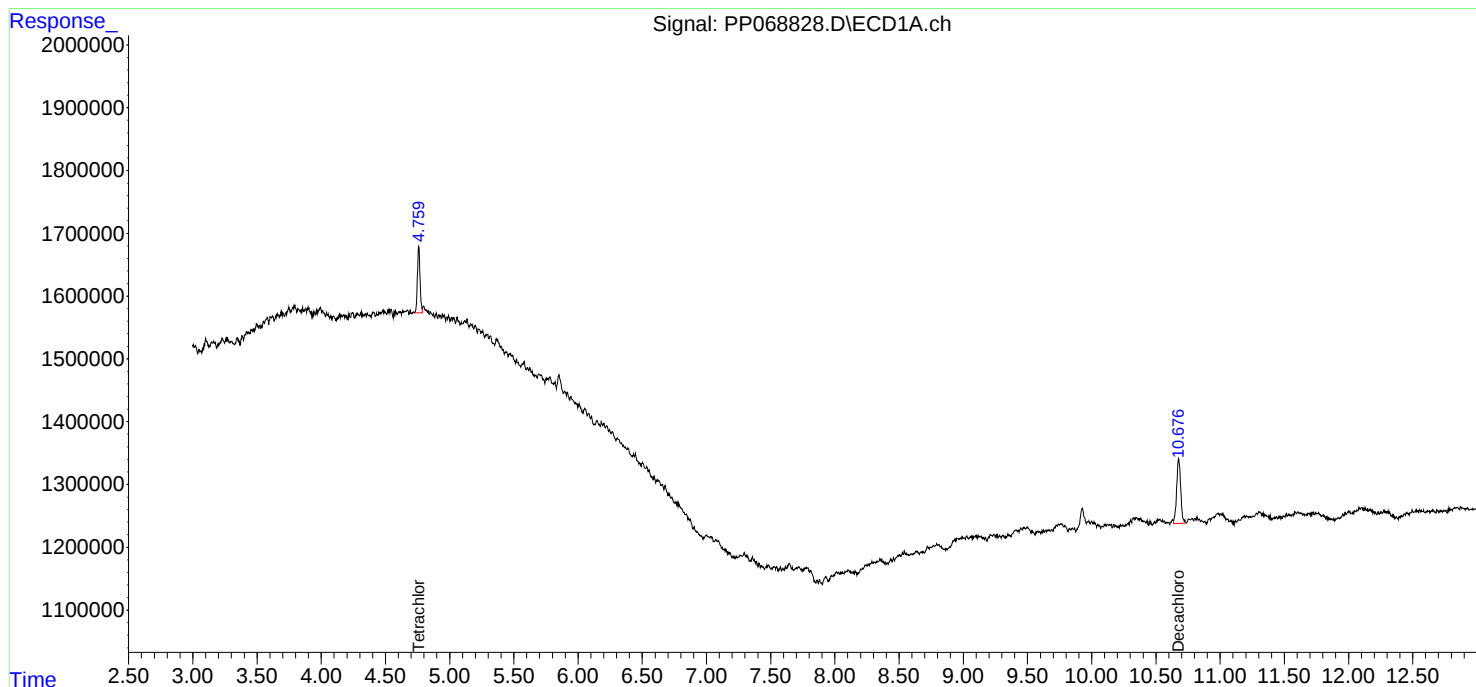

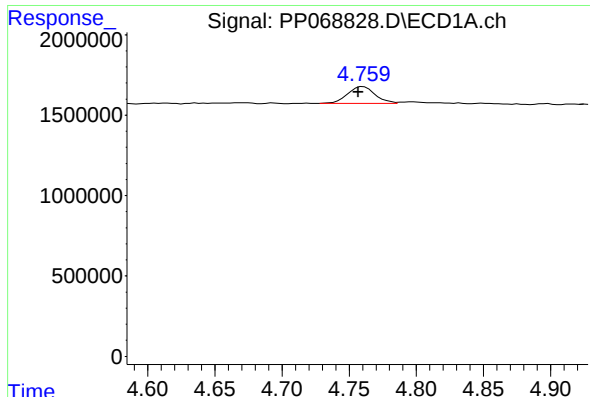


#1 Tetrachloro-m-xylene

R.T.: 4.759 min
Delta R.T.: 0.002 min
Response: 1509262
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC247637-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

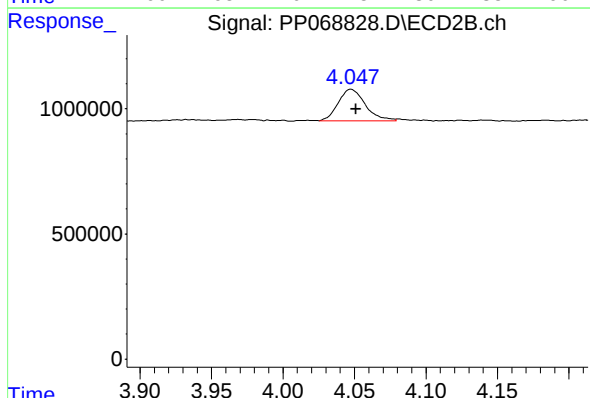


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: -0.004 min
Response: 1668576
Conc: 1.72 ng/ml m

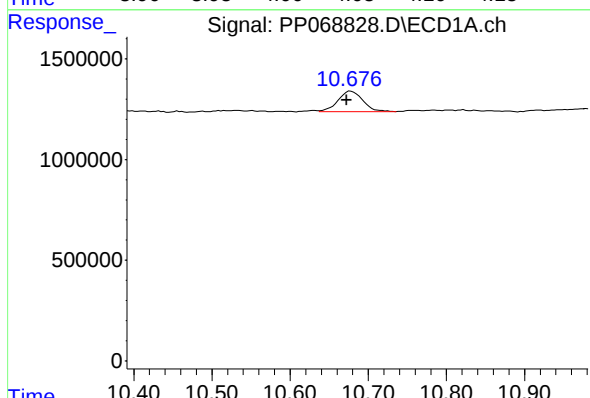

#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: 0.005 min
Response: 2266816
Conc: 1.81 ng/ml

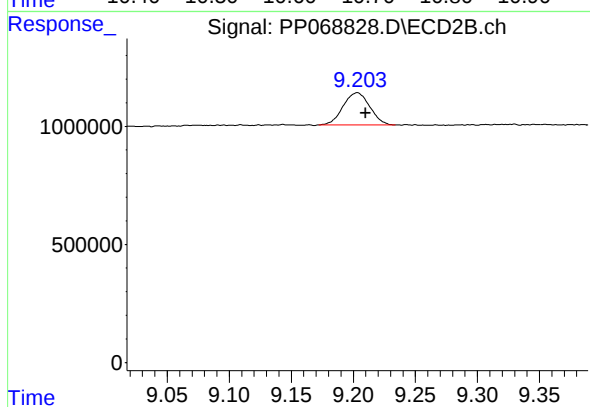

#2 Decachlorobiphenyl

R.T.: 9.203 min
Delta R.T.: -0.007 min
Response: 2048138
Conc: 1.81 ng/ml m