

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
 Data File : PP041639.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Dec 2021 12:52
 Operator : AJ\MA
 Sample : M4904-05 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 23:51:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.745	3.750	32620	54353	1.447	1.789
2) SA Decachlor...	10.639	9.007	28211	25303	1.310	1.637
Target Compounds						
4) L1 AR-1016-2	6.110f	0.000	1713	0	1.438	N.D. #
13) L3 AR-1232-3	6.110f	0.000	1713	0	3.462	N.D. #
17) L4 AR-1242-2	6.110f	0.000	1713	0	1.866	N.D. #
29) L6 AR-1254-4	7.858f	0.000	1379	0	1.329	N.D. #
32) L7 AR-1260-2	7.983f	0.000	8997	0	7.161	N.D. #
34) L7 AR-1260-4	8.579f	0.000	1518	0	1.419	N.D. #
45) L9 AR-1268-5	10.345f	0.000	568	0	0.079	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
Data File : PP041639.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Dec 2021 12:52
Operator : AJ\MA
Sample : M4904-05 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 23:51:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

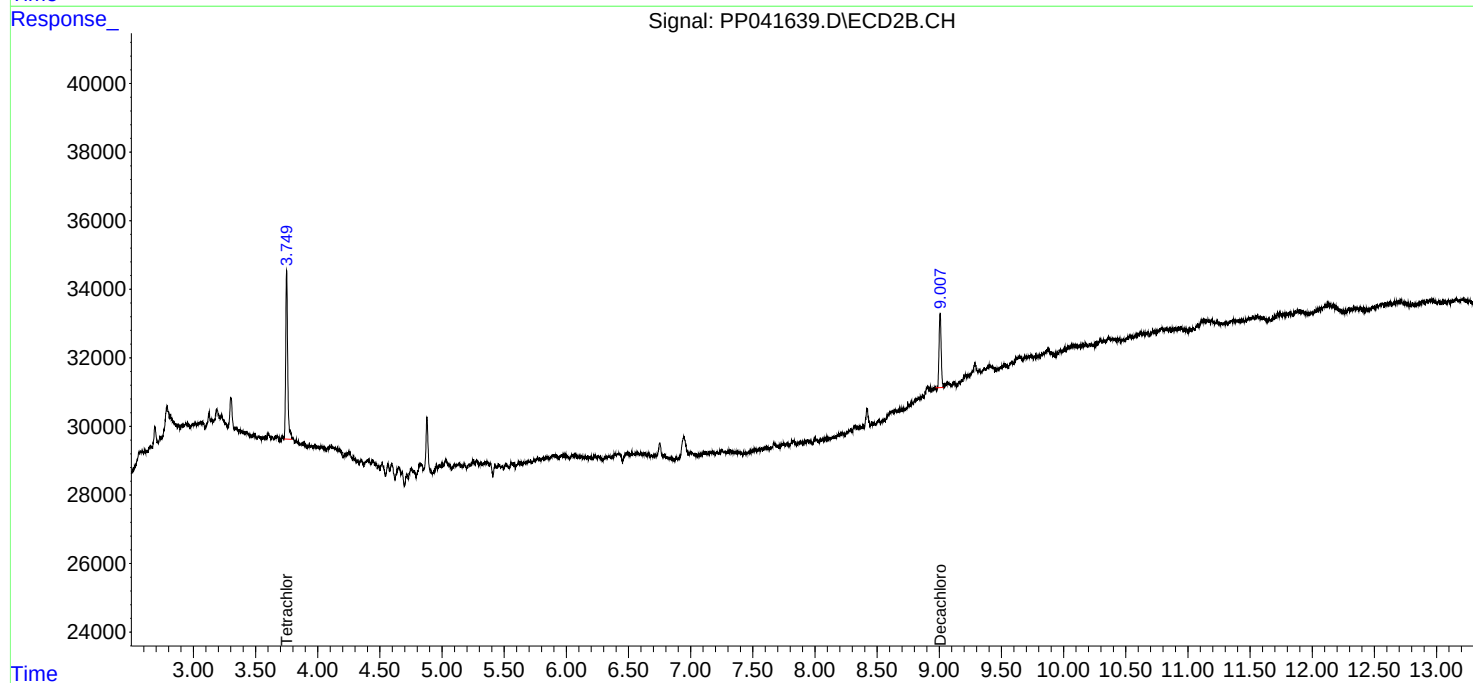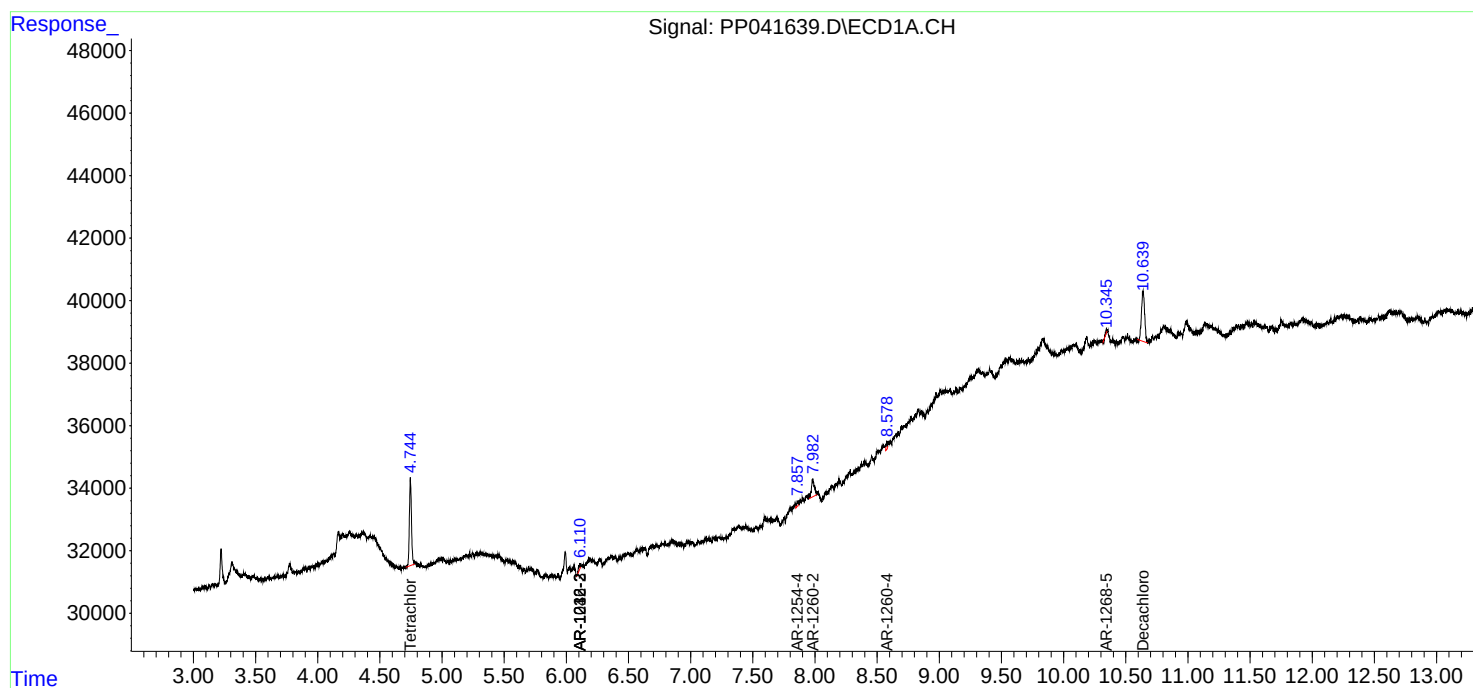


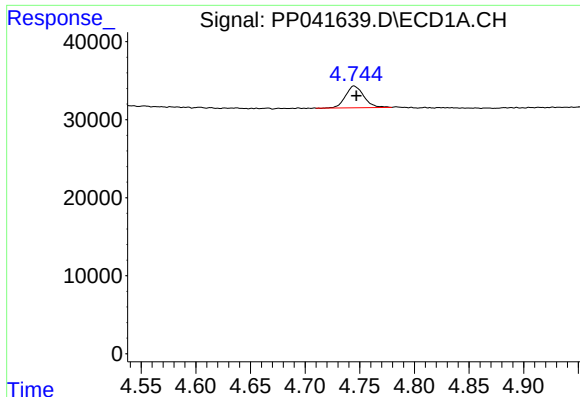

#1 Tetrachloro-m-xylene


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 32620
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

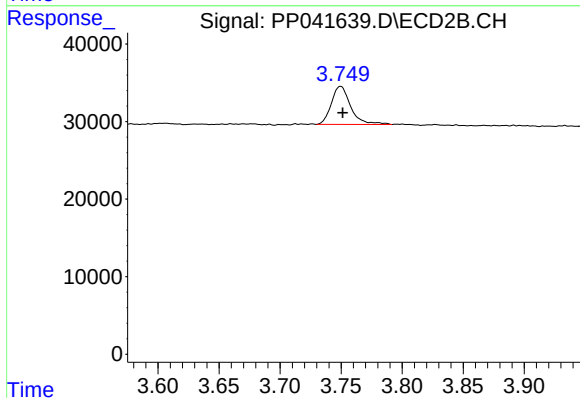


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.002 min
Response: 54353
Conc: 1.79 ng/ml

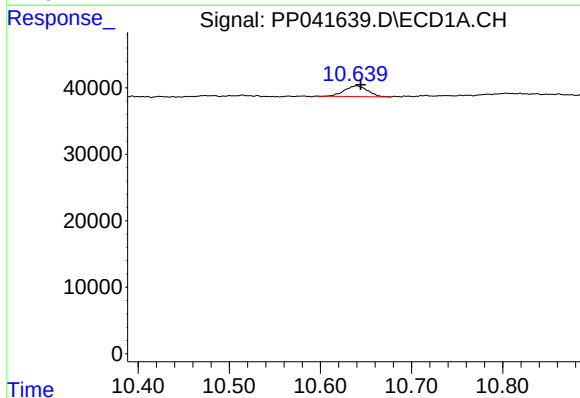


#2 Decachlorobiphenyl

R.T.: 10.639 min
Delta R.T.: -0.005 min
Response: 28211
Conc: 1.31 ng/ml

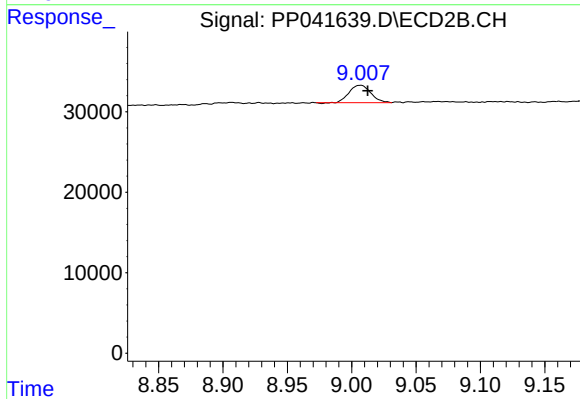

#2 Decachlorobiphenyl


R.T.: 9.007 min
Delta R.T.: -0.005 min
Response: 25303
Conc: 1.64 ng/ml

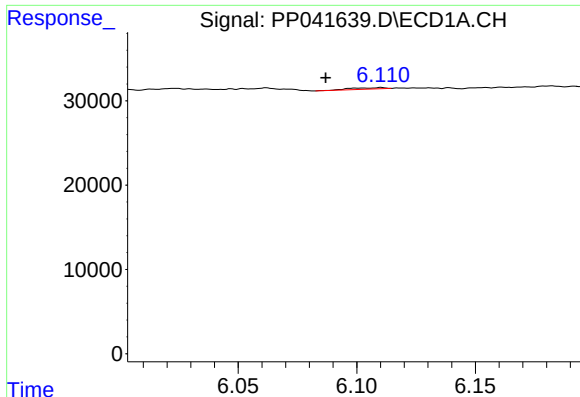

#4 AR-1016-2


R.T.: 6.110 min
Delta R.T.: 0.023 min
Response: 1713
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

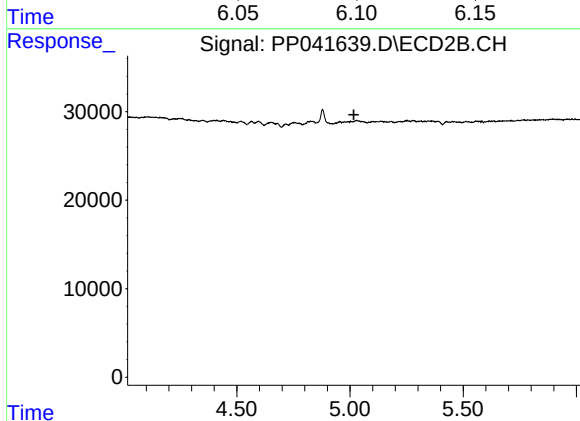


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.017 min
Response: 0
Conc: N.D.

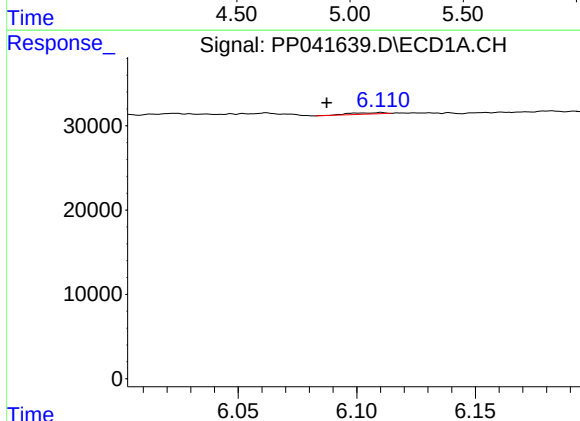


#13 AR-1232-3

R.T.: 6.110 min
Delta R.T.: 0.023 min
Response: 1713
Conc: 3.46 ng/ml

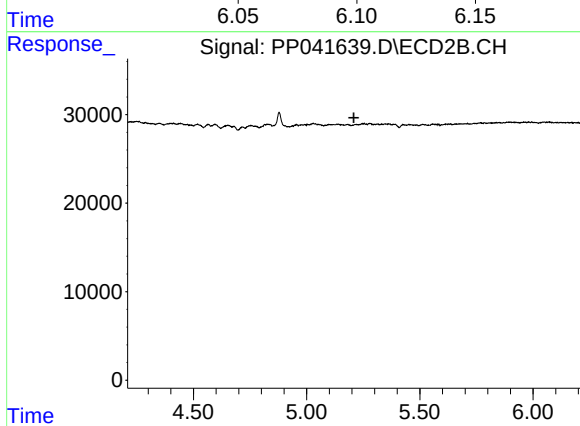

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

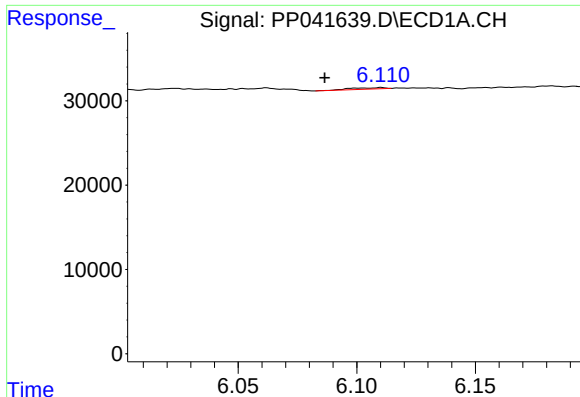

#17 AR-1242-2


R.T.: 6.110 min
Delta R.T.: 0.024 min
Response: 1713
Conc: 1.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

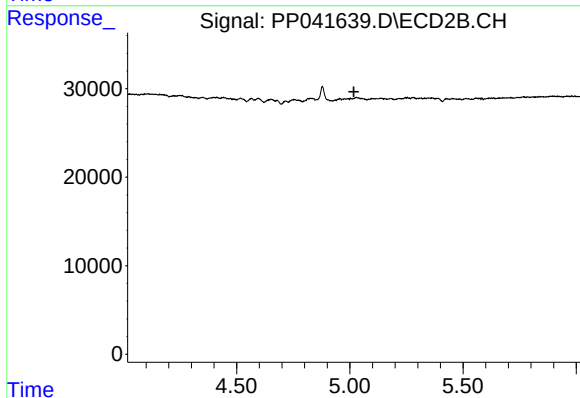


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.018 min
Response: 0
Conc: N.D.

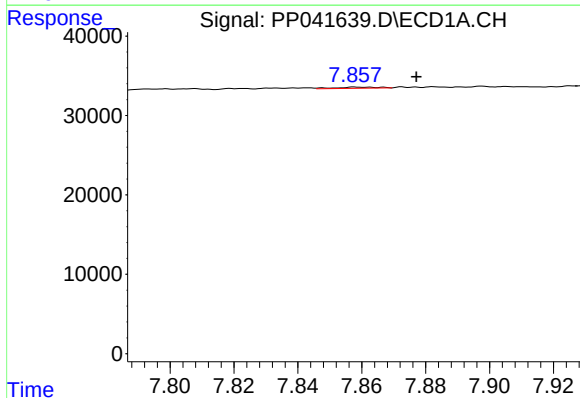


#29 AR-1254-4

R.T.: 7.858 min
Delta R.T.: -0.019 min
Response: 1379
Conc: 1.33 ng/ml

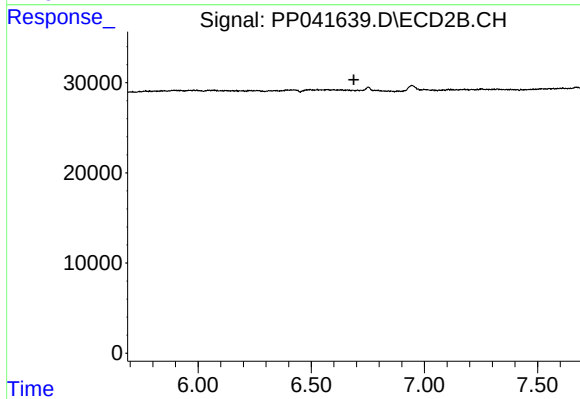

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.688 min
Response: 0
Conc: N.D.

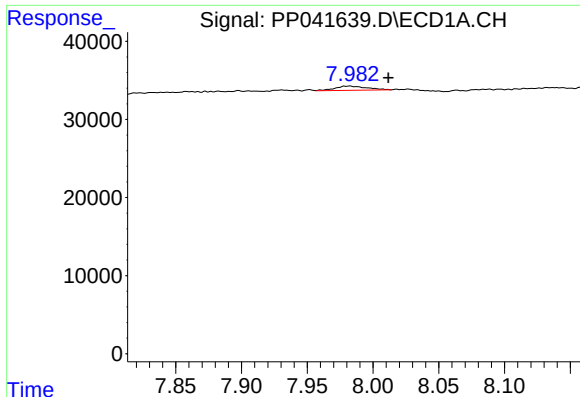

#32 AR-1260-2


R.T.: 7.983 min
Delta R.T.: -0.029 min
Response: 8997
Conc: 7.16 ng/ml

Instrument :
ECD_P
ClientSampleId :

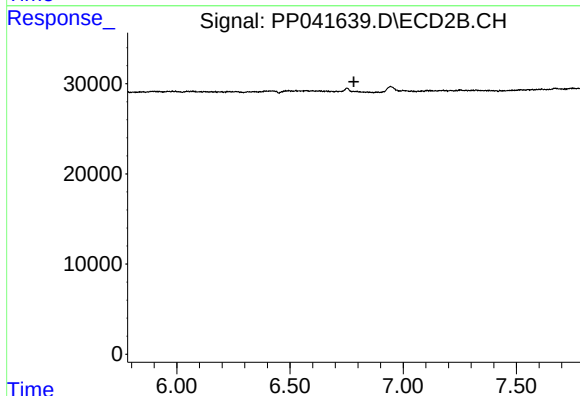


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

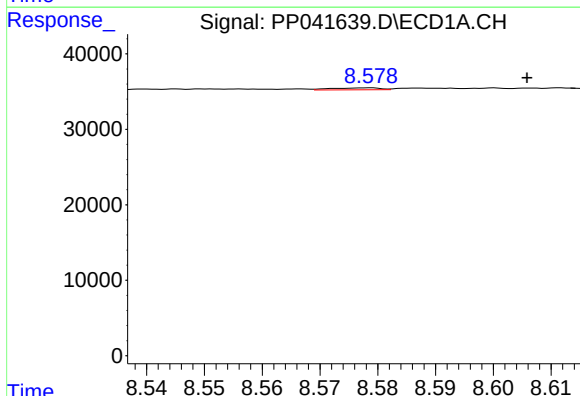


#34 AR-1260-4

R.T.: 8.579 min
Delta R.T.: -0.027 min
Response: 1518
Conc: 1.42 ng/ml

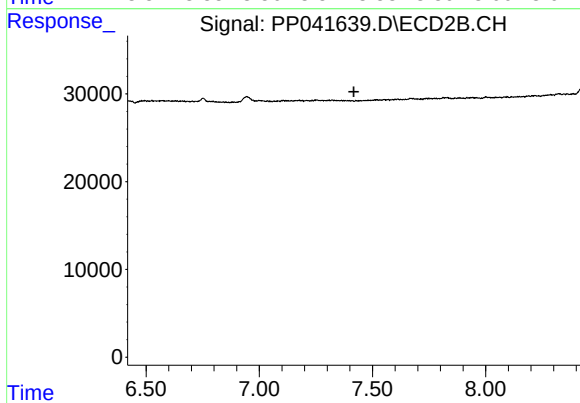

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

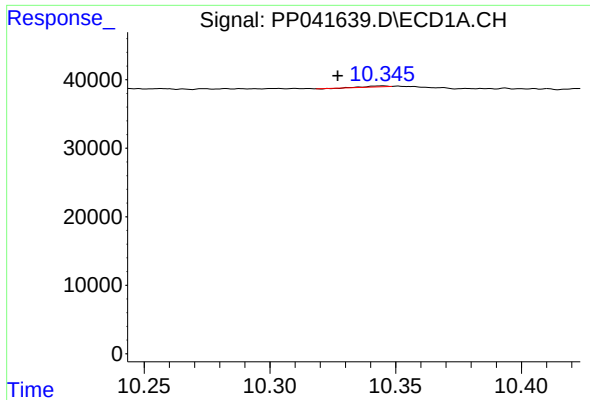

#45 AR-1268-5

R.T.: 10.345 min
Delta R.T.: 0.018 min
Response: 568
Conc: 0.08 ng/ml

Instrument :
ECD_P
ClientSampleId :

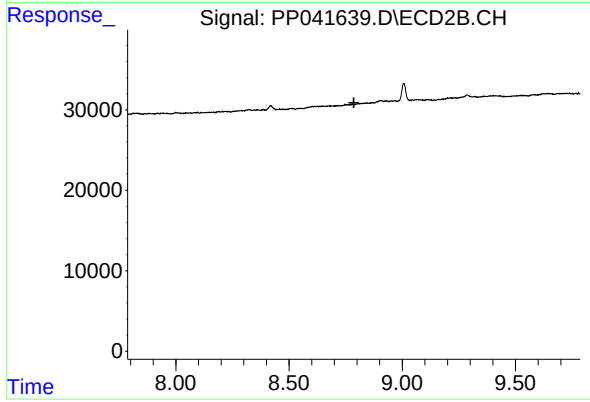

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.786 min
Response: 0
Conc: N.D.