

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
 Data File : PP041640.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Dec 2021 13:09
 Operator : AJ\MA
 Sample : M4904-06 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 23:52:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.745	3.750	34803	58410	1.543	1.923
2) SA Decachlor...	10.641	9.005	30277	28215	1.406	1.826 #
Target Compounds						
32) L7 AR-1260-2	7.988f	0.000	8935	0	7.111	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
Data File : PP041640.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Dec 2021 13:09
Operator : AJ\MA
Sample : M4904-06 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 23:52:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

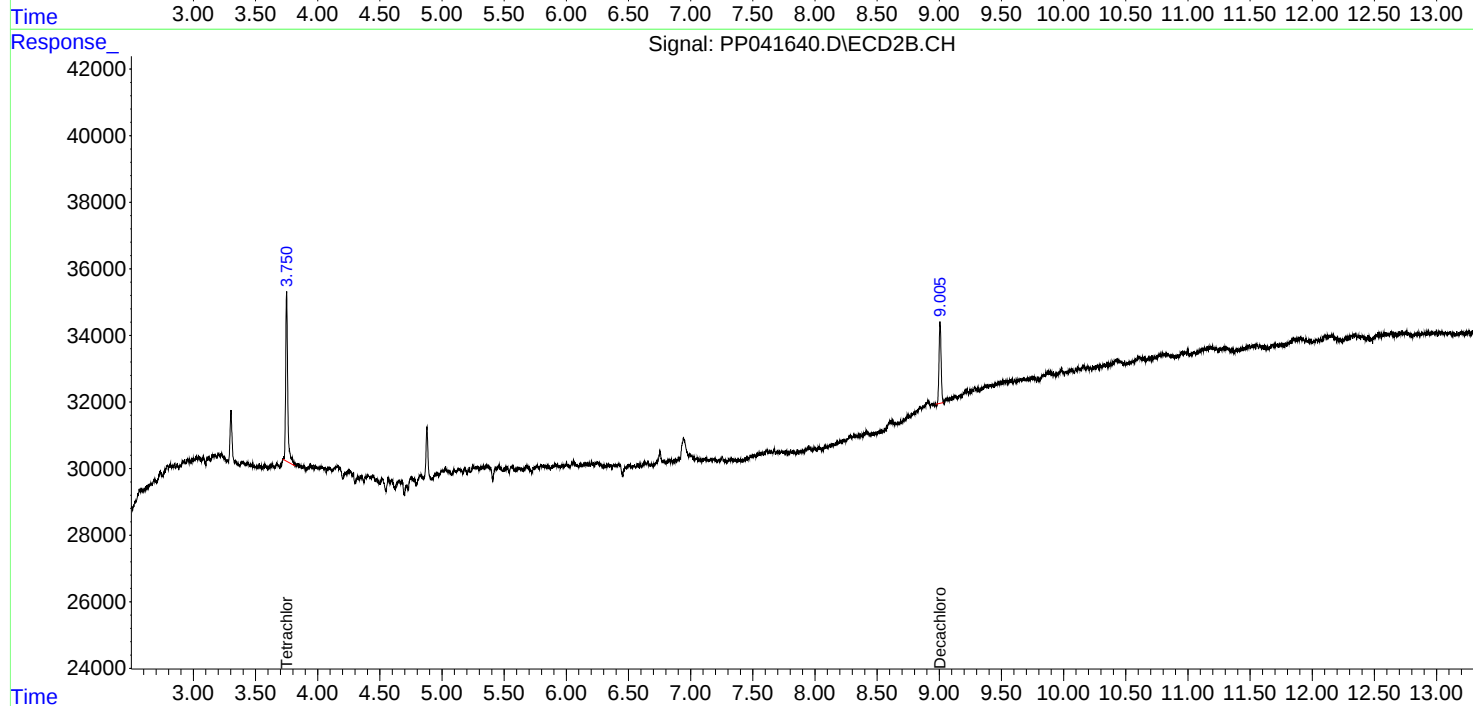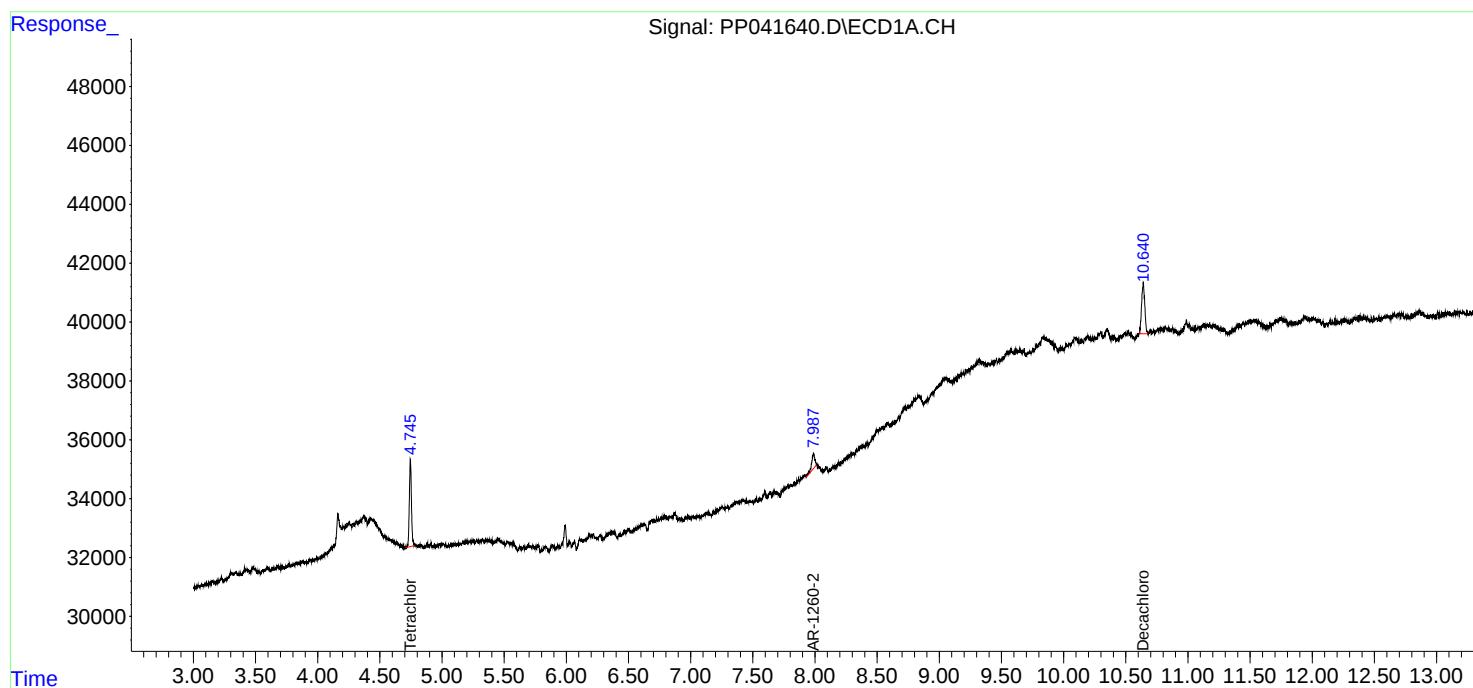


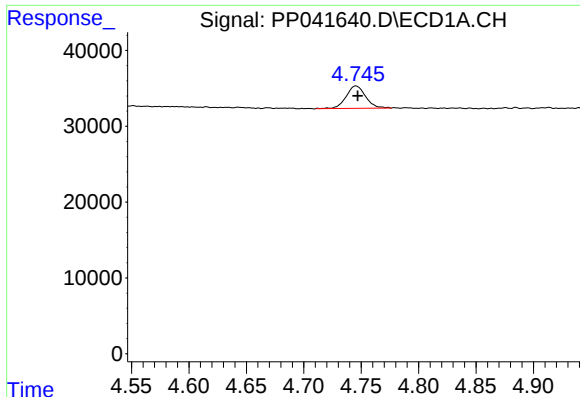

#1 Tetrachloro-m-xylene


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 34803
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

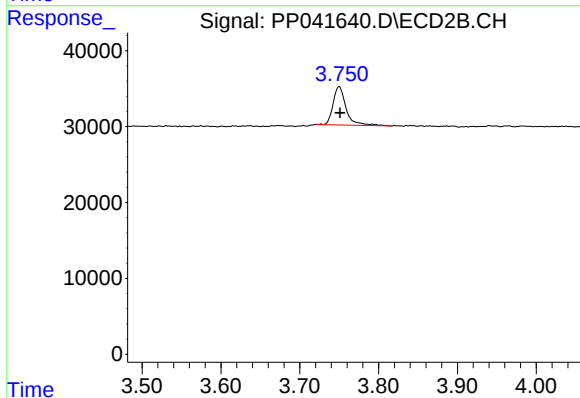


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.001 min
Response: 58410
Conc: 1.92 ng/ml

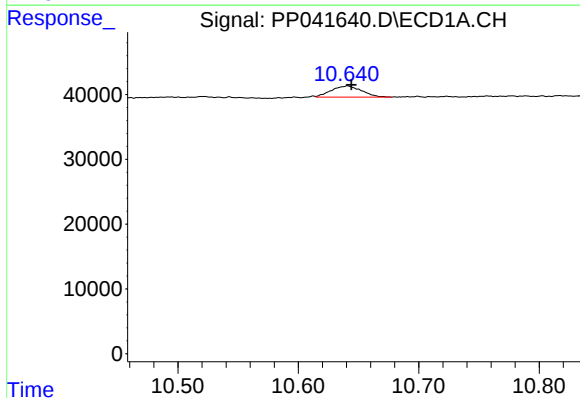


#2 Decachlorobiphenyl

R.T.: 10.641 min
Delta R.T.: -0.003 min
Response: 30277
Conc: 1.41 ng/ml

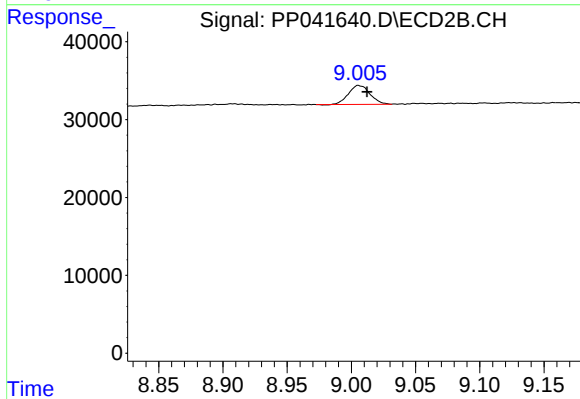

#2 Decachlorobiphenyl


R.T.: 9.005 min
Delta R.T.: -0.007 min
Response: 28215
Conc: 1.83 ng/ml

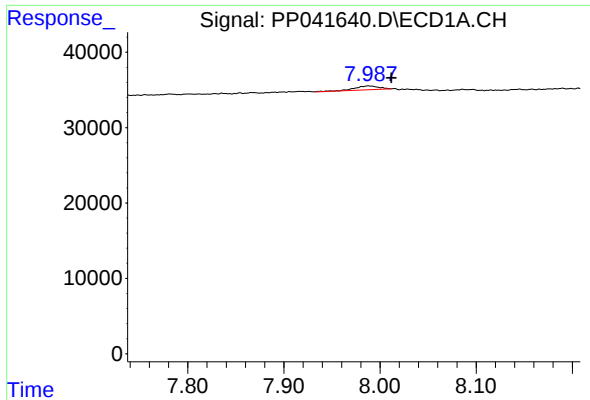

#32 AR-1260-2

R.T.: 7.988 min
Delta R.T.: -0.024 min
Response: 8935
Conc: 7.11 ng/ml

Instrument :
ECD_P
ClientSampleId :

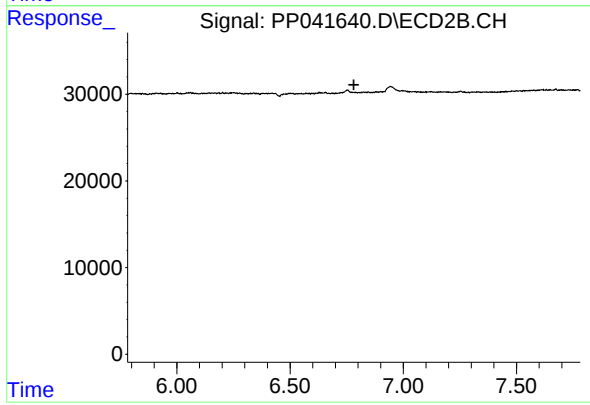

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.