

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
 Data File : PP041651.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Dec 2021 16:13
 Operator : AJ\MA
 Sample : M4904-12 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC157517-1-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/07/2021
 Supervised By :mohammad ahmed 12/07/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 23:56:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.744	3.750	38857	52775	1.723	1.737
2) SA Decachlor...	10.643	9.007	30880	28786	1.434	1.863m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
Data File : PP041651.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Dec 2021 16:13
Operator : AJ\MA
Sample : M4904-12 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
BC157517-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/07/2021
Supervised By :mohammad ahmed 12/07/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 23:56:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

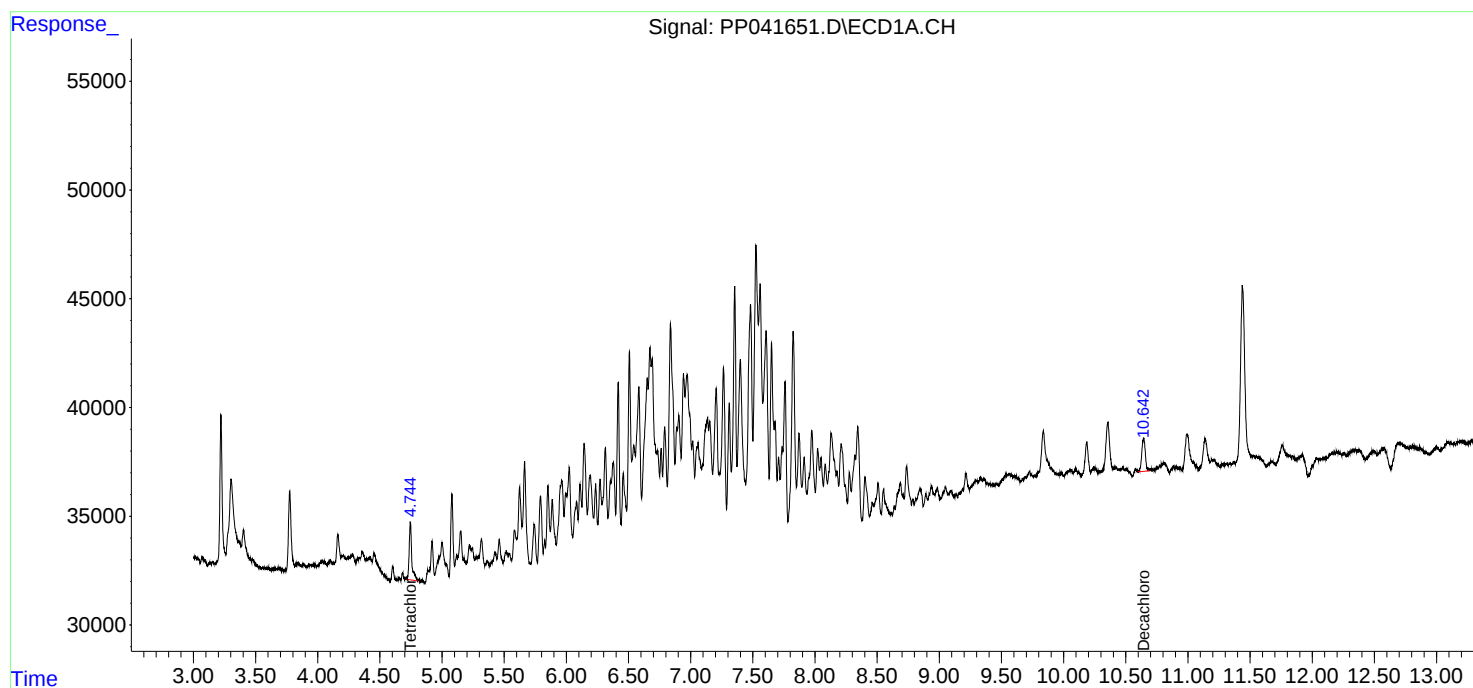

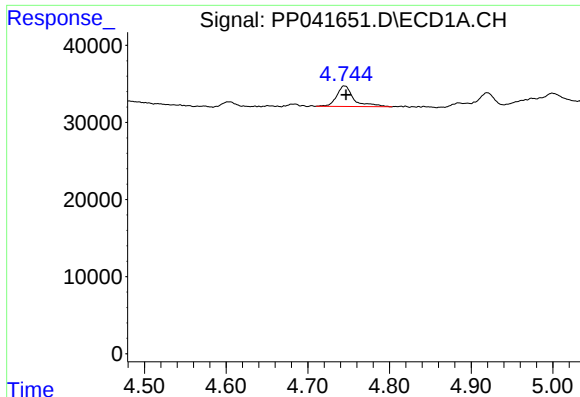

#1 Tetrachloro-m-xylene

R.T.: 4.744 min
Delta R.T.: -0.003 min
Response: 38857
Conc: 1.72 ng/ml

Instrument :

ECD_P


ClientSampleId :

BC157517-1-2

Manual Integrations


APPROVED

Reviewed By :Ankita Jodhani 12/07/2021
Supervised By :mohammad ahmed 12/07/2021

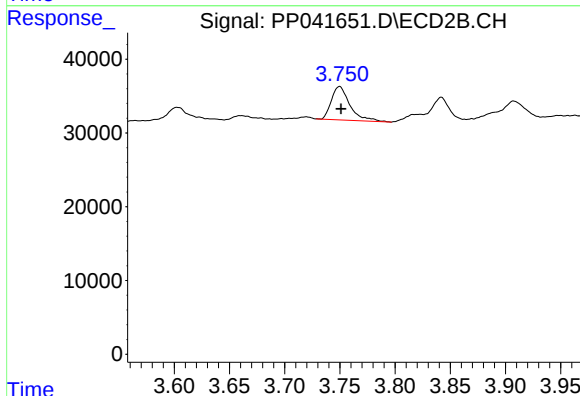


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: -0.001 min
Response: 52775
Conc: 1.74 ng/ml

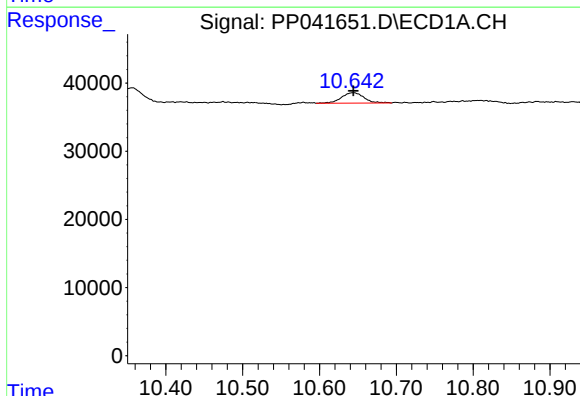

#2 Decachlorobiphenyl

R.T.: 10.643 min
Delta R.T.: 0.000 min
Response: 30880
Conc: 1.43 ng/ml

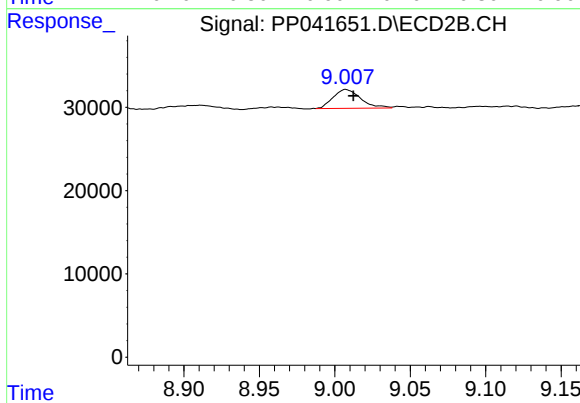

#2 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.006 min
Response: 28786
Conc: 1.86 ng/ml m