

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
 Data File : PP041708.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Dec 2021 9:00
 Operator : AJ\MA
 Sample : M4934-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 17098

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 11:13:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.745	3.751	344554	447646	15.280	14.737
2) SA Decachlor...	10.635	9.002	430839	320745	20.009	20.753

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120621\
Data File : PP041708.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Dec 2021 9:00
Operator : AJ\MA
Sample : M4934-04
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
17098

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 11:13:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

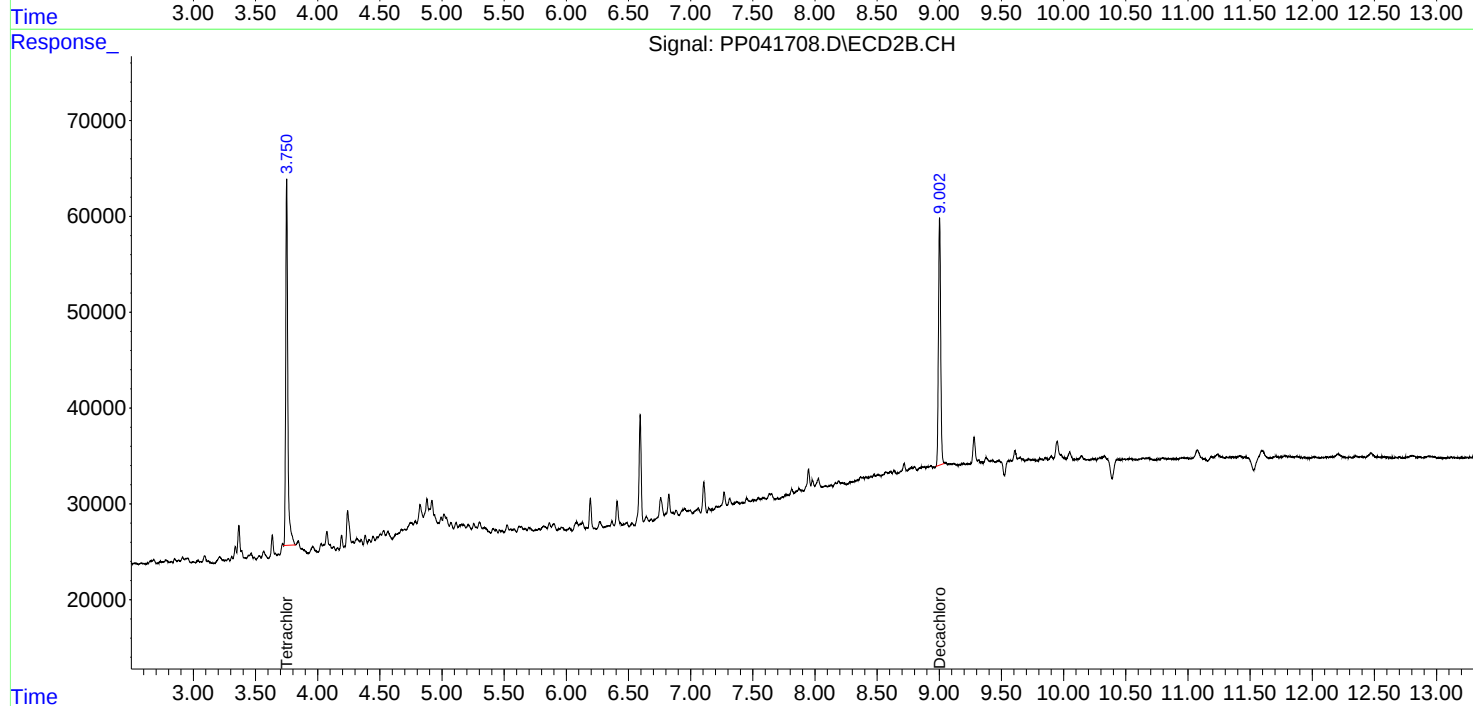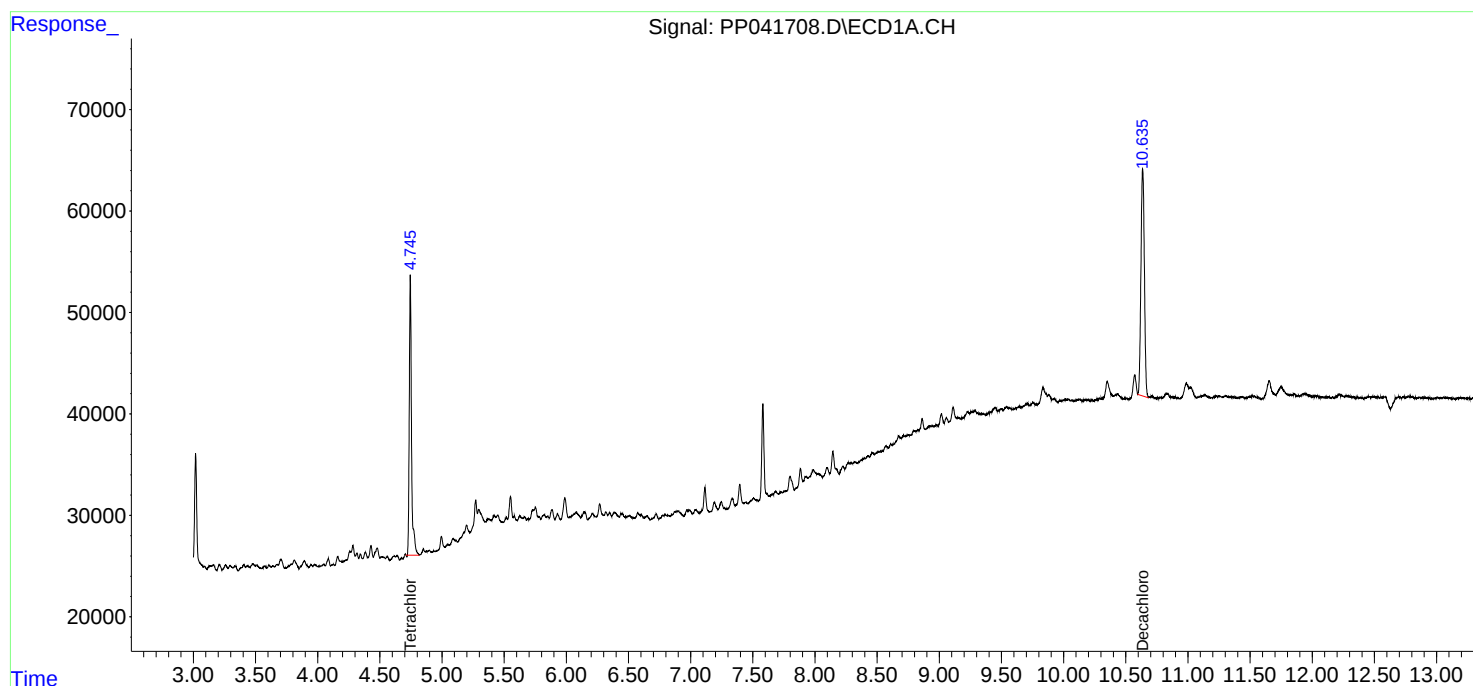


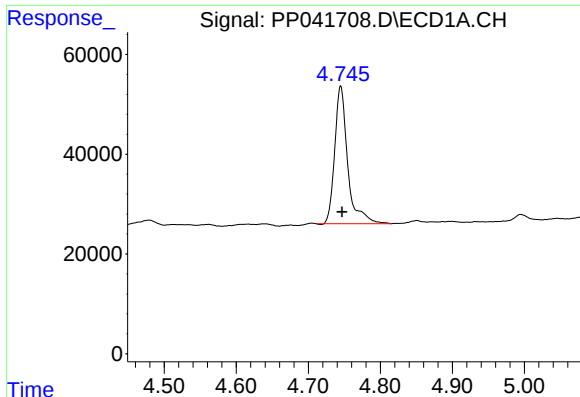

#1 Tetrachloro-m-xylene


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 344554
Conc: 15.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
17098

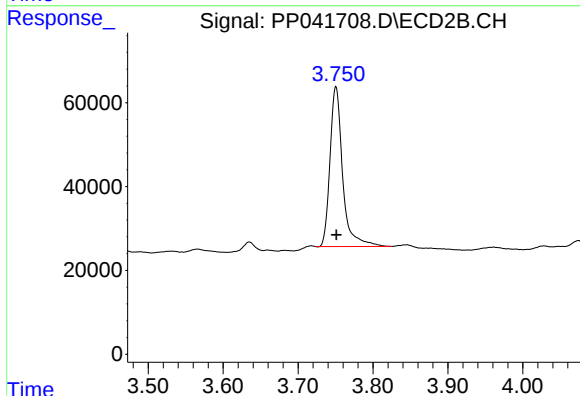


#1 Tetrachloro-m-xylene

R.T.: 3.751 min
Delta R.T.: 0.000 min
Response: 447646
Conc: 14.74 ng/ml

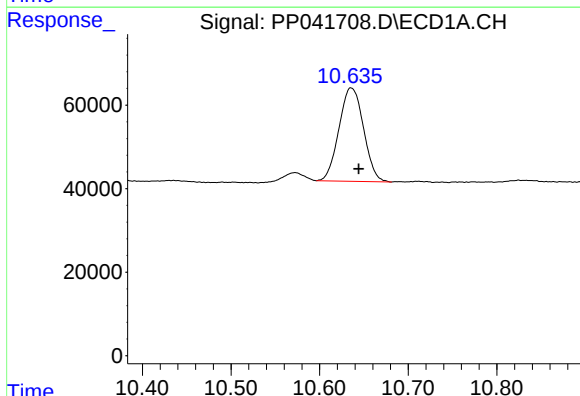

#2 Decachlorobiphenyl

R.T.: 10.635 min
Delta R.T.: -0.009 min
Response: 430839
Conc: 20.01 ng/ml

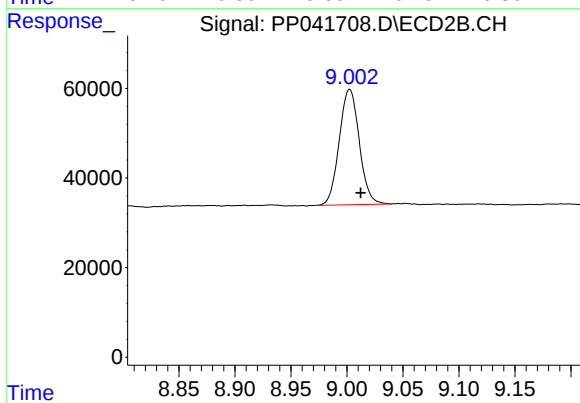

#2 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: -0.010 min
Response: 320745
Conc: 20.75 ng/ml