

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120718\
 Data File : PP028351.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Dec 2018 9:55
 Operator : EI\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 14:02:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP120718.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 07 14:01:32 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

15) T	Picloram	0.000	18.342	0	18618133	N.D.	0.119 #
-------	----------	-------	--------	---	----------	------	---------



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120718\
Data File : PP028351.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Dec 2018 9:55
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 14:02:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP120718.M
Quant Title : 8080.M
QLast Update : Fri Dec 07 14:01:32 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

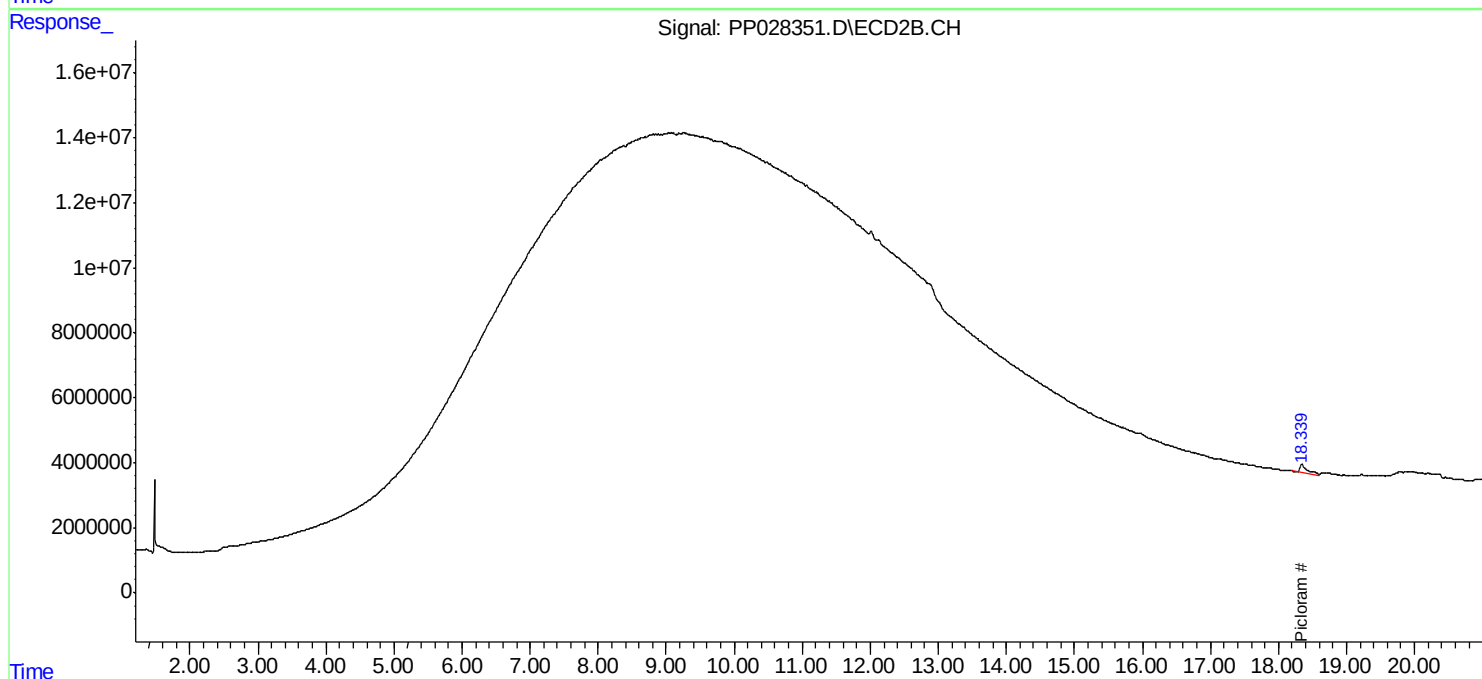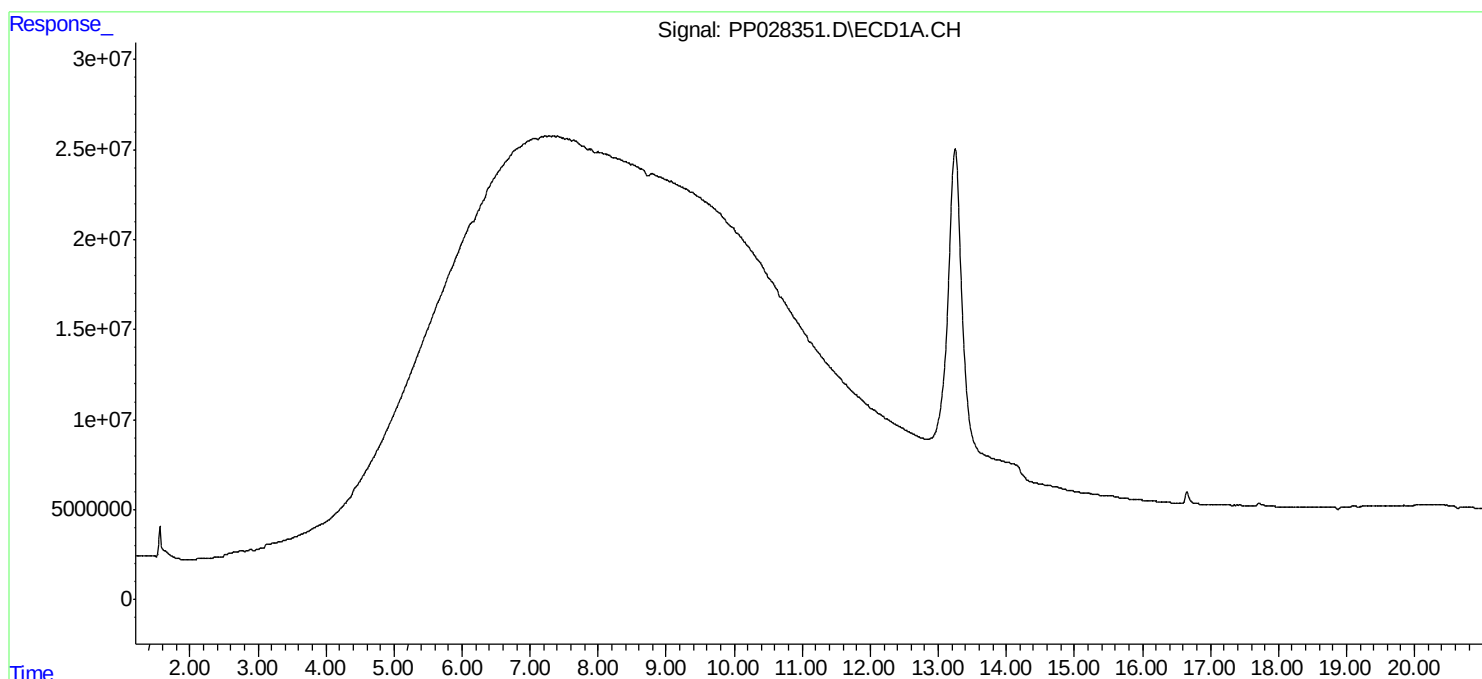

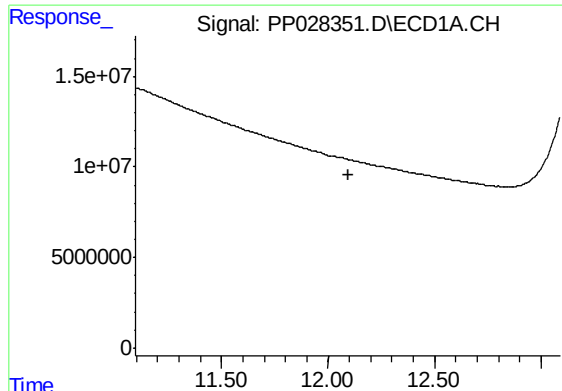

#4 2,4-DCAA


R.T.: 0.000 min

Exp R.T. : 12.094 min

Response: 0

Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

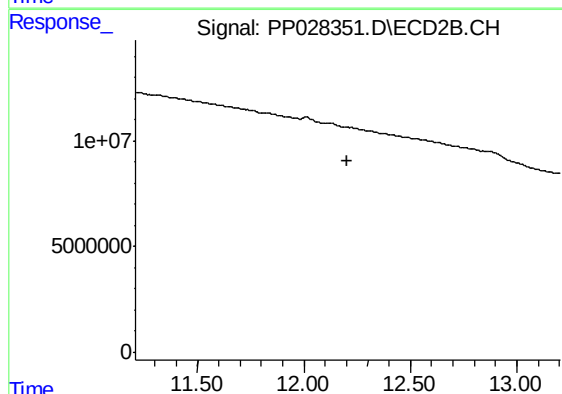


#4 2,4-DCAA

R.T.: 0.000 min

Exp R.T. : 12.207 min

Response: 0

Conc: N.D.

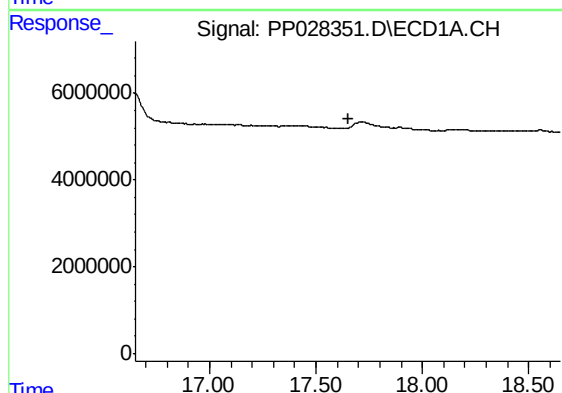


#15 Picloram

R.T.: 0.000 min

Exp R.T. : 17.651 min

Response: 0

Conc: N.D.

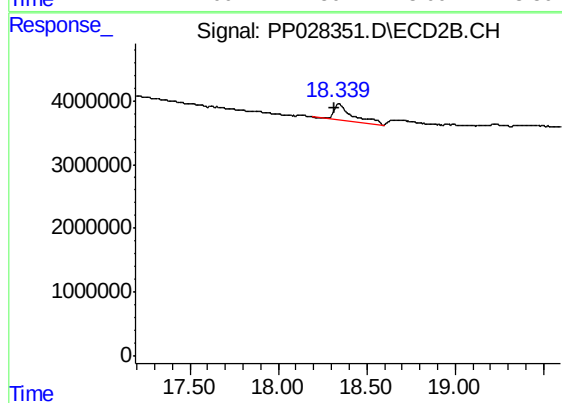

#15 Picloram

R.T.: 18.342 min

Delta R.T.: 0.027 min

Response: 18618133

Conc: 0.12 ng/ml