

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120718\
 Data File : PS002528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2018 16:12
 Operator : EI\SJ
 Sample : J6214-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 22:22:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 07 03:48:18 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.414	10.909	101.1E6	89889835	318.430	232.479 #
Target Compounds							
3) T	4-Nitroph...	10.979	10.067	3861946	7653970	24.488	43.335 #
5) T	DICAMBA	0.000	11.150	0	17383950	N.D.	12.196 #
6) T	MCP	12.087	11.373	28242764	2321384	28.405	2.483 #
7) T	MCPA	12.234	11.741	4971538	8110638	3.302	5.330 #
8) T	DICHLORPROP	0.000	12.367	0	991658	N.D.	2.774 #
10) T	Pentachlo...	0.000	13.347	0	207876	N.D.	0.040 #
11) T	2,4,5-TP ...	0.000	13.873	0	10702083	N.D.	5.097 #
12) T	2,4,5-T	0.000	14.448	0	2203104	N.D.	1.288 #
13) T	2,4-DB	15.703	15.092	9266202	3000279	41.107	12.424 #
14) T	DINOSEB	0.000	15.585	0	8042193	N.D.	5.270 #
15) T	Picloram	16.862	16.781	11285478	3218994	4.447	1.122 #
16) T	DCPA	0.000	16.781	0	3218994	N.D.	1.134 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120718\
Data File : PS002528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2018 16:12
Operator : EI\SJ
Sample : J6214-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 22:22:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Fri Dec 07 03:48:18 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

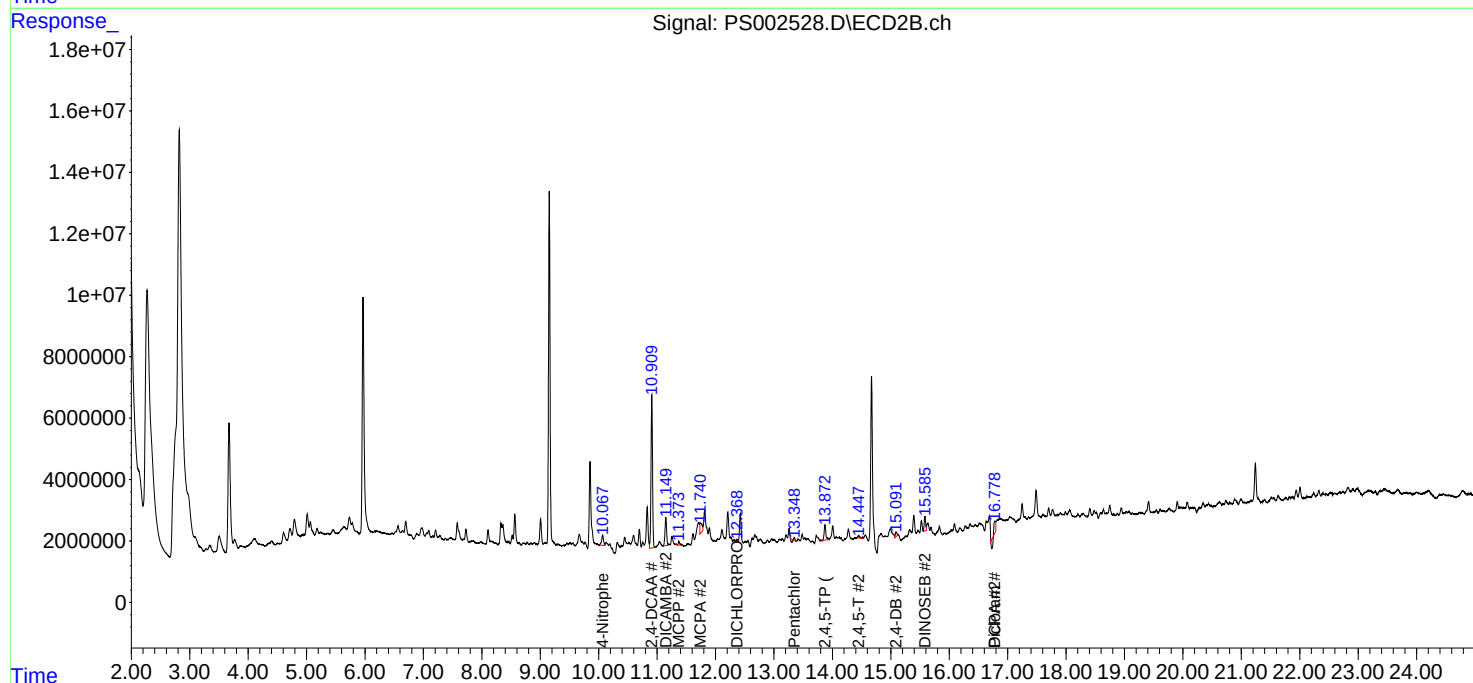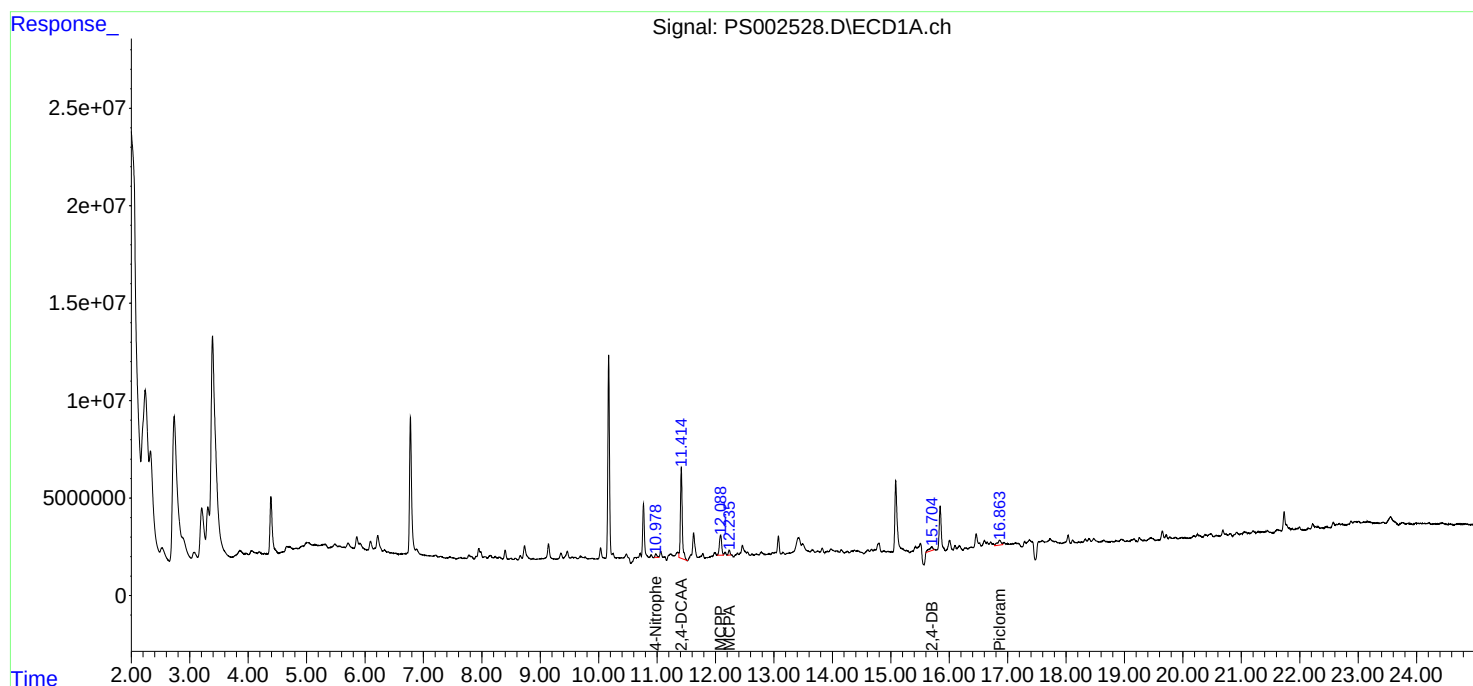


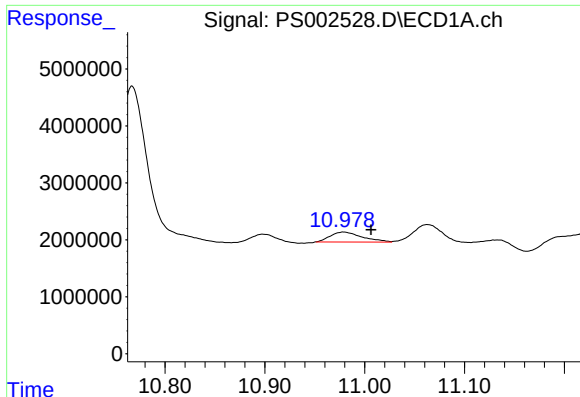

#3 4-Nitrophenol


R.T.: 10.979 min
Delta R.T.: -0.027 min
Response: 3861946
Conc: 24.49 ng/ml

Instrument :
ECD_P
ClientSampleId :

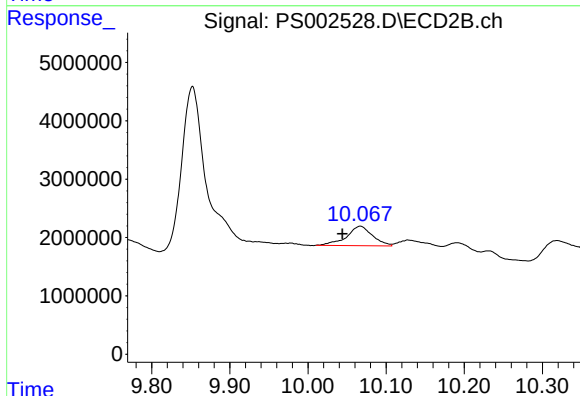


#3 4-Nitrophenol

R.T.: 10.067 min
Delta R.T.: 0.023 min
Response: 7653970
Conc: 43.34 ng/ml

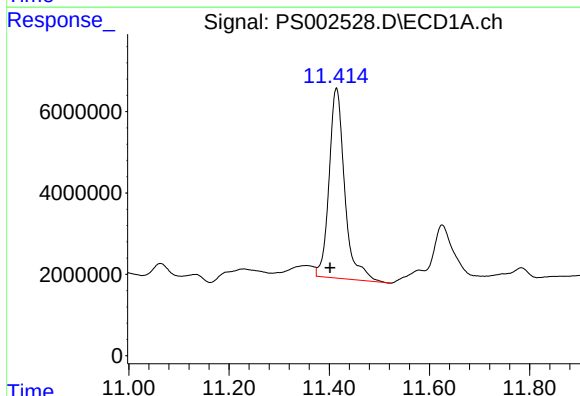


#4 2,4-DCAA

R.T.: 11.414 min
Delta R.T.: 0.013 min
Response: 101076081
Conc: 318.43 ng/ml

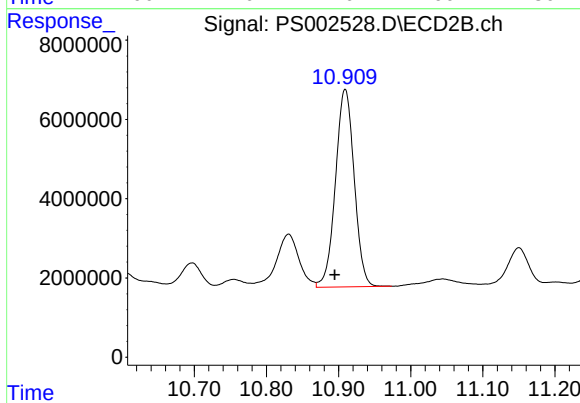

#4 2,4-DCAA


R.T.: 10.909 min
Delta R.T.: 0.014 min
Response: 89889835
Conc: 232.48 ng/ml

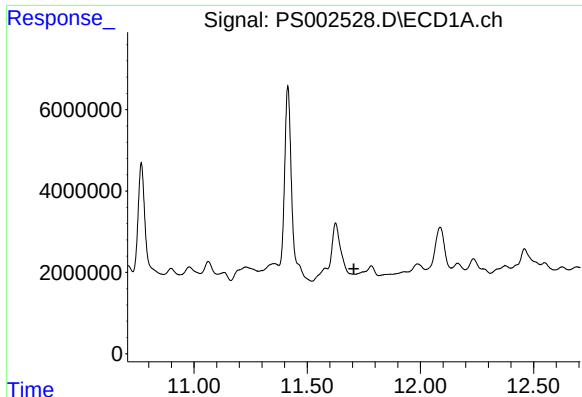

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

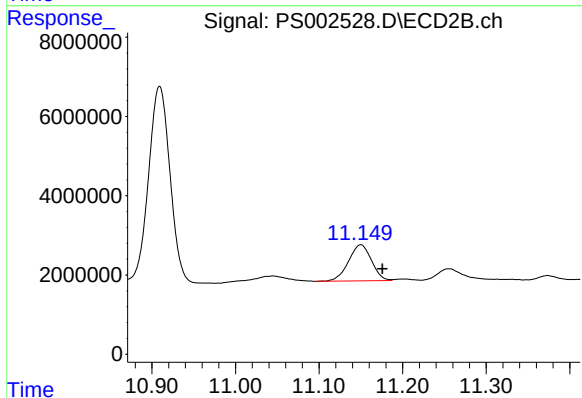


#5 DICAMBA

R.T.: 11.150 min
Delta R.T.: -0.026 min
Response: 17383950
Conc: 12.20 ng/ml

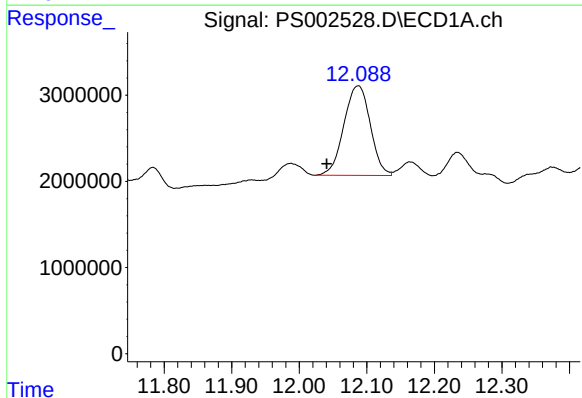


#6 MCP

R.T.: 12.087 min
Delta R.T.: 0.046 min
Response: 28242764
Conc: 28.40 ug/ml

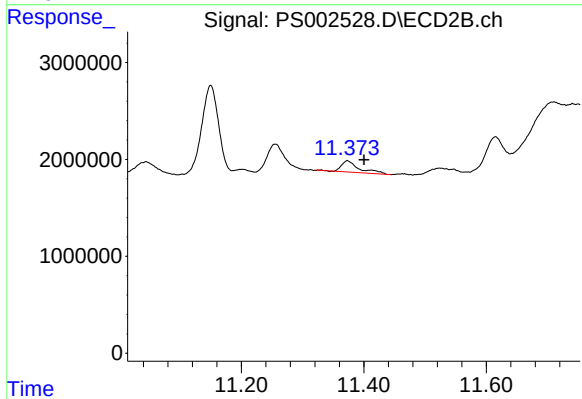

#6 MCP


R.T.: 11.373 min
Delta R.T.: -0.027 min
Response: 2321384
Conc: 2.48 ug/ml

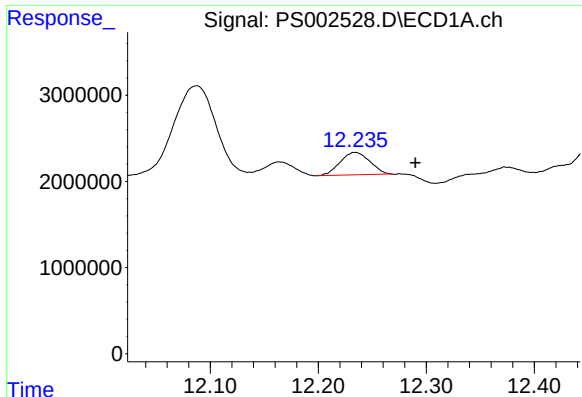

#7 MCPA


R.T.: 12.234 min
Delta R.T.: -0.056 min
Response: 4971538
Conc: 3.30 ug/ml

Instrument :
ECD_P
ClientSampleId :

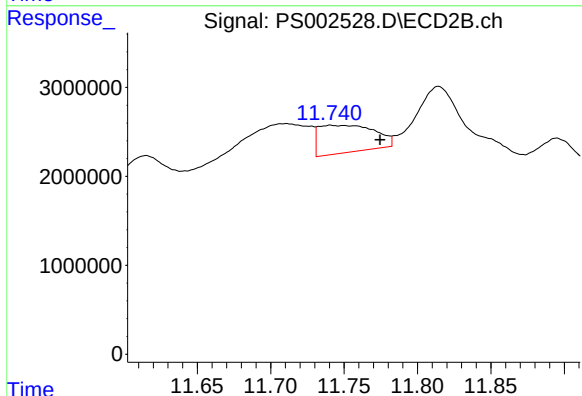


#7 MCPA

R.T.: 11.741 min
Delta R.T.: -0.033 min
Response: 8110638
Conc: 5.33 ug/ml

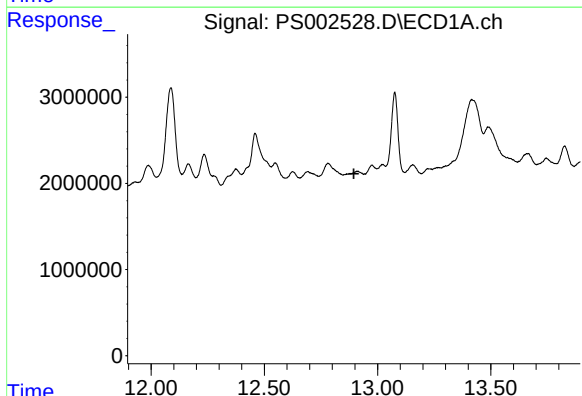


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.895 min
Response: 0
Conc: N.D.

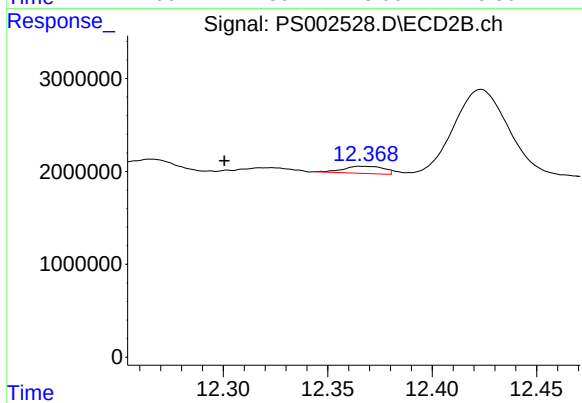

#8 DICHLORPROP


R.T.: 12.367 min
Delta R.T.: 0.067 min
Response: 991658
Conc: 2.77 ng/ml

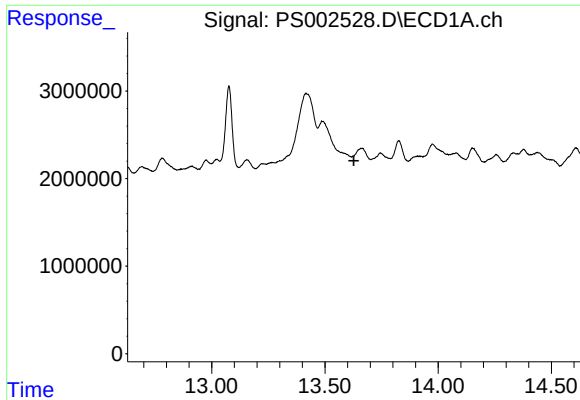

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

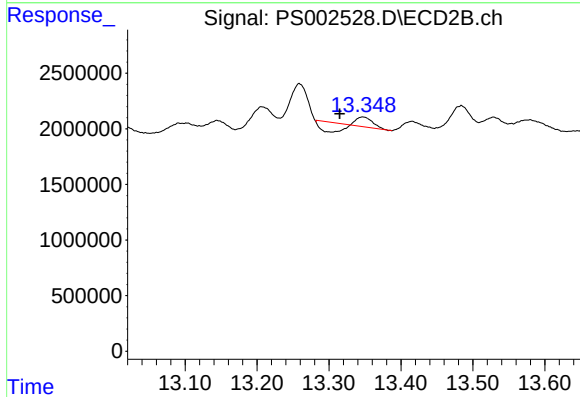


#10 Pentachlorophenol

R.T.: 13.347 min
Delta R.T.: 0.032 min
Response: 207876
Conc: 0.04 ng/ml

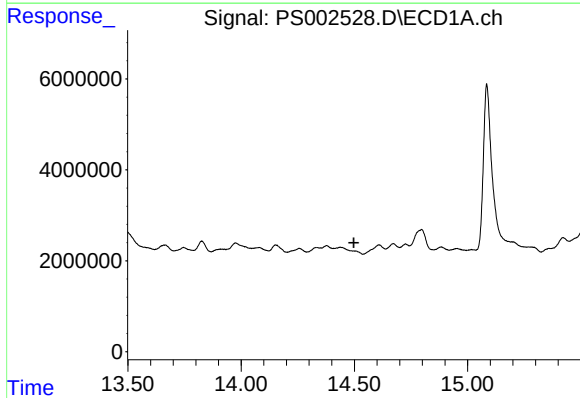


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.498 min
Response: 0
Conc: N.D.

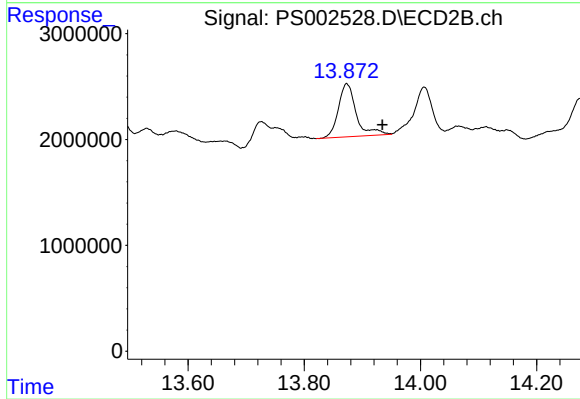

#11 2,4,5-TP (SILVEX)


R.T.: 13.873 min
Delta R.T.: -0.061 min
Response: 10702083
Conc: 5.10 ng/ml

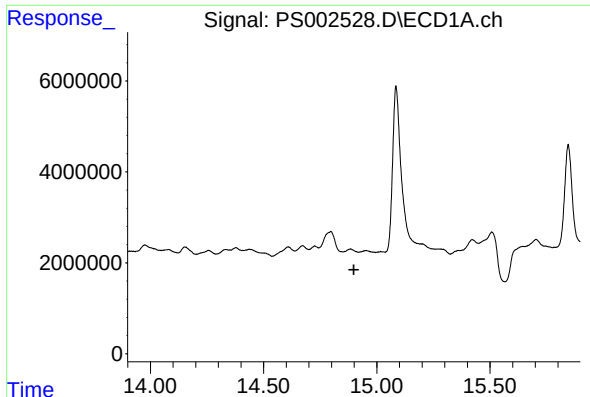

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.899 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

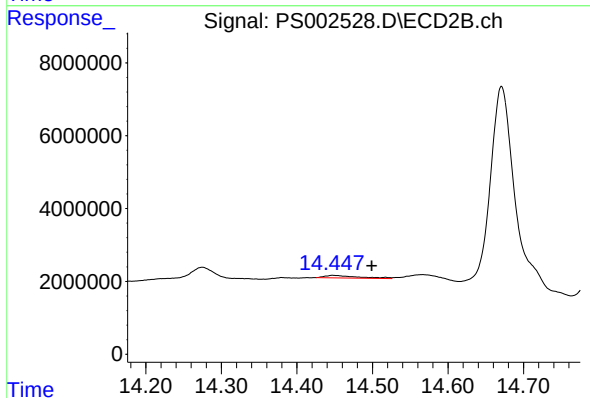


#12 2,4,5-T

R.T.: 14.448 min
Delta R.T.: -0.051 min
Response: 2203104
Conc: 1.29 ng/ml

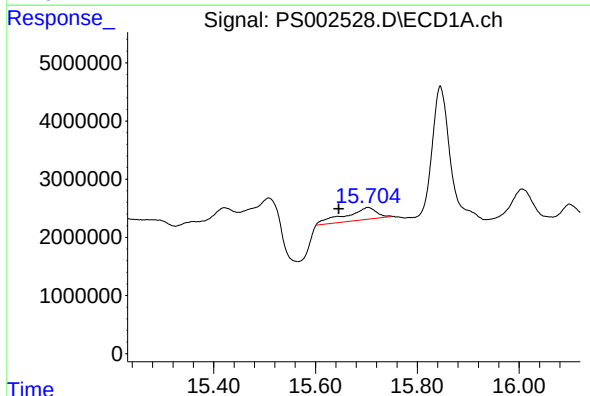


#13 2,4-DB

R.T.: 15.703 min
Delta R.T.: 0.057 min
Response: 9266202
Conc: 41.11 ng/ml

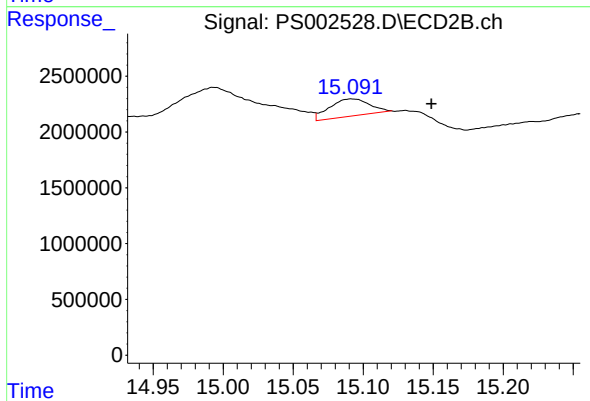

#13 2,4-DB


R.T.: 15.092 min
Delta R.T.: -0.057 min
Response: 3000279
Conc: 12.42 ng/ml

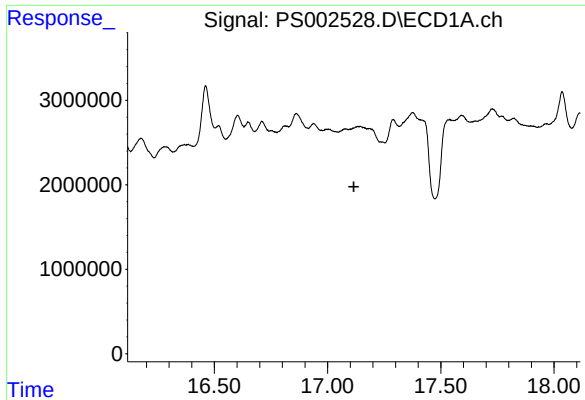

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

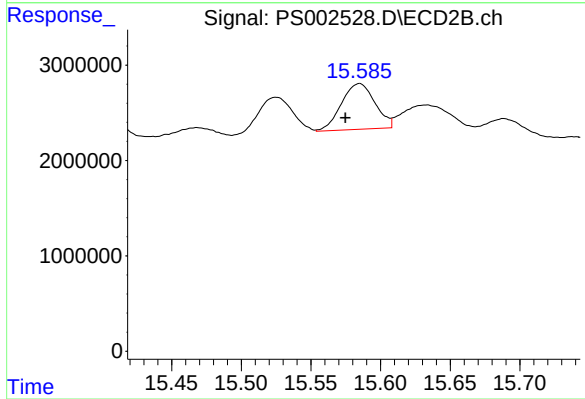


#14 DINOSEB

R.T.: 15.585 min
Delta R.T.: 0.010 min
Response: 8042193
Conc: 5.27 ng/ml

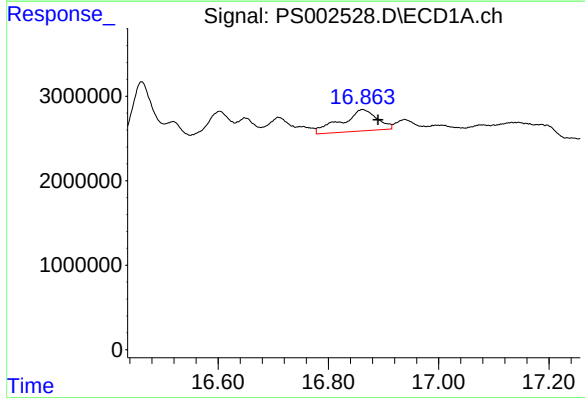


#15 Picloram

R.T.: 16.862 min
Delta R.T.: -0.028 min
Response: 11285478
Conc: 4.45 ng/ml

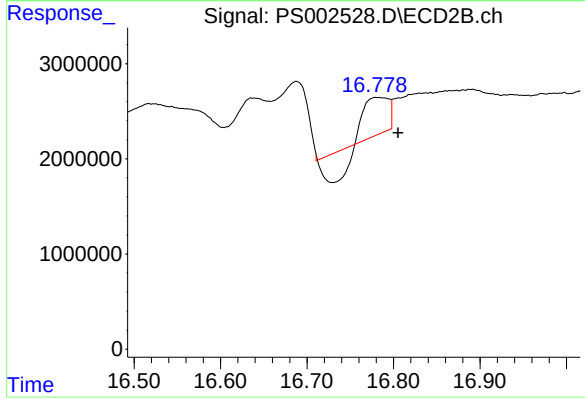

#15 Picloram


R.T.: 16.781 min
Delta R.T.: -0.024 min
Response: 3218994
Conc: 1.12 ng/ml

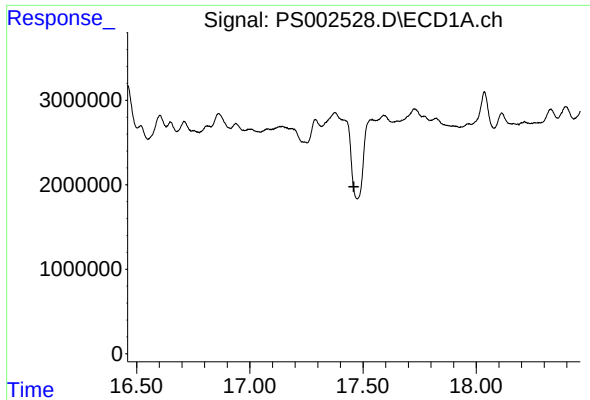

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

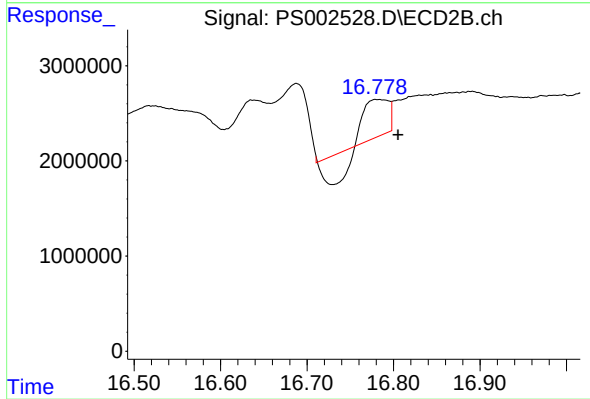

#16 DCPA

R.T.: 16.781 min
Delta R.T.: -0.024 min
Response: 3218994
Conc: 1.13 ng/ml