

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120721\
 Data File : PP041713.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Dec 2021 10:39
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 00:00:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	7.036	5.888f	21015	9850	43.730 15.134 #
24)	L5	AR-1248-4	7.003	0.000	7104	0	8.482 N.D. #
25)	L5	AR-1248-5	7.036	5.888f	21015	9850	25.254 11.001 #
26)	L6	AR-1254-1	6.978	5.888f	57764	9850	68.061 7.076 #
28)	L6	AR-1254-3	7.594	0.000	22070	0	15.495 N.D. #
32)	L7	AR-1260-2	8.030f	0.000	4982	0	3.965 N.D. #
33)	L7	AR-1260-3	8.360f	0.000	1271	0	1.404 N.D. #
35)	L7	AR-1260-5	8.949f	0.000	38649	0	18.653 N.D. #
36)	L8	AR-1262-1	8.360	0.000	1271	0	1.001 N.D. #
37)	L8	AR-1262-2	8.949f	0.000	38649	0	17.106 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120721\
Data File : PP041713.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Dec 2021 10:39
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 00:00:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

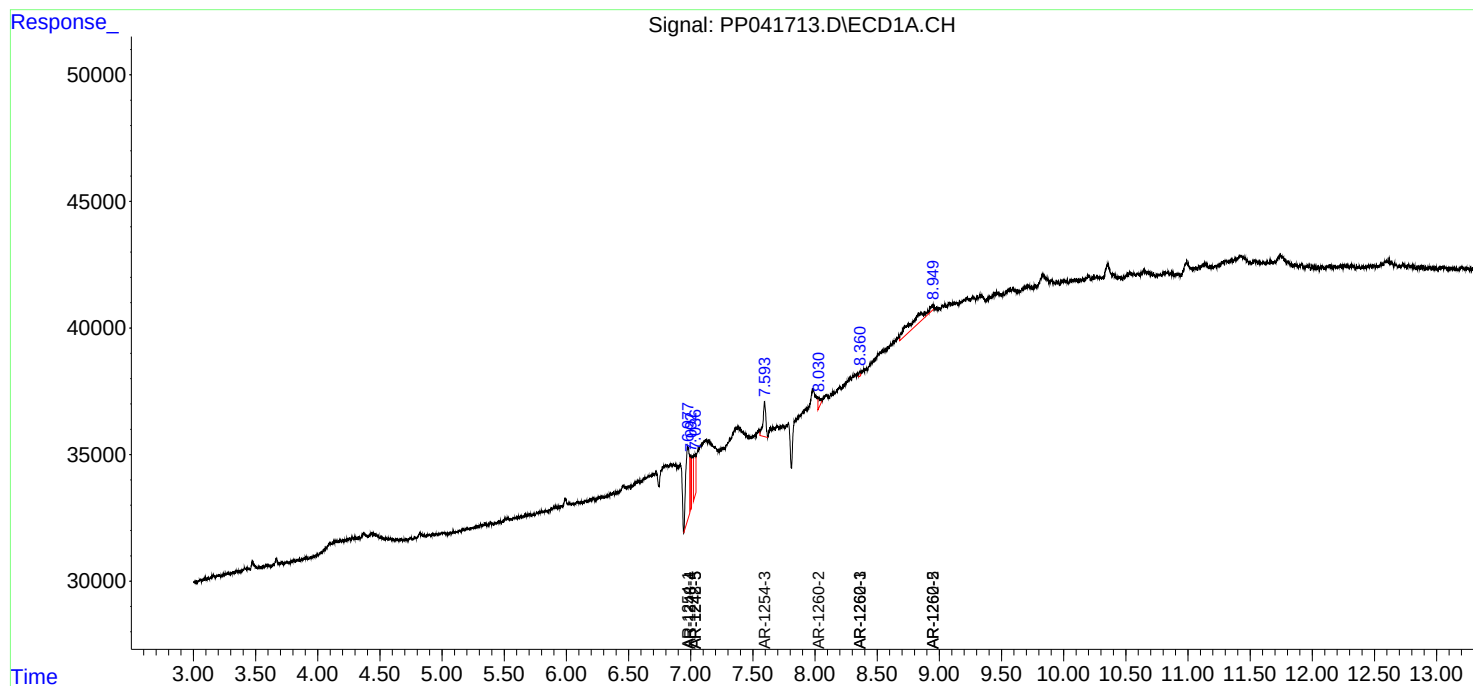


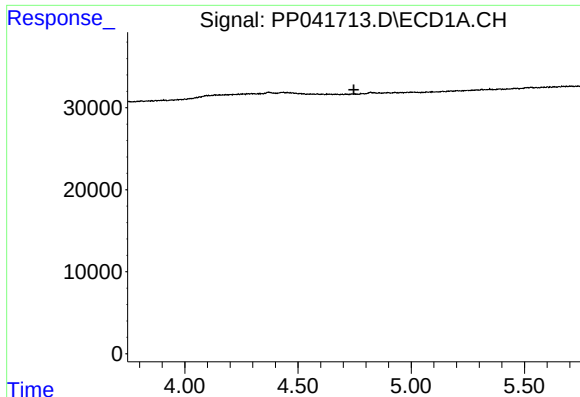

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

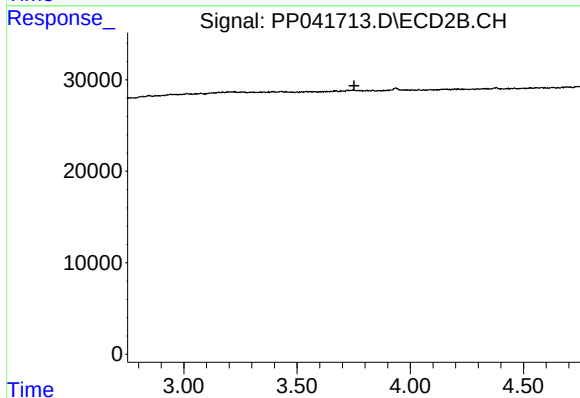


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.751 min
Response: 0
Conc: N.D.

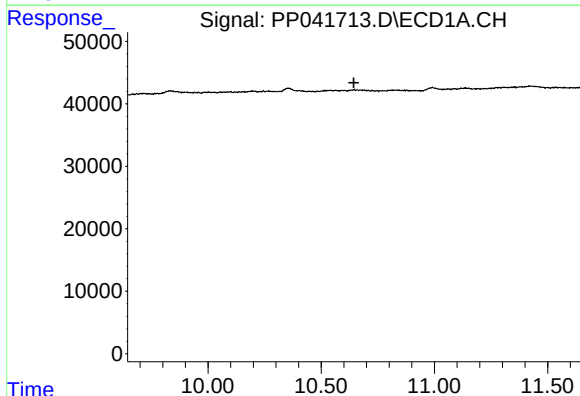


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.644 min
Response: 0
Conc: N.D.

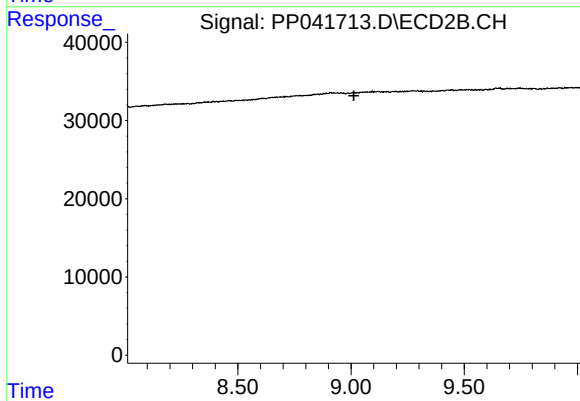

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.012 min
Response: 0
Conc: N.D.

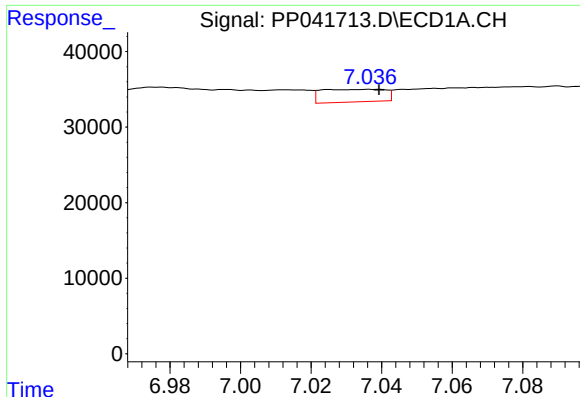

#20 AR-1242-5


R.T.: 7.036 min
Delta R.T.: -0.003 min
Response: 21015
Conc: 43.73 ng/ml

Instrument :
ECD_P
ClientSampleId :

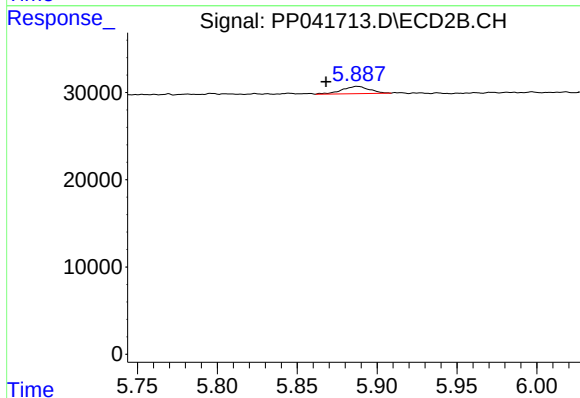


#20 AR-1242-5

R.T.: 5.888 min
Delta R.T.: 0.019 min
Response: 9850
Conc: 15.13 ng/ml

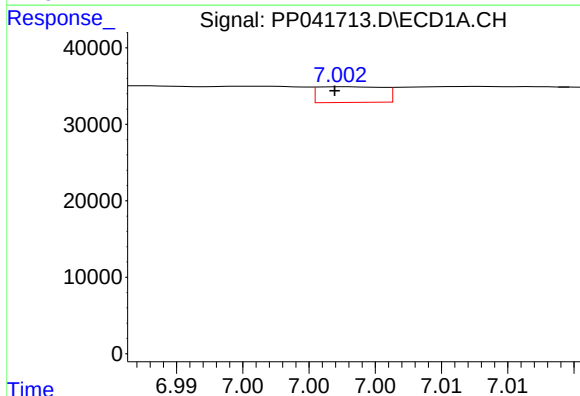


#24 AR-1248-4

R.T.: 7.003 min
Delta R.T.: 0.000 min
Response: 7104
Conc: 8.48 ng/ml

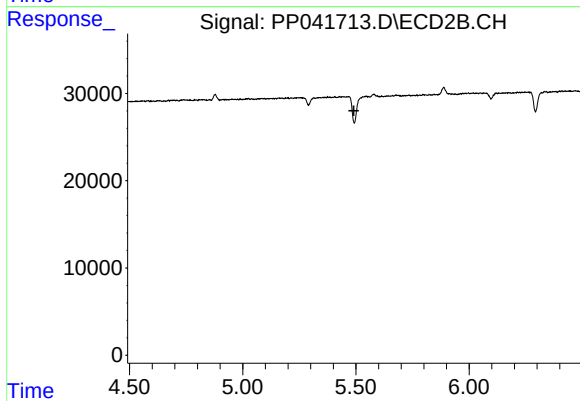

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

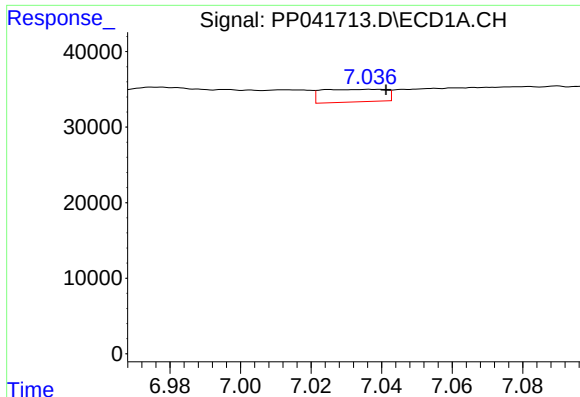

#25 AR-1248-5


R.T.: 7.036 min
Delta R.T.: -0.005 min
Response: 21015
Conc: 25.25 ng/ml

Instrument :
ECD_P
ClientSampleId :

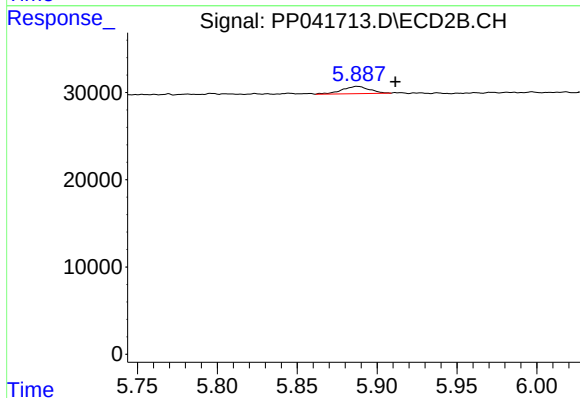


#25 AR-1248-5

R.T.: 5.888 min
Delta R.T.: -0.024 min
Response: 9850
Conc: 11.00 ng/ml

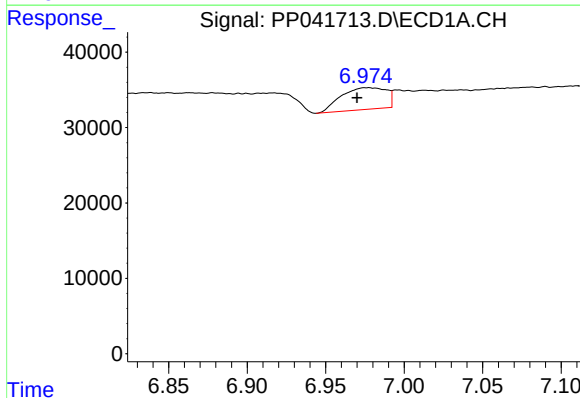


#26 AR-1254-1

R.T.: 6.978 min
Delta R.T.: 0.008 min
Response: 57764
Conc: 68.06 ng/ml

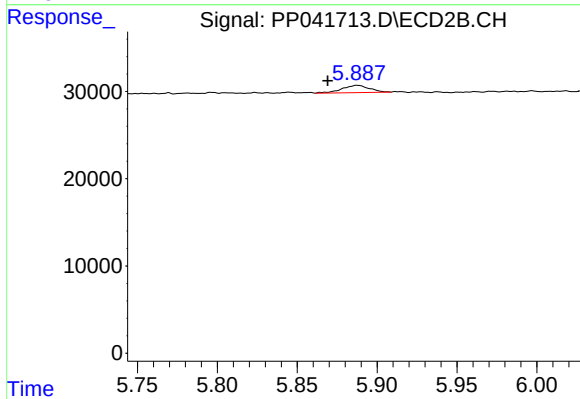

#26 AR-1254-1


R.T.: 5.888 min
Delta R.T.: 0.018 min
Response: 9850
Conc: 7.08 ng/ml

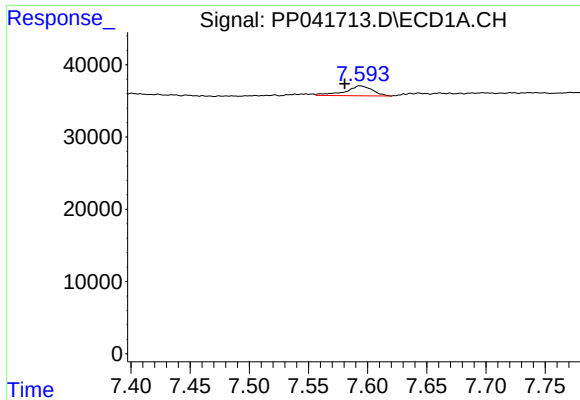

#28 AR-1254-3


R.T.: 7.594 min
Delta R.T.: 0.013 min
Response: 22070
Conc: 15.49 ng/ml

Instrument :
ECD_P
ClientSampleId :

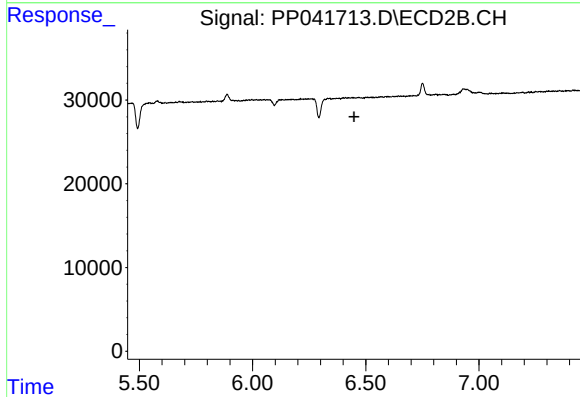


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.448 min
Response: 0
Conc: N.D.

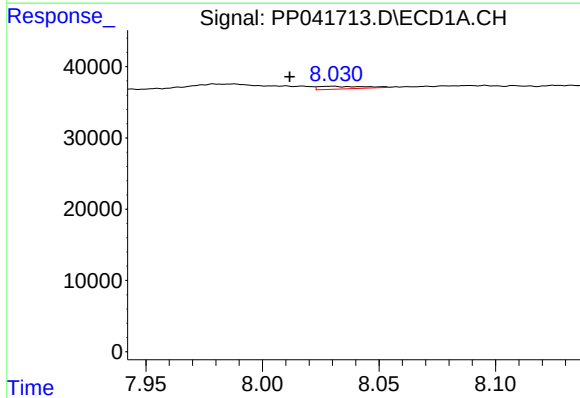


#32 AR-1260-2

R.T.: 8.030 min
Delta R.T.: 0.018 min
Response: 4982
Conc: 3.97 ng/ml

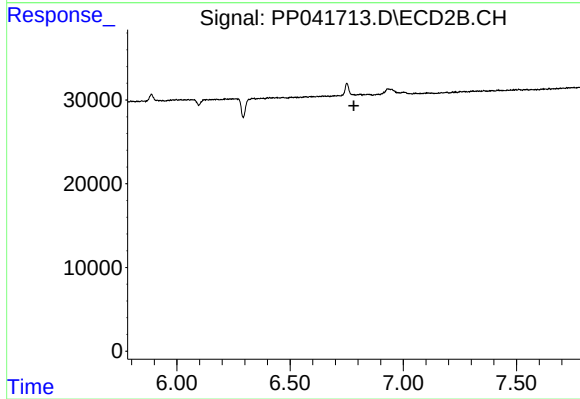

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

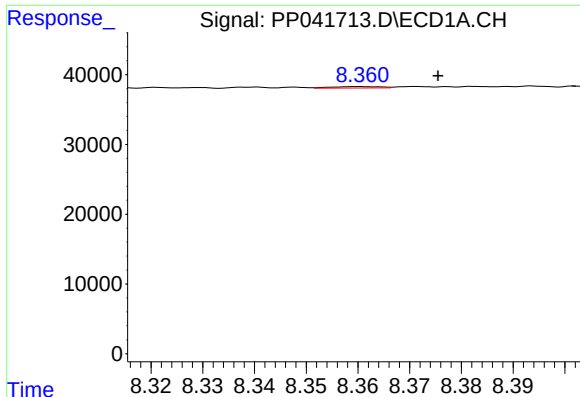

#33 AR-1260-3


R.T.: 8.360 min
Delta R.T.: -0.015 min
Response: 1271
Conc: 1.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

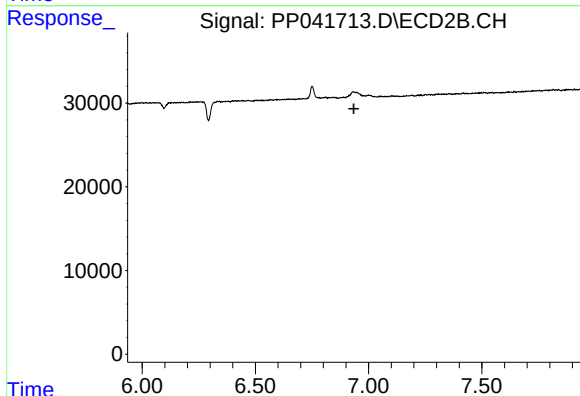


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

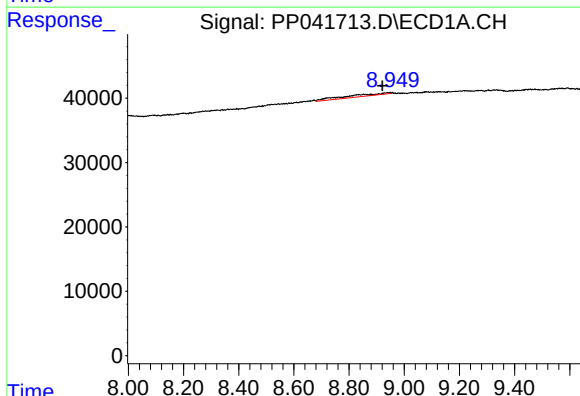


#35 AR-1260-5

R.T.: 8.949 min
Delta R.T.: 0.028 min
Response: 38649
Conc: 18.65 ng/ml

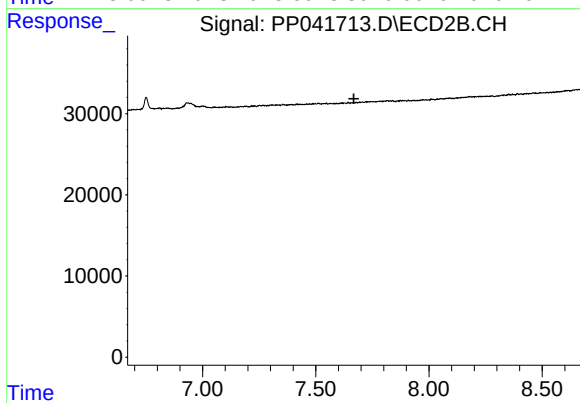

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

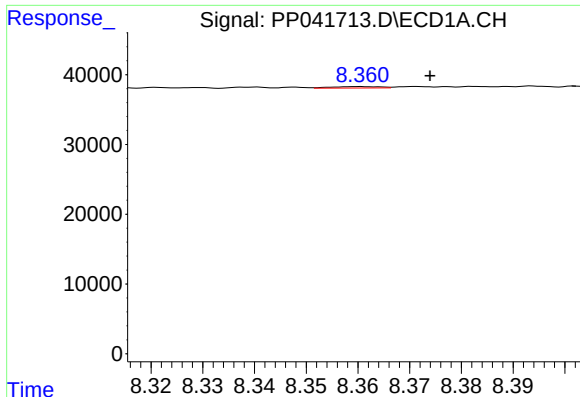

#36 AR-1262-1


R.T.: 8.360 min
Delta R.T.: -0.014 min
Response: 1271
Conc: 1.00 ng/ml

Instrument :
ECD_P
ClientSampleId :

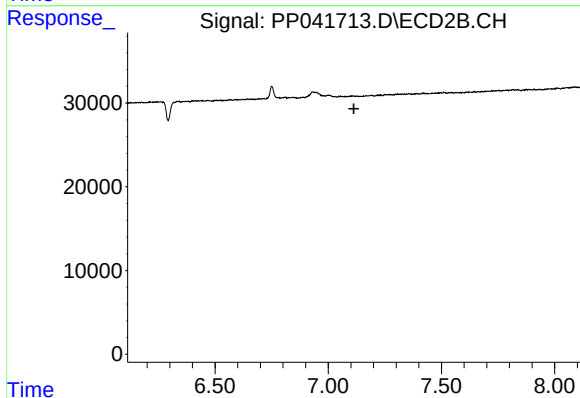


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

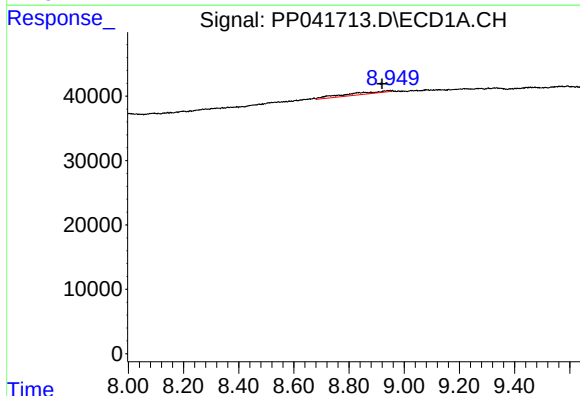

#37 AR-1262-2

R.T.: 8.949 min
Delta R.T.: 0.029 min
Response: 38649
Conc: 17.11 ng/ml

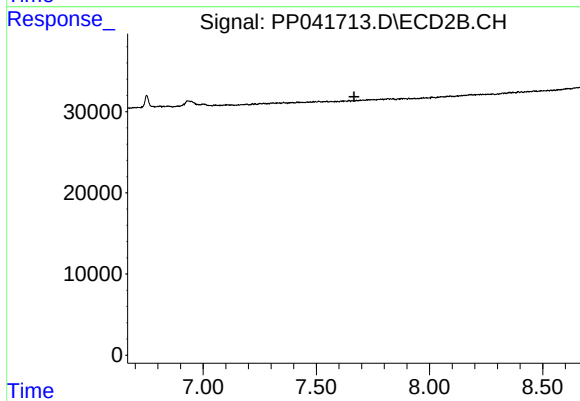

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.666 min
Response: 0
Conc: N.D.