

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120721\
 Data File : PP041744.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Dec 2021 20:44
 Operator : AJ\MA
 Sample : 500 PPB SPIKE TEST
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 500 PPB SPIKE TEST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 00:12:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
3)	L1	AR-1016-1	6.058	4.993	299722	348137	374.589	374.729
4)	L1	AR-1016-2	6.082	5.012	453393	534344	380.533	376.409
5)	L1	AR-1016-3	6.147	5.202	280903	287350	376.961	357.901
6)	L1	AR-1016-4	6.254	5.256	225495	223827	371.451	355.214
7)	L1	AR-1016-5	6.566	5.483	217750	282022	371.588	379.135
31)	L7	AR-1260-1	7.739	6.576	423559	461023	429.055	402.486
32)	L7	AR-1260-2	8.004	6.774	498127	542459	396.468	413.252
33)	L7	AR-1260-3	8.369	6.927	316612	502637	349.644	375.782
34)	L7	AR-1260-4	8.599	7.409	401521	348023	375.210	353.450
35)	L7	AR-1260-5	8.912	7.660	739943	750738	357.120	363.203


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120721\
Data File : PP041744.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Dec 2021 20:44
Operator : AJ\MA
Sample : 500 PPB SPIKE TEST
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 00:12:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

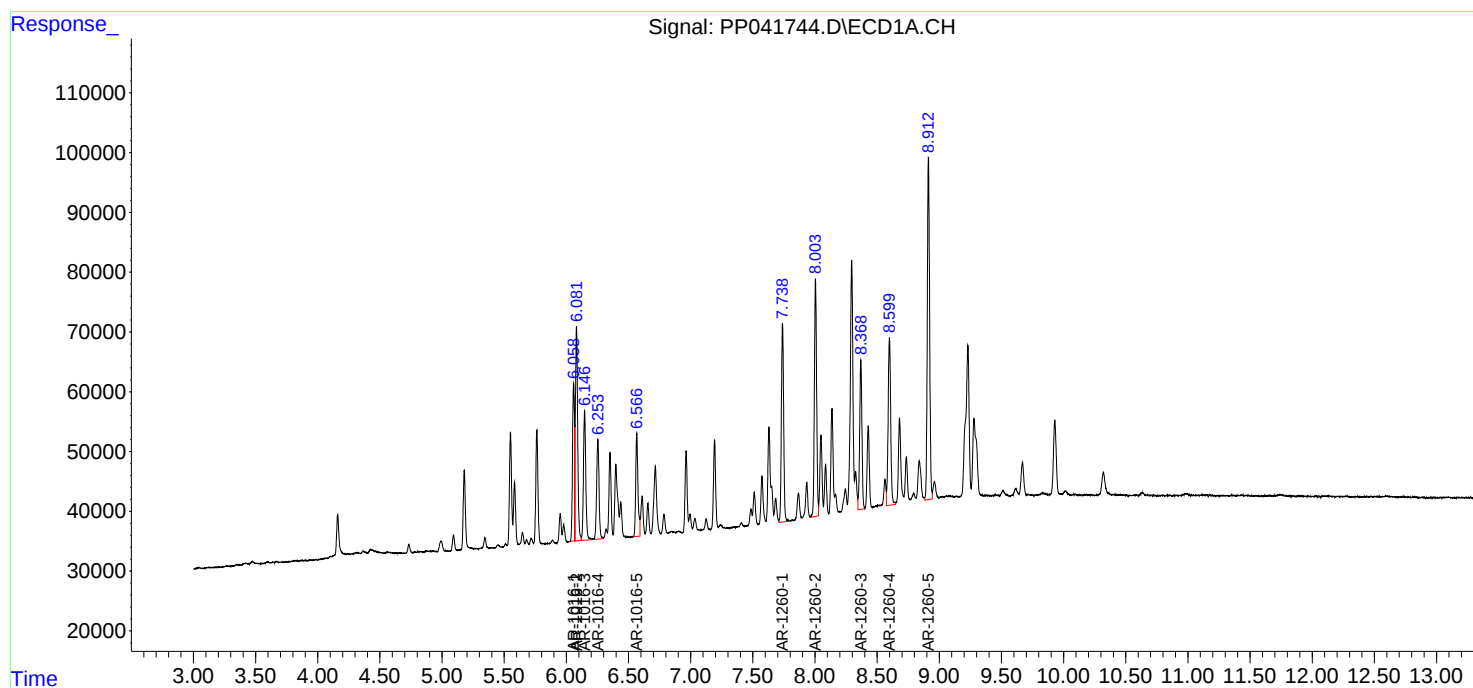


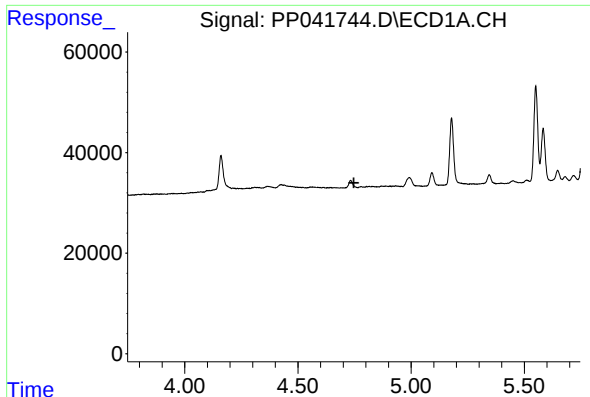

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

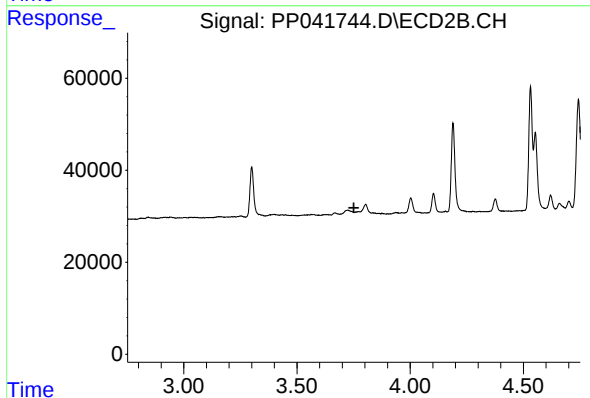


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.751 min
Response: 0
Conc: N.D.

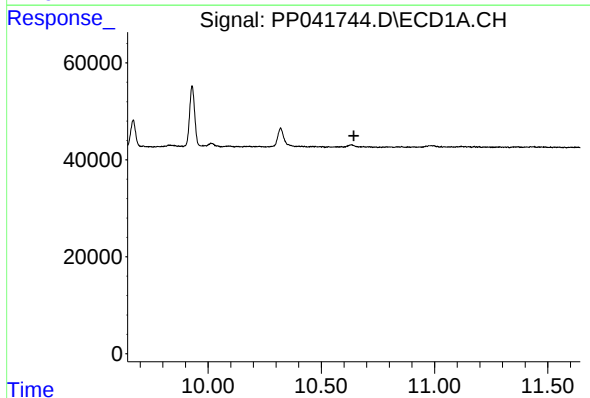


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.644 min
Response: 0
Conc: N.D.

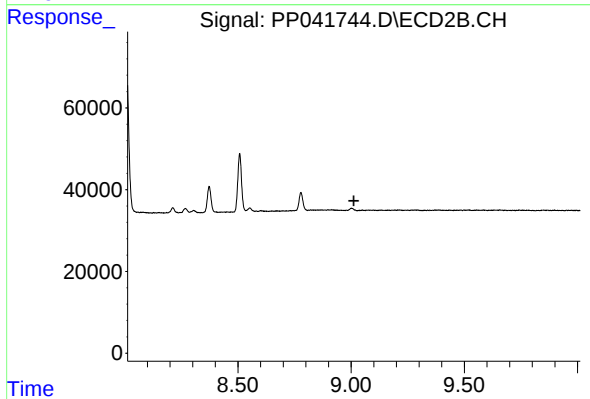

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.012 min
Response: 0
Conc: N.D.

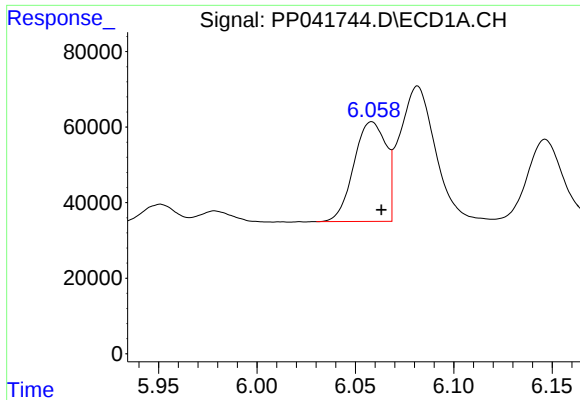

#3 AR-1016-1


R.T.: 6.058 min
Delta R.T.: -0.005 min
Response: 299722
Conc: 374.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

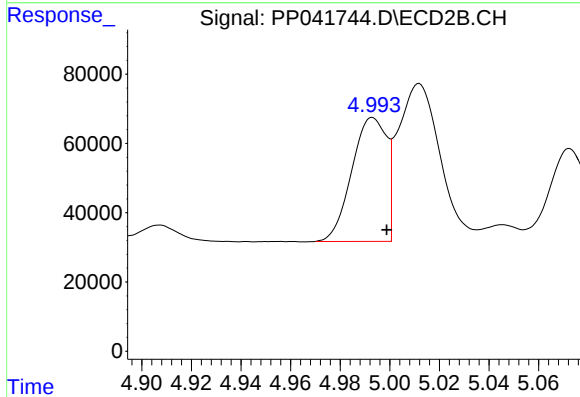


#3 AR-1016-1

R.T.: 4.993 min
Delta R.T.: -0.006 min
Response: 348137
Conc: 374.73 ng/ml

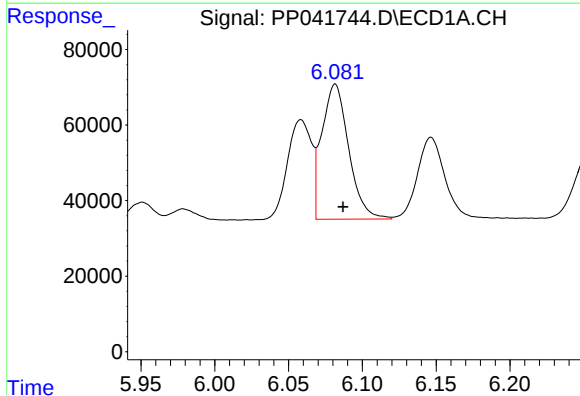


#4 AR-1016-2

R.T.: 6.082 min
Delta R.T.: -0.005 min
Response: 453393
Conc: 380.53 ng/ml

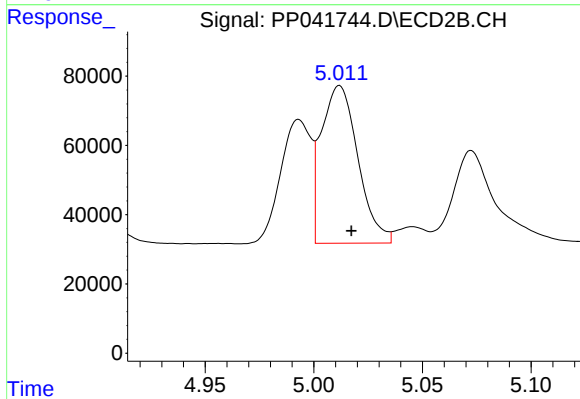

#4 AR-1016-2


R.T.: 5.012 min
Delta R.T.: -0.006 min
Response: 534344
Conc: 376.41 ng/ml

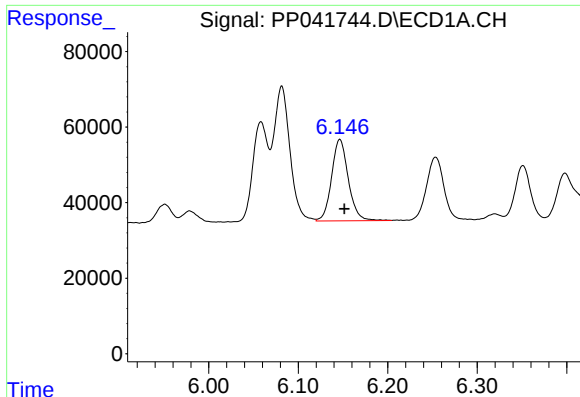

#5 AR-1016-3


R.T.: 6.147 min
Delta R.T.: -0.005 min
Response: 280903
Conc: 376.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

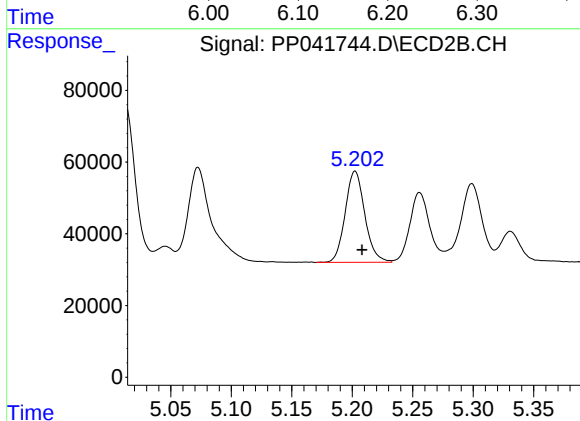


#5 AR-1016-3

R.T.: 5.202 min
Delta R.T.: -0.006 min
Response: 287350
Conc: 357.90 ng/ml

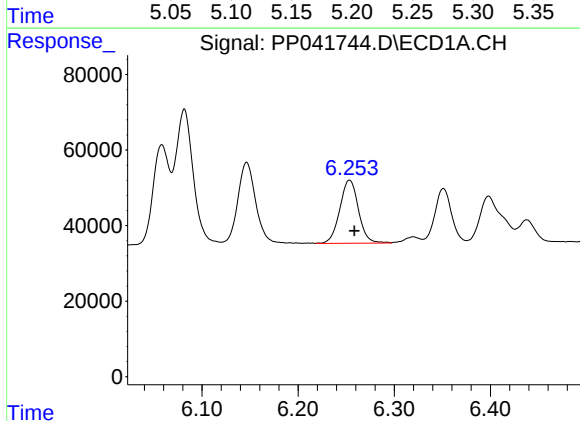


#6 AR-1016-4

R.T.: 6.254 min
Delta R.T.: -0.005 min
Response: 225495
Conc: 371.45 ng/ml

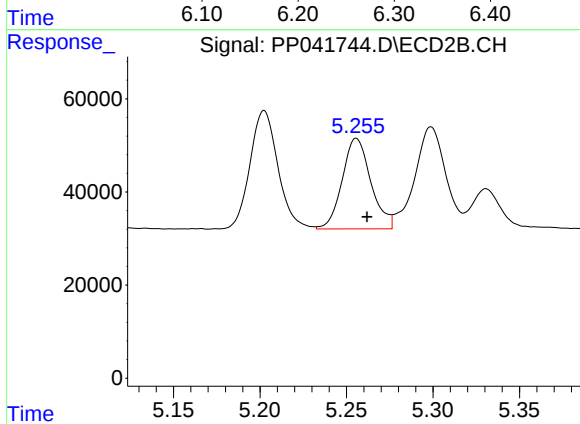

#6 AR-1016-4


R.T.: 5.256 min
Delta R.T.: -0.006 min
Response: 223827
Conc: 355.21 ng/ml

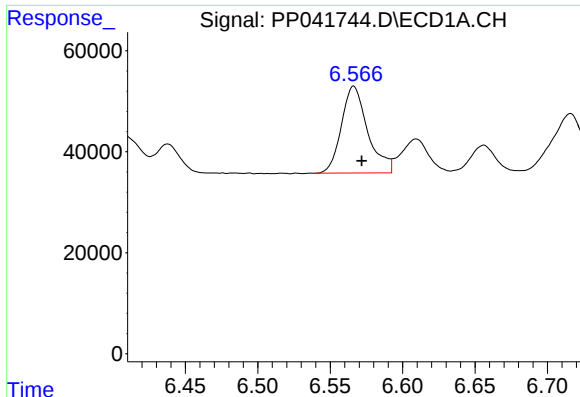

#7 AR-1016-5


R.T.: 6.566 min
Delta R.T.: -0.006 min
Response: 217750
Conc: 371.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

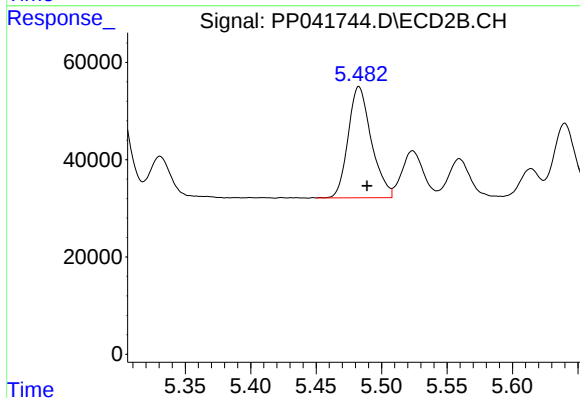


#7 AR-1016-5

R.T.: 5.483 min
Delta R.T.: -0.006 min
Response: 282022
Conc: 379.13 ng/ml

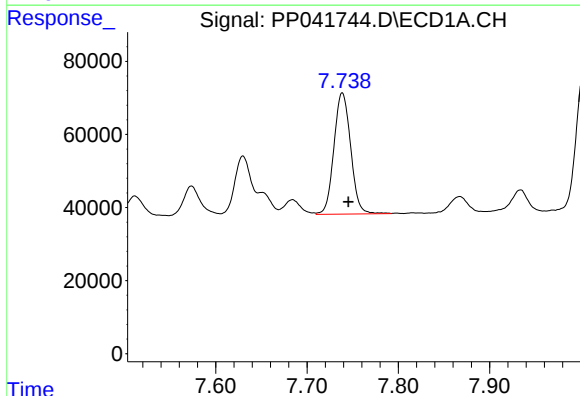


#31 AR-1260-1

R.T.: 7.739 min
Delta R.T.: -0.007 min
Response: 423559
Conc: 429.05 ng/ml

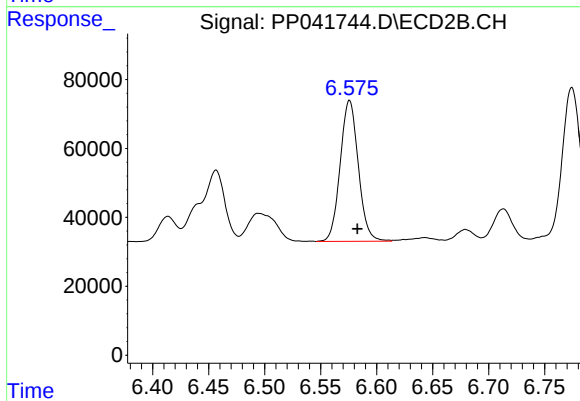

#31 AR-1260-1


R.T.: 6.576 min
Delta R.T.: -0.007 min
Response: 461023
Conc: 402.49 ng/ml

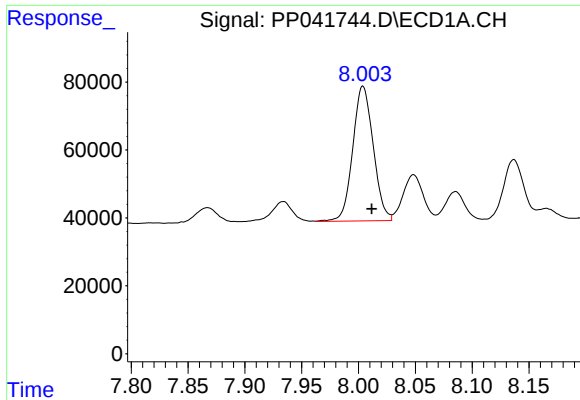

#32 AR-1260-2


R.T.: 8.004 min
Delta R.T.: -0.008 min
Response: 498127
Conc: 396.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

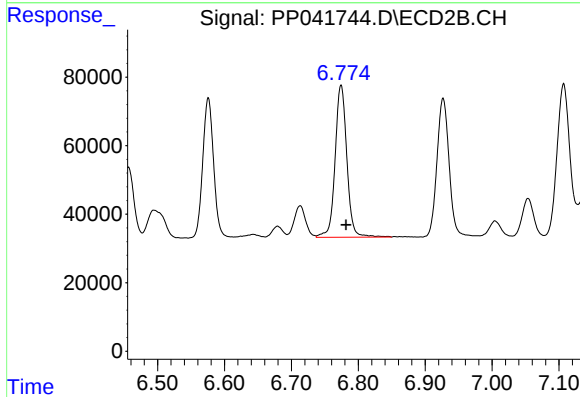


#32 AR-1260-2

R.T.: 6.774 min
Delta R.T.: -0.008 min
Response: 542459
Conc: 413.25 ng/ml

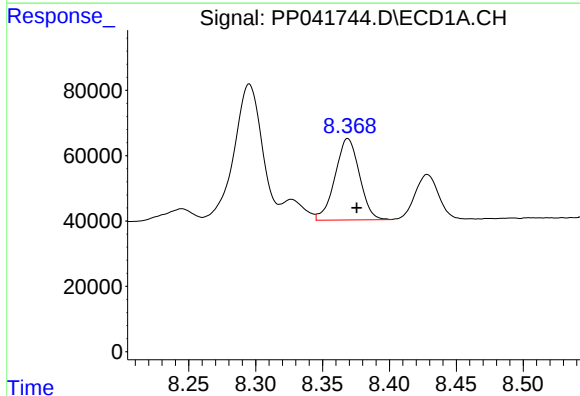


#33 AR-1260-3

R.T.: 8.369 min
Delta R.T.: -0.007 min
Response: 316612
Conc: 349.64 ng/ml

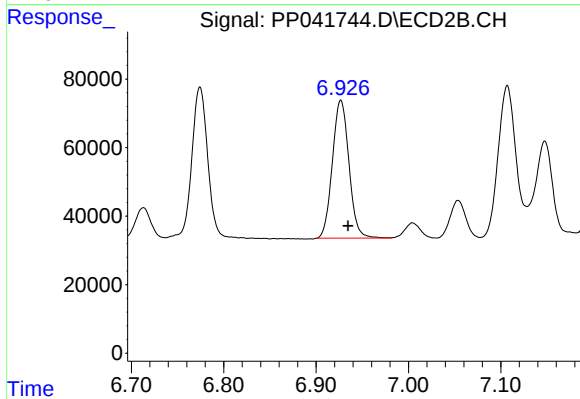

#33 AR-1260-3


R.T.: 6.927 min
Delta R.T.: -0.008 min
Response: 502637
Conc: 375.78 ng/ml

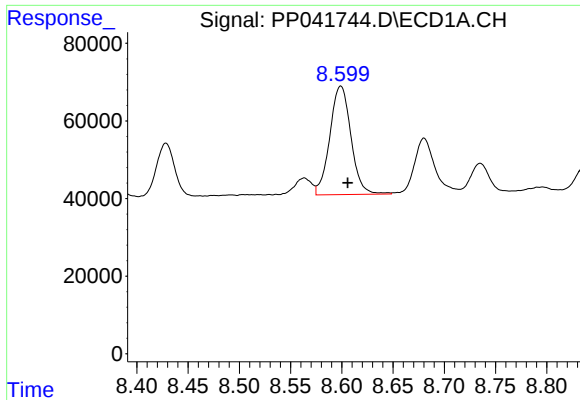

#34 AR-1260-4


R.T.: 8.599 min
Delta R.T.: -0.007 min
Response: 401521
Conc: 375.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

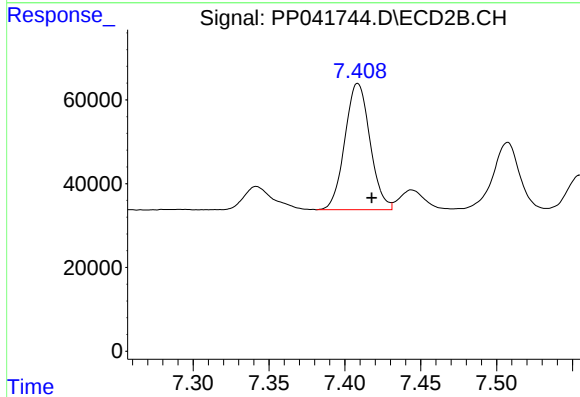


#34 AR-1260-4

R.T.: 7.409 min
Delta R.T.: -0.009 min
Response: 348023
Conc: 353.45 ng/ml

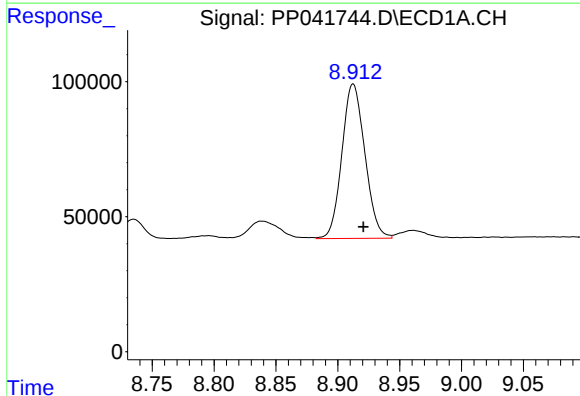

#35 AR-1260-5

R.T.: 8.912 min
Delta R.T.: -0.008 min
Response: 739943
Conc: 357.12 ng/ml

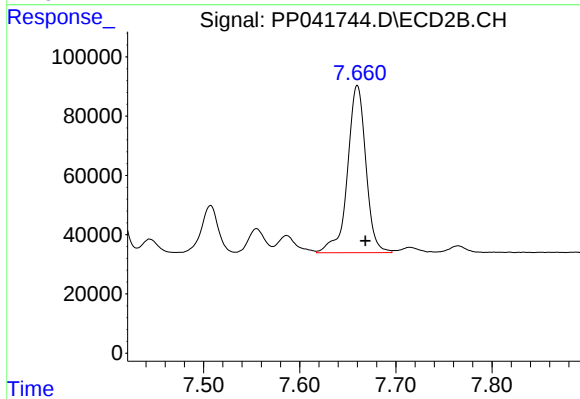

#35 AR-1260-5

R.T.: 7.660 min
Delta R.T.: -0.008 min
Response: 750738
Conc: 363.20 ng/ml